

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
 Data File : PL042060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2018 17:39
 Operator : AJ\SJ
 Sample : J5907-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-S

Manual Integrations
 APPROVED

sohil
 11/17/2018 4:18:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 03:36:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	47477175	25237603	7.689	8.518
28)	SA Decachlor...	8.206	9.230	52947883	21365584	7.729	8.377
Target Compounds							
12)	B 4,4'-DDE	5.624	6.460	51939247	34398530	7.592m	10.077 #
17)	MA 4,4'-DDT	6.376	7.251	42473653	11755401	7.467m	4.360m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
Data File : PL042060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2018 17:39
Operator : AJ\SJ
Sample : J5907-15
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-4-S


Manual Integrations
APPROVED

sohil
11/17/2018 4:18:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 03:36:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

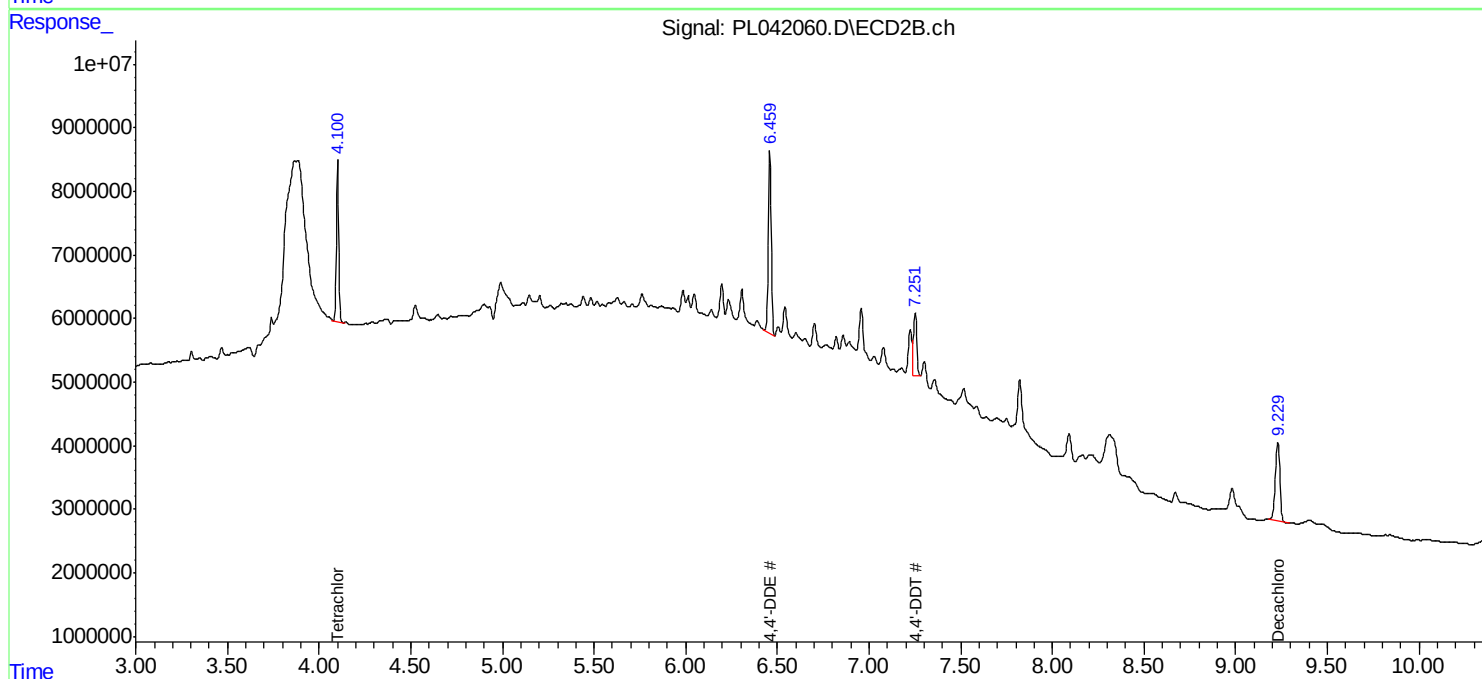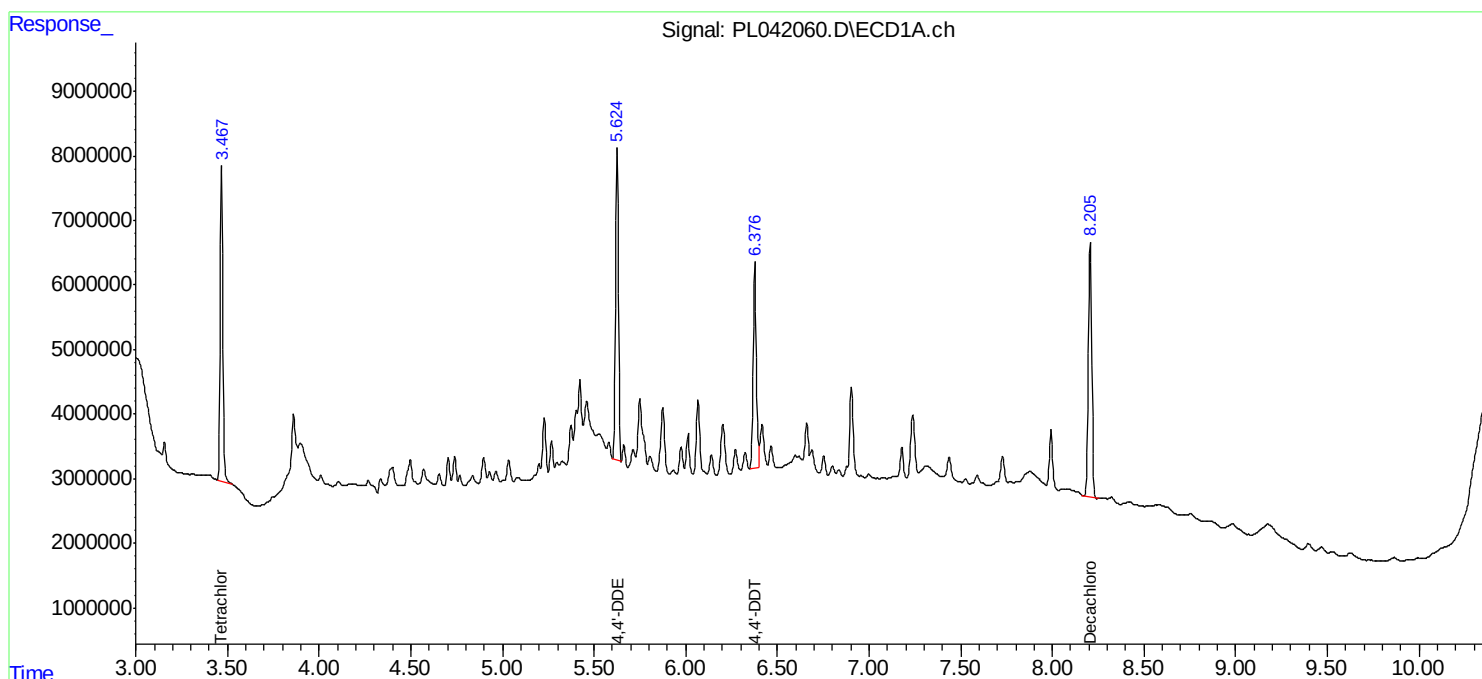

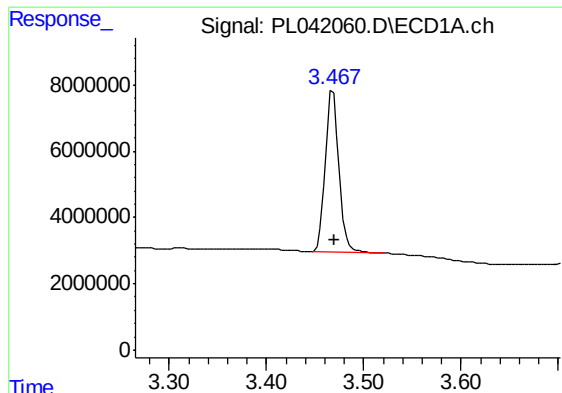


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: -0.002 min
Response: 47477175
Conc: 7.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-S


Manual Integrations
APPROVED

sohil
11/17/2018 4:18:18 AM

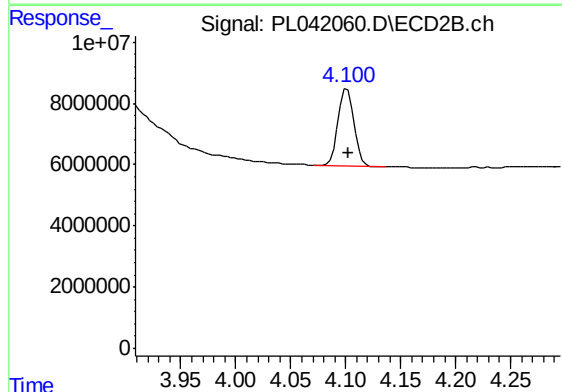


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 25237603
Conc: 8.52 ng/ml

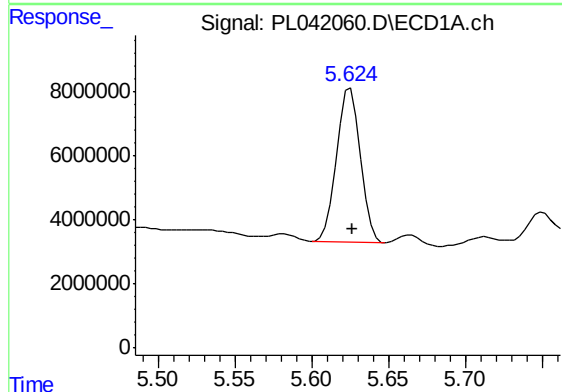


#12 4,4'-DDE

R.T.: 5.624 min
Delta R.T.: -0.003 min
Response: 51939247
Conc: 7.59 ng/ml m

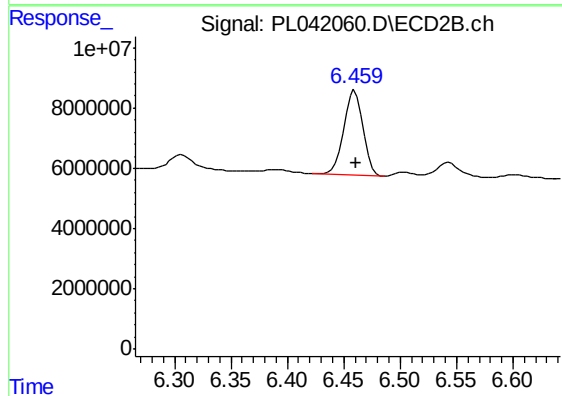

#12 4,4'-DDE

R.T.: 6.460 min
Delta R.T.: 0.000 min
Response: 34398530
Conc: 10.08 ng/ml

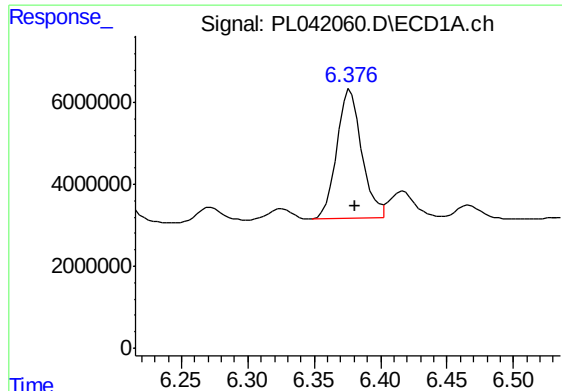


#17 4,4'-DDT

R.T.: 6.376 min
Delta R.T.: -0.005 min
Response: 42473653
Conc: 7.47 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-4-S


Manual Integrations
APPROVED

sohil
11/17/2018 4:18:18 AM

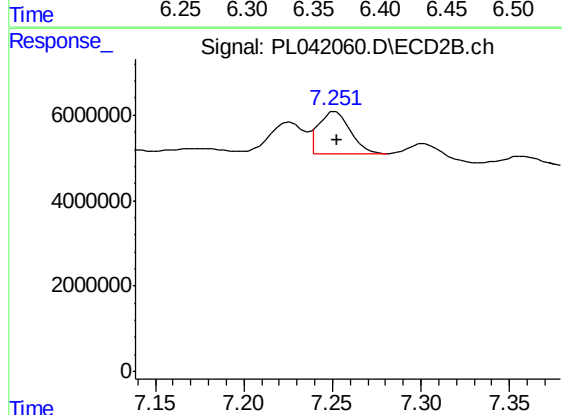


#17 4,4'-DDT

R.T.: 7.251 min
Delta R.T.: -0.002 min
Response: 11755401
Conc: 4.36 ng/ml m

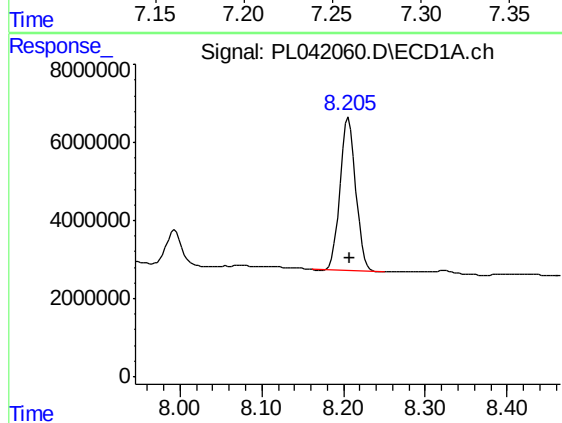

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.002 min
Response: 52947883
Conc: 7.73 ng/ml

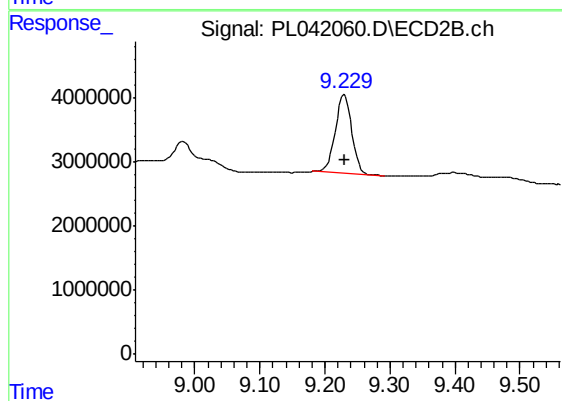

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.000 min
Response: 21365584
Conc: 8.38 ng/ml