

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111219\
 Data File : PL054191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2019 11:59
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:30:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	4.044	228.5E6	54799018	21.078	21.899
28)	SA Decachlor...	8.325	9.125	196.4E6	53213094	20.019	18.897
Target Compounds							
8)	B Heptachlo...	0.000	5.909f	0	364355	N.D.	0.125 #
9)	A Endosulfan I	5.637	6.267	4710628	407347	0.383	0.150 #
11)	B alpha-Chl...	5.562	0.000	6060048	0	0.456	N.D. #
12)	B 4,4'-DDE	5.732	0.000	4462361	0	0.376	N.D. #
14)	MA Endrin	6.128	0.000	6571882	0	0.567	N.D. #
17)	MA 4,4'-DDT	0.000	7.183	0	4004489	N.D.	1.732 #
22)	Mirex	0.000	8.258f	0	2732750	N.D.	1.351 #
26)	Chlordane-4	5.562	0.000	6060048	0	6.464	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111219\
Data File : PL054191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2019 11:59
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:30:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

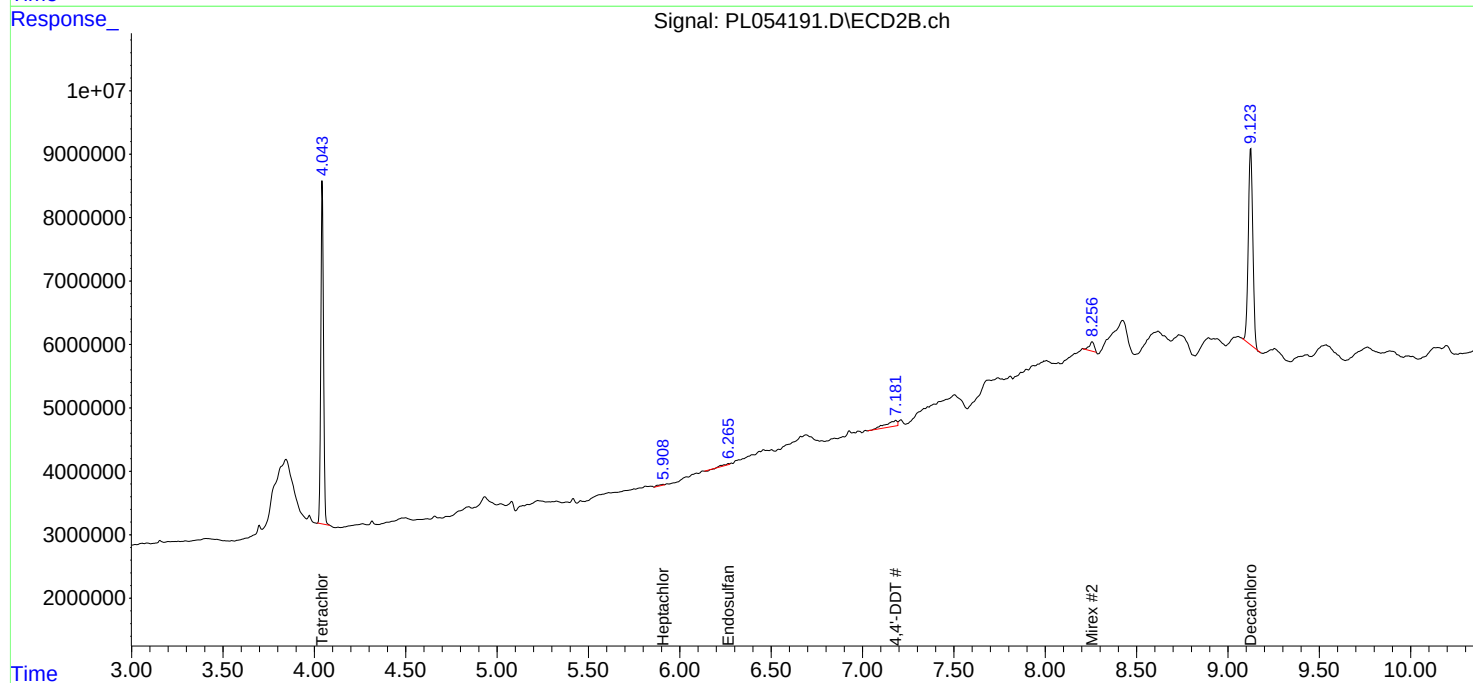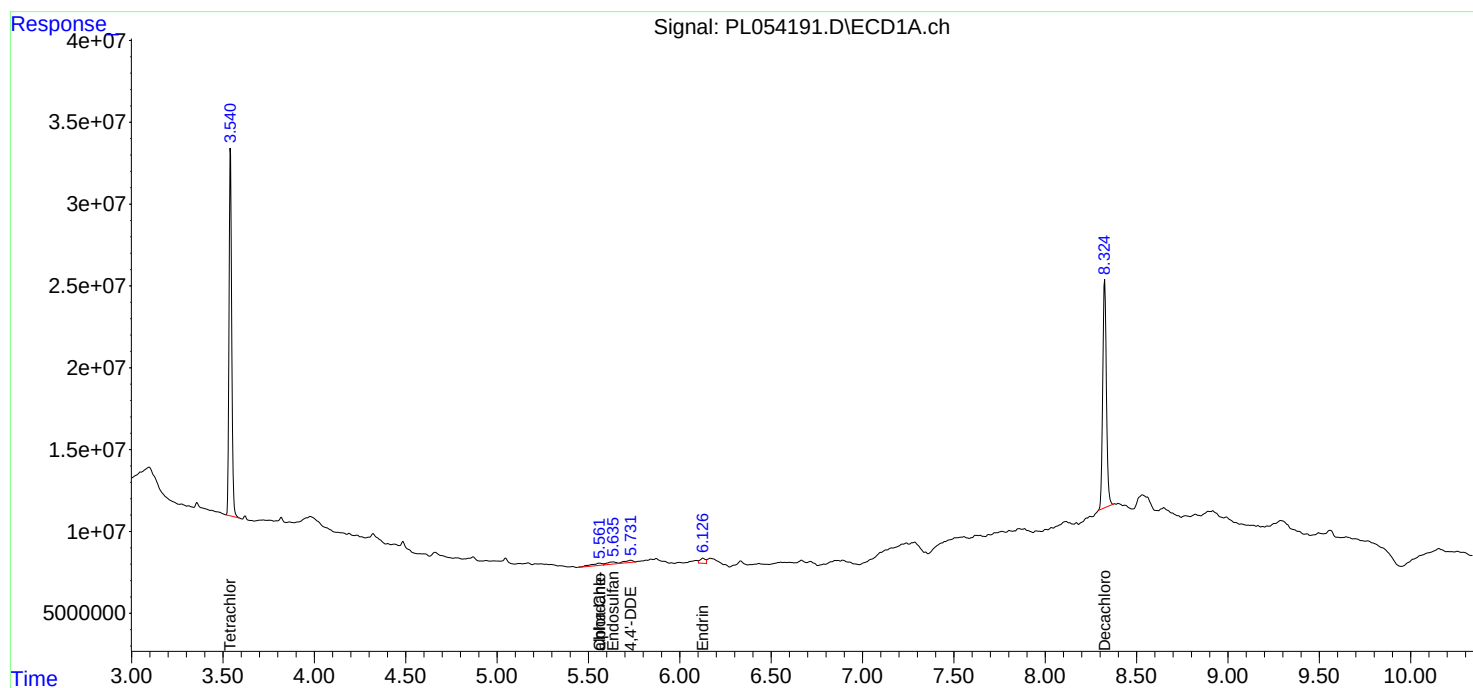


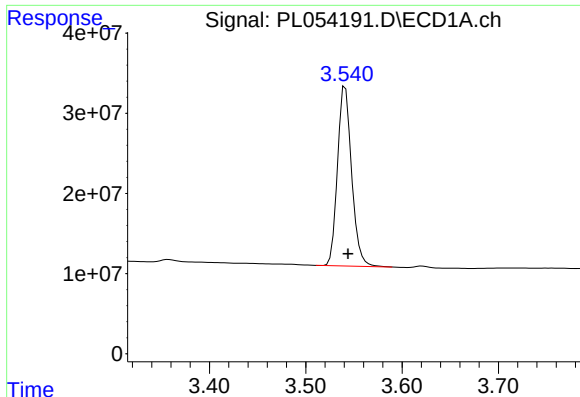

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: -0.003 min
Response: 228467815
Conc: 21.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

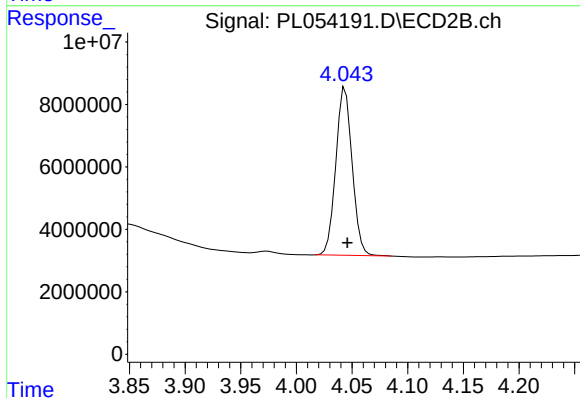


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 54799018
Conc: 21.90 ng/ml

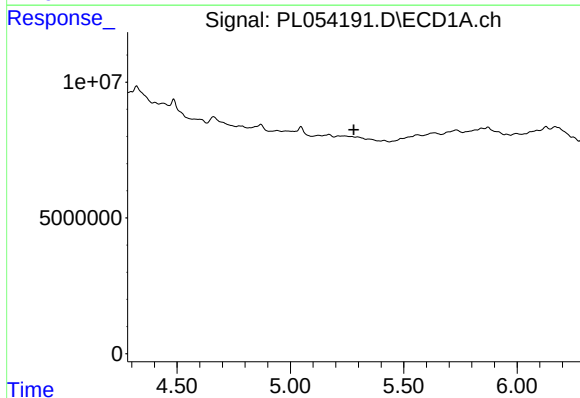


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

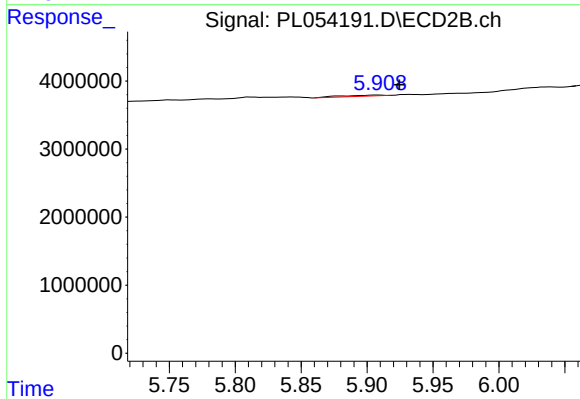

#8 Heptachlor epoxide


R.T.: 5.909 min
Delta R.T.: -0.015 min
Response: 364355
Conc: 0.12 ng/ml

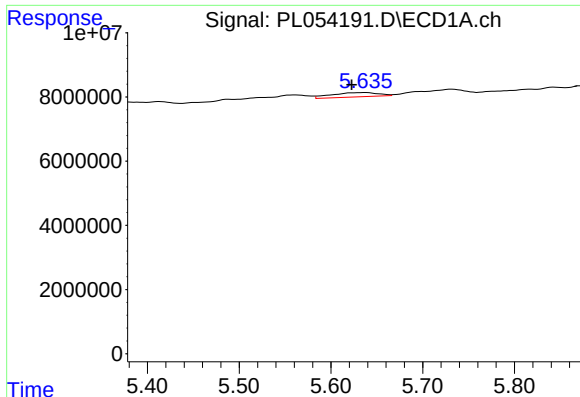

#9 Endosulfan I


R.T.: 5.637 min
Delta R.T.: 0.014 min
Response: 4710628
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

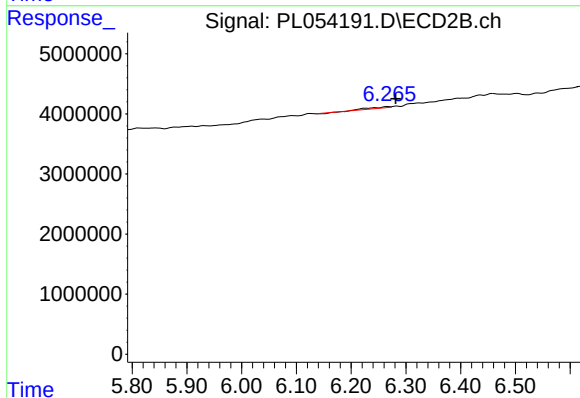


#9 Endosulfan I

R.T.: 6.267 min
Delta R.T.: -0.015 min
Response: 407347
Conc: 0.15 ng/ml

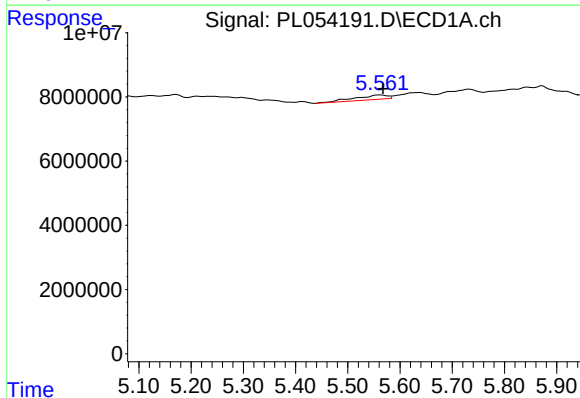


#11 alpha-Chlordane

R.T.: 5.562 min
Delta R.T.: -0.006 min
Response: 6060048
Conc: 0.46 ng/ml

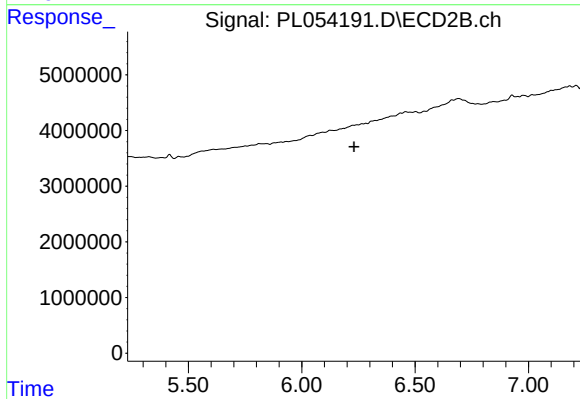

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

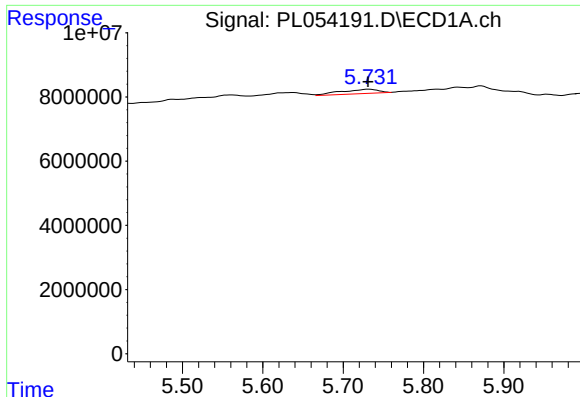

#12 4,4'-DDE


R.T.: 5.732 min
Delta R.T.: 0.002 min
Response: 4462361
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

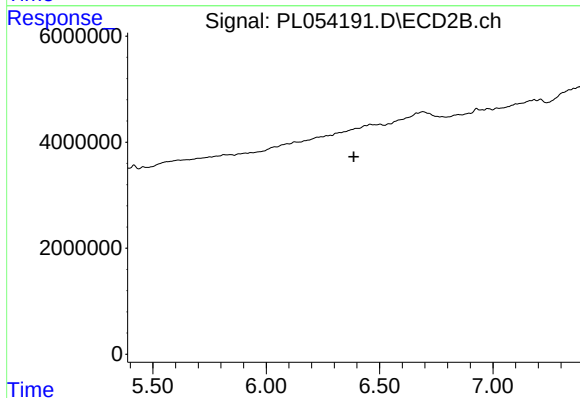


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

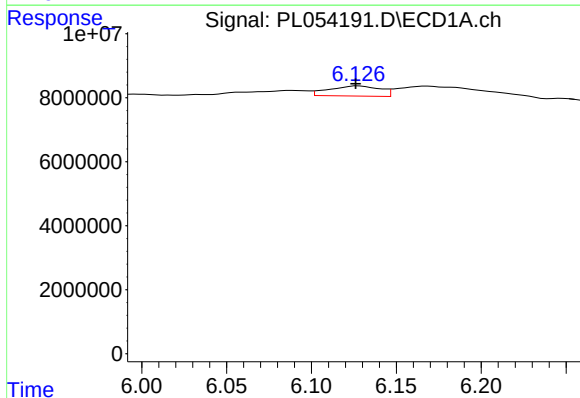


#14 Endrin

R.T.: 6.128 min
Delta R.T.: 0.001 min
Response: 6571882
Conc: 0.57 ng/ml

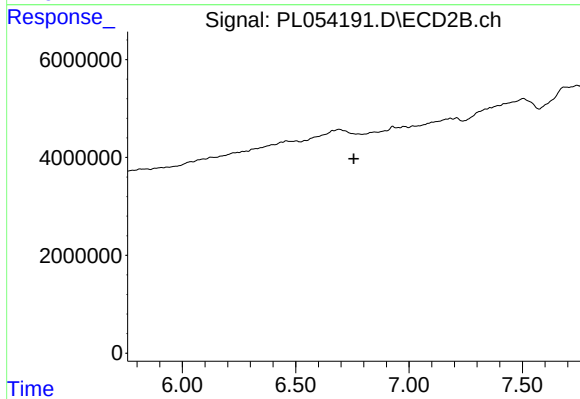

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.756 min
Response: 0
Conc: N.D.

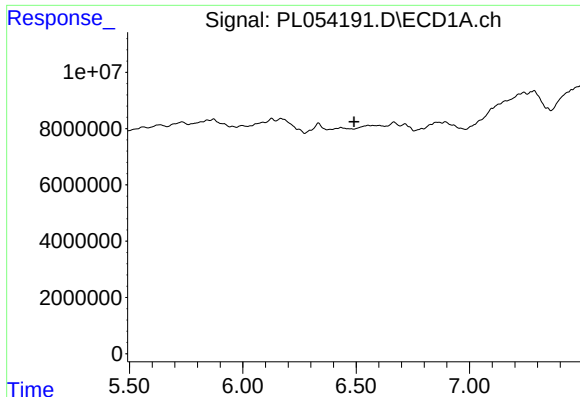

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

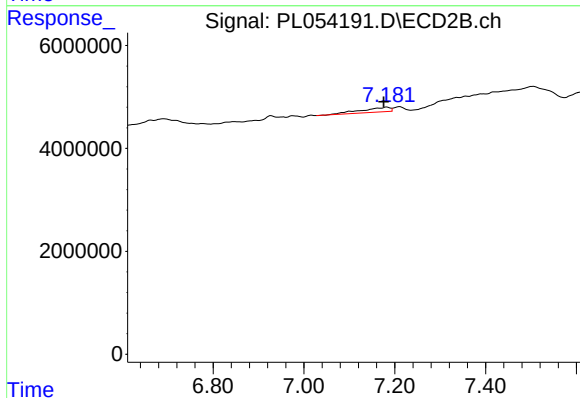


#17 4,4'-DDT

R.T.: 7.183 min
Delta R.T.: 0.007 min
Response: 4004489
Conc: 1.73 ng/ml

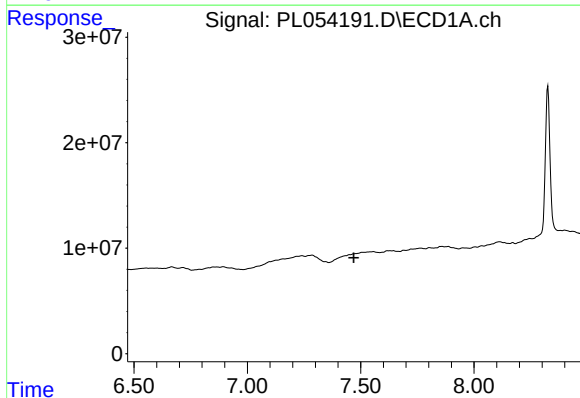


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.469 min
Response: 0
Conc: N.D.

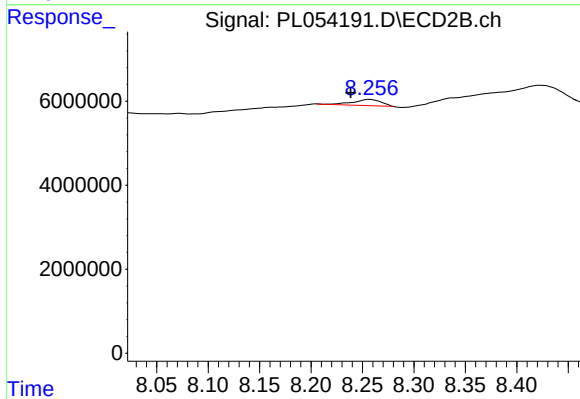

#22 Mirex


R.T.: 8.258 min
Delta R.T.: 0.019 min
Response: 2732750
Conc: 1.35 ng/ml

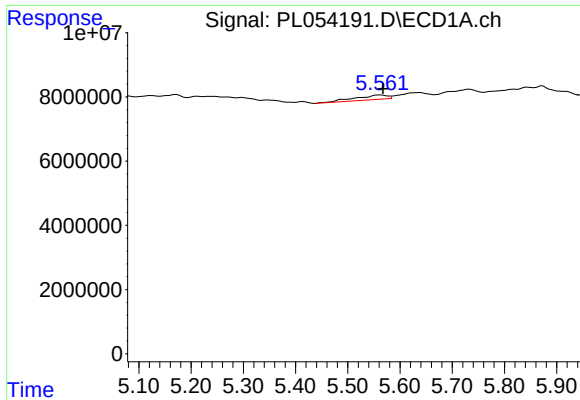

#26 Chlordane-4


R.T.: 5.562 min
Delta R.T.: -0.006 min
Response: 6060048
Conc: 6.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

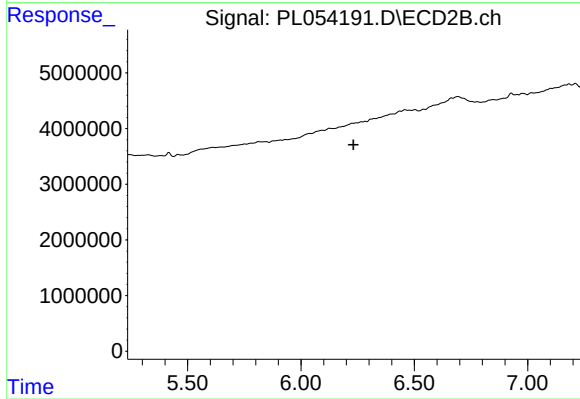


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

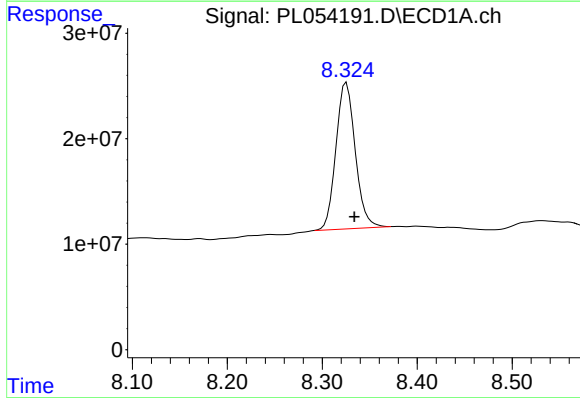

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 196414508
Conc: 20.02 ng/ml

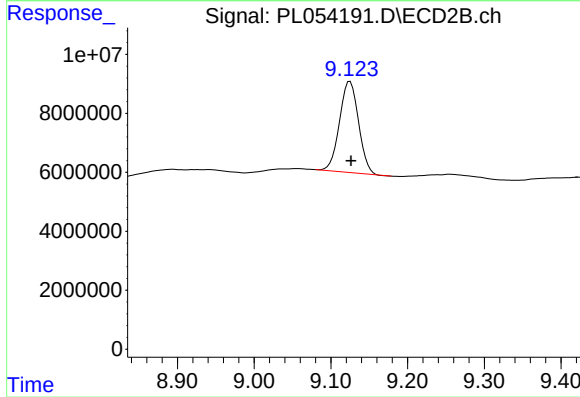

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: -0.001 min
Response: 53213094
Conc: 18.90 ng/ml