

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111219\
 Data File : PL054194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2019 13:51
 Operator : SG\AJ
 Sample : PB124716BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:30:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.044	226.4E6	51629473	20.884	20.632
28)	SA Decachlor...	8.327	9.126	194.9E6	55012465	19.869	19.536
Target Compounds							
3)	MA gamma-BHC...	4.278	0.000	1083488	0	0.070	N.D. #
4)	MA Heptachlor	4.586	0.000	9119869	0	0.578	N.D. #
6)	B beta-BHC	4.537	0.000	3298367	0	0.501	N.D. #
7)	B delta-BHC	4.732	5.083f	1442626	2046819	0.095	0.678 #
8)	B Heptachlo...	5.279	0.000	7203700	0	0.534	N.D. #
22)	Mirex	7.442f	0.000	3810181	0	0.445	N.D. #
23)	Chlordane-1	4.446f	0.000	5625203	0	15.860	N.D. #
24)	Chlordane-2	4.956f	5.500	4030849	5972659	10.461	60.808 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111219\
Data File : PL054194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2019 13:51
Operator : SG\AJ
Sample : PB124716BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:30:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

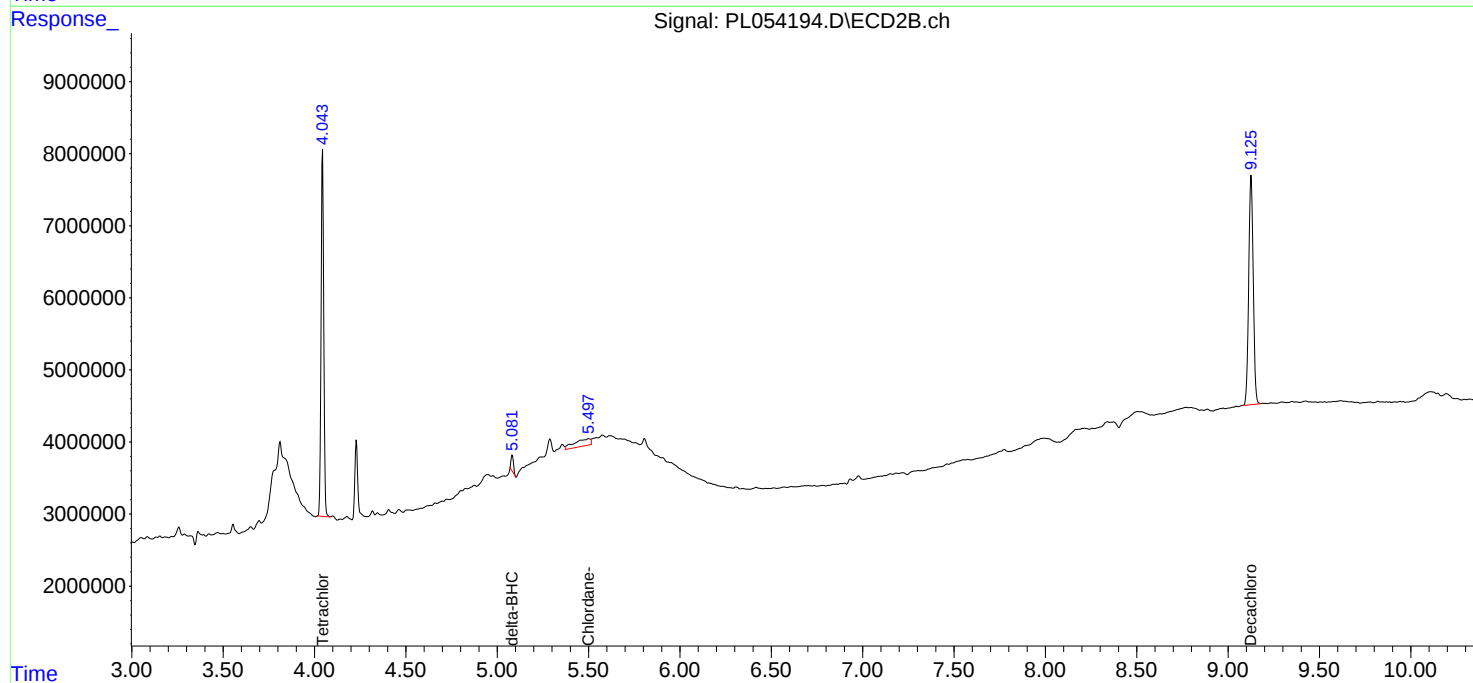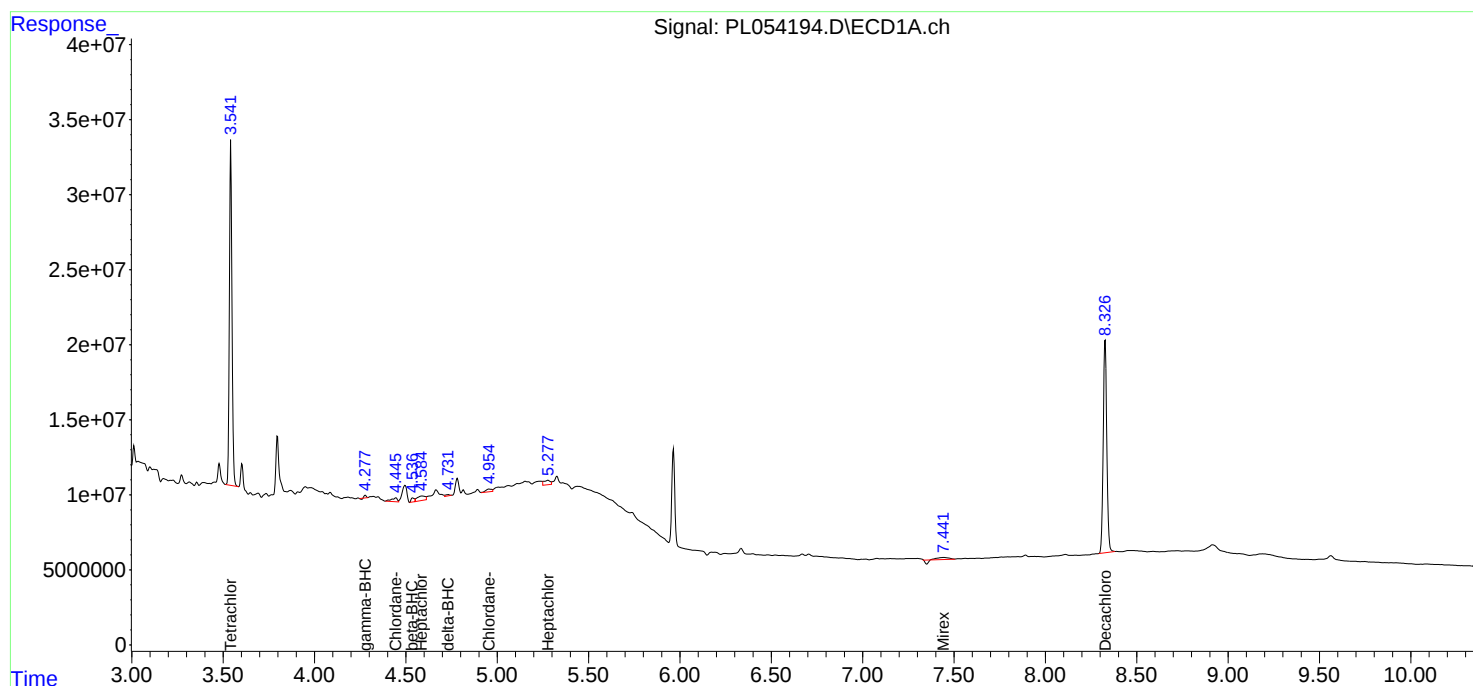


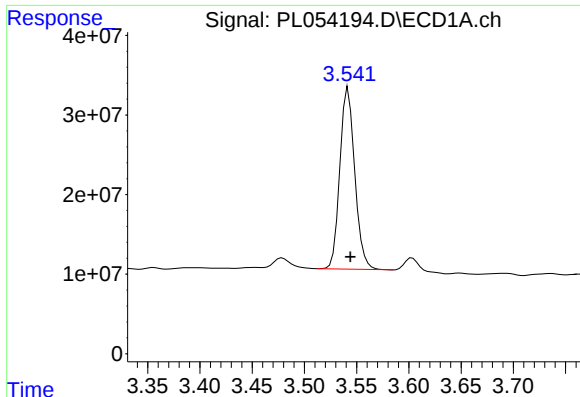

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 226371421
Conc: 20.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

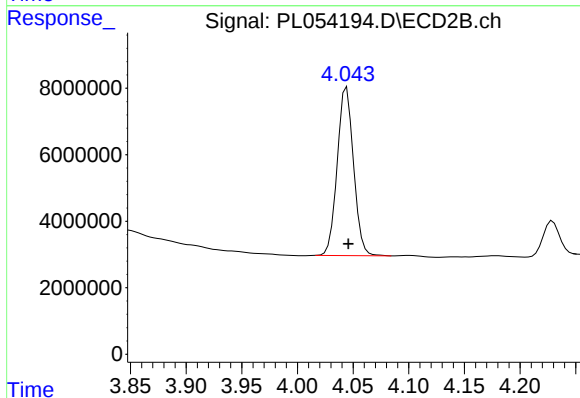


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 51629473
Conc: 20.63 ng/ml

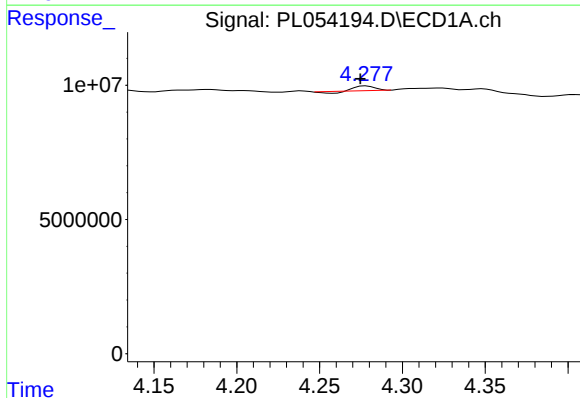


#3 gamma-BHC (Lindane)

R.T.: 4.278 min
Delta R.T.: 0.003 min
Response: 1083488
Conc: 0.07 ng/ml

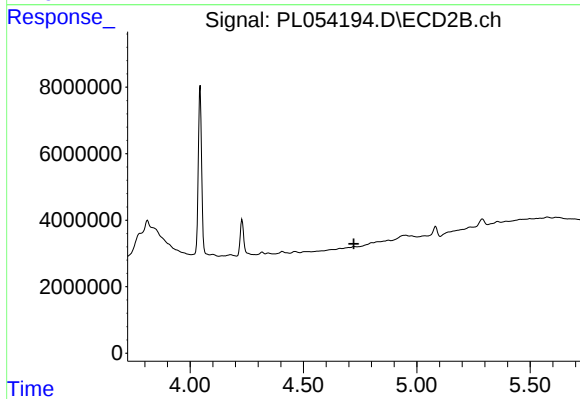

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.722 min
Response: 0
Conc: N.D.

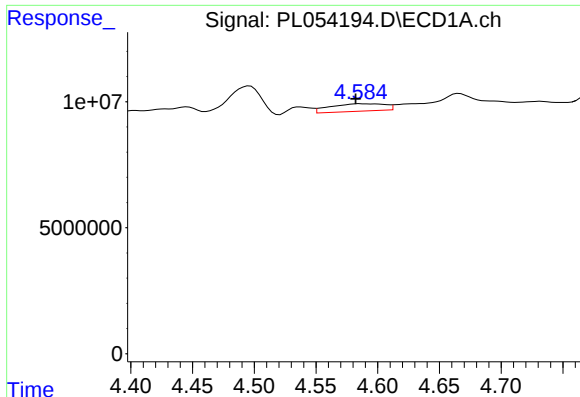

#4 Heptachlor


R.T.: 4.586 min
Delta R.T.: 0.004 min
Response: 9119869
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

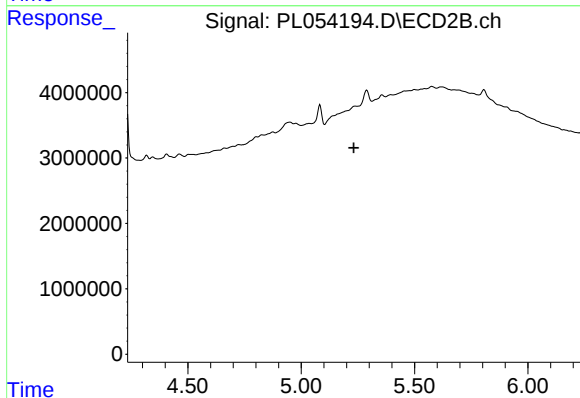


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.232 min
Response: 0
Conc: N.D.

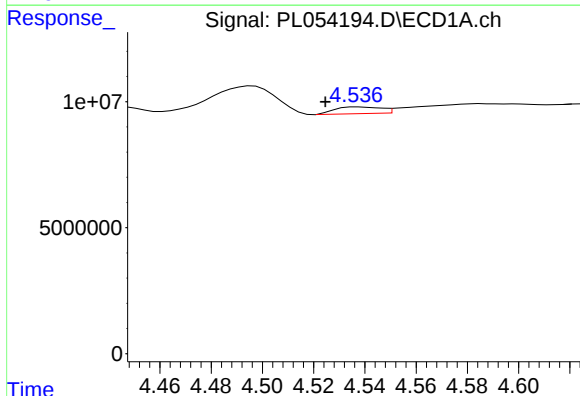


#6 beta-BHC

R.T.: 4.537 min
Delta R.T.: 0.013 min
Response: 3298367
Conc: 0.50 ng/ml

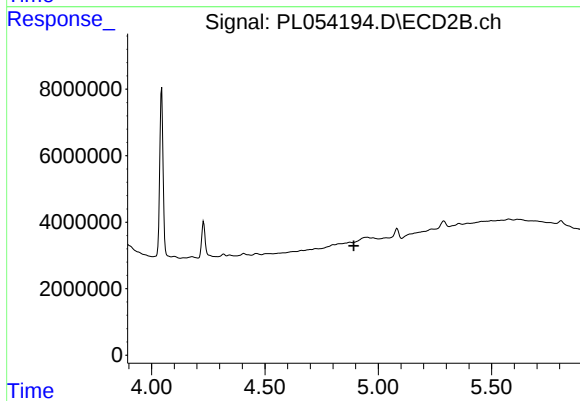

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

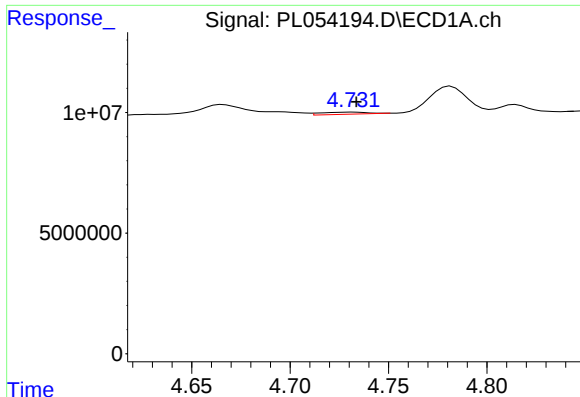

#7 delta-BHC


R.T.: 4.732 min
Delta R.T.: -0.002 min
Response: 1442626
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

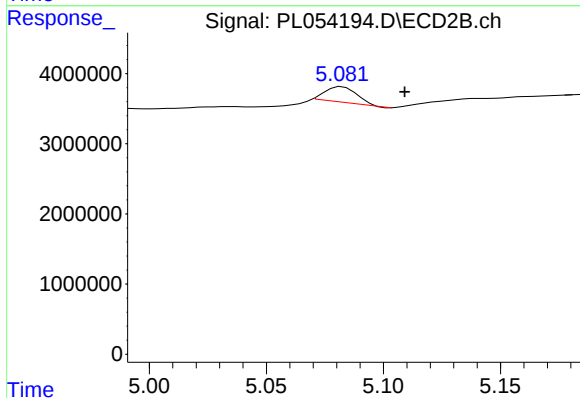


#7 delta-BHC

R.T.: 5.083 min
Delta R.T.: -0.027 min
Response: 2046819
Conc: 0.68 ng/ml

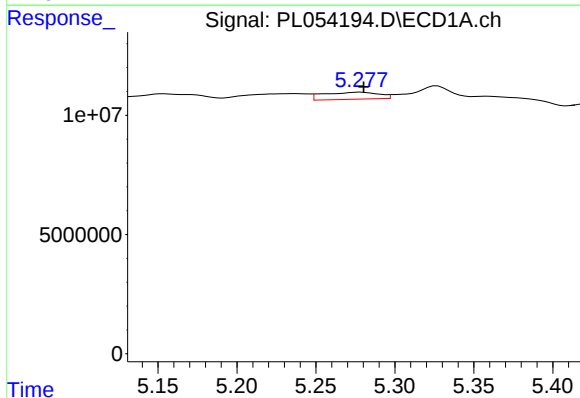


#8 Heptachlor epoxide

R.T.: 5.279 min
Delta R.T.: -0.002 min
Response: 7203700
Conc: 0.53 ng/ml

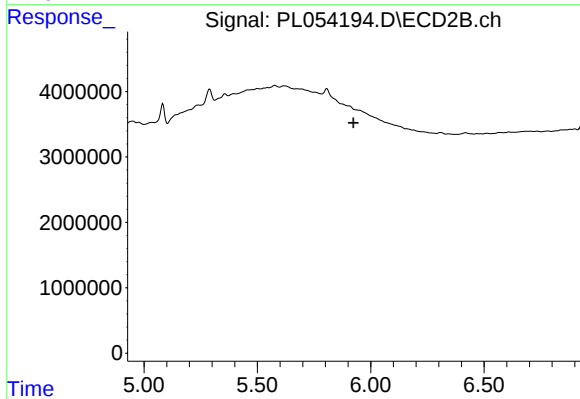

#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

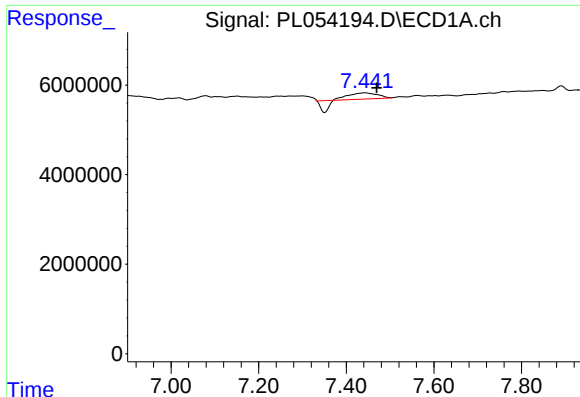

#22 Mirex


R.T.: 7.442 min

Delta R.T.: -0.027 min

Response: 3810181

Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

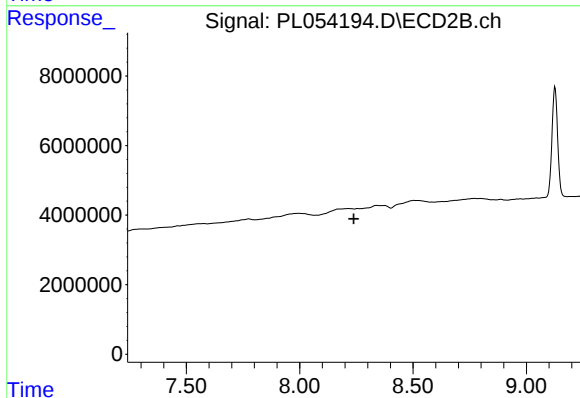


#22 Mirex

R.T.: 0.000 min

Exp R.T. : 8.239 min

Response: 0

Conc: N.D.

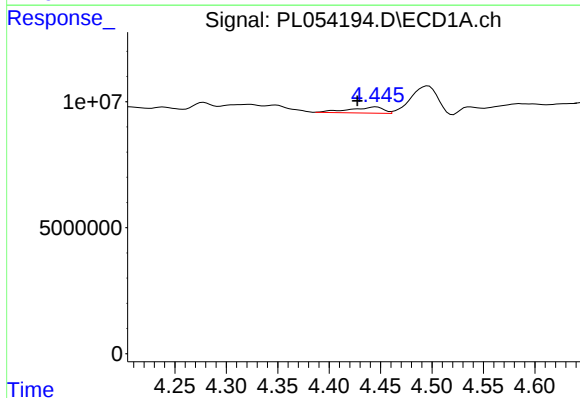


#23 Chlordane-1

R.T.: 4.446 min

Delta R.T.: 0.018 min

Response: 5625203

Conc: 15.86 ng/ml

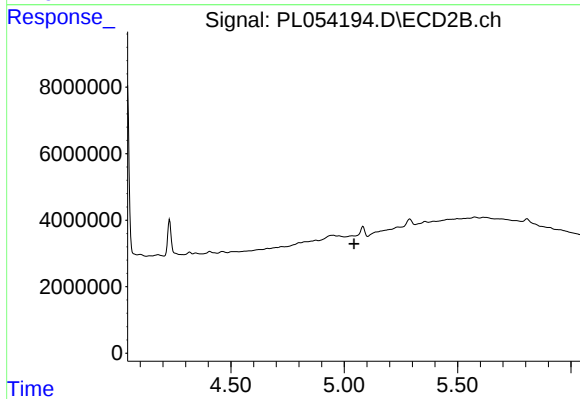


#23 Chlordane-1

R.T.: 0.000 min

Exp R.T. : 5.043 min

Response: 0


Conc: N.D.

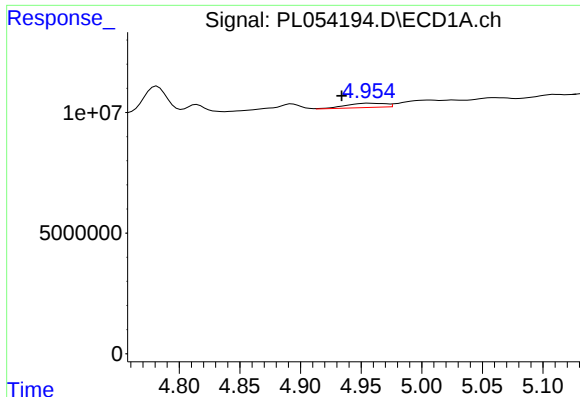

#24 Chlordane-2


R.T.: 4.956 min
Delta R.T.: 0.022 min
Response: 4030849
Conc: 10.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

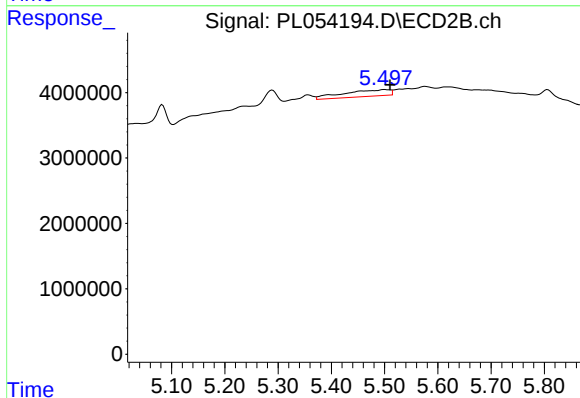


#24 Chlordane-2

R.T.: 5.500 min
Delta R.T.: -0.011 min
Response: 5972659
Conc: 60.81 ng/ml

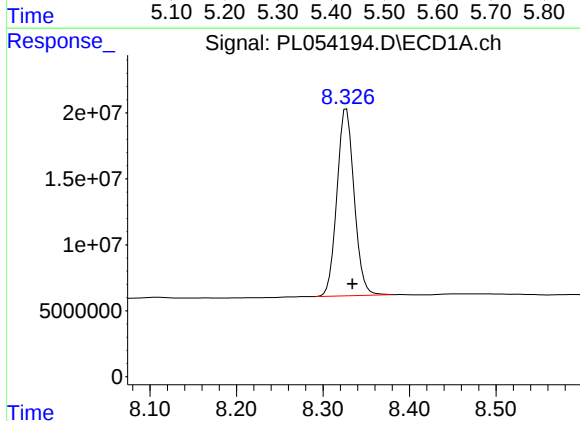

#28 Decachlorobiphenyl

R.T.: 8.327 min
Delta R.T.: -0.007 min
Response: 194947330
Conc: 19.87 ng/ml

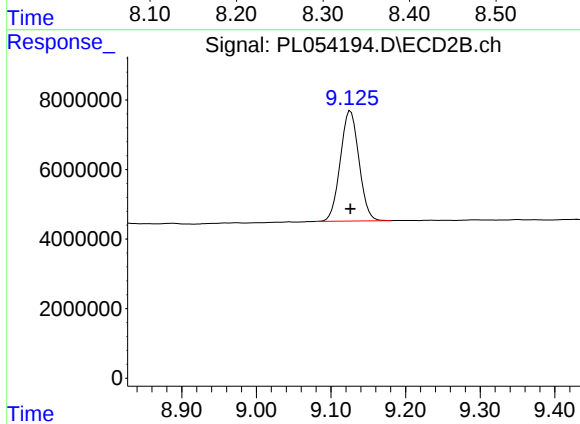

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 55012465
Conc: 19.54 ng/ml