

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111219\
 Data File : PL054219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2019 19:52
 Operator : SG\AJ
 Sample : K5760-13
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:35:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.044	201.8E6	49387683	18.617	19.736
28)	SA Decachlor...	8.324	9.123	157.5E6	47143221	16.051	16.741
Target Compounds							
7)	B delta-BHC	0.000	5.083f	0	2345871	N.D.	0.777 #
23)	Chlordane-1	4.457f	0.000	12612210	0	35.560	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111219\
Data File : PL054219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2019 19:52
Operator : SG\AJ
Sample : K5760-13
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:35:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

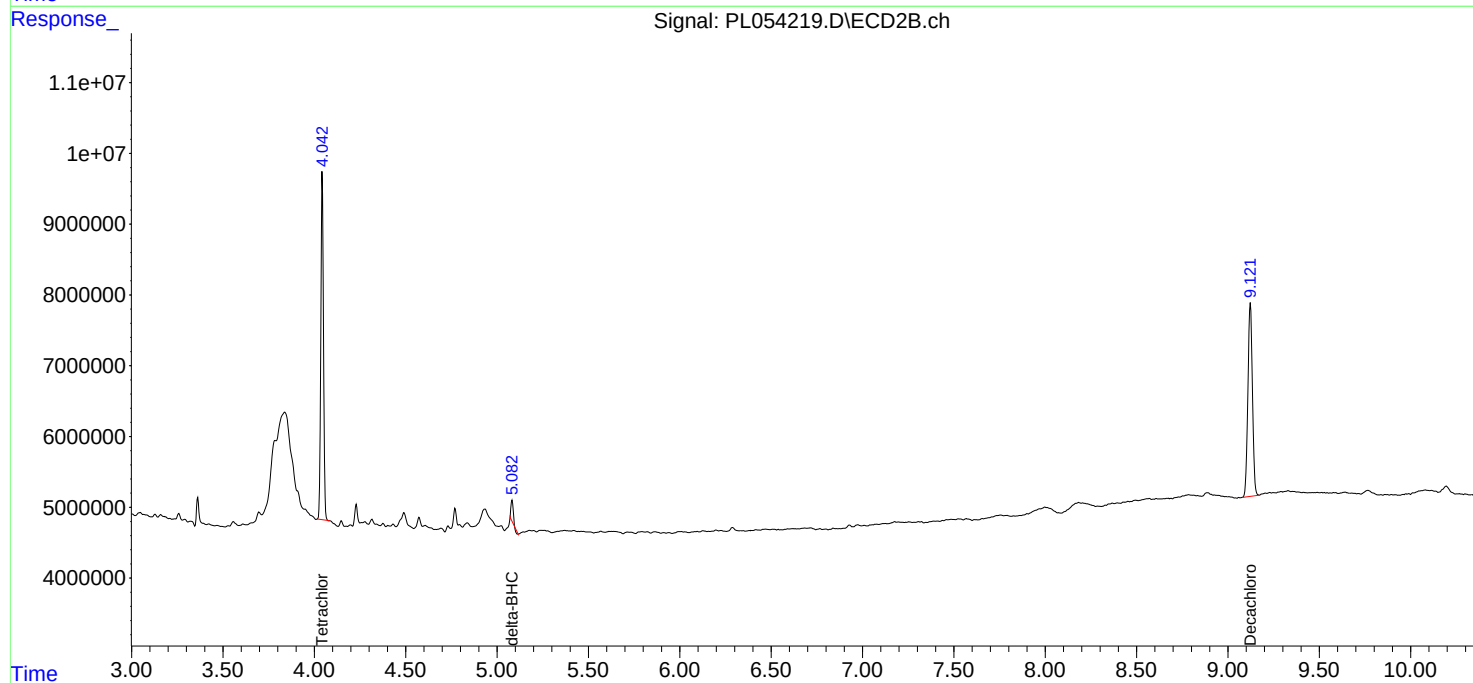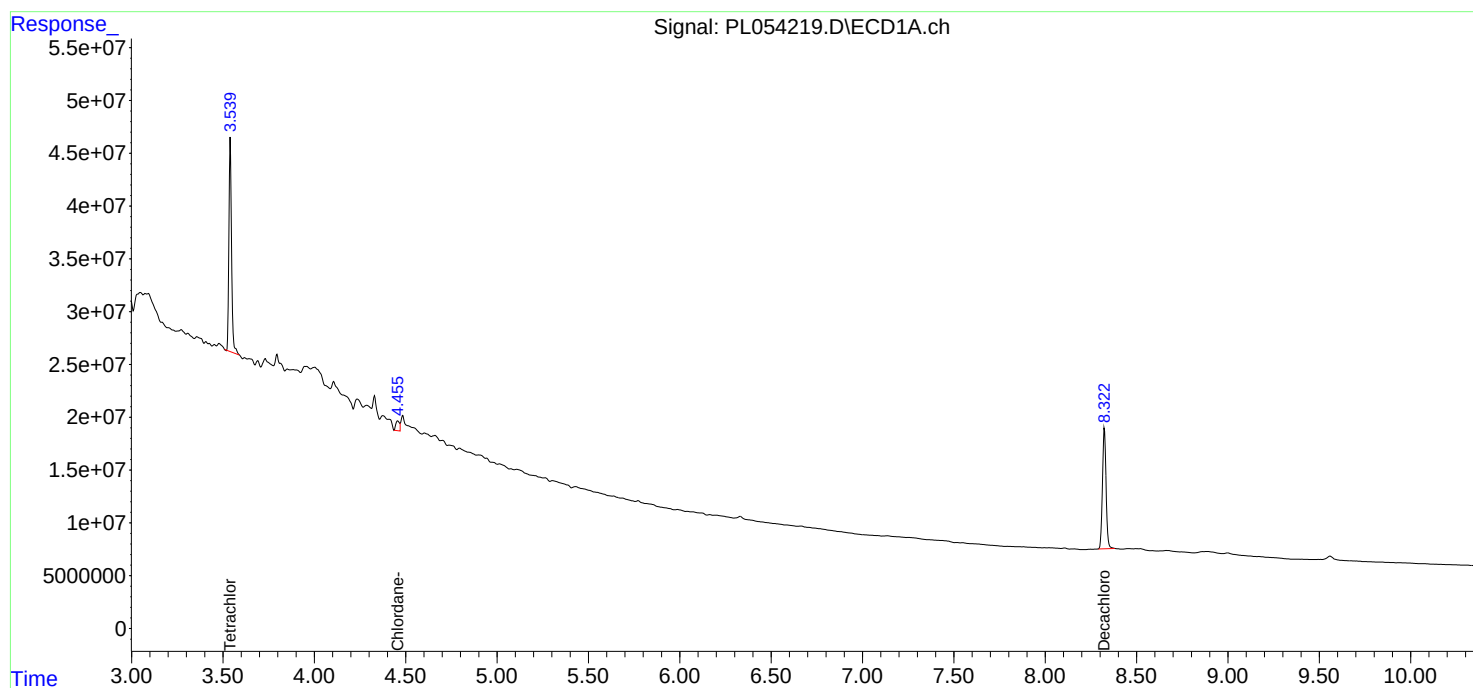


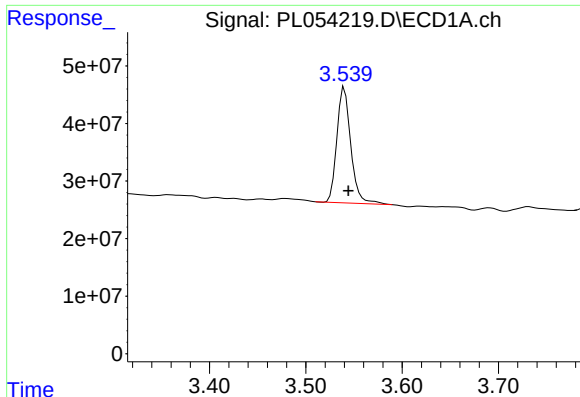

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 201800881
Conc: 18.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

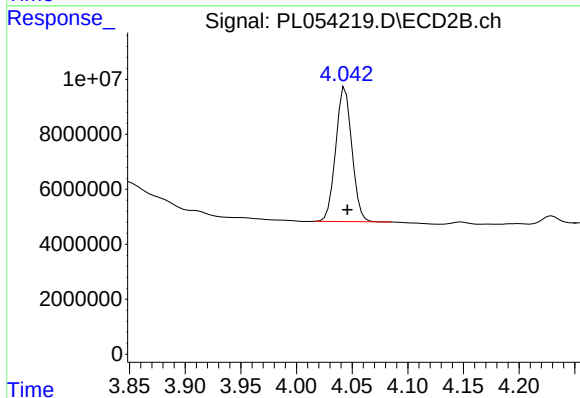


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 49387683
Conc: 19.74 ng/ml

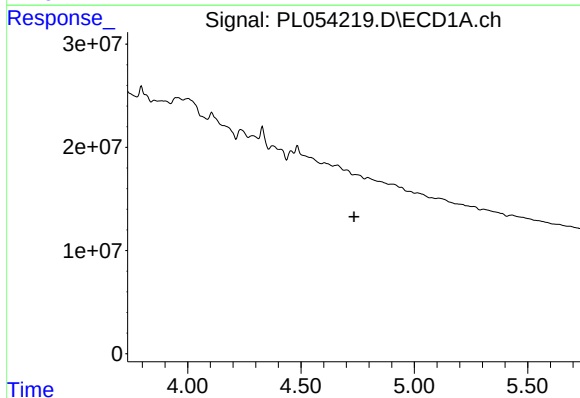


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

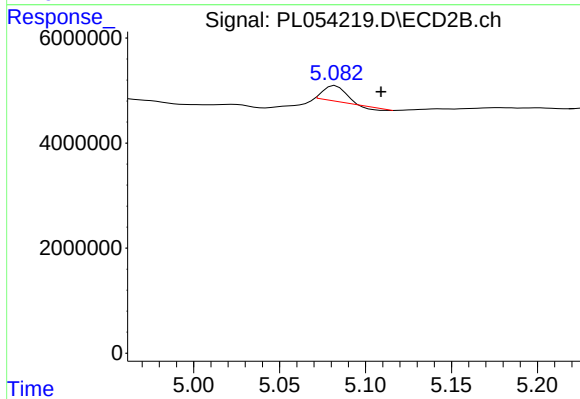

#7 delta-BHC


R.T.: 5.083 min
Delta R.T.: -0.026 min
Response: 2345871
Conc: 0.78 ng/ml

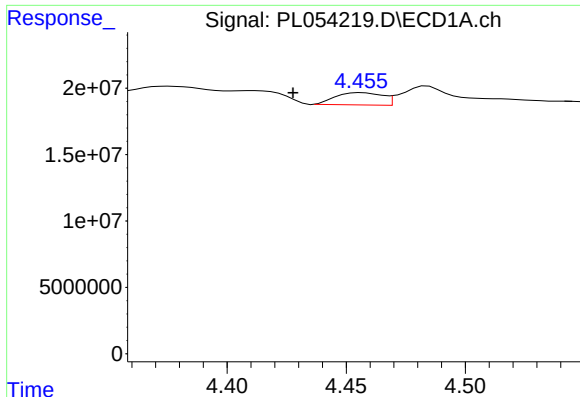

#23 Chlordane-1


R.T.: 4.457 min
Delta R.T.: 0.029 min
Response: 12612210
Conc: 35.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

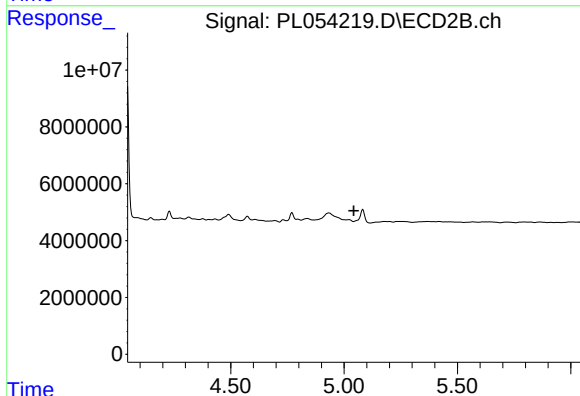


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

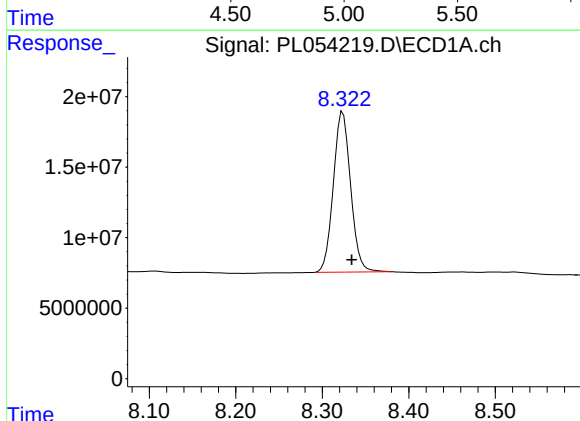

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.010 min
Response: 157480867
Conc: 16.05 ng/ml

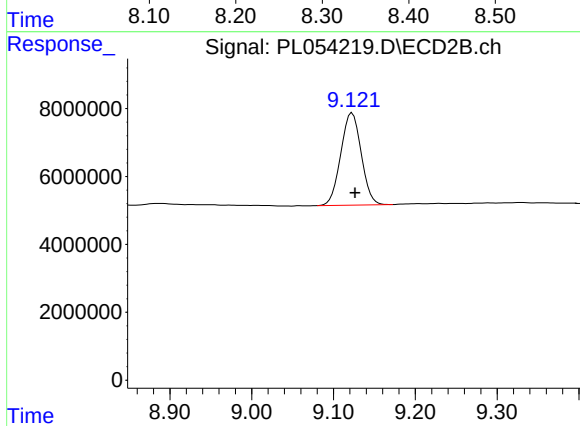

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 47143221
Conc: 16.74 ng/ml