

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111219\
 Data File : PL054220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2019 20:06
 Operator : SG\AJ
 Sample : K5670-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:35:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6) B	beta-BHC	4.529	4.900	10133590	4427136	1.538 2.866 #
7) B	delta-BHC	0.000	5.084f	0	3538750	N.D. 1.172 #
10) B	gamma-Chl...	5.512	0.000	181.9E6	0	13.330 N.D. #
23)	Chlordane-1	4.415	5.031	6259707	1347006	17.649 16.061
25)	Chlordane-3	5.512	0.000	181.9E6	0	157.777 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111219\
Data File : PL054220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2019 20:06
Operator : SG\AJ
Sample : K5670-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:35:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

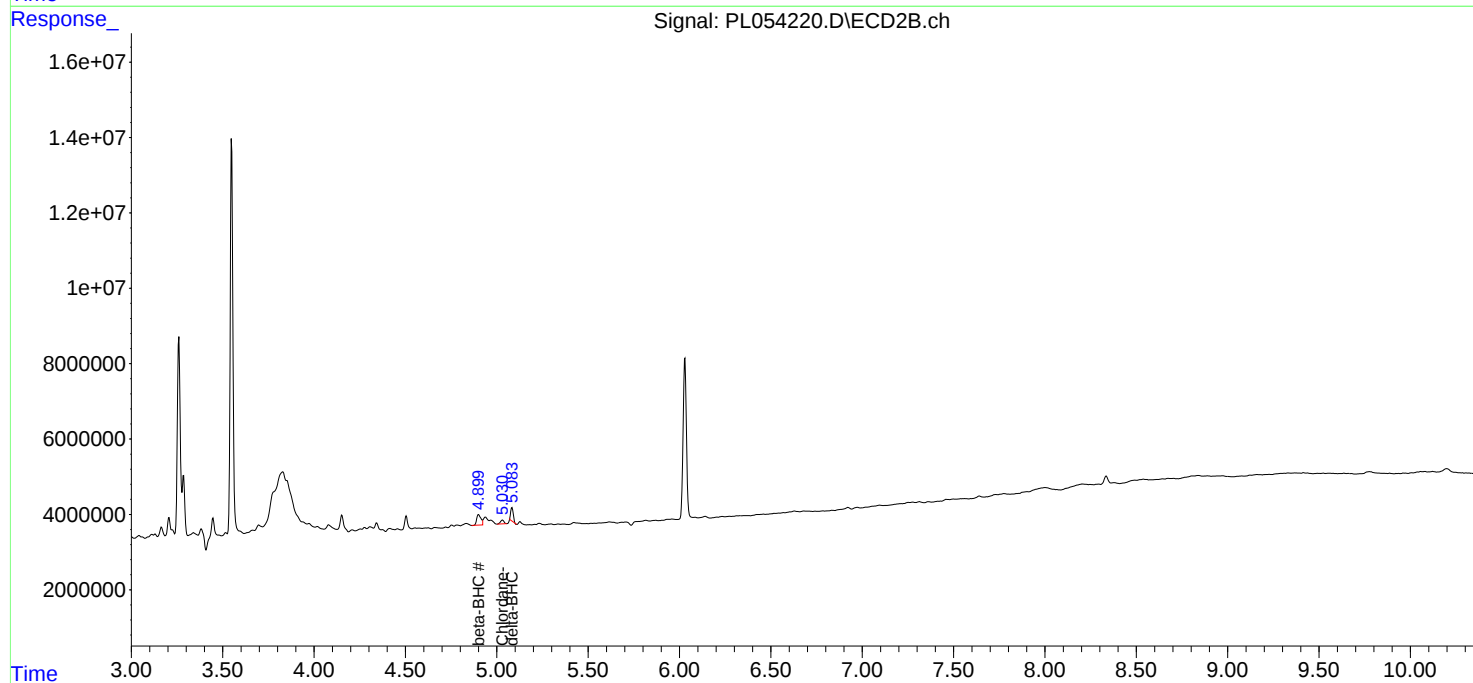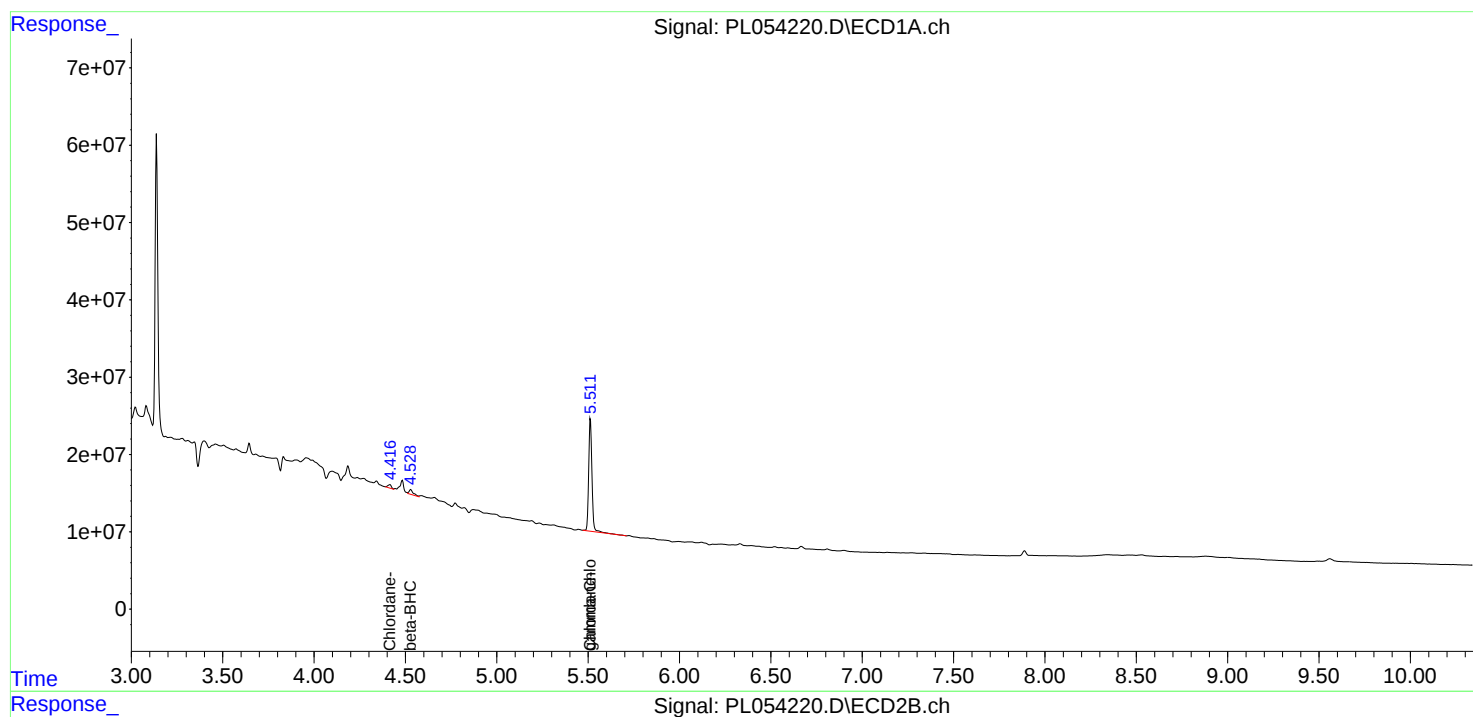


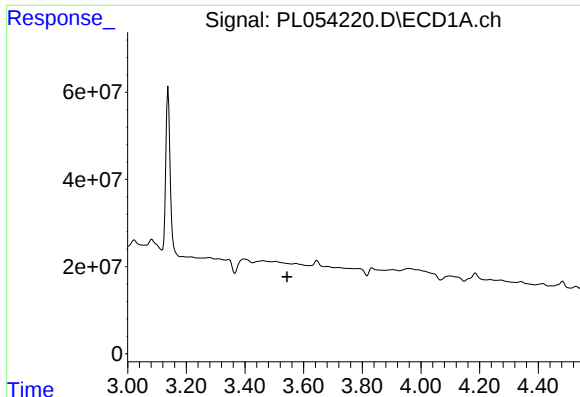

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.544 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

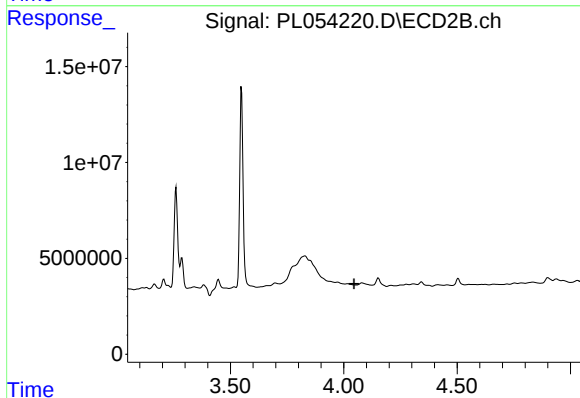


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.046 min
Response: 0
Conc: N.D.

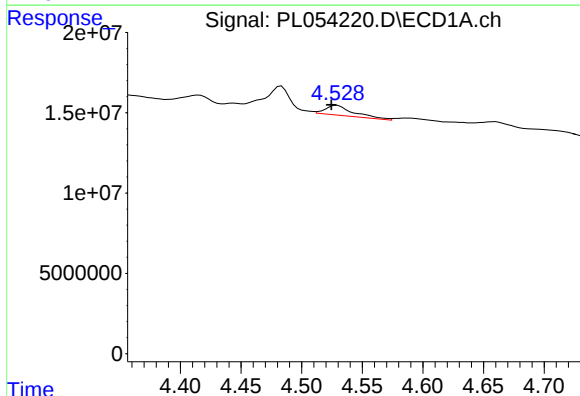


#6 beta-BHC

R.T.: 4.529 min
Delta R.T.: 0.004 min
Response: 10133590
Conc: 1.54 ng/ml

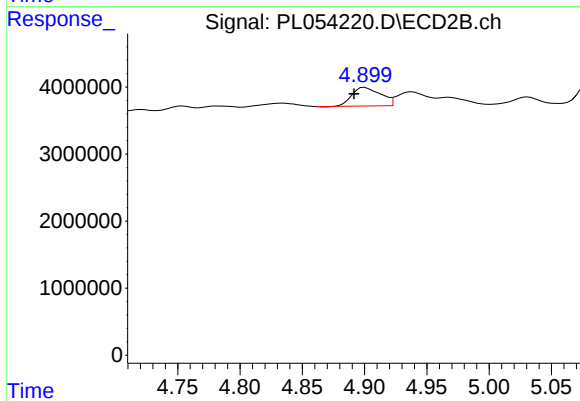

#6 beta-BHC


R.T.: 4.900 min
Delta R.T.: 0.009 min
Response: 4427136
Conc: 2.87 ng/ml

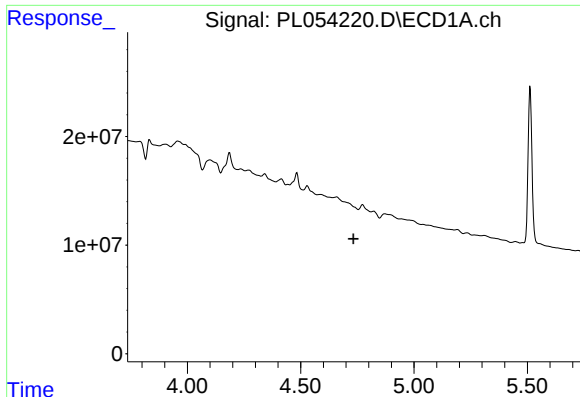

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

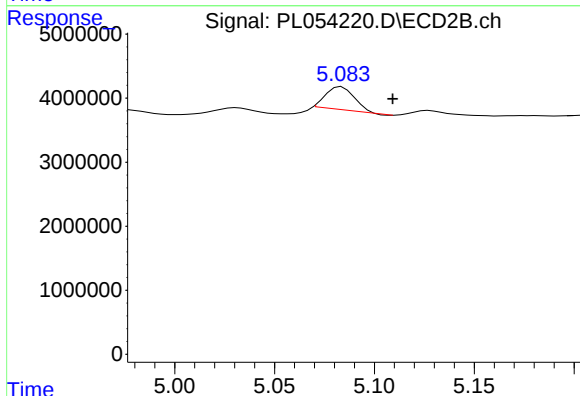


#7 delta-BHC

R.T.: 5.084 min
Delta R.T.: -0.026 min
Response: 3538750
Conc: 1.17 ng/ml

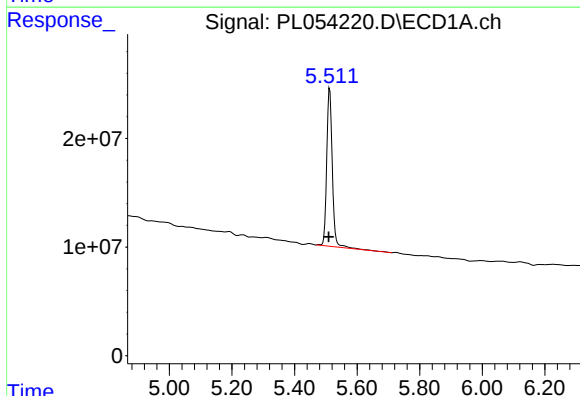


#10 gamma-Chlordane

R.T.: 5.512 min
Delta R.T.: 0.003 min
Response: 181867842
Conc: 13.33 ng/ml

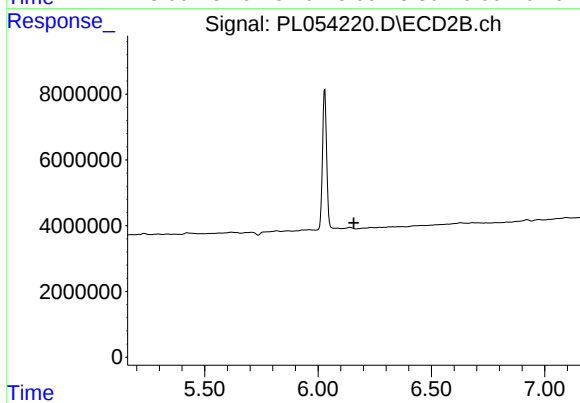

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

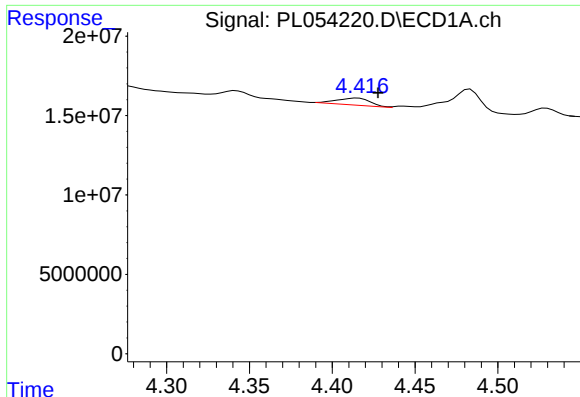

#23 Chlordane-1


R.T.: 4.415 min
Delta R.T.: -0.012 min
Response: 6259707
Conc: 17.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

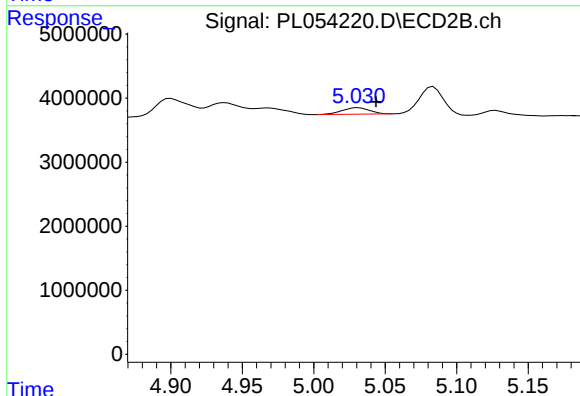


#23 Chlordane-1

R.T.: 5.031 min
Delta R.T.: -0.012 min
Response: 1347006
Conc: 16.06 ng/ml

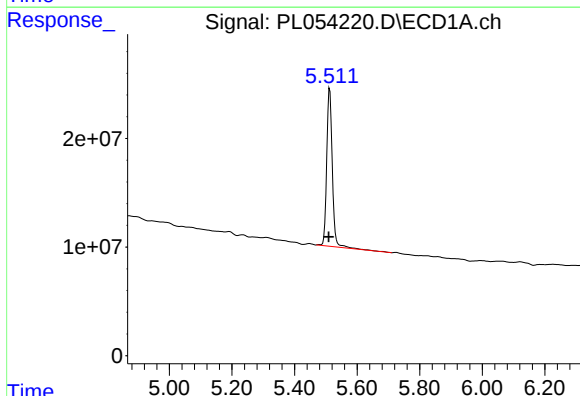


#25 Chlordane-3

R.T.: 5.512 min
Delta R.T.: 0.004 min
Response: 181867842
Conc: 157.78 ng/ml

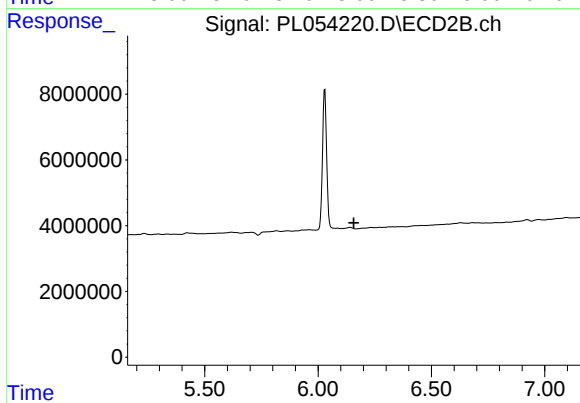

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

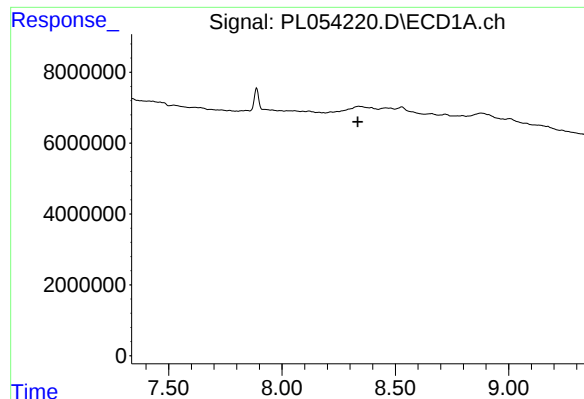

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

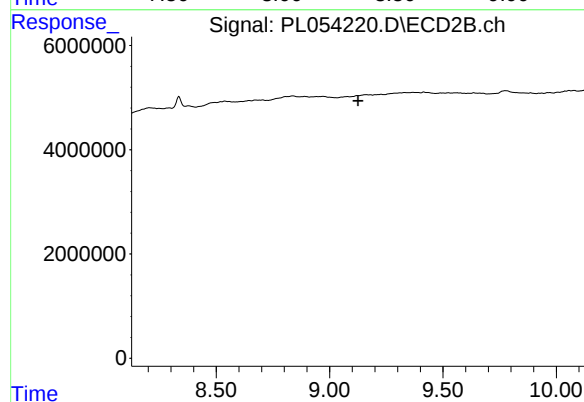

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.126 min
Response: 0
Conc: N.D.