

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111220\
 Data File : PL062977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2020 12:30
 Operator : DD\AJ
 Sample : PB132955BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:26:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	3.951	35989284	57101596	20.923	19.431
28)	SA Decachlor...	8.137	8.995	33757898	45408786	21.042	21.696
Target Compounds							
9)	A Endosulfan I	0.000	6.150f	0	4119024	N.D.	1.306 #
11)	B alpha-Chl...	0.000	6.150f	0	4119024	N.D.	1.223 #
13)	MA Dieldrin	0.000	6.420	0	11900684	N.D.	3.718 #
15)	B Endosulfa...	0.000	6.836f	0	3769945	N.D.	1.319 #
16)	A 4,4'-DDD	0.000	6.787f	0	3130649	N.D.	1.223 #
17)	MA 4,4'-DDT	6.294	0.000	2389299	0	1.790	N.D. #
22)	Mirex	7.282f	0.000	2106604	0	1.486	N.D. #
23)	Chlordane-1	4.256	0.000	28397	0	0.551	N.D. #
26)	Chlordane-4	0.000	6.150f	0	4119024	N.D.	8.505 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111220\
Data File : PL062977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2020 12:30
Operator : DD\AJ
Sample : PB132955BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:26:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

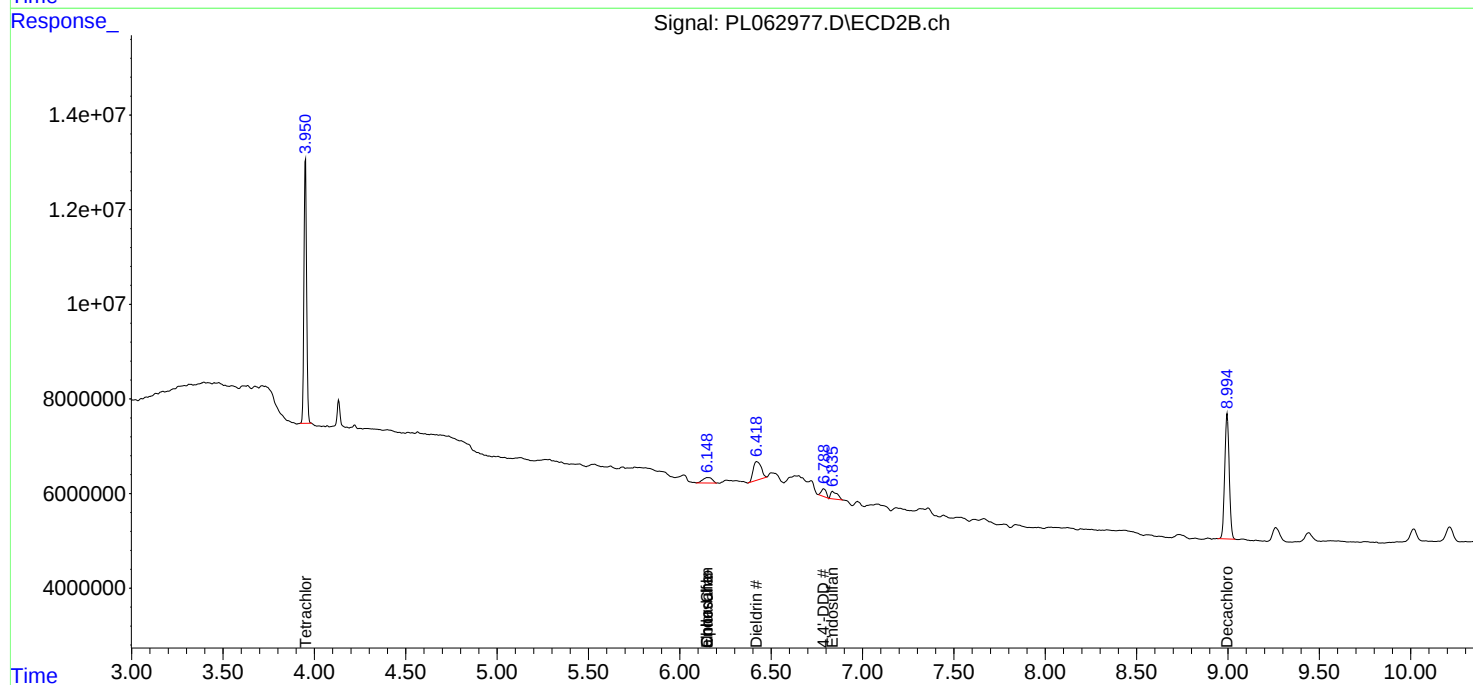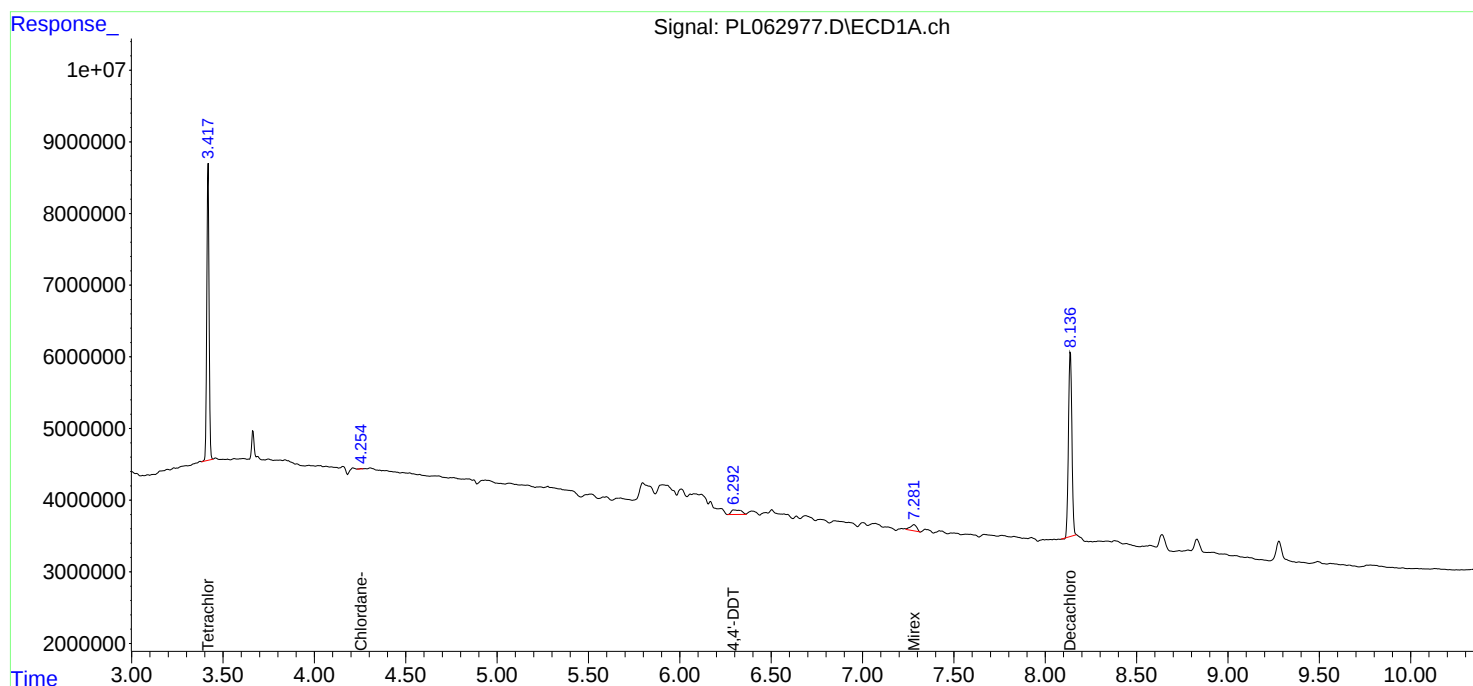


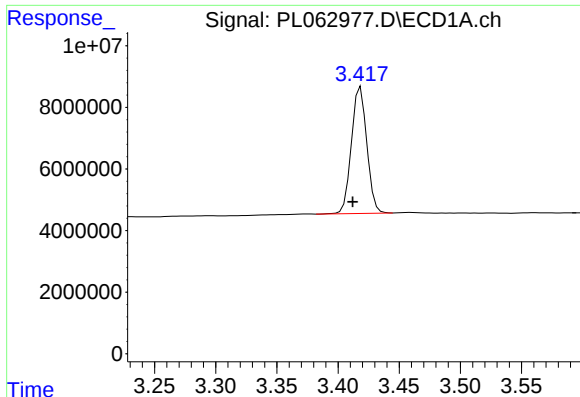

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: 0.006 min
Response: 35989284
Conc: 20.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

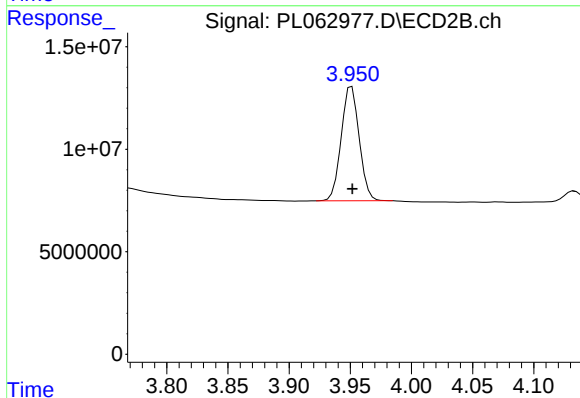


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 57101596
Conc: 19.43 ng/ml

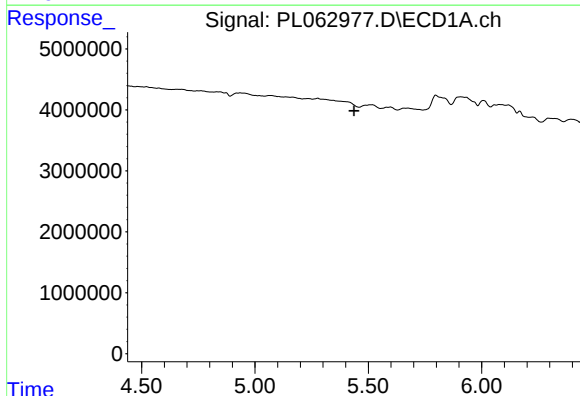


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.438 min
Response: 0
Conc: N.D.

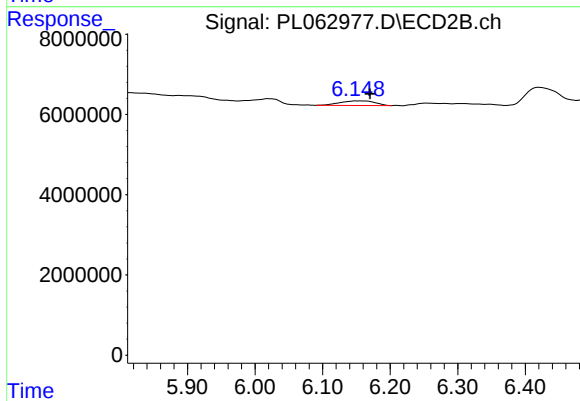

#9 Endosulfan I


R.T.: 6.150 min
Delta R.T.: -0.020 min
Response: 4119024
Conc: 1.31 ng/ml

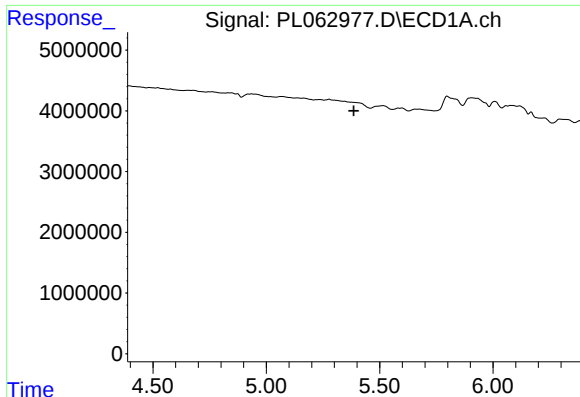

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

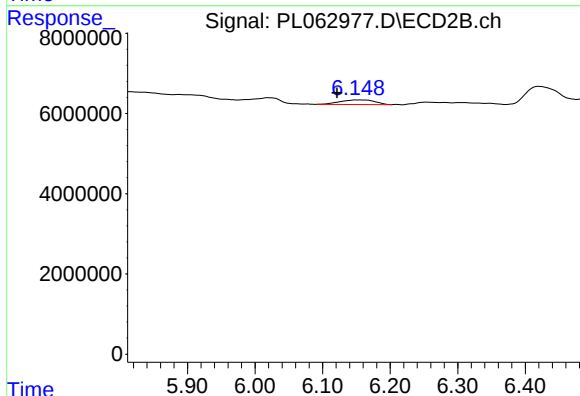


#11 alpha-Chlordane

R.T.: 6.150 min
Delta R.T.: 0.029 min
Response: 4119024
Conc: 1.22 ng/ml

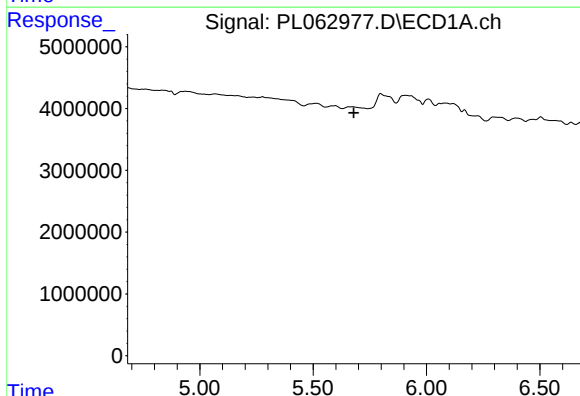


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.679 min
Response: 0
Conc: N.D.

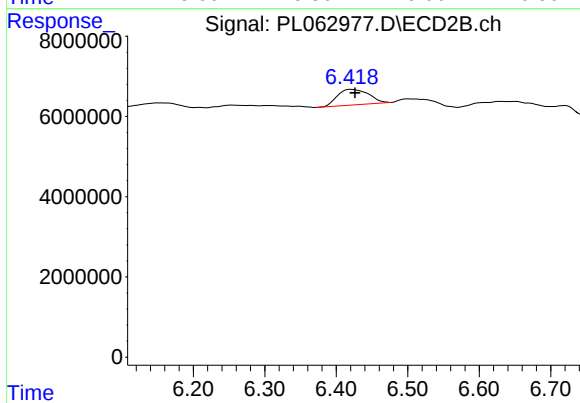

#13 Dieldrin


R.T.: 6.420 min
Delta R.T.: -0.006 min
Response: 11900684
Conc: 3.72 ng/ml

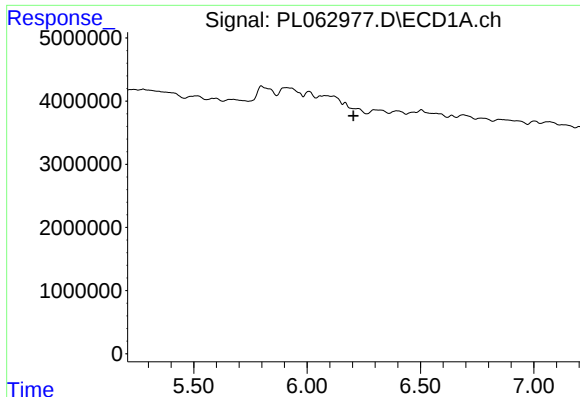

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

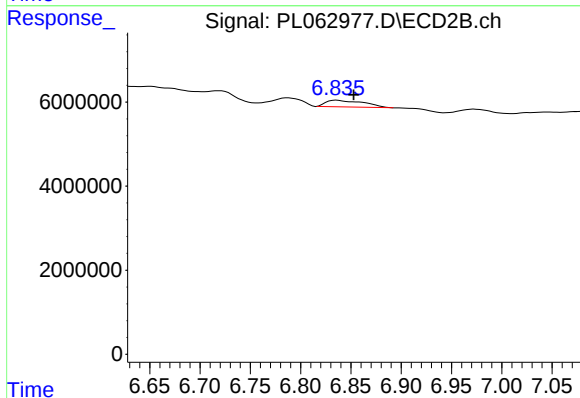


#15 Endosulfan II

R.T.: 6.836 min
Delta R.T.: -0.017 min
Response: 3769945
Conc: 1.32 ng/ml

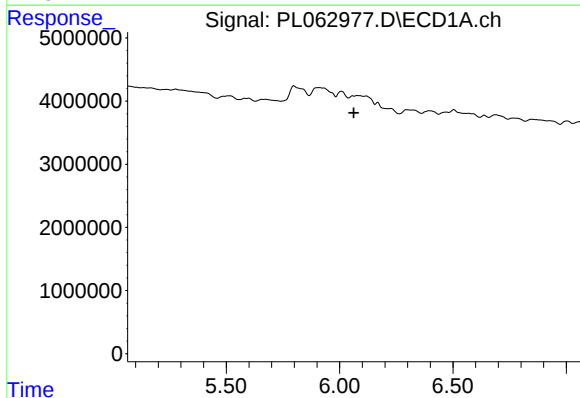


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.062 min
Response: 0
Conc: N.D.

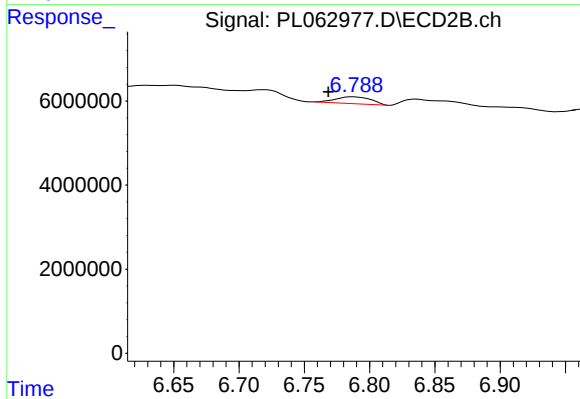

#16 4,4'-DDD


R.T.: 6.787 min
Delta R.T.: 0.019 min
Response: 3130649
Conc: 1.22 ng/ml

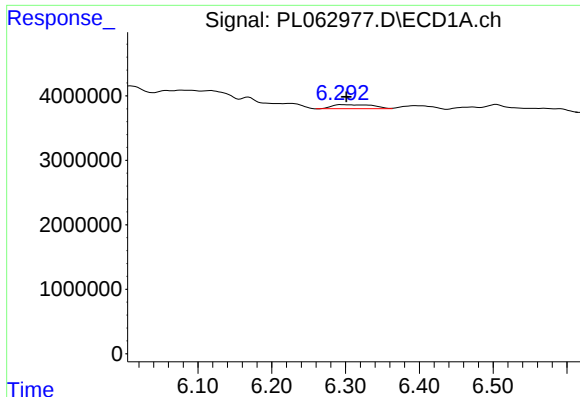

#17 4,4'-DDT


R.T.: 6.294 min
Delta R.T.: -0.007 min
Response: 2389299
Conc: 1.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

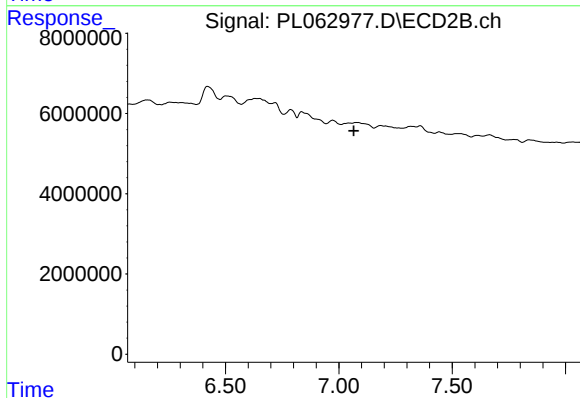


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.066 min
Response: 0
Conc: N.D.

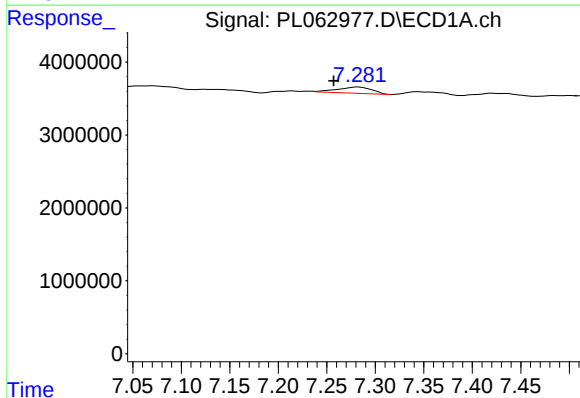


#22 Mirex

R.T.: 7.282 min
Delta R.T.: 0.025 min
Response: 2106604
Conc: 1.49 ng/ml

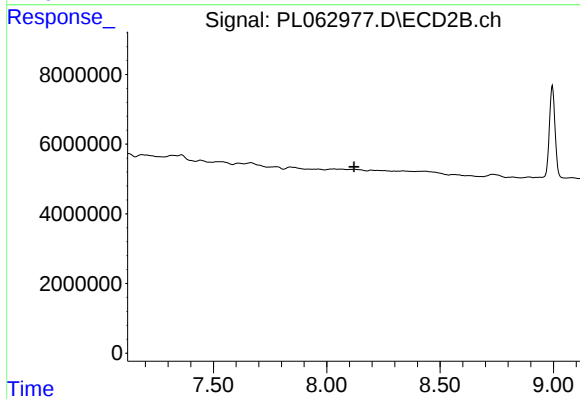

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.121 min
Response: 0
Conc: N.D.

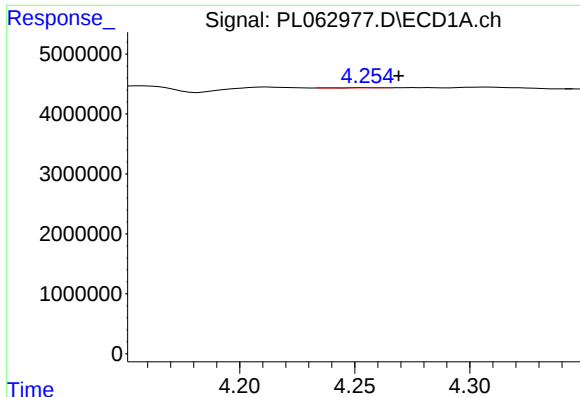

#23 Chlordane-1


R.T.: 4.256 min
Delta R.T.: -0.013 min
Response: 28397
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

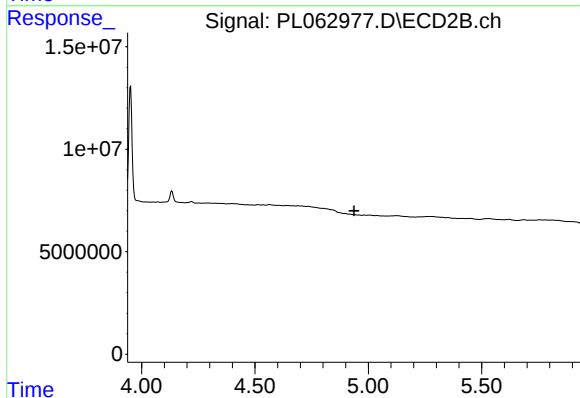


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

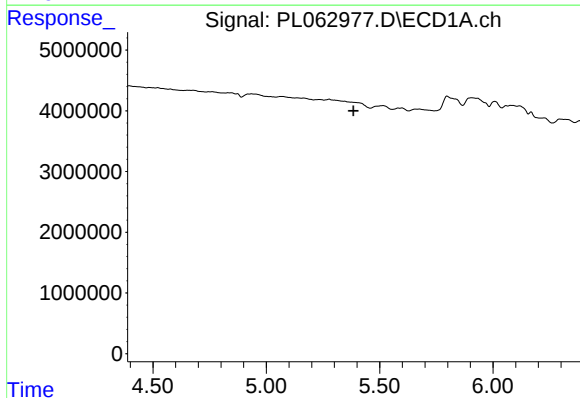


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.385 min
Response: 0
Conc: N.D.

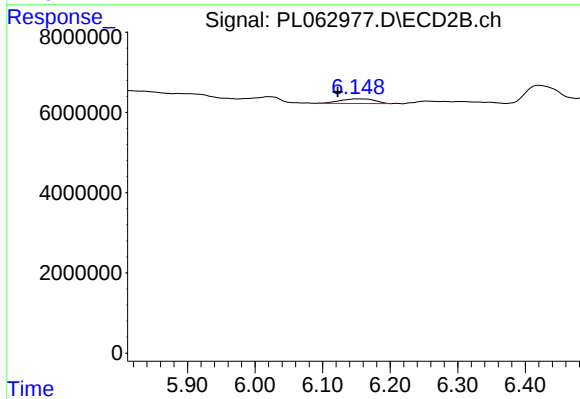

#26 Chlordane-4


R.T.: 6.150 min
Delta R.T.: 0.027 min
Response: 4119024
Conc: 8.51 ng/ml

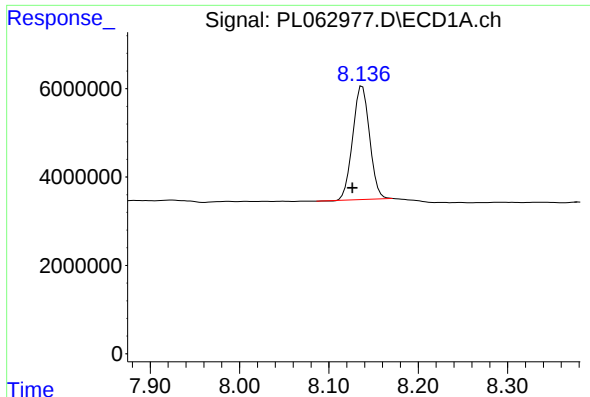

#28 Decachlorobiphenyl

R.T.: 8.137 min
Delta R.T.: 0.011 min
Response: 33757898
Conc: 21.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

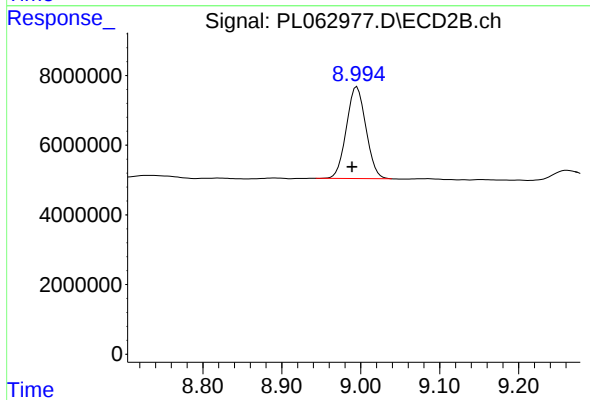

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.006 min
Response: 45408786
Conc: 21.70 ng/ml