

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111220\
 Data File : PL062979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2020 12:59
 Operator : DD\AJ
 Sample : L4587-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:27:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.950	25526710	37239723	14.840	12.672
28)	SA Decachlor...	8.127	8.990	23113147	29783223	14.407	14.230
Target Compounds							
2)	A alpha-BHC	0.000	4.323	0	2602283	N.D.	0.586 #
3)	MA gamma-BHC...	0.000	4.624	0	2876333	N.D.	0.689 #
5)	MB Aldrin	4.660	0.000	1657367	0	0.868	N.D. #
8)	B Heptachlo...	0.000	5.828	0	3454862	N.D.	1.067 #
9)	A Endosulfan I	5.448	0.000	2079453	0	1.244	N.D. #
10)	B gamma-Chl...	0.000	6.044	0	4582011	N.D.	1.361 #
12)	B 4,4'-DDE	5.551	6.270	948192	8394421	0.573	2.605 #
15)	B Endosulfa...	0.000	6.824f	0	1651006	N.D.	0.578 #
23)	Chlordane-1	4.258	4.953f	1350190	1025878	26.192	10.220 #
25)	Chlordane-3	0.000	6.044	0	4582011	N.D.	11.343 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111220\
Data File : PL062979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2020 12:59
Operator : DD\AJ
Sample : L4587-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:27:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

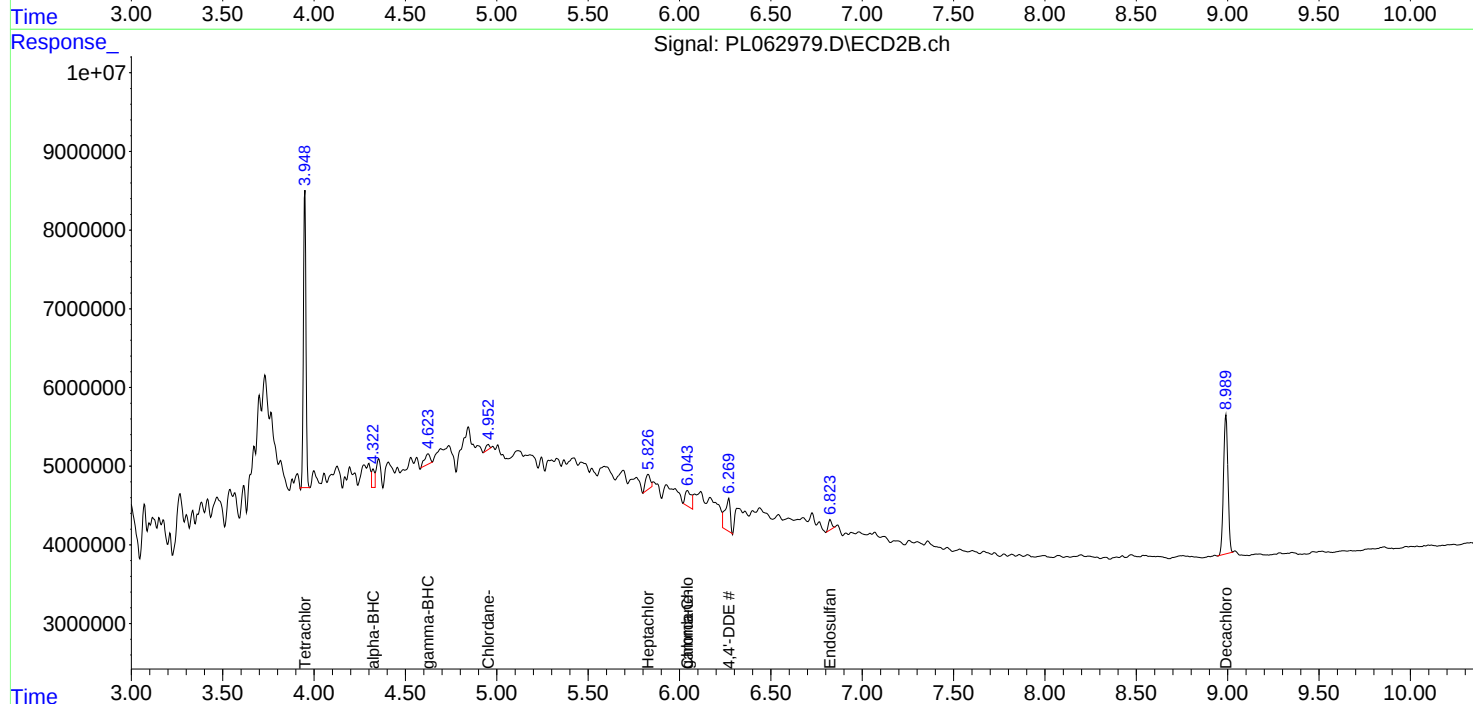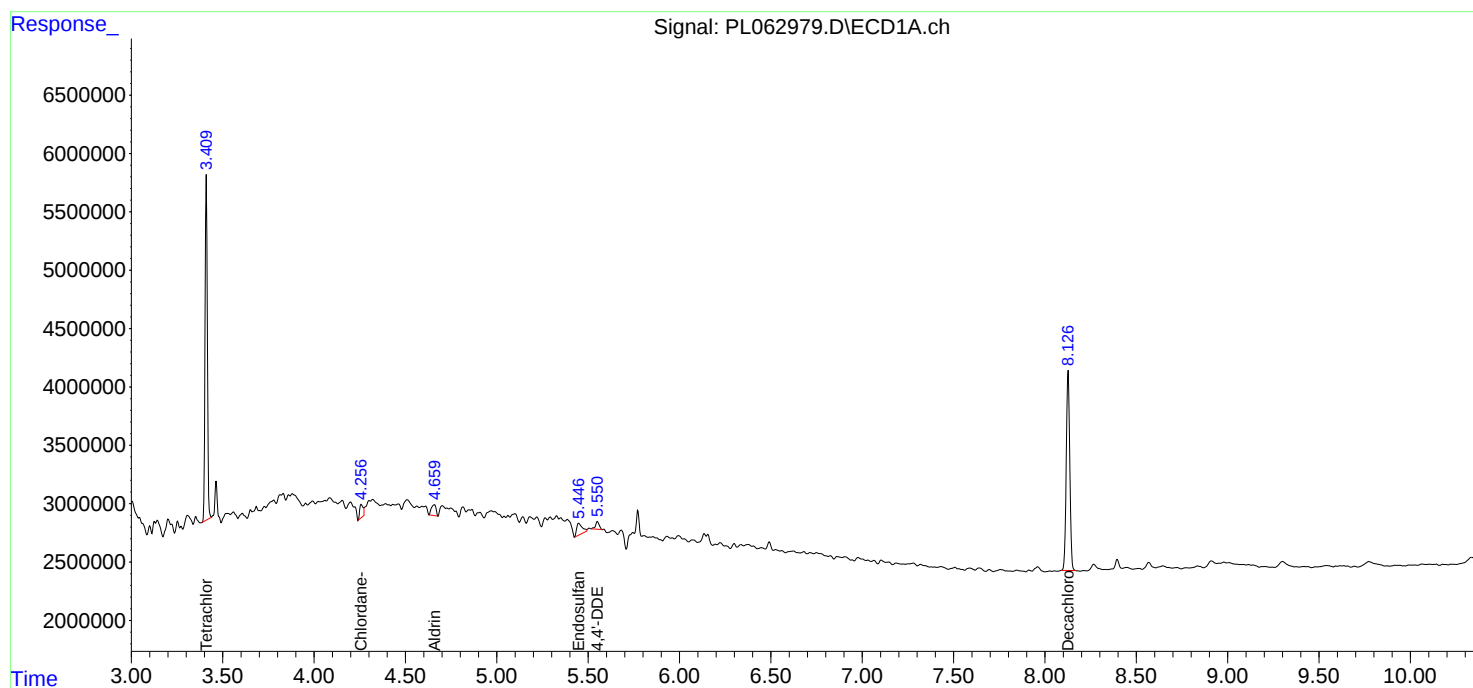


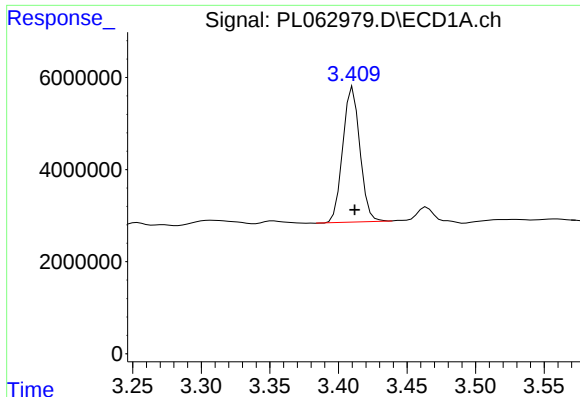

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 25526710
Conc: 14.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

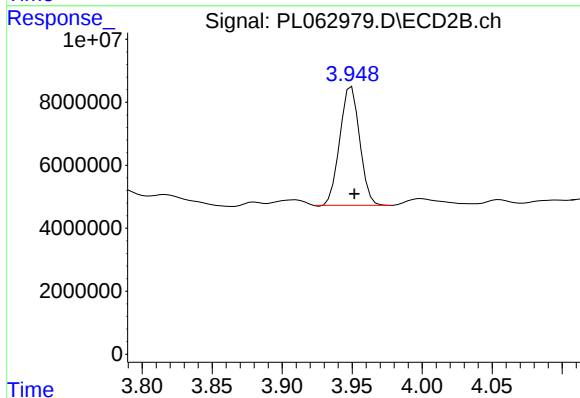


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 37239723
Conc: 12.67 ng/ml

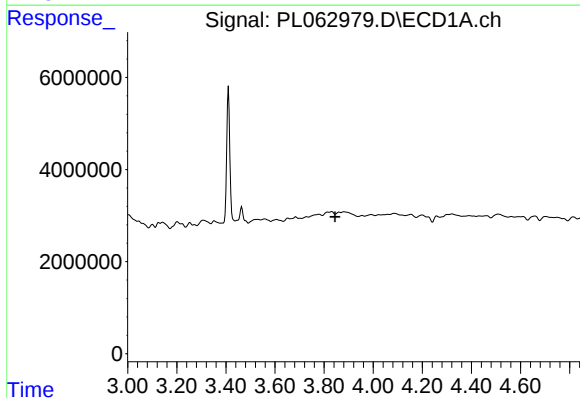


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.844 min
Response: 0
Conc: N.D.

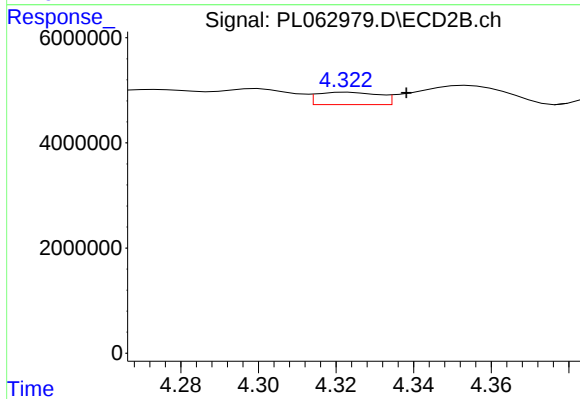

#2 alpha-BHC


R.T.: 4.323 min
Delta R.T.: -0.015 min
Response: 2602283
Conc: 0.59 ng/ml

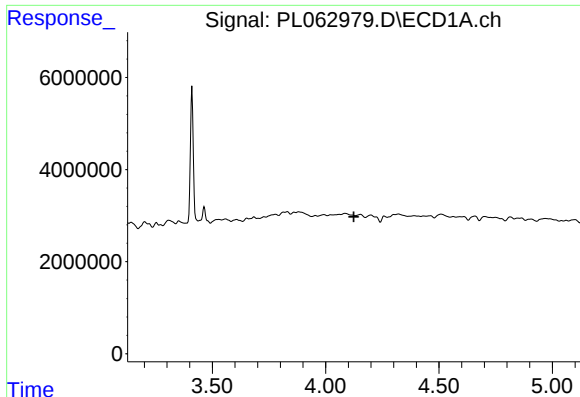

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

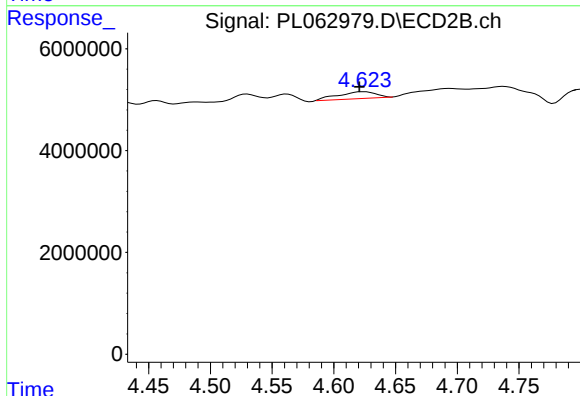


#3 gamma-BHC (Lindane)

R.T.: 4.624 min
Delta R.T.: 0.004 min
Response: 2876333
Conc: 0.69 ng/ml

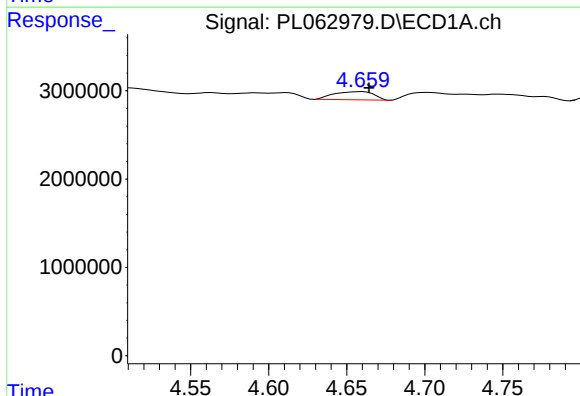


#5 Aldrin

R.T.: 4.660 min
Delta R.T.: -0.004 min
Response: 1657367
Conc: 0.87 ng/ml

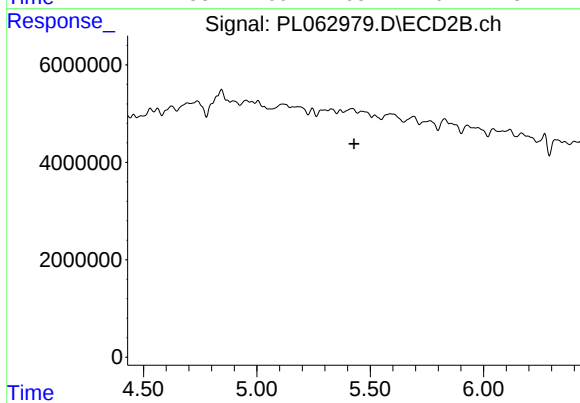

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.429 min
Response: 0
Conc: N.D.

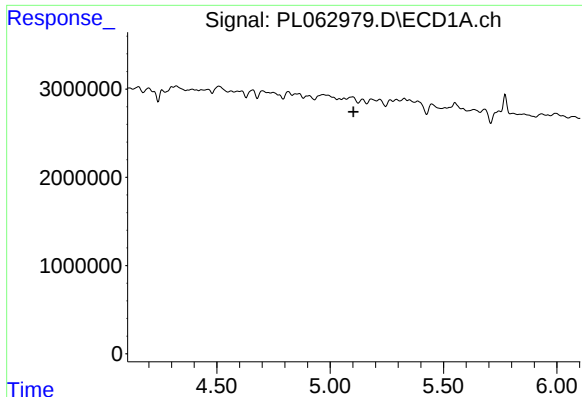

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.103 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

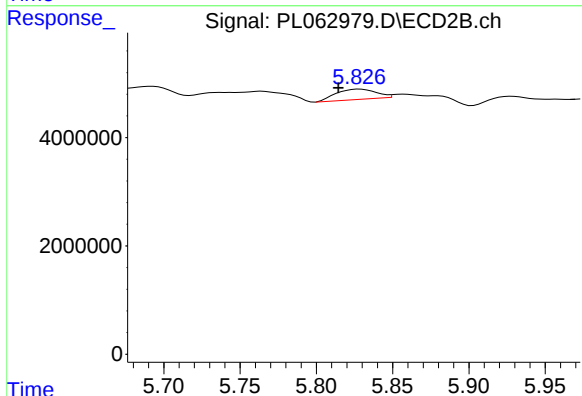


#8 Heptachlor epoxide

R.T.: 5.828 min
Delta R.T.: 0.014 min
Response: 3454862
Conc: 1.07 ng/ml

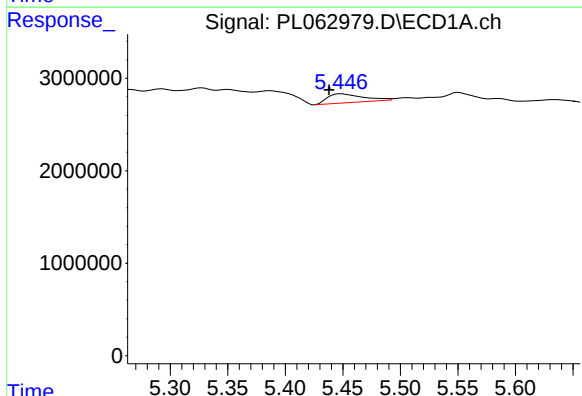


#9 Endosulfan I

R.T.: 5.448 min
Delta R.T.: 0.011 min
Response: 2079453
Conc: 1.24 ng/ml

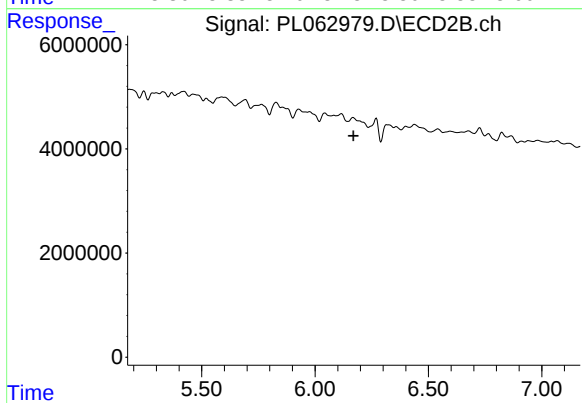

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.170 min
Response: 0
Conc: N.D.

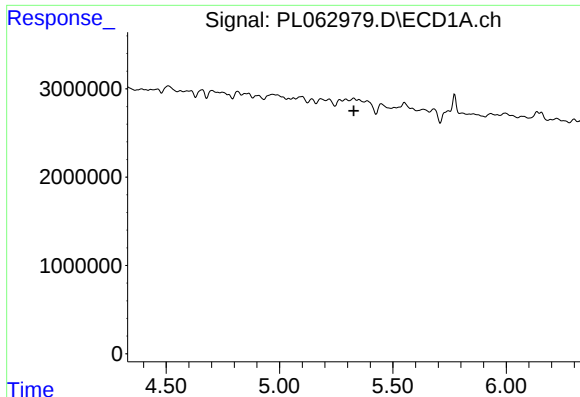

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

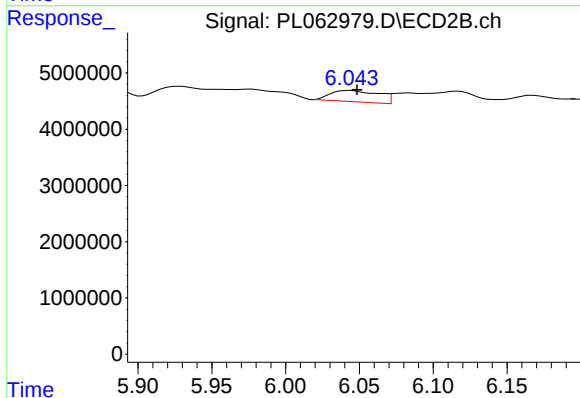


#10 gamma-Chlordane

R.T.: 6.044 min
Delta R.T.: -0.005 min
Response: 4582011
Conc: 1.36 ng/ml

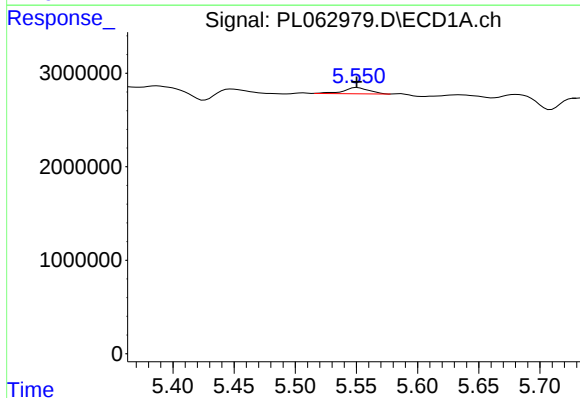


#12 4,4'-DDE

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 948192
Conc: 0.57 ng/ml

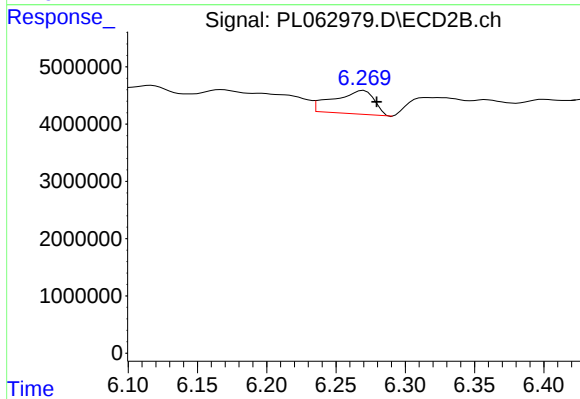

#12 4,4'-DDE


R.T.: 6.270 min
Delta R.T.: -0.009 min
Response: 8394421
Conc: 2.61 ng/ml

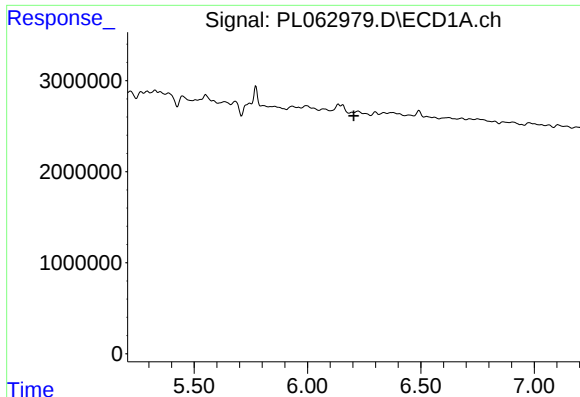

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

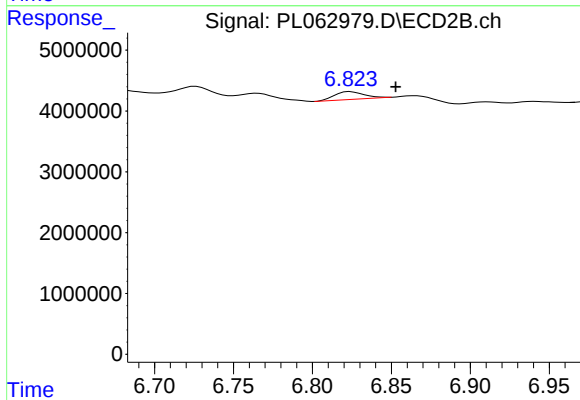


#15 Endosulfan II

R.T.: 6.824 min
Delta R.T.: -0.029 min
Response: 1651006
Conc: 0.58 ng/ml

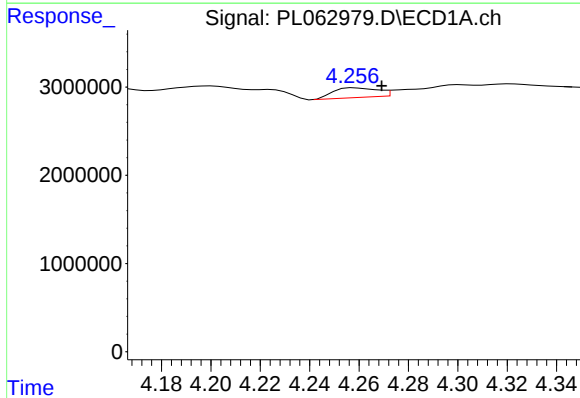


#23 Chlordane-1

R.T.: 4.258 min
Delta R.T.: -0.011 min
Response: 1350190
Conc: 26.19 ng/ml

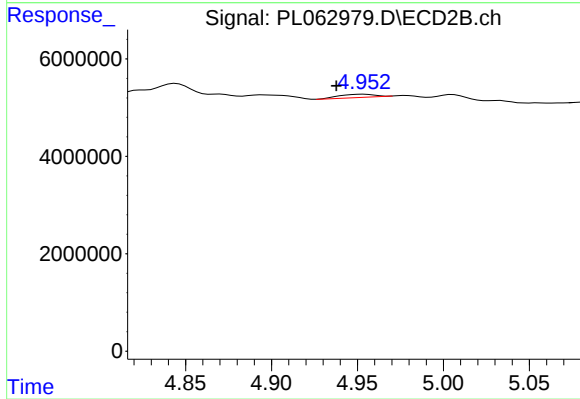

#23 Chlordane-1


R.T.: 4.953 min
Delta R.T.: 0.016 min
Response: 1025878
Conc: 10.22 ng/ml

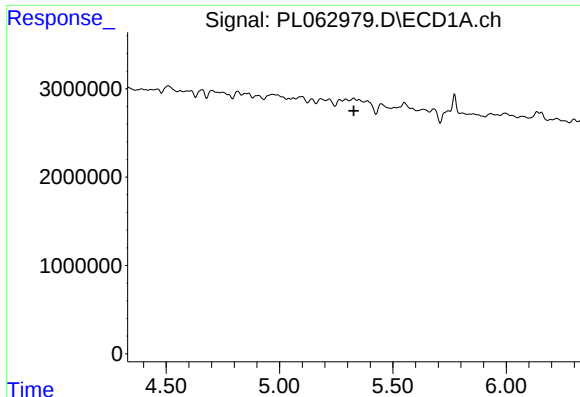

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

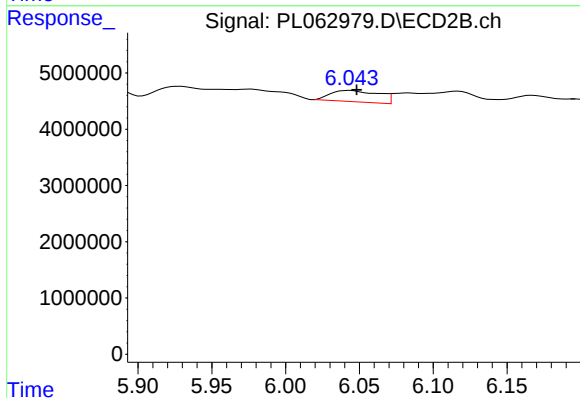


#25 Chlordane-3

R.T.: 6.044 min
Delta R.T.: -0.004 min
Response: 4582011
Conc: 11.34 ng/ml

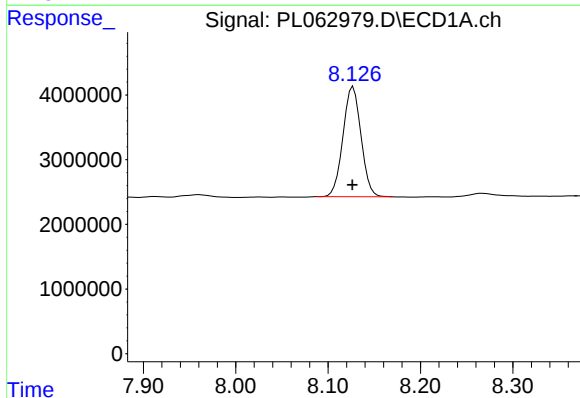

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 23113147
Conc: 14.41 ng/ml

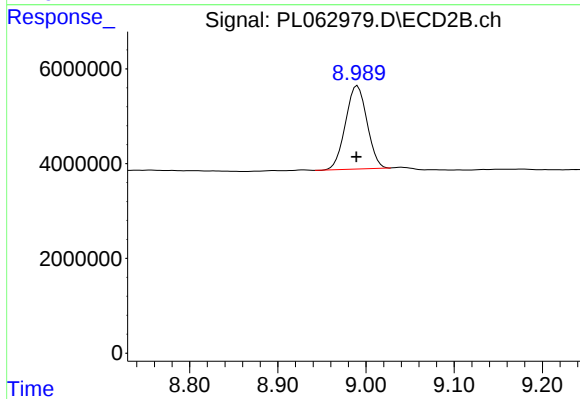

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.001 min
Response: 29783223
Conc: 14.23 ng/ml