

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111220\
 Data File : PL062986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2020 14:38
 Operator : DD\AJ
 Sample : L4702-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 M-6(0-10)

Manual Integrations
 APPROVED

Ankita
 11/13/2020 12:12:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:29:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.411	3.949	25855087	35854274	15.031	12.201m
28) SA Decachlor...	8.126	8.991	20604189	23879432	12.843m	11.409
Target Compounds						
10) B gamma-Chl...	5.327	6.047	3205138	7953646	1.779m	2.363m#
11) B alpha-Chl...	5.384	6.119	3785975	10635630	2.094m	3.157m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111220\
Data File : PL062986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2020 14:38
Operator : DD\AJ
Sample : L4702-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
M-6(0-10)


Manual Integrations
APPROVED

Ankita
11/13/2020 12:12:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:29:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

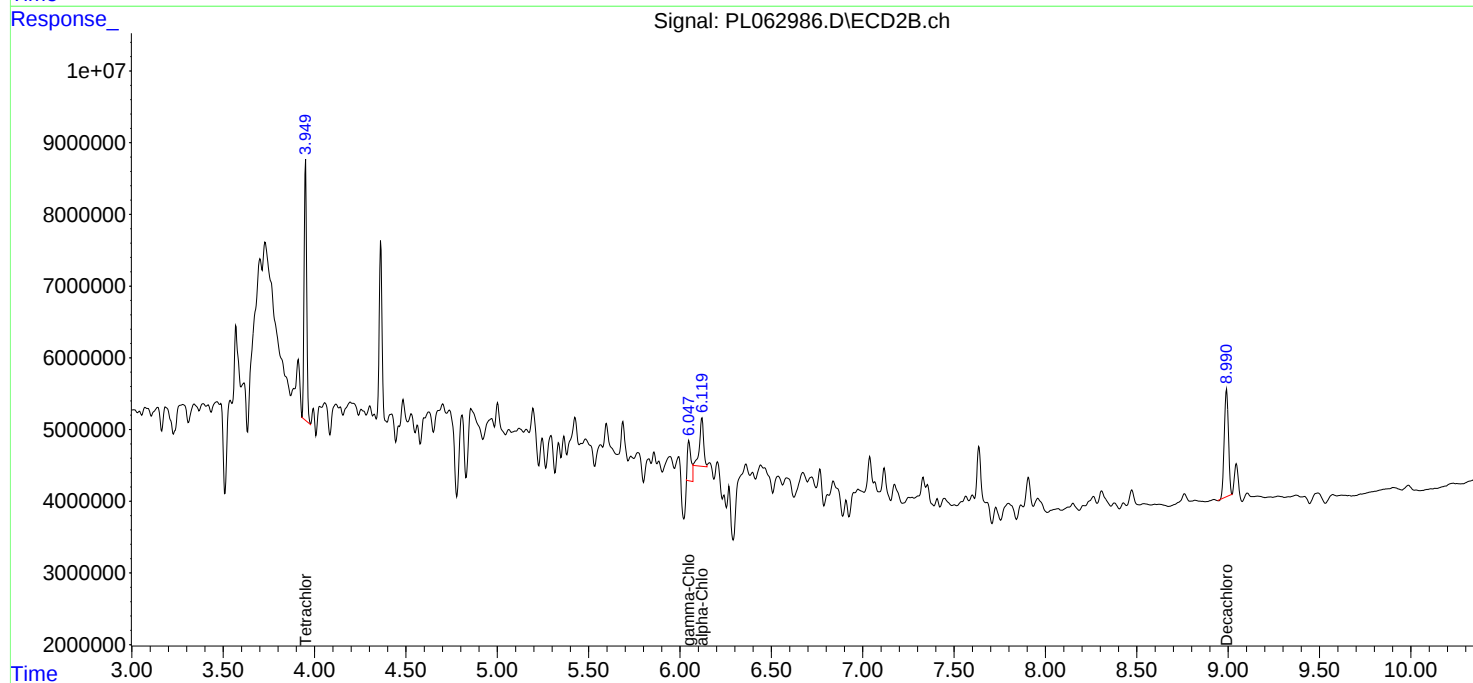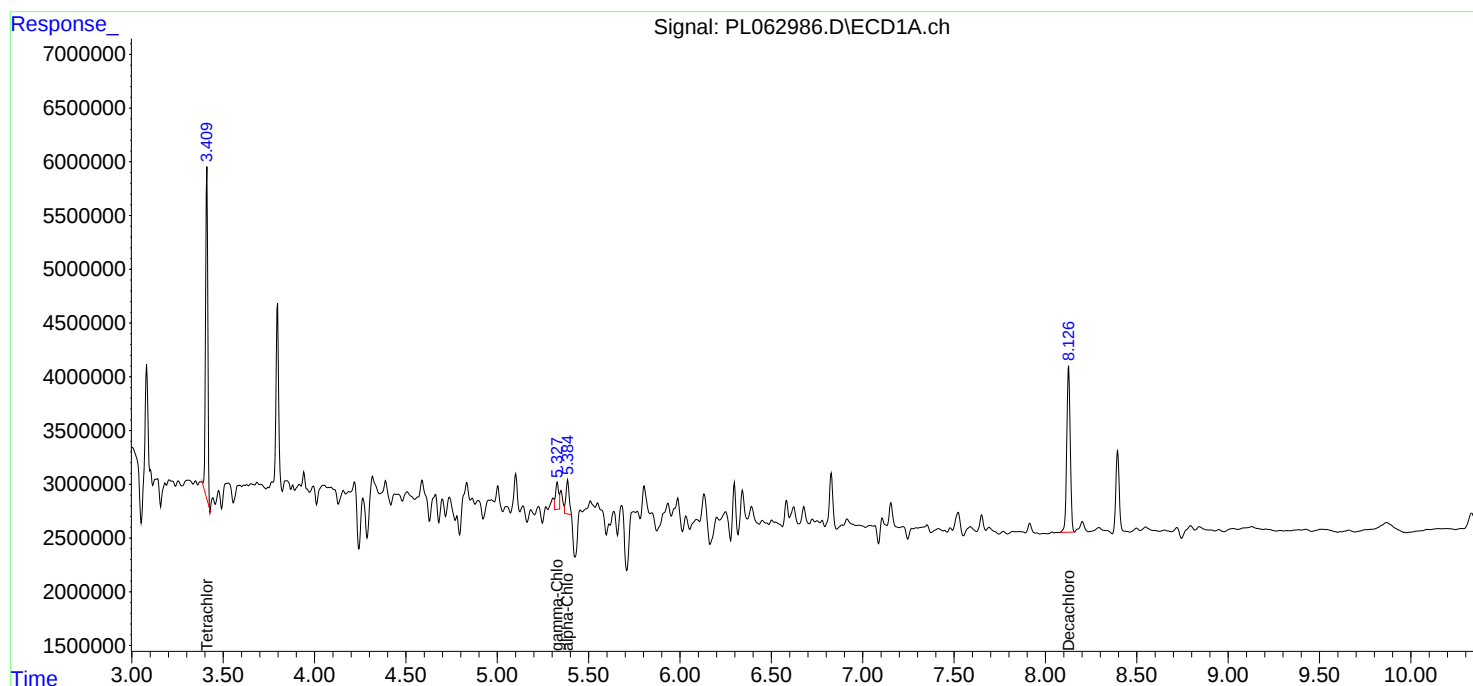

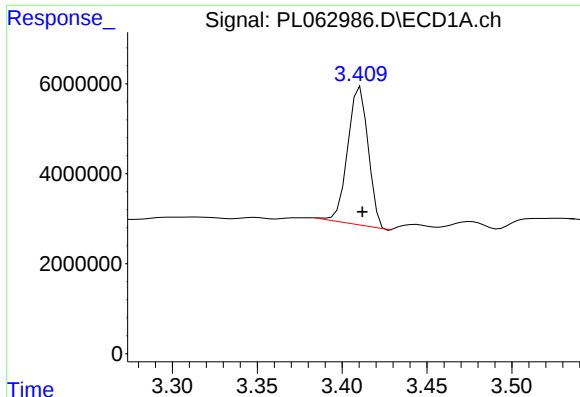


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 25855087
Conc: 15.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-6(0-10)


Manual Integrations
APPROVED

Ankita
11/13/2020 12:12:40 PM

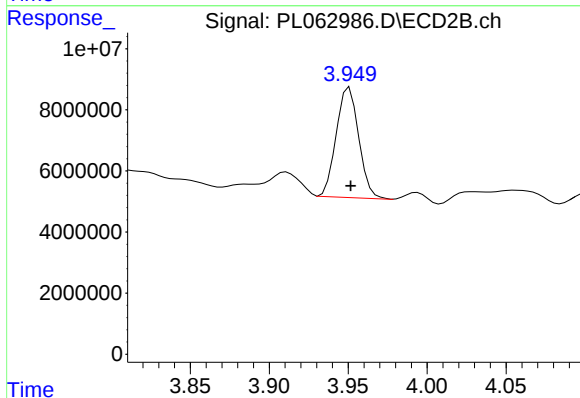


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.002 min
Response: 35854274
Conc: 12.20 ng/ml m

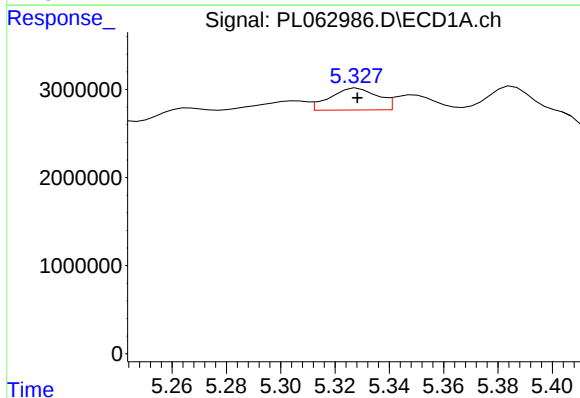


#10 gamma-Chlordane

R.T.: 5.327 min
Delta R.T.: -0.001 min
Response: 3205138
Conc: 1.78 ng/ml m

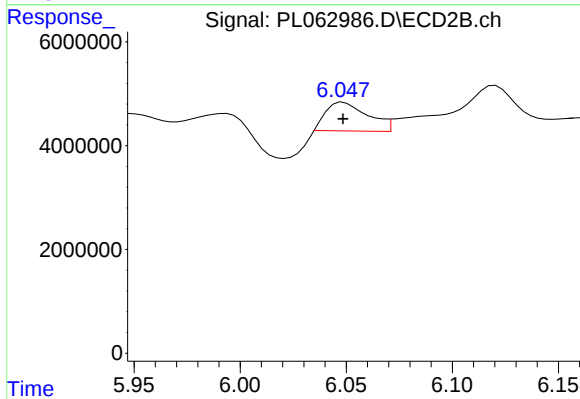

#10 gamma-Chlordane

R.T.: 6.047 min
Delta R.T.: -0.001 min
Response: 7953646
Conc: 2.36 ng/ml m

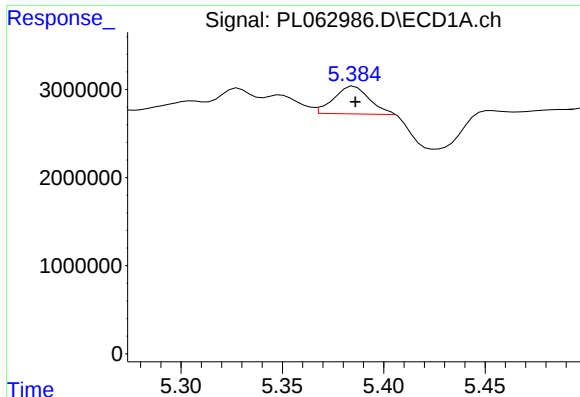


#11 alpha-Chlordane

R.T.: 5.384 min
Delta R.T.: -0.002 min
Response: 3785975
Conc: 2.09 ng/ml m

Instrument :
ECD_L
ClientSampleId :
M-6(0-10)


Manual Integrations
APPROVED

Ankita
11/13/2020 12:12:40 PM

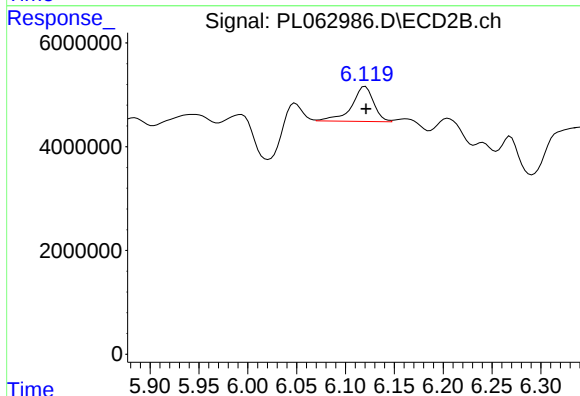


#11 alpha-Chlordane

R.T.: 6.119 min
Delta R.T.: -0.002 min
Response: 10635630
Conc: 3.16 ng/ml m

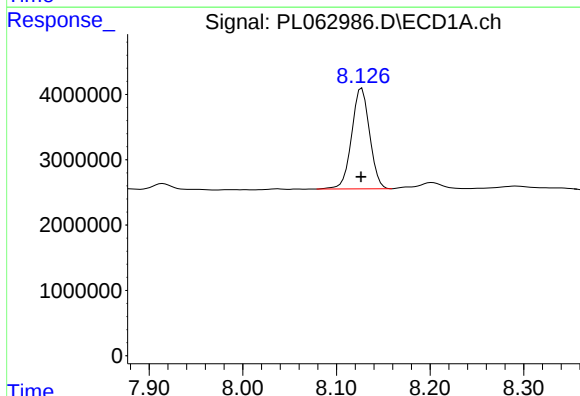

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 20604189
Conc: 12.84 ng/ml m

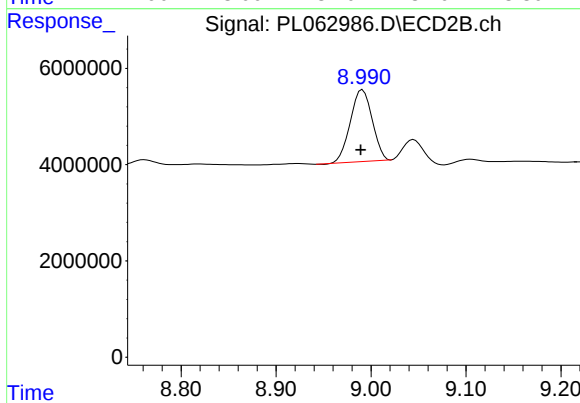

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 23879432
Conc: 11.41 ng/ml