

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111220\
 Data File : PL062987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2020 14:53
 Operator : DD\AJ
 Sample : L4702-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 M-99(0-10)

Manual Integrations
 APPROVED

Ankita
 11/13/2020 12:12:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:29:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.949	26598223	38329506	15.463	13.043m
28)	SA Decachlor...	8.127	8.990	21405729	25265513	13.343	12.072
Target Compounds							
10)	B gamma-Chl...	5.327	6.047	3805474	6187202	2.112m	1.838m
11)	B alpha-Chl...	5.384	6.119	4116486	9481205	2.277m	2.814m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111220\
Data File : PL062987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2020 14:53
Operator : DD\AJ
Sample : L4702-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
M-99(0-10)


Manual Integrations
APPROVED

Ankita
11/13/2020 12:12:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:29:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

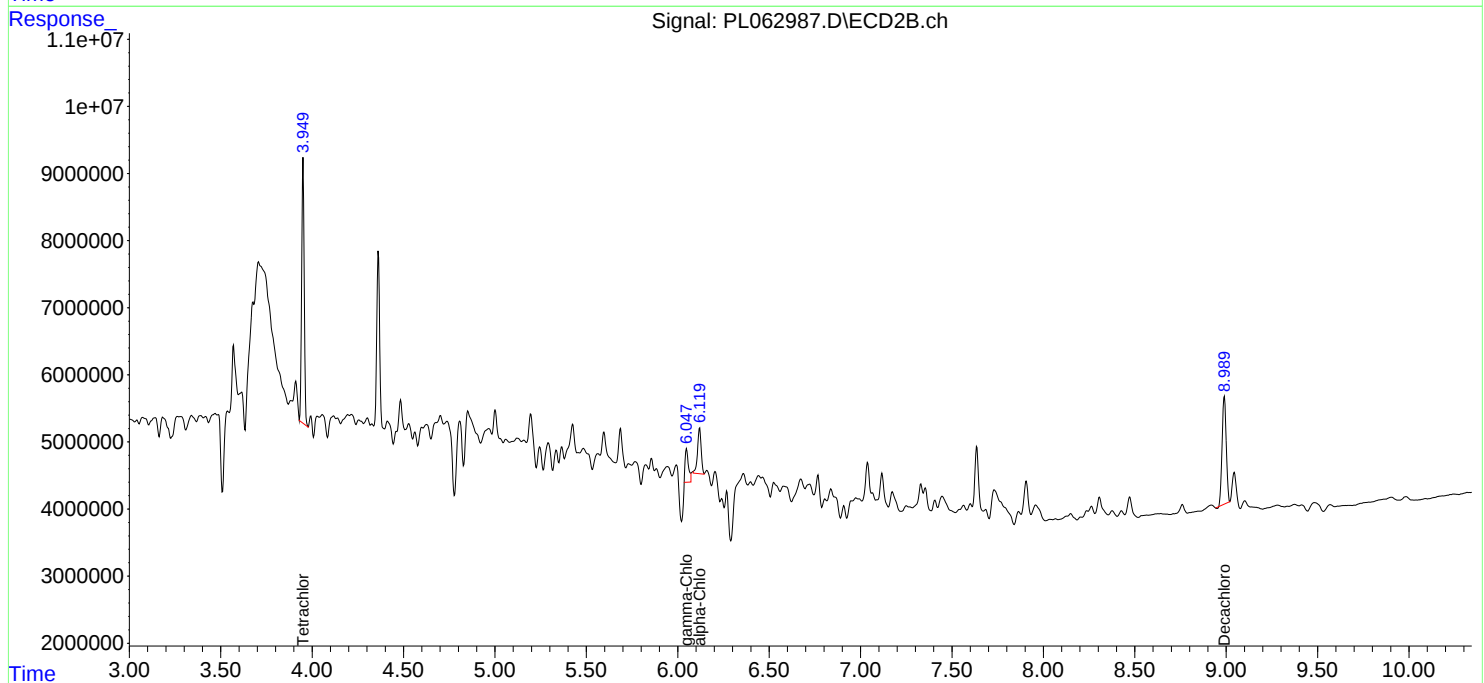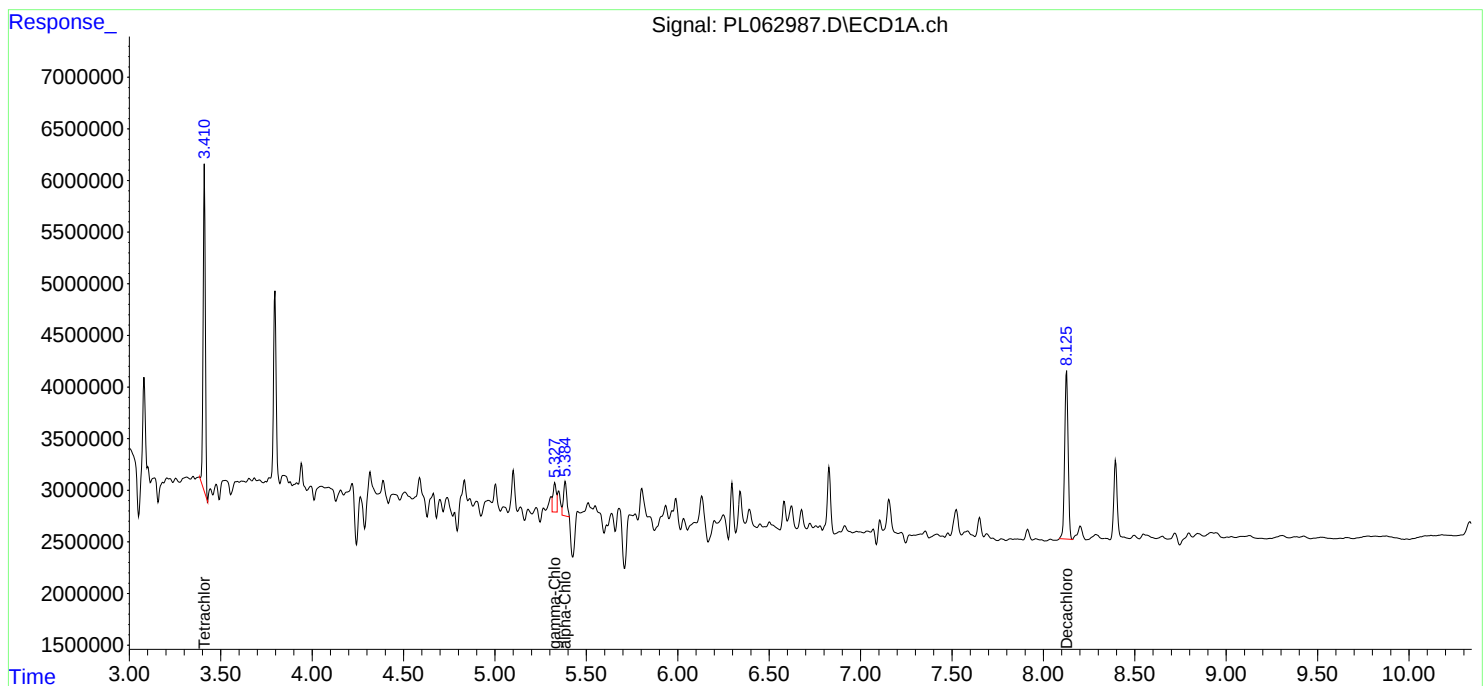

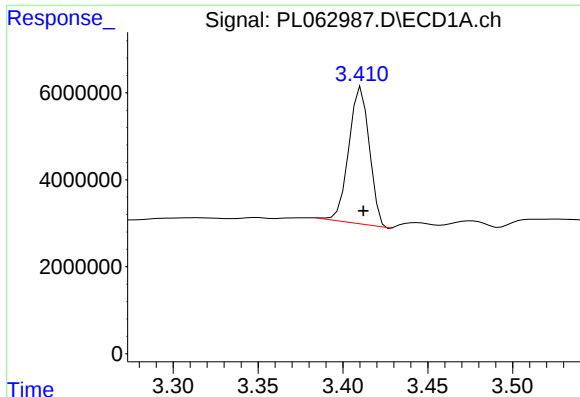


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 26598223
Conc: 15.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-99(0-10)


Manual Integrations
APPROVED

Ankita
11/13/2020 12:12:41 PM

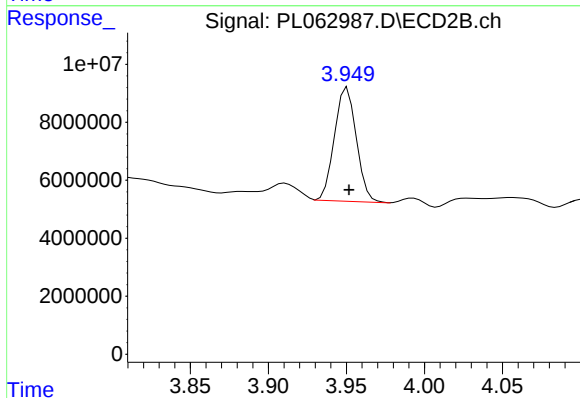


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.002 min
Response: 38329506
Conc: 13.04 ng/ml m

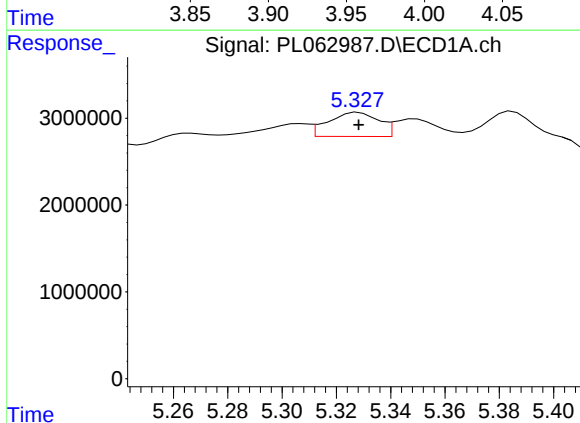


#10 gamma-Chlordane

R.T.: 5.327 min
Delta R.T.: -0.002 min
Response: 3805474
Conc: 2.11 ng/ml m

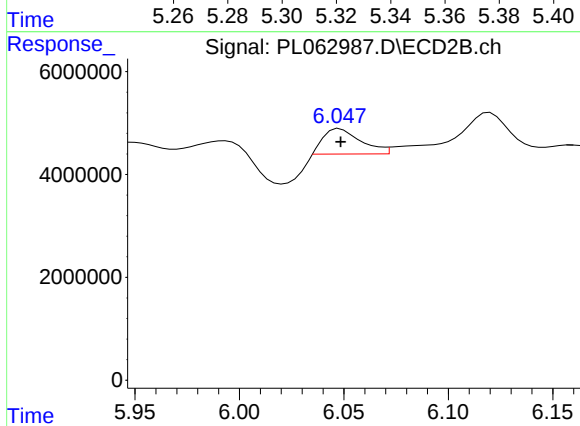

#10 gamma-Chlordane

R.T.: 6.047 min
Delta R.T.: -0.002 min
Response: 6187202
Conc: 1.84 ng/ml m

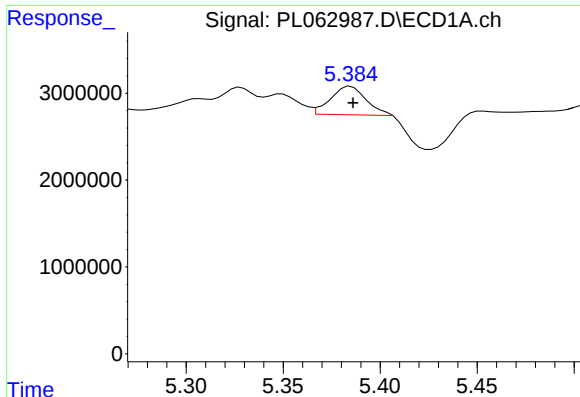


#11 alpha-Chlordane

R.T.: 5.384 min
Delta R.T.: -0.003 min
Response: 4116486
Conc: 2.28 ng/ml m

Instrument :
ECD_L
ClientSampleId :
M-99(0-10)


Manual Integrations
APPROVED

Ankita
11/13/2020 12:12:41 PM

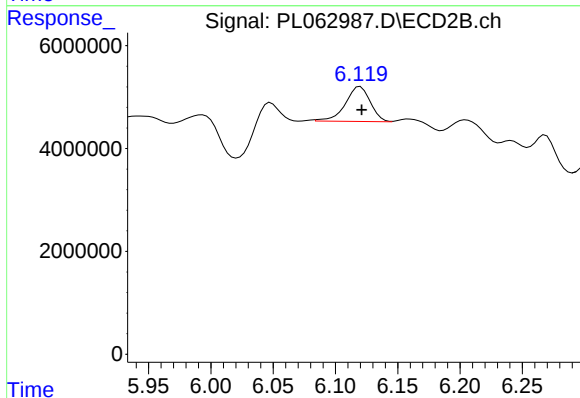


#11 alpha-Chlordane

R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 9481205
Conc: 2.81 ng/ml m

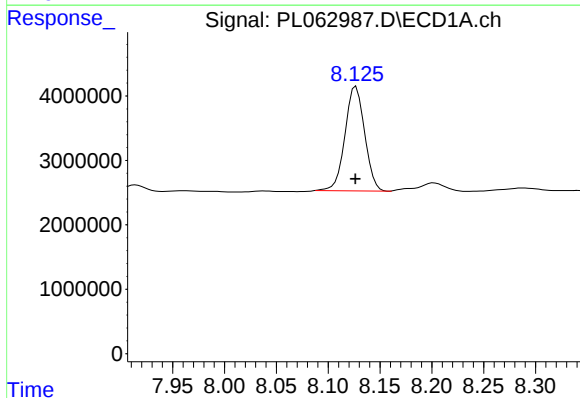

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 21405729
Conc: 13.34 ng/ml

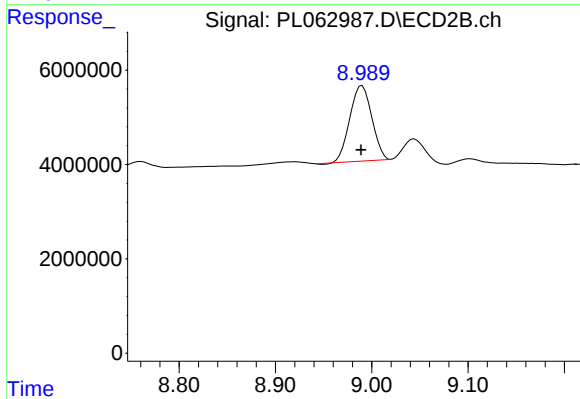

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.001 min
Response: 25265513
Conc: 12.07 ng/ml