

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111221\
 Data File : PL070942.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2021 08:35
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:41:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
7) B	delta-BHC	0.000	7.024f	0	2836903	N.D. 1.696 #
8) B	Heptachlo...	0.000	7.972	0	2987415	N.D. 1.960 #
9) A	Endosulfan I	0.000	8.391f	0	784392	N.D. 0.545 #
11) B	alpha-Chl...	0.000	8.331f	0	701707	N.D. 0.461 #
14) MA	Endrin	0.000	8.902	0	4379495	N.D. 3.781 #
17) MA	4,4'-DDT	0.000	9.379f	0	1612099	N.D. 1.278 #
18) B	Endrin al...	0.000	9.266	0	1297304	N.D. 1.342 #
20) A	Methoxychlor	0.000	9.824f	0	1056240	N.D. 1.561 #
21) B	Endrin ke...	9.207f	0.000	1398348	0	1.956 N.D. #
22)	Mirex	0.000	10.459	0	2025122	N.D. 1.944 #
26)	Chlordane-4	0.000	8.331f	0	701707	N.D. 2.892 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111221\
Data File : PL070942.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2021 08:35
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:41:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

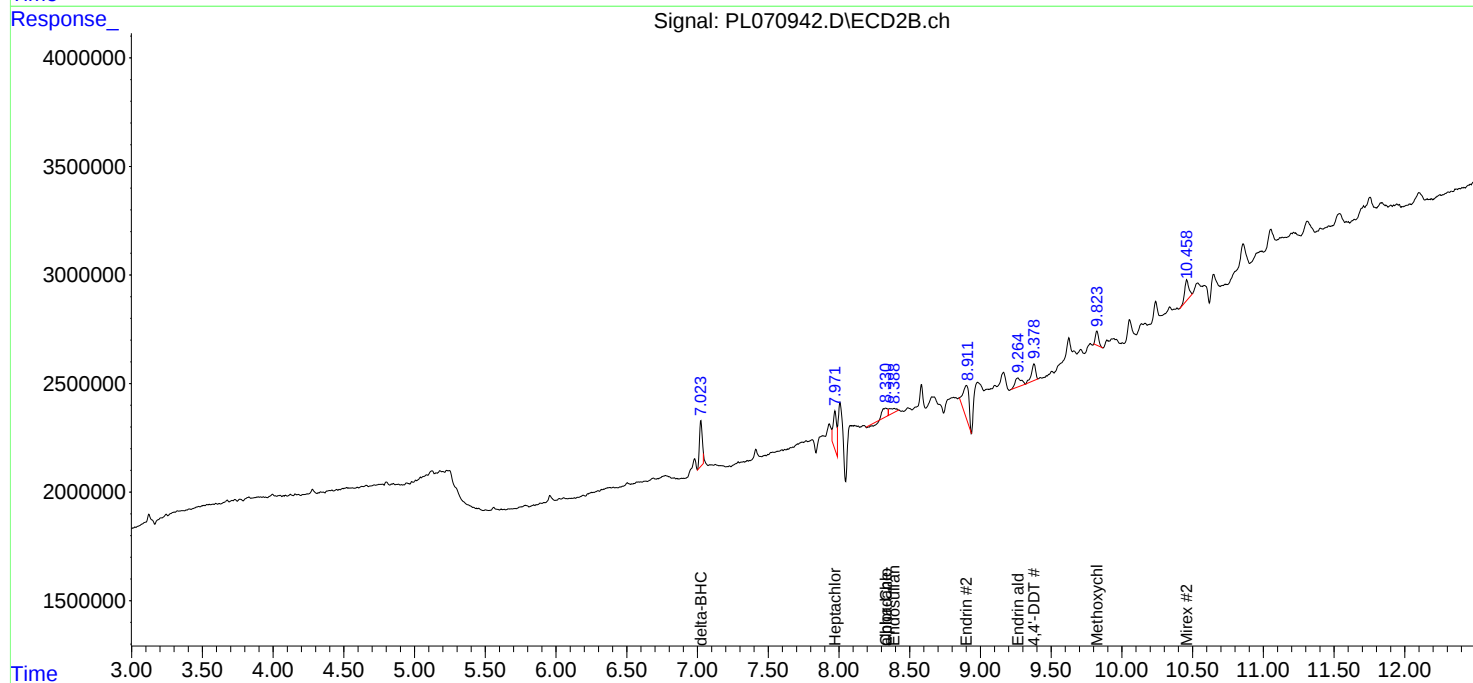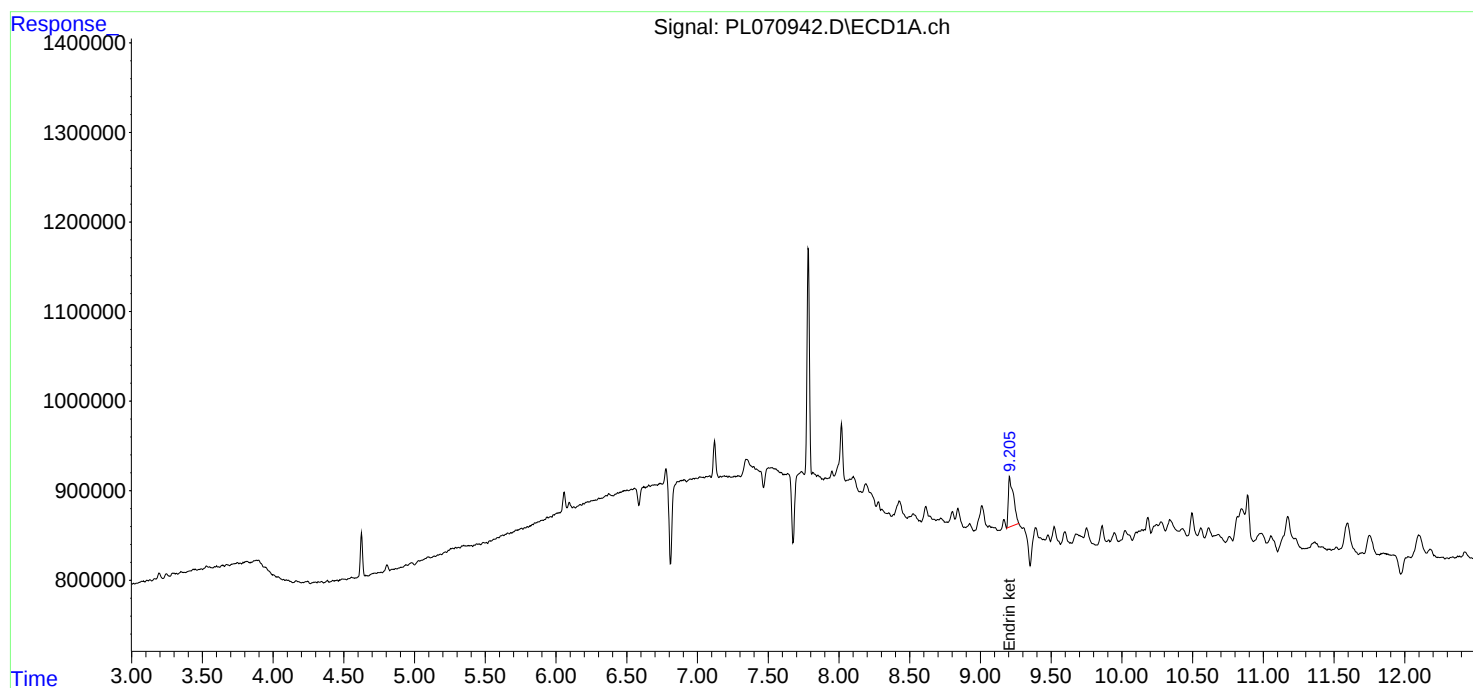


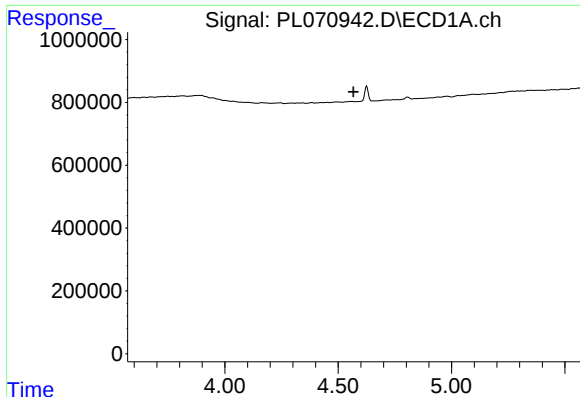

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

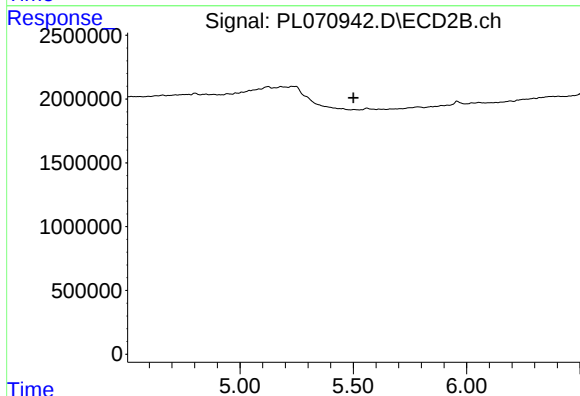


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

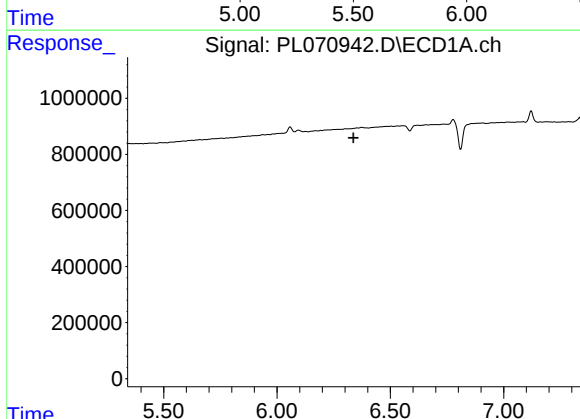


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.338 min
Response: 0
Conc: N.D.

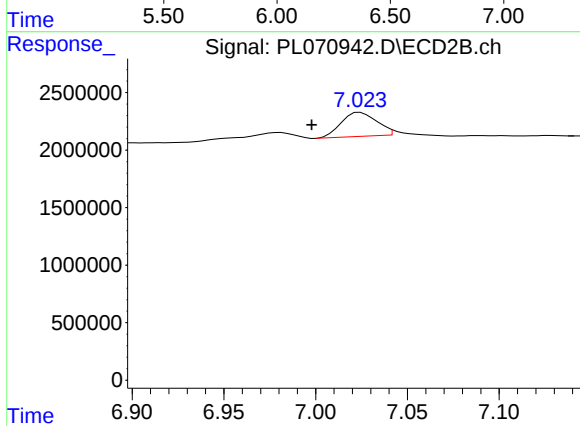

#7 delta-BHC


R.T.: 7.024 min
Delta R.T.: 0.026 min
Response: 2836903
Conc: 1.70 ng/ml

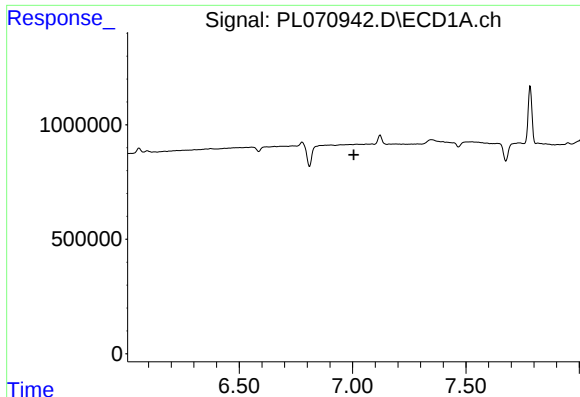

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

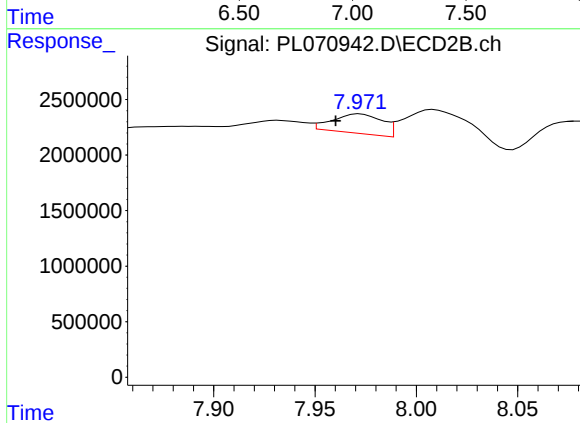


#8 Heptachlor epoxide

R.T.: 7.972 min
Delta R.T.: 0.012 min
Response: 2987415
Conc: 1.96 ng/ml

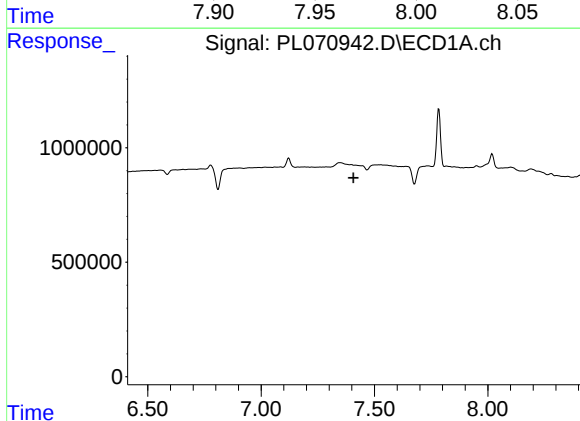


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.408 min
Response: 0
Conc: N.D.

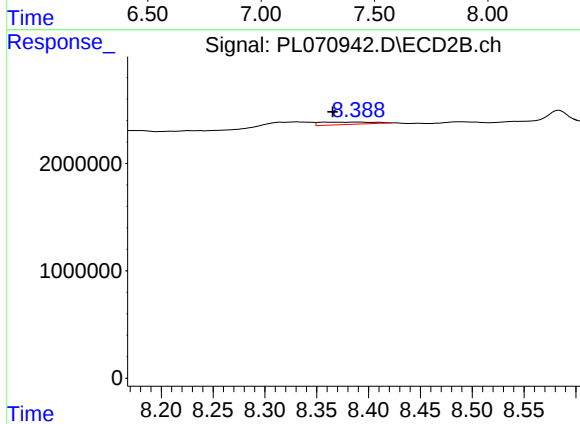

#9 Endosulfan I


R.T.: 8.391 min
Delta R.T.: 0.026 min
Response: 784392
Conc: 0.55 ng/ml

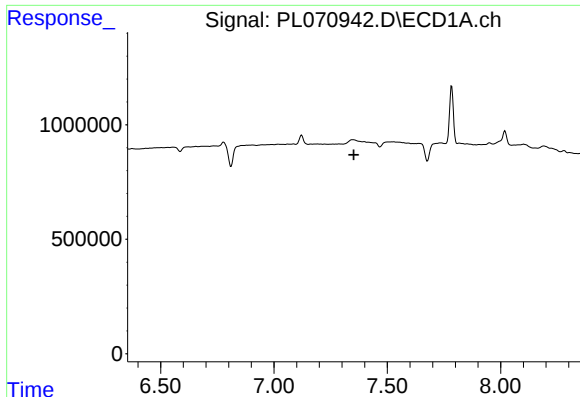

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

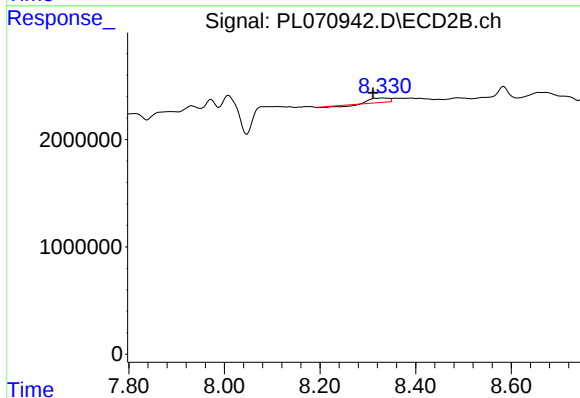


#11 alpha-Chlordane

R.T.: 8.331 min
Delta R.T.: 0.020 min
Response: 701707
Conc: 0.46 ng/ml

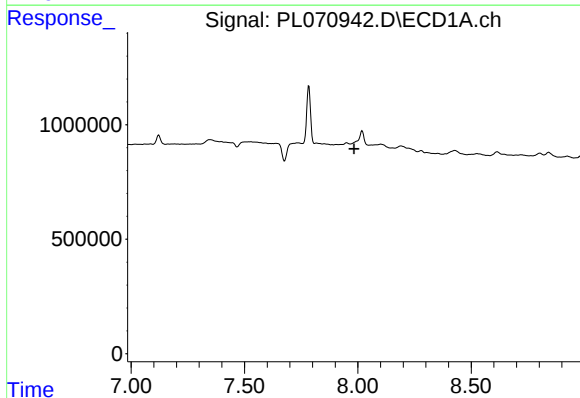


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 7.984 min
Response: 0
Conc: N.D.

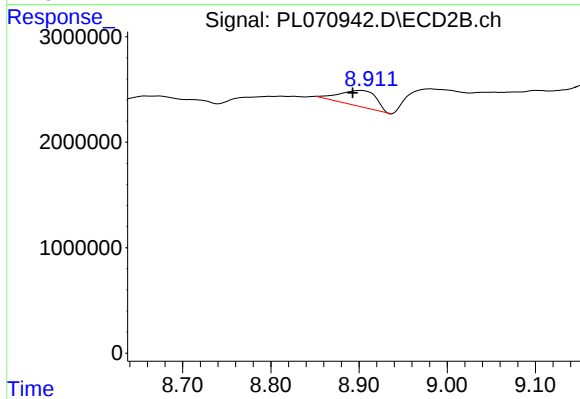

#14 Endrin


R.T.: 8.902 min
Delta R.T.: 0.009 min
Response: 4379495
Conc: 3.78 ng/ml

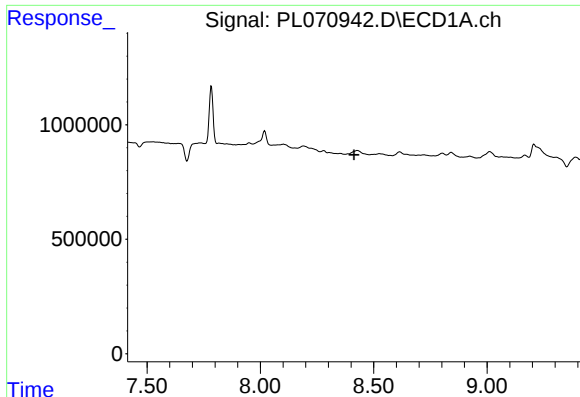

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.413 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

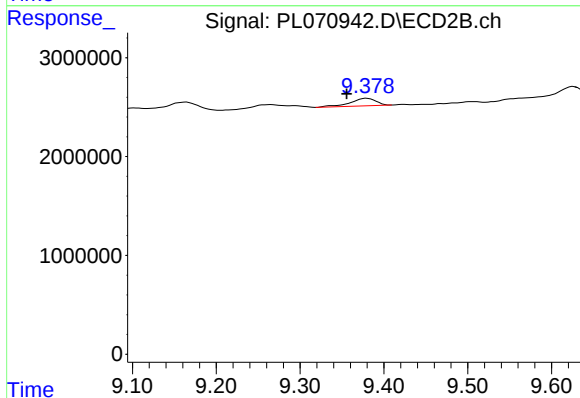


#17 4,4'-DDT

R.T.: 9.379 min
Delta R.T.: 0.024 min
Response: 1612099
Conc: 1.28 ng/ml

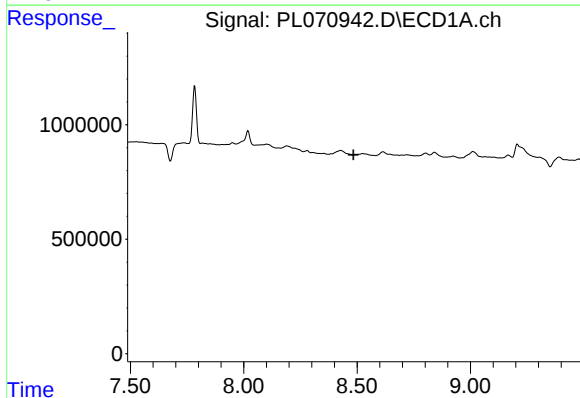


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.484 min
Response: 0
Conc: N.D.

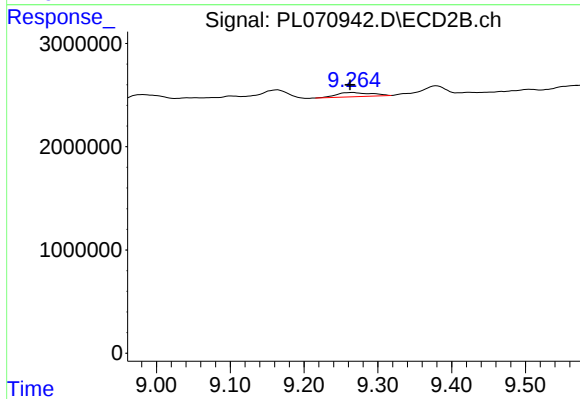

#18 Endrin aldehyde


R.T.: 9.266 min
Delta R.T.: 0.003 min
Response: 1297304
Conc: 1.34 ng/ml

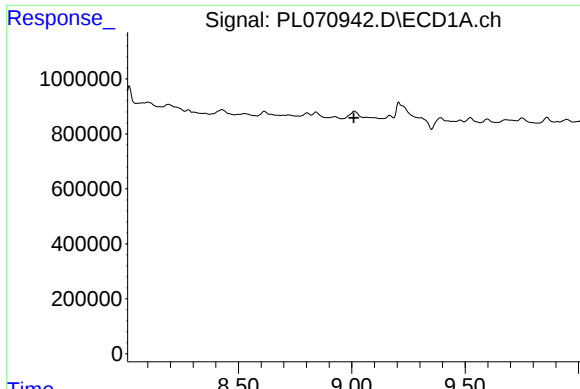

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

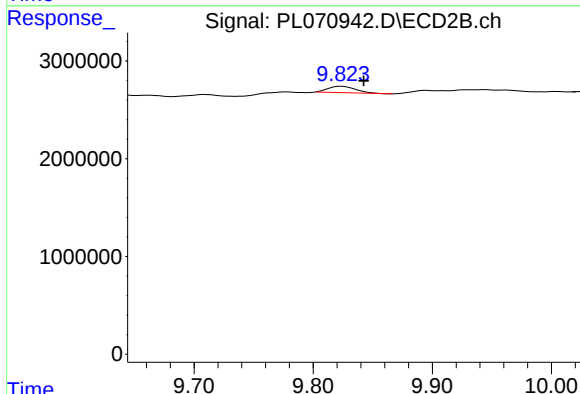


#20 Methoxychlor

R.T.: 9.824 min
Delta R.T.: -0.018 min
Response: 1056240
Conc: 1.56 ng/ml

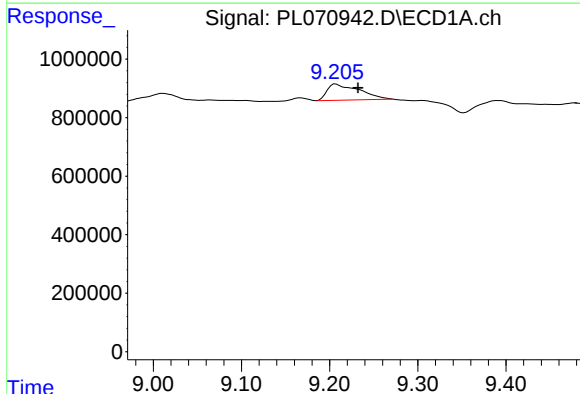


#21 Endrin ketone

R.T.: 9.207 min
Delta R.T.: -0.025 min
Response: 1398348
Conc: 1.96 ng/ml

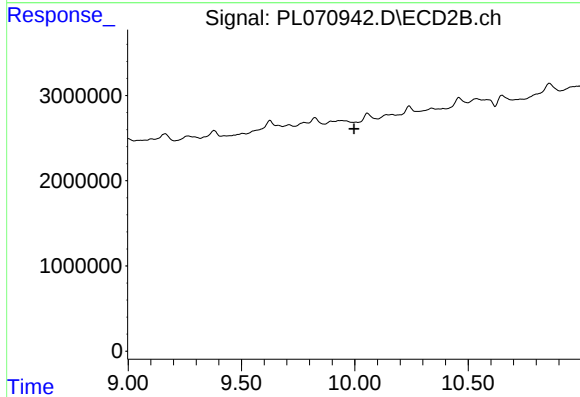

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.996 min
Response: 0
Conc: N.D.

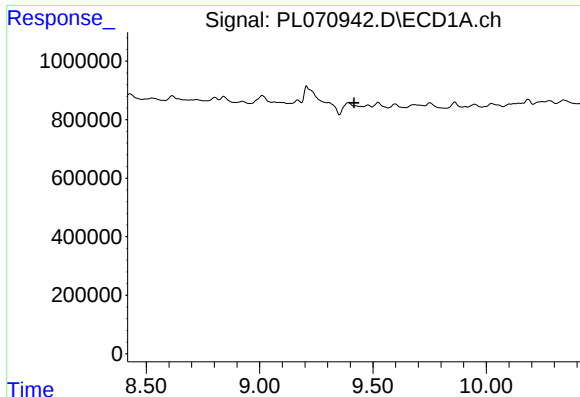

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

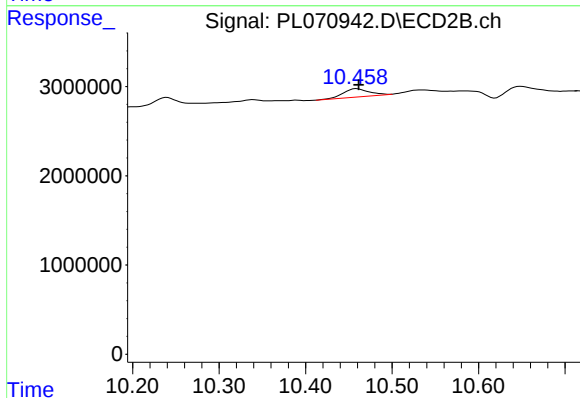


#22 Mirex

R.T.: 10.459 min
Delta R.T.: -0.002 min
Response: 2025122
Conc: 1.94 ng/ml

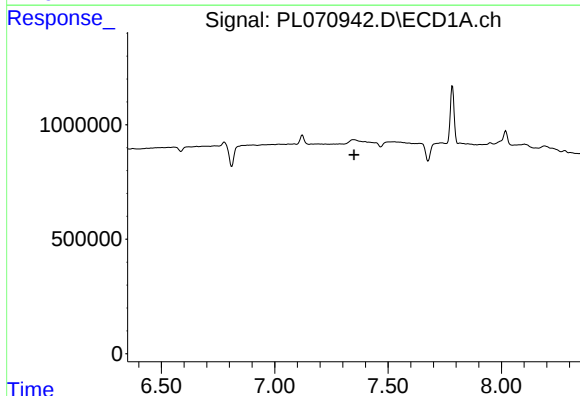


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

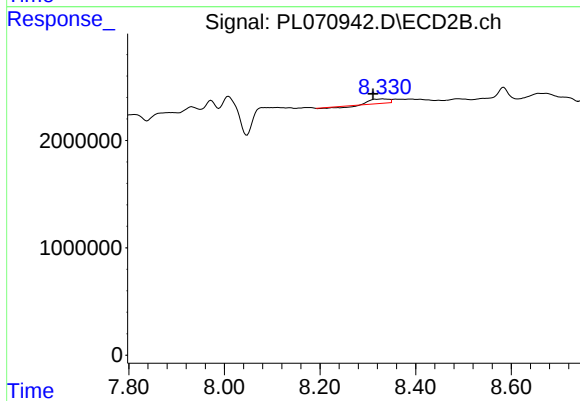

#26 Chlordane-4


R.T.: 8.331 min
Delta R.T.: 0.020 min
Response: 701707
Conc: 2.89 ng/ml

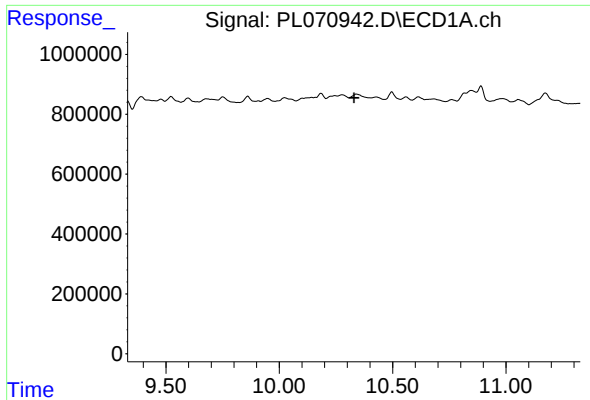

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.330 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

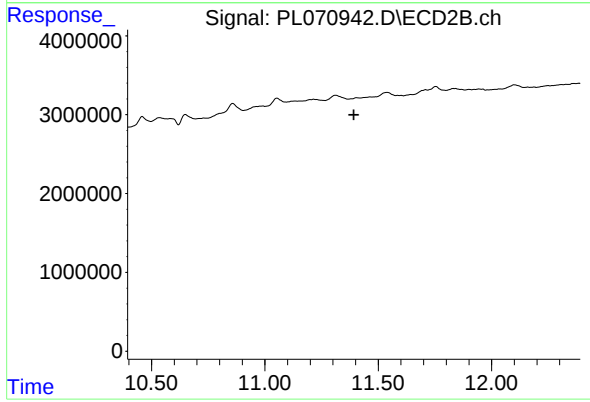

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.392 min
Response: 0
Conc: N.D.