

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111223\
 Data File : PL086591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2023 12:35
 Operator : AR\AJ
 Sample : 05310-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/13/2023
 Supervised By : Ankita Jodhani 11/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 21:00:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 13:04:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	2.619	33544358	20948139	10.331m	21.275 #
2)	SA Decachlor...	8.859	7.769	52355964	20053081	17.886	16.606

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111223\
Data File : PL086591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2023 12:35
Operator : AR\AJ
Sample : 05310-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/13/2023
Supervised By : Ankita Jodhani 11/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 21:00:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 13:04:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

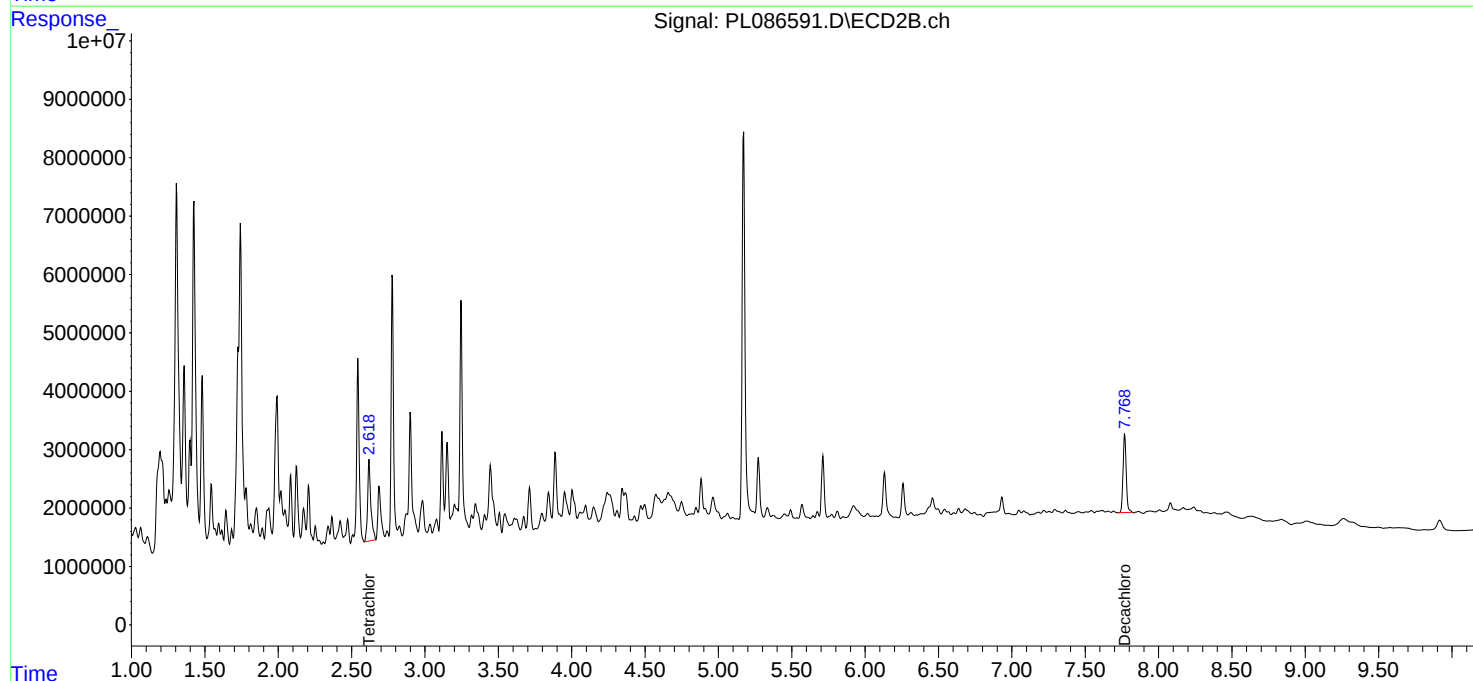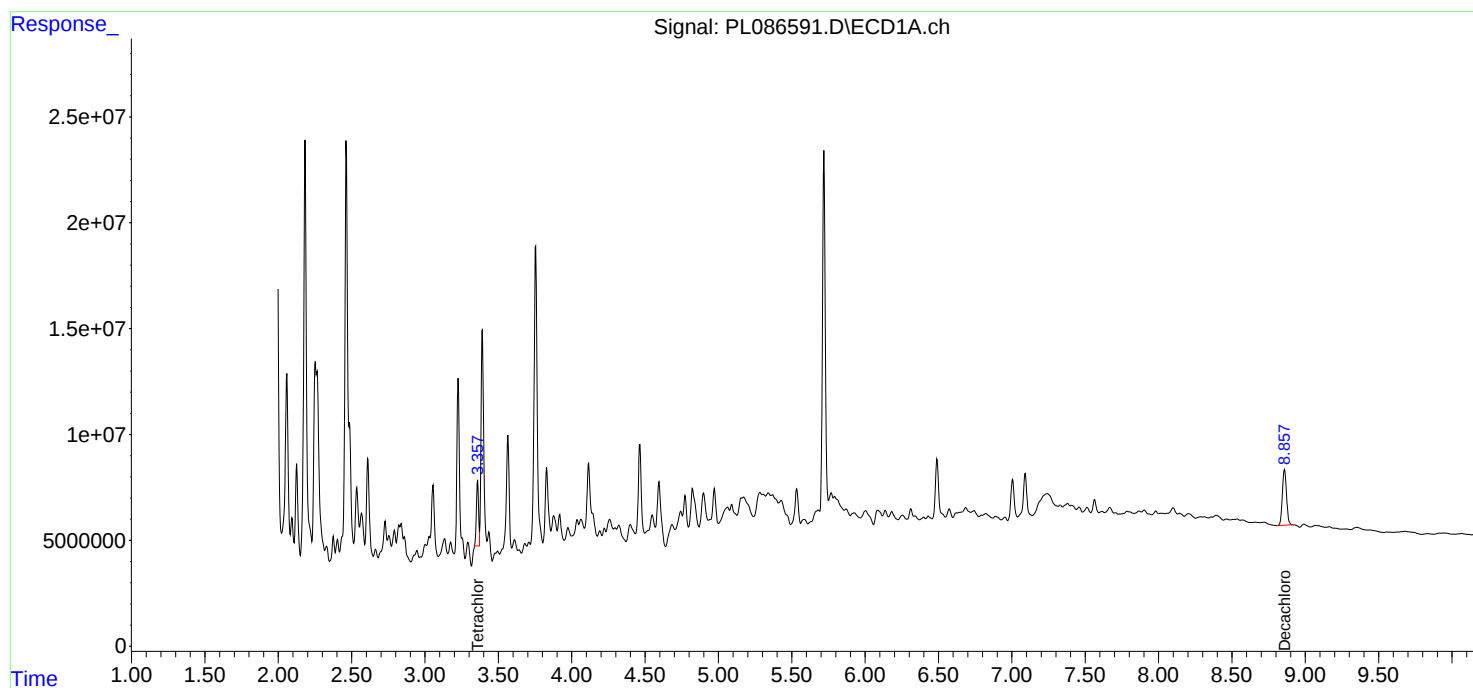

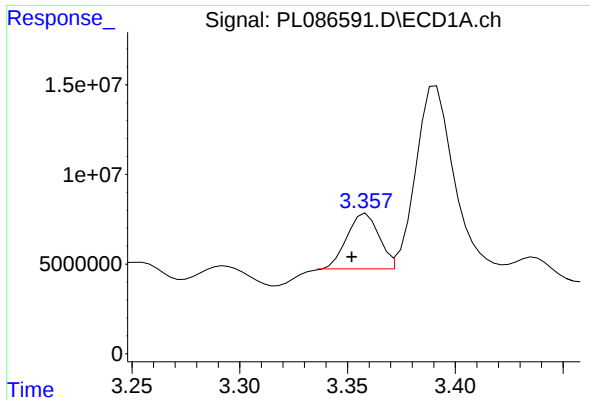


#1 Tetrachloro-m-xylene

R.T.: 3.357 min
Delta R.T.: 0.005 min
Response: 33544358
Conc: 10.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

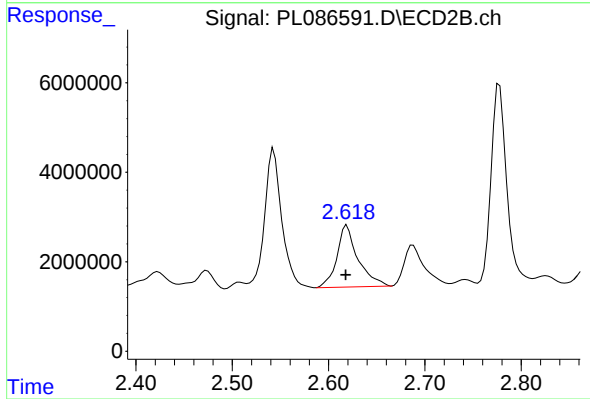


#1 Tetrachloro-m-xylene

R.T.: 2.619 min
Delta R.T.: 0.001 min
Response: 20948139
Conc: 21.27 ng/ml

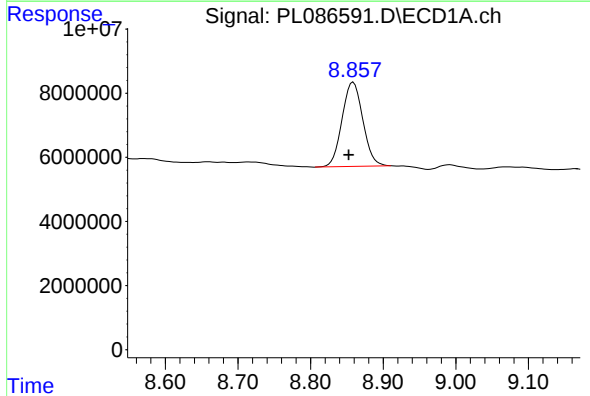

#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.006 min
Response: 52355964
Conc: 17.89 ng/ml

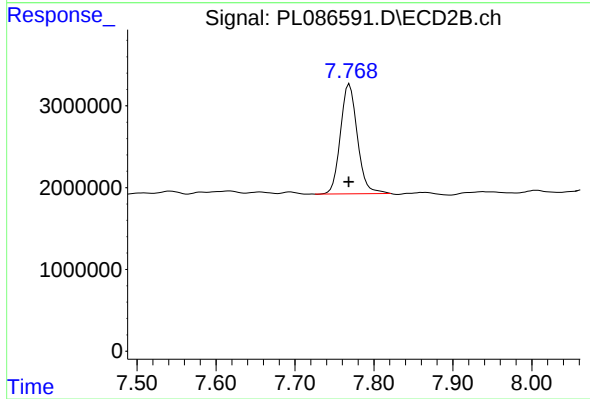

#28 Decachlorobiphenyl

R.T.: 7.769 min
Delta R.T.: 0.001 min
Response: 20053081
Conc: 16.61 ng/ml