

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111318\
 Data File : PL042102.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 11:56
 Operator : AJ\SJ
 Sample : J5847-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C0AK7

Manual Integrations
 APPROVED

Sohil
 11/14/2018 4:20:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 04:01:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 24 01:06:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	117.4E6	63474438	18.364	19.643
27)	SA Decachlor...	8.210	9.235	163.1E6	69825515	25.415	26.037
Target Compounds							
8)	B Heptachlo...	5.178	6.000	465.1E6	240.0E6	59.748	69.705
10)	B trans-Chl...	5.404	6.234	129.4E6	80852082	16.780	24.952 #
11)	B cis-Chlor...	5.461	6.307	123.7E6	73576007	16.277	23.239m#
15)	B Endosulfa...	6.295	7.044	32885294	5982054	4.930m	2.228m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111318\
Data File : PL042102.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2018 11:56
Operator : AJ\SJ
Sample : J5847-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 04:01:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 24 01:06:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

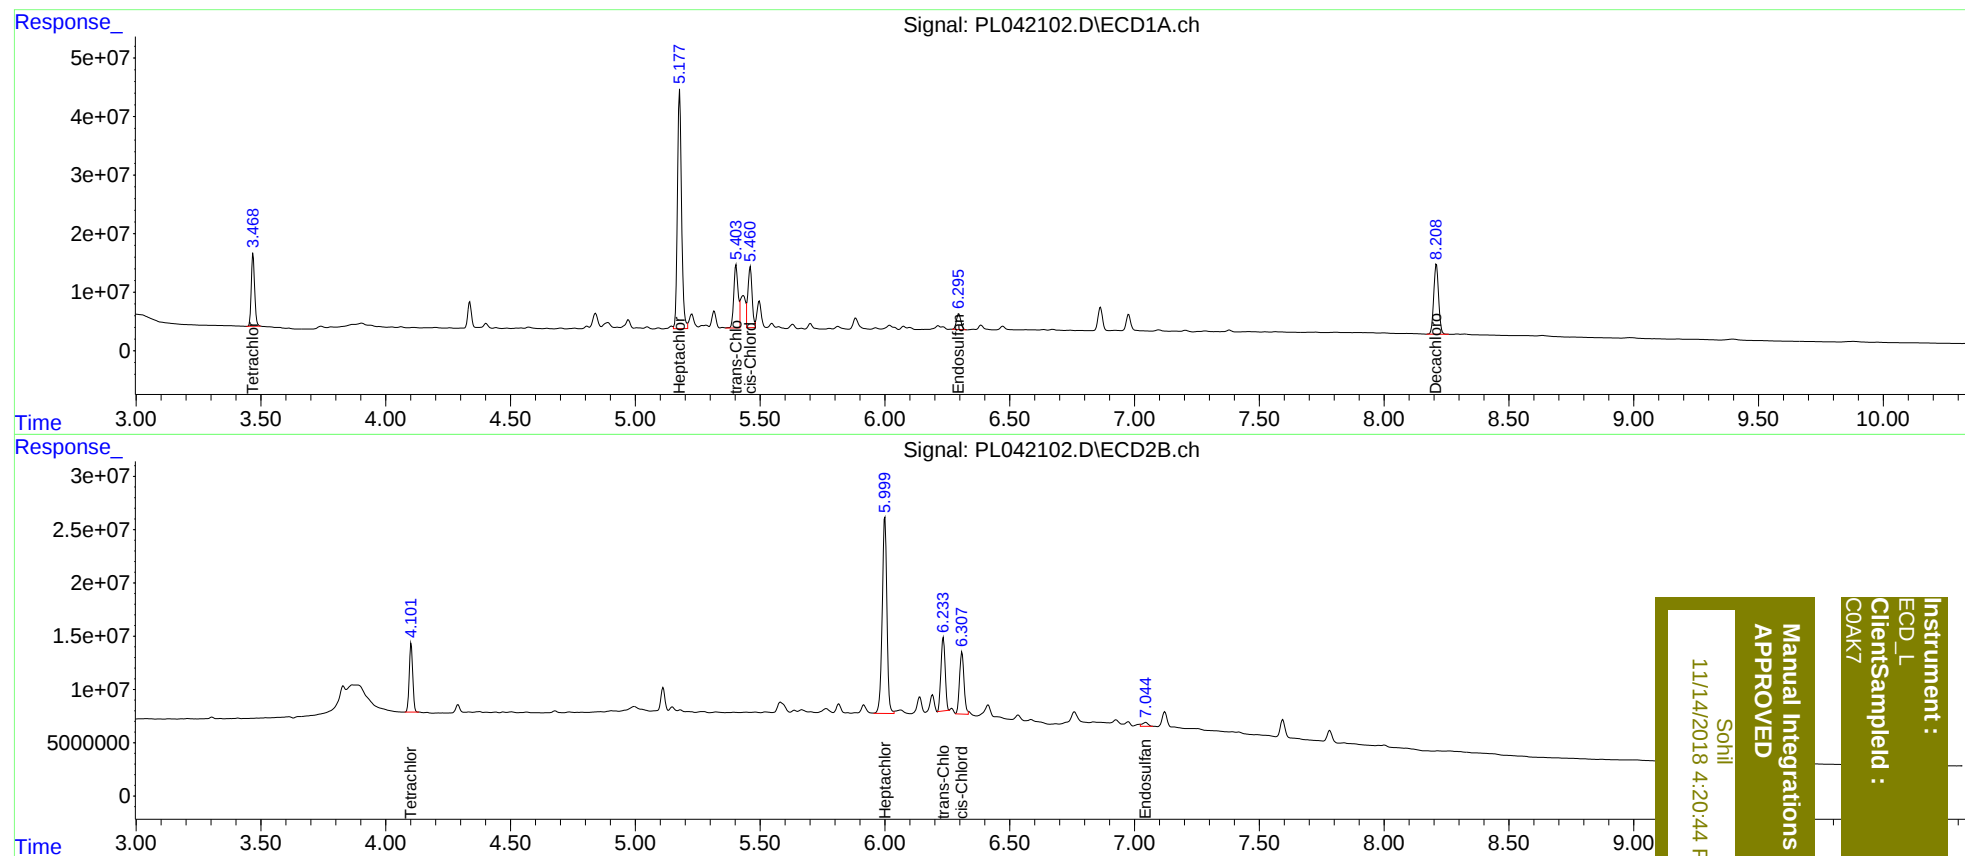

Manual Integrations
APPROVED

Sohil
11/14/2018 4:20:44 PM

Instrument :
ECD_L
ClientSampled :
COAK7