

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111318\
 Data File : PL042097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 10:46
 Operator : AJ\SJ
 Sample : J5847-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1


Instrument :
 ECD_L
 ClientSampleId :
 C0AH3MSD

Manual Integrations
 APPROVED

Sohil
 11/14/2018 4:15:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 04:00:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 24 01:06:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

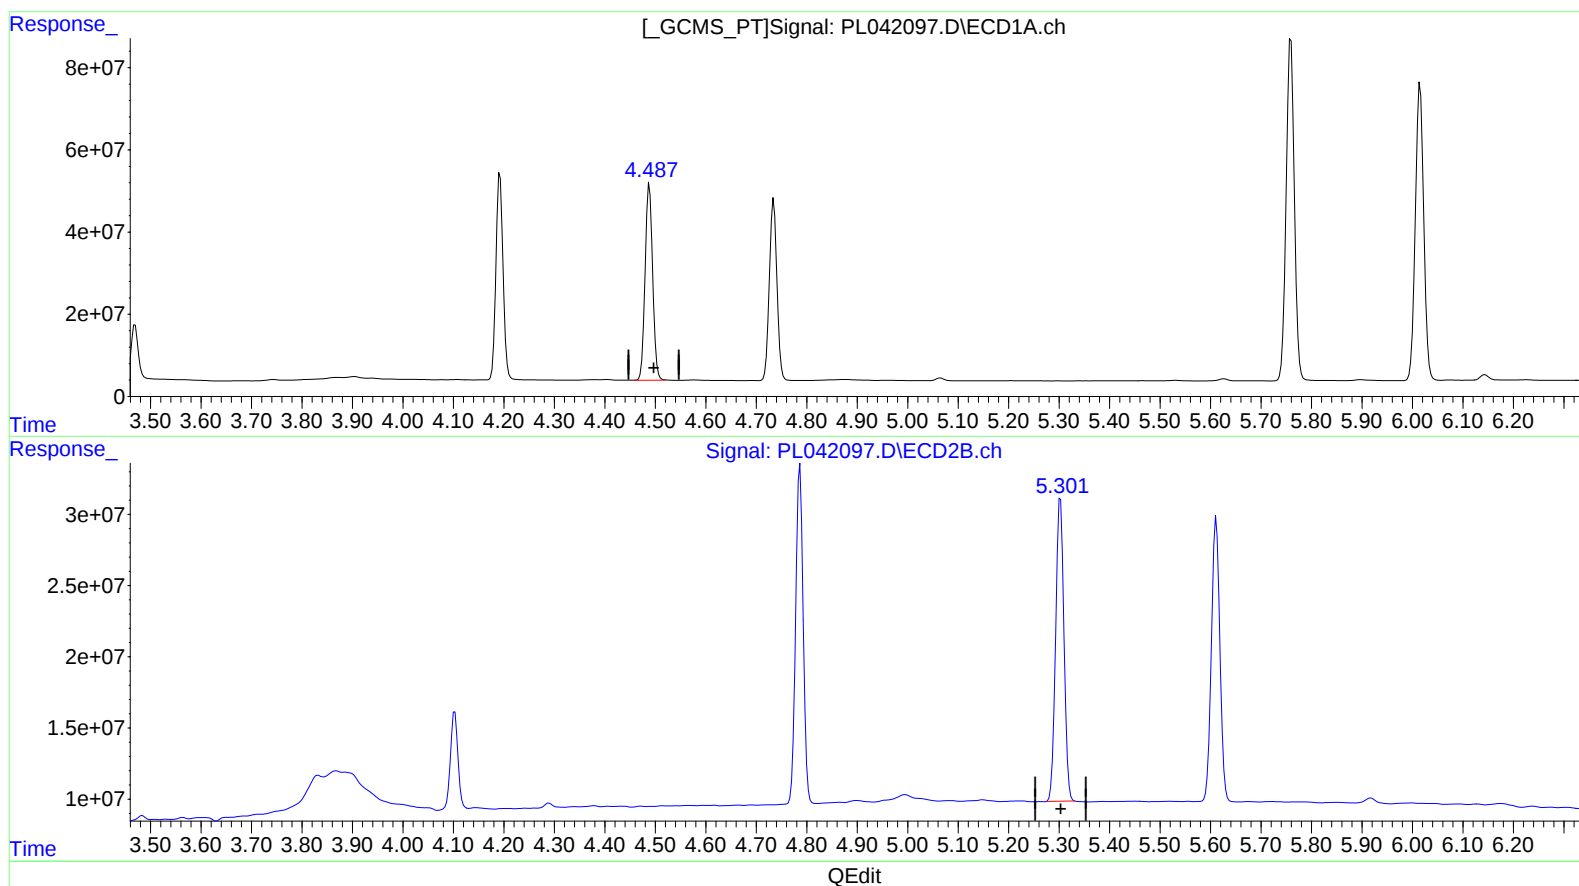

(4) Heptachlor (MA)
 4.487min 54.287 ng/ml m
 response 496153917

(4) Heptachlor #2 (MA)
 5.303min 57.070 ng/ml
 response 243546592

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111318\
 Data File : PL042097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 10:46
 Operator : AJ\SJ
 Sample : J5847-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 Client Sample ID :
 C0AH3MSD

Manual Integrations
 APPROVED

Sohil
 11/14/2018 4:15:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 04:00:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102318CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 24 01:06:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.2
 Signal #2 Phase: ZB-MR1
 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.469	4.103	127.1E6	70201987	19.888	21.725
27) SA Decachlor...	8.210	9.235	170.0E6	73463836	26.494	27.394
Target Compounds						
3) MA gamma-BHC...	4.192	4.787	485.9E6	246.8E6	55.905	57.165
4) MA Heptachlor	4.487	5.303	496.2E6	243.5E6	54.287m	57.070
5) MB Aldrin	4.734	5.611	461.3E6	232.6E6	58.879	63.577
13) MA Dieldrin	5.759	6.618	943.3E6	436.9E6	113.923	129.611
14) MA Endrin	6.015	6.838	832.8E6	357.2E6	118.224	133.126
17) MA 4,4'-DDT	6.382	7.255	696.3E6	315.9E6	111.574	119.642

} SJ 11/17/18

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.