

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111323\
 Data File : PL086619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2023 16:11
 Operator : AR\AJ
 Sample : 05385-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-03-11102023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 20:05:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 13:04:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.619	12631896	3911200	3.890	3.972
28)	SA Decachlor...	8.852	7.767	19067792	7114830	6.514	5.892
Target Compounds							
12)	B 4,4'-DDE	6.013	5.074	2260876	701277	0.652	0.683


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111323\
Data File : PL086619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2023 16:11
Operator : AR\AJ
Sample : 05385-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HR-03-11102023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 20:05:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 13:04:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

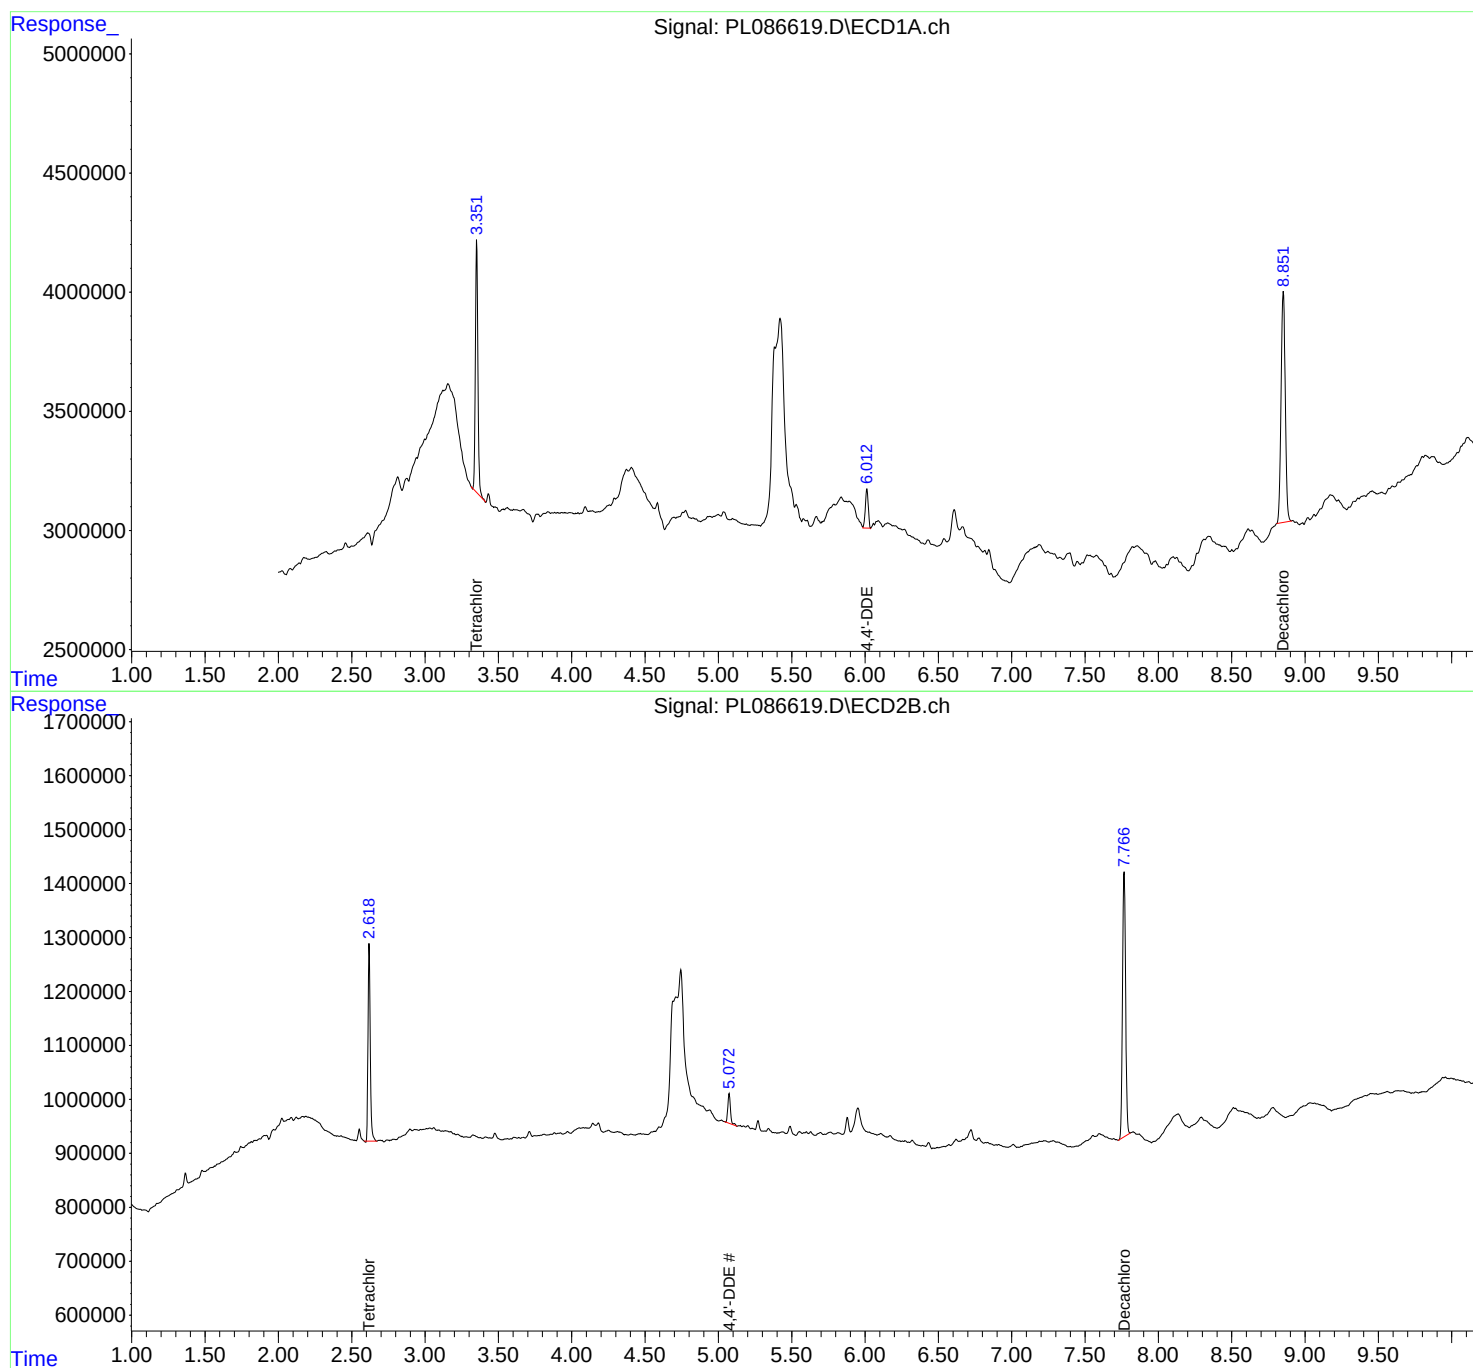


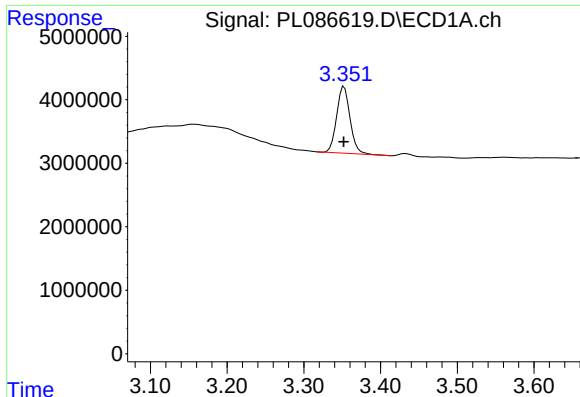

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 12631896
Conc: 3.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-03-11102023

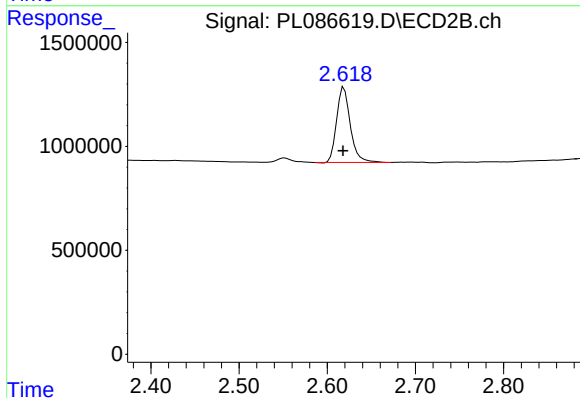


#1 Tetrachloro-m-xylene

R.T.: 2.619 min
Delta R.T.: 0.001 min
Response: 3911200
Conc: 3.97 ng/ml

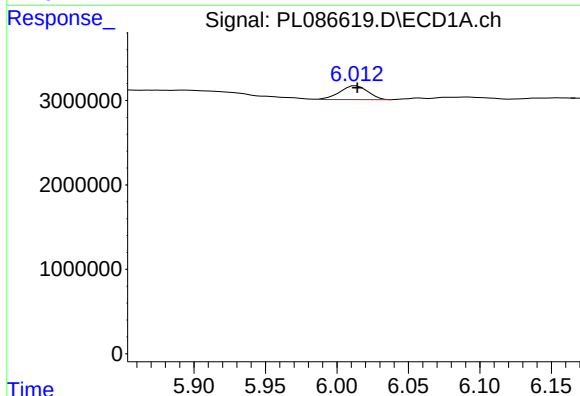


#12 4,4'-DDE

R.T.: 6.013 min
Delta R.T.: 0.000 min
Response: 2260876
Conc: 0.65 ng/ml

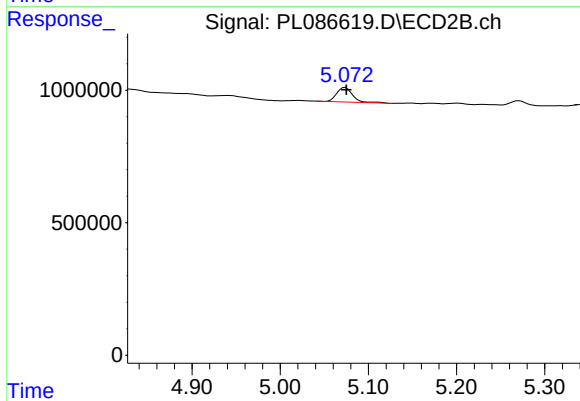

#12 4,4'-DDE


R.T.: 5.074 min
Delta R.T.: -0.001 min
Response: 701277
Conc: 0.68 ng/ml

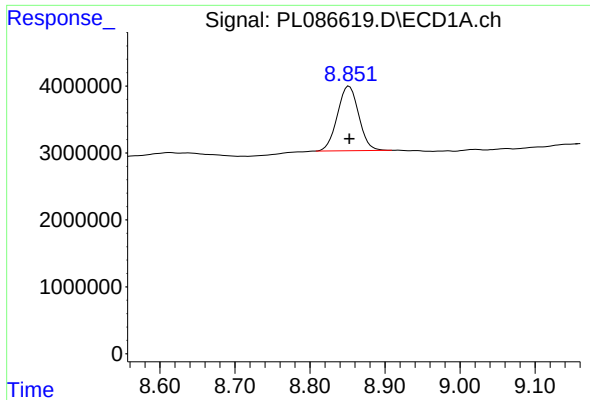

#28 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: 0.000 min
Response: 19067792
Conc: 6.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-03-11102023

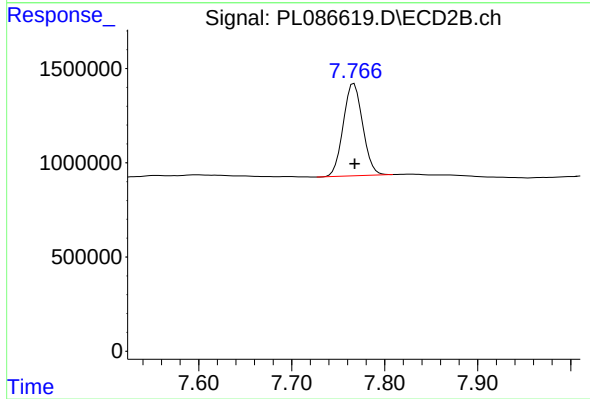

#28 Decachlorobiphenyl

R.T.: 7.767 min
Delta R.T.: 0.000 min
Response: 7114830
Conc: 5.89 ng/ml