

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 18:37
 Operator : AJ\SJ
 Sample : J5908-23
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:41:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	55494508	30147217	8.987	10.176
28)	SA Decachlor...	8.208	9.232	50312779	20769223	7.345	8.143
Target Compounds							
6)	B beta-BHC	4.403f	0.000	8438697	0	2.287	N.D. #
9)	A Endosulfan I	0.000	6.307f	0	3768189	N.D.	1.155 #
10)	B gamma-Chl...	0.000	6.242	0	6165094	N.D.	1.739 #
11)	B alpha-Chl...	0.000	6.307	0	3768189	N.D.	1.083 #
13)	MA Dieldrin	5.818f	0.000	1705593	0	0.219	N.D. #
16)	A 4,4'-DDD	6.206f	0.000	2221066	0	0.402	N.D. #
17)	MA 4,4'-DDT	6.376	0.000	2043686	0	0.359	N.D. #
20)	A Methoxychlor	6.906	0.000	1150400	0	0.361	N.D. #
23)	Chlordane-1	4.403	0.000	8438697	0	28.276	N.D. #
25)	Chlordane-3	0.000	6.242	0	6165094	N.D.	12.072 #
26)	Chlordane-4	0.000	6.307	0	3768189	N.D.	6.311 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2018 18:37
Operator : AJ\SJ
Sample : J5908-23
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:41:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

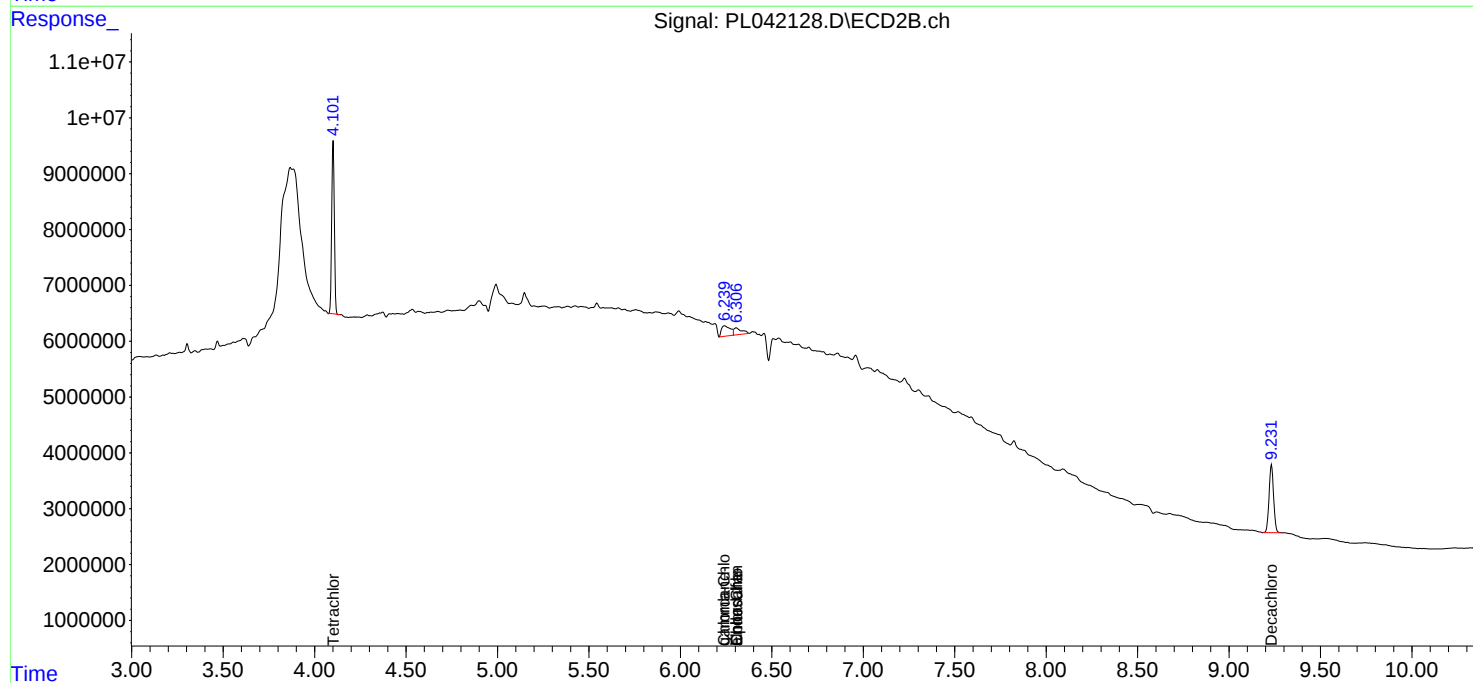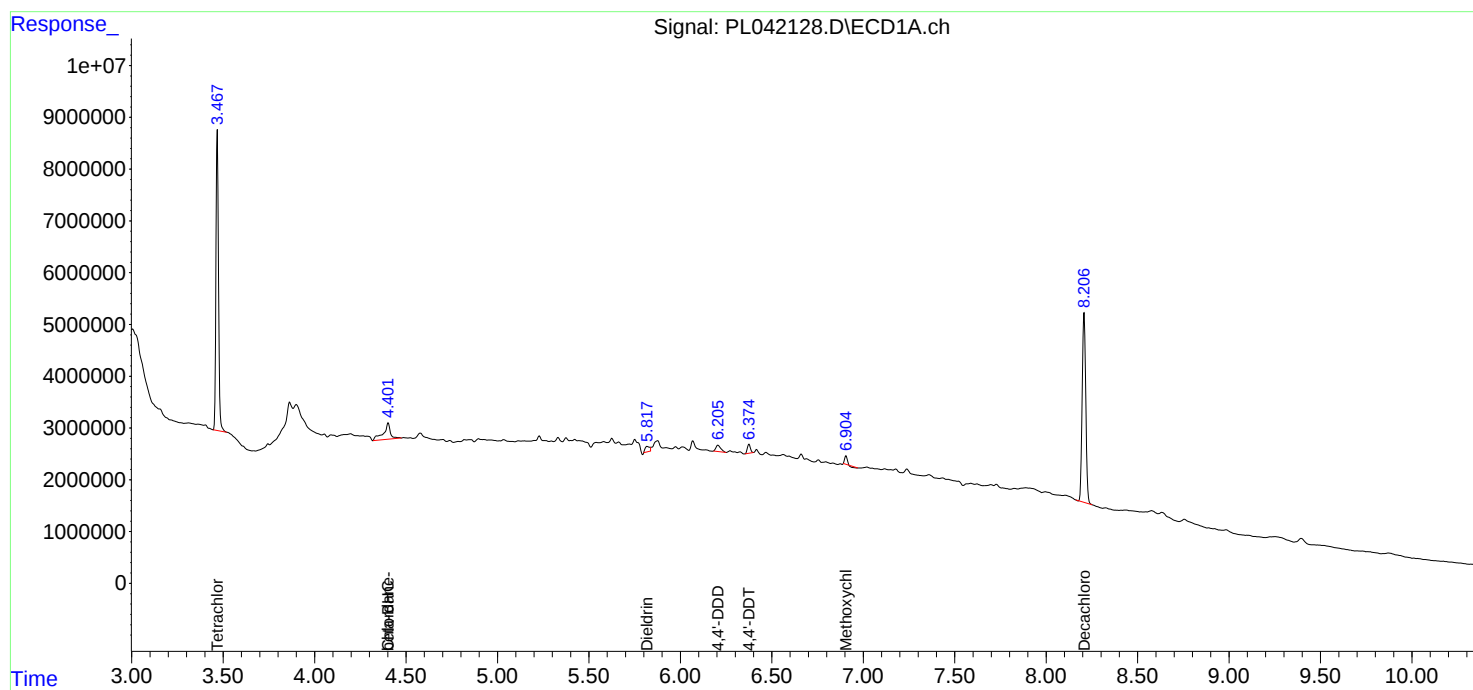


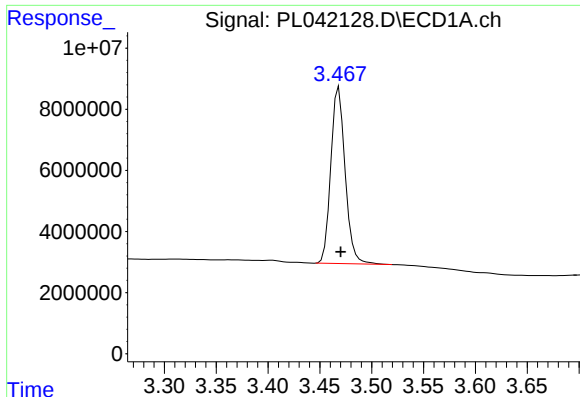

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: -0.002 min
Response: 55494508
Conc: 8.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

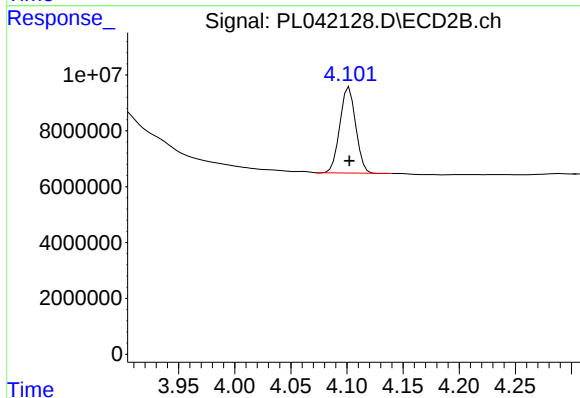


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 30147217
Conc: 10.18 ng/ml

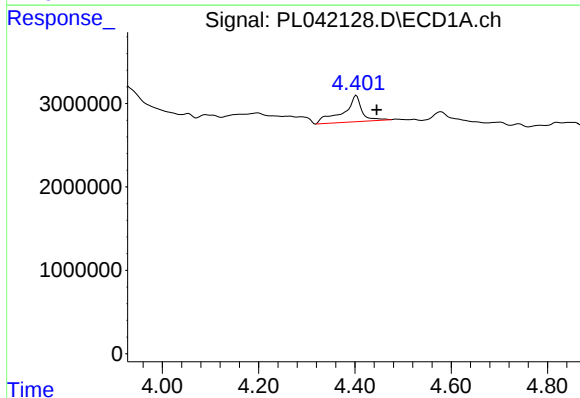


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: -0.043 min
Response: 8438697
Conc: 2.29 ng/ml

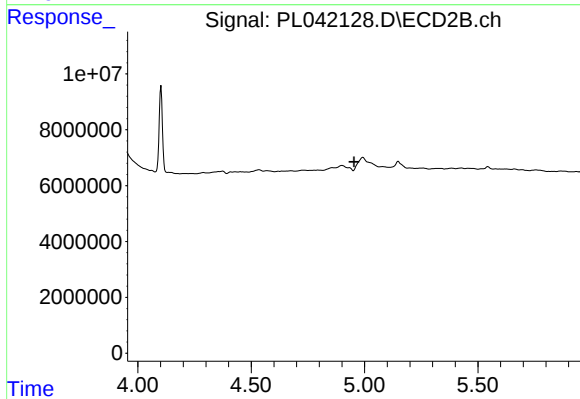

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

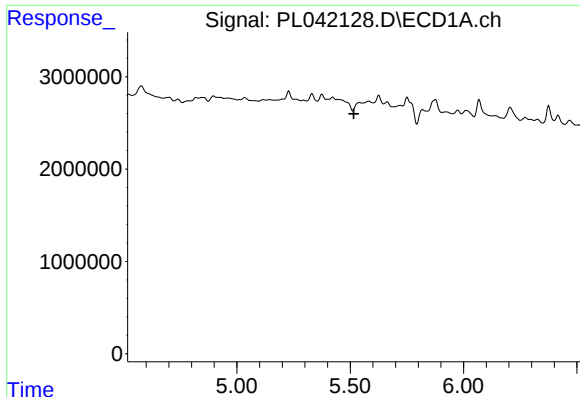

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.515 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

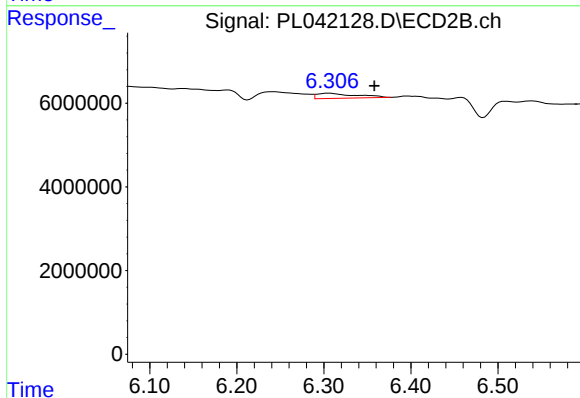


#9 Endosulfan I

R.T.: 6.307 min
Delta R.T.: -0.052 min
Response: 3768189
Conc: 1.16 ng/ml

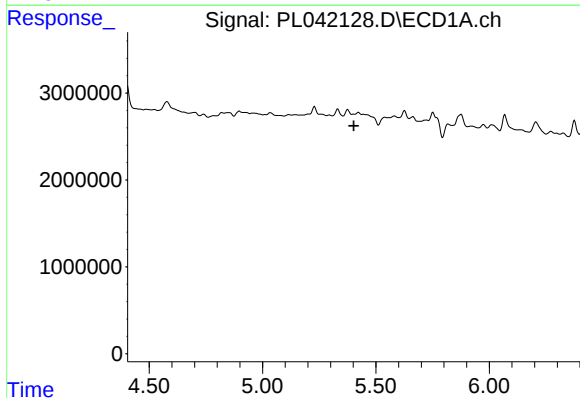


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.403 min
Response: 0
Conc: N.D.

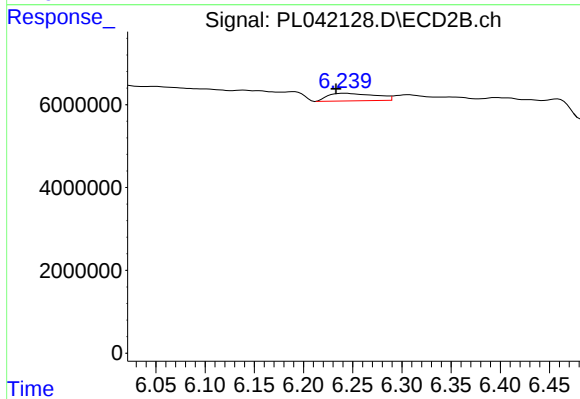

#10 gamma-Chlordane


R.T.: 6.242 min
Delta R.T.: 0.008 min
Response: 6165094
Conc: 1.74 ng/ml

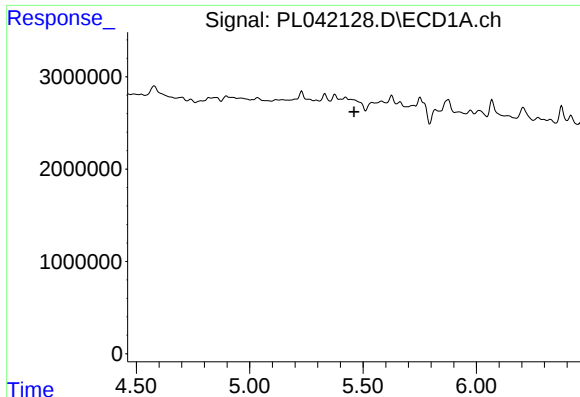

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

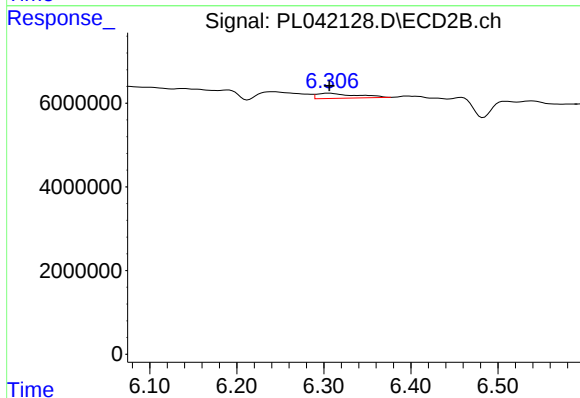


#11 alpha-Chlordane

R.T.: 6.307 min
Delta R.T.: 0.000 min
Response: 3768189
Conc: 1.08 ng/ml

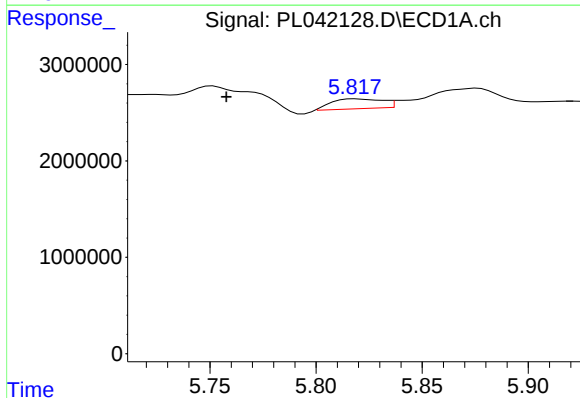


#13 Dieldrin

R.T.: 5.818 min
Delta R.T.: 0.061 min
Response: 1705593
Conc: 0.22 ng/ml

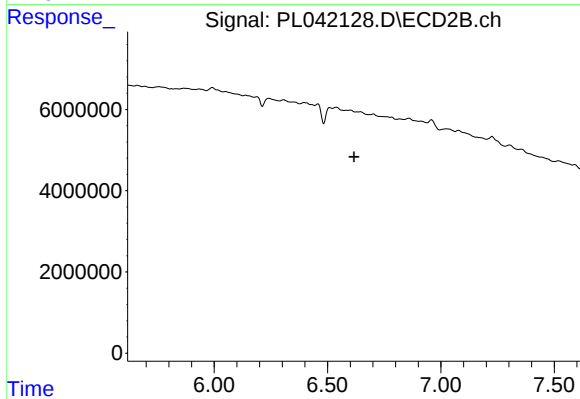

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

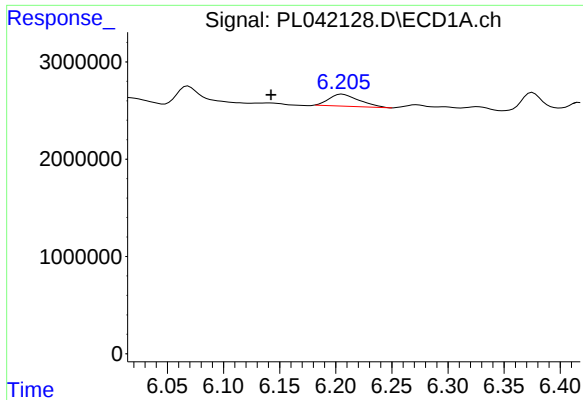

#16 4,4'-DDD


R.T.: 6.206 min
Delta R.T.: 0.064 min
Response: 2221066
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

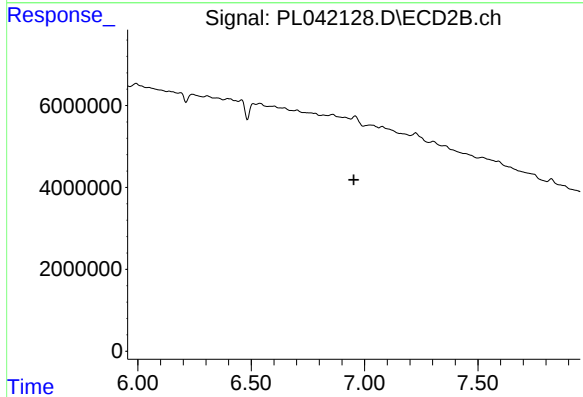


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

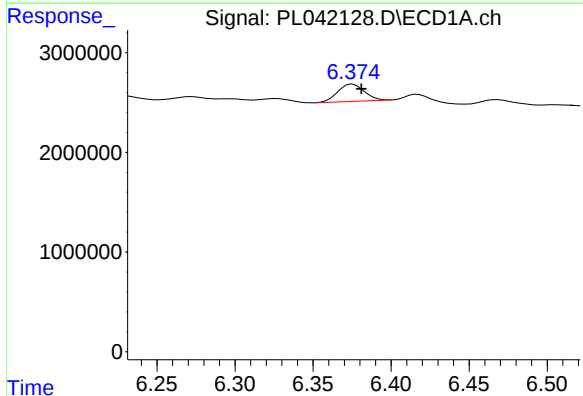


#17 4,4'-DDT

R.T.: 6.376 min
Delta R.T.: -0.005 min
Response: 2043686
Conc: 0.36 ng/ml

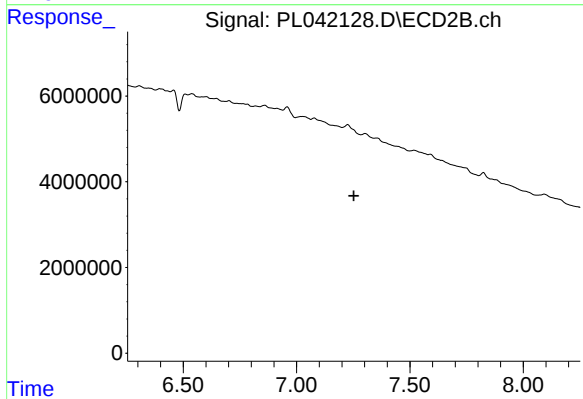

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

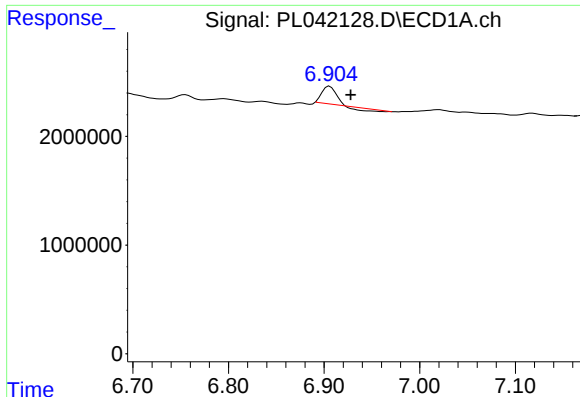

#20 Methoxychlor


R.T.: 6.906 min
Delta R.T.: -0.022 min
Response: 1150400
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

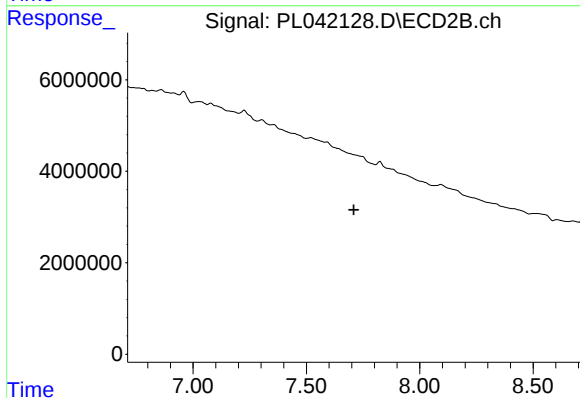


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

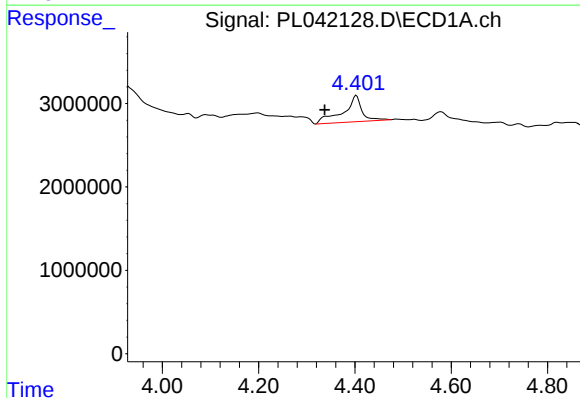


#23 Chlordane-1

R.T.: 4.403 min
Delta R.T.: 0.065 min
Response: 8438697
Conc: 28.28 ng/ml

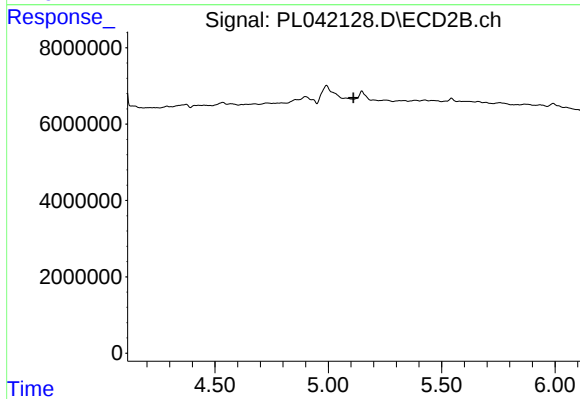

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

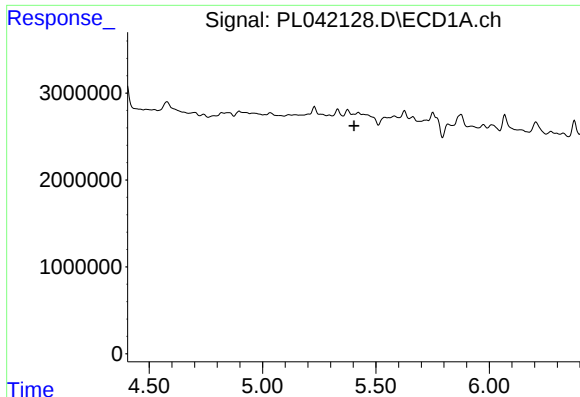

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

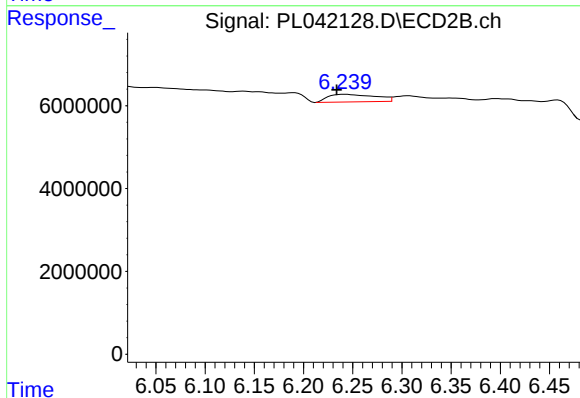


#25 Chlordane-3

R.T.: 6.242 min
Delta R.T.: 0.008 min
Response: 6165094
Conc: 12.07 ng/ml

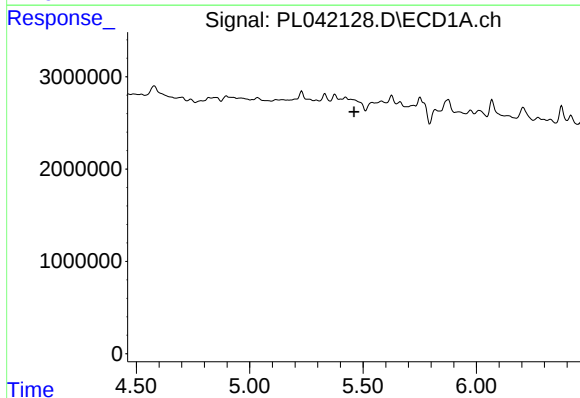


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.461 min
Response: 0
Conc: N.D.

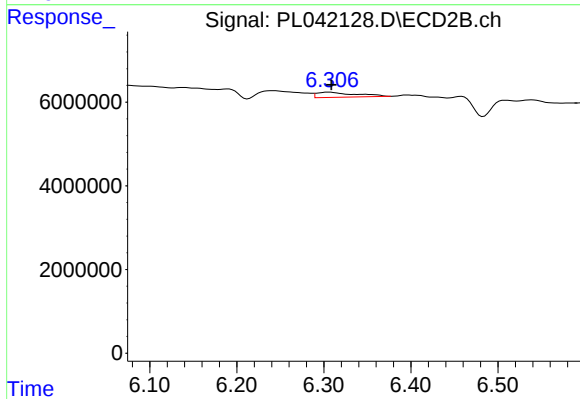

#26 Chlordane-4


R.T.: 6.307 min
Delta R.T.: -0.002 min
Response: 3768189
Conc: 6.31 ng/ml

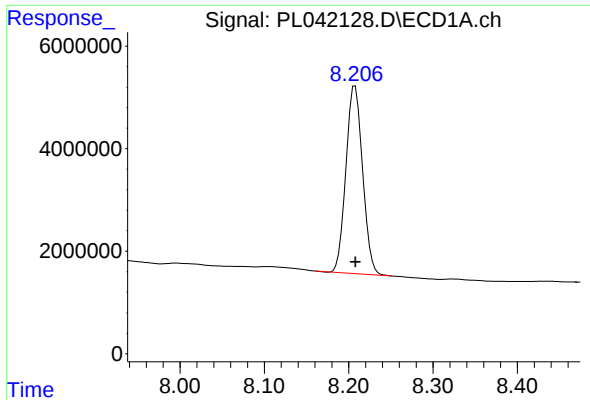

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 50312779
Conc: 7.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

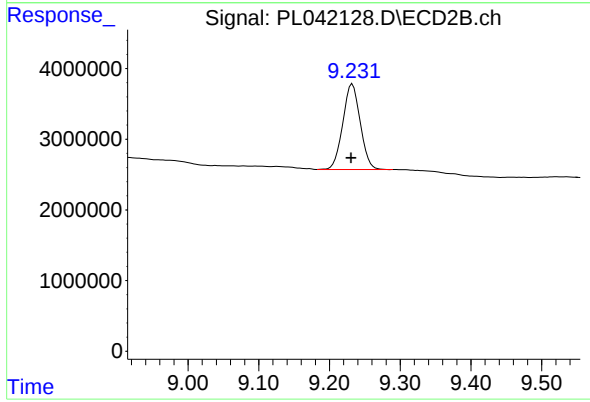

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.002 min
Response: 20769223
Conc: 8.14 ng/ml