

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 18:51
 Operator : AJ\SJ
 Sample : J5908-27
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:41:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	47965482	23928877	7.768	8.077
28)	SA Decachlor...	8.208	9.233	44560399	18846972	6.505	7.389
Target Compounds							
5)	MB Aldrin	0.000	5.607	0	1947025	N.D.	0.518 #
9)	A Endosulfan I	5.550	0.000	2000862	0	0.275	N.D. #
10)	B gamma-Chl...	0.000	6.245	0	38240138	N.D.	10.788 #
11)	B alpha-Chl...	0.000	6.245f	0	38240138	N.D.	10.992 #
12)	B 4,4'-DDE	0.000	6.527f	0	4862428	N.D.	1.424 #
23)	Chlordane-1	4.343	0.000	4591943	0	15.386	N.D. #
24)	Chlordane-2	0.000	5.607	0	1947025	N.D.	13.369 #
25)	Chlordane-3	0.000	6.245	0	38240138	N.D.	74.879 #
26)	Chlordane-4	0.000	6.245	0	38240138	N.D.	64.041 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2018 18:51
Operator : AJ\SJ
Sample : J5908-27
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:41:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

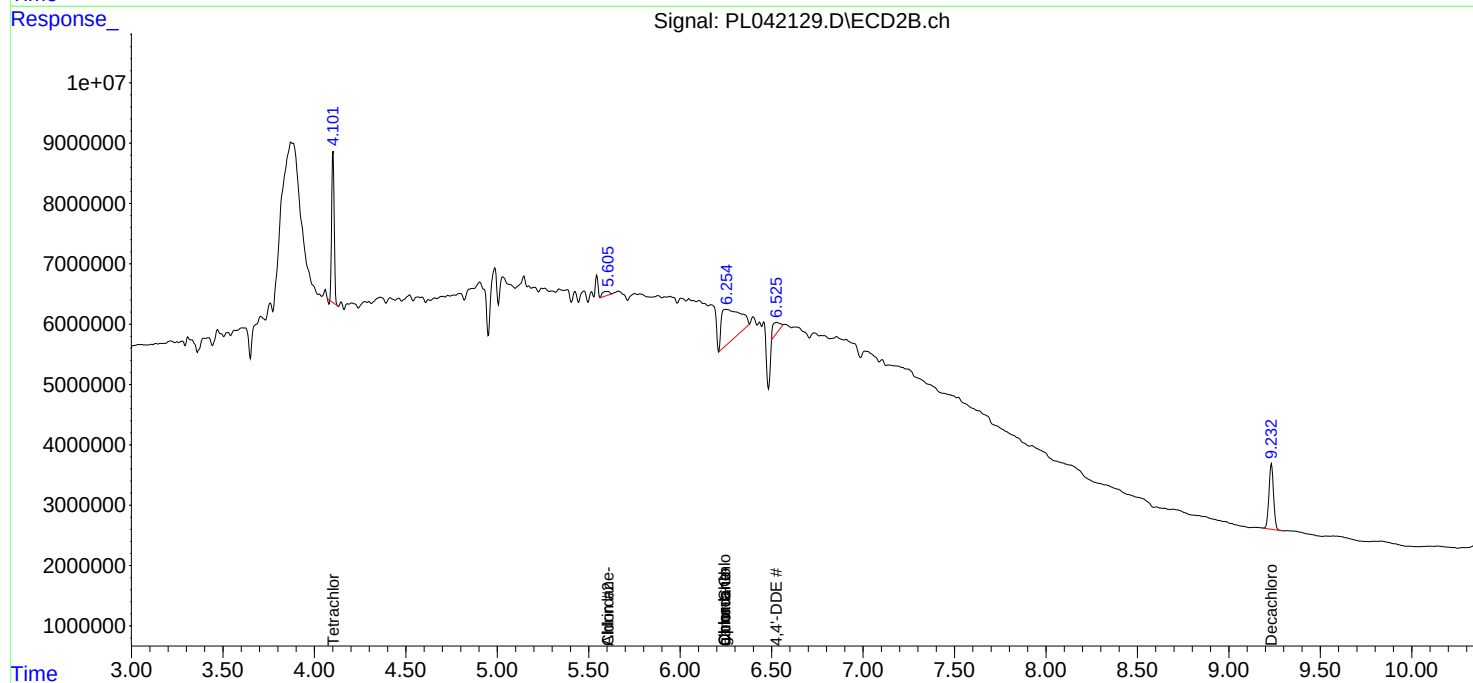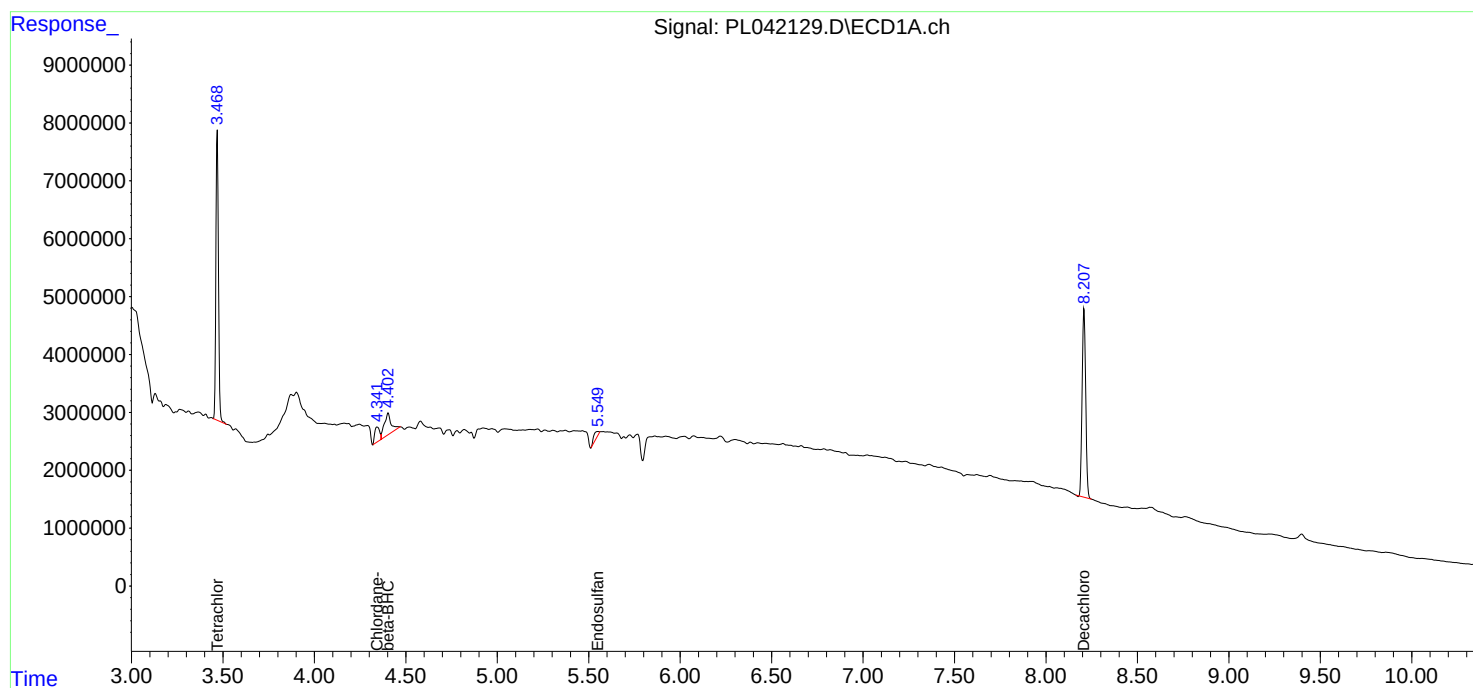


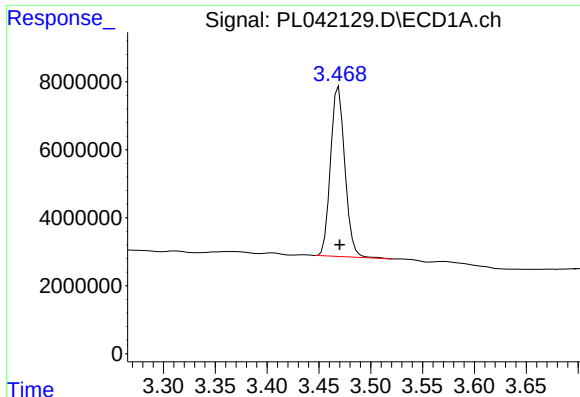

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 47965482
Conc: 7.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

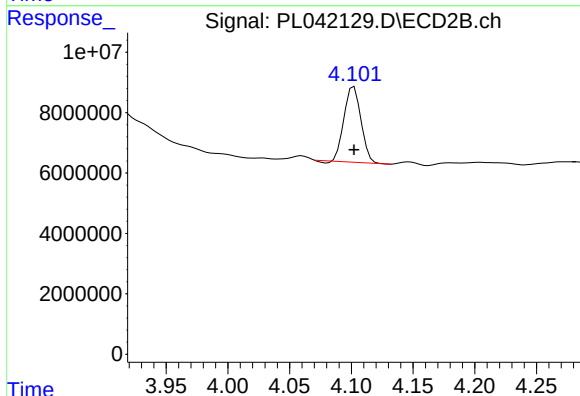


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 23928877
Conc: 8.08 ng/ml

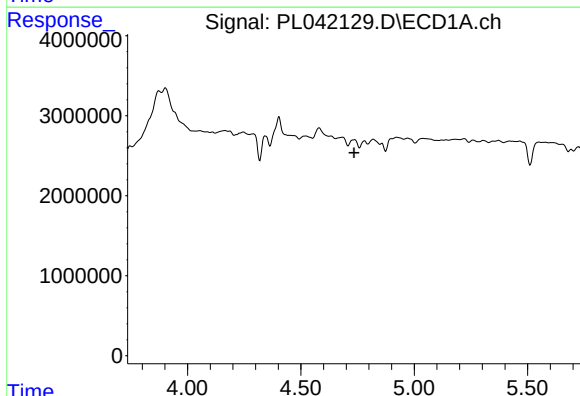


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

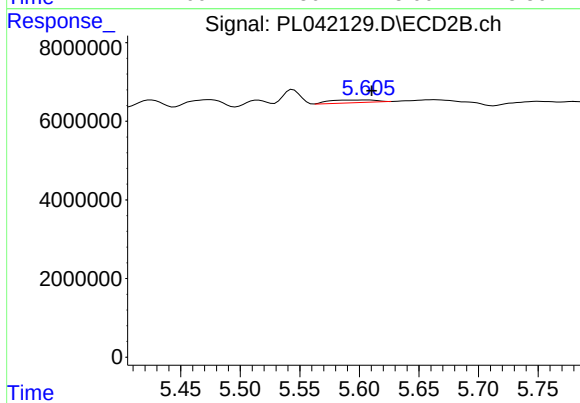

#5 Aldrin


R.T.: 5.607 min
Delta R.T.: -0.004 min
Response: 1947025
Conc: 0.52 ng/ml

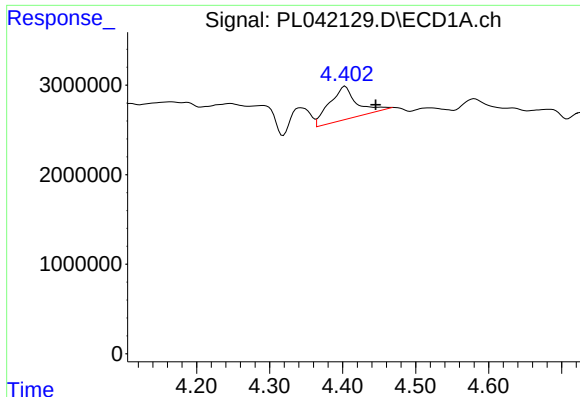

#6 beta-BHC


R.T.: 4.404 min
Delta R.T.: -0.042 min
Response: 9632000
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

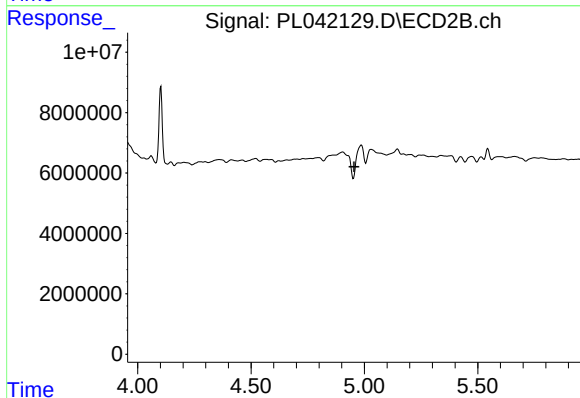


#6 beta-BHC

R.T.: 4.987 min
Delta R.T.: 0.032 min
Response: -5053301
Conc: N.D.

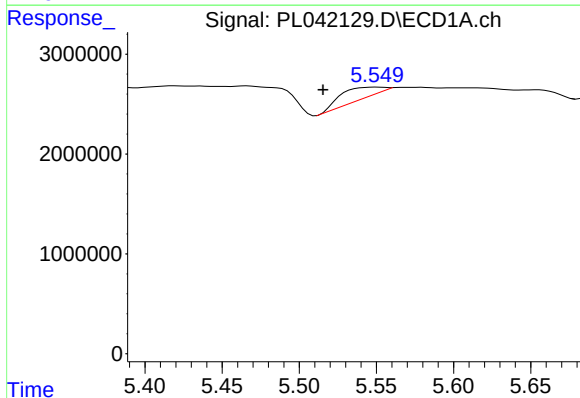


#9 Endosulfan I

R.T.: 5.550 min
Delta R.T.: 0.035 min
Response: 2000862
Conc: 0.27 ng/ml

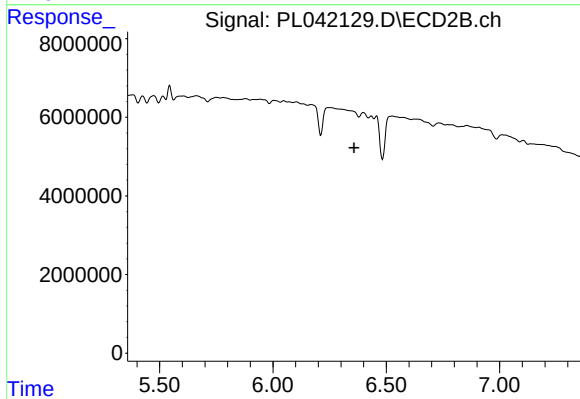

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

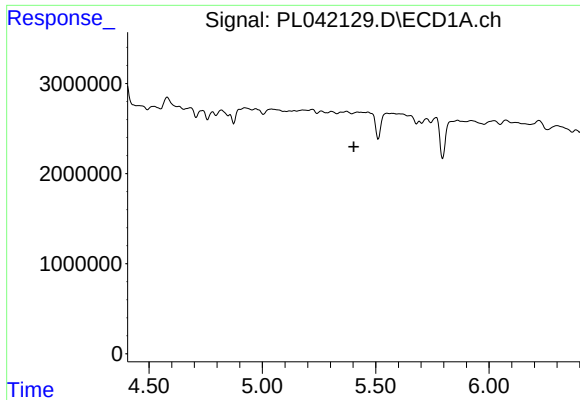

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.403 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

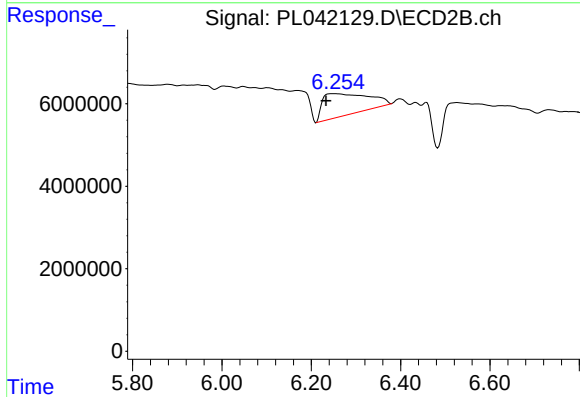


#10 gamma-Chlordane

R.T.: 6.245 min
Delta R.T.: 0.012 min
Response: 38240138
Conc: 10.79 ng/ml

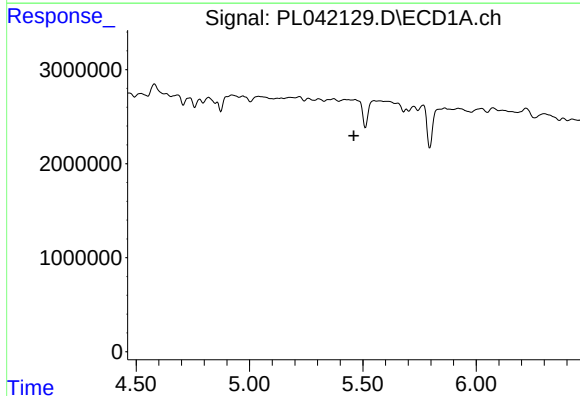


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

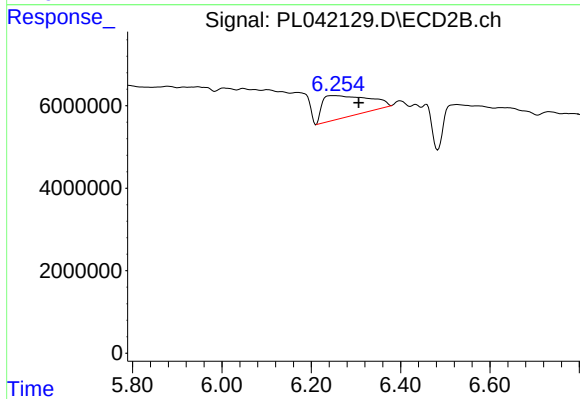

#11 alpha-Chlordane


R.T.: 6.245 min
Delta R.T.: -0.061 min
Response: 38240138
Conc: 10.99 ng/ml

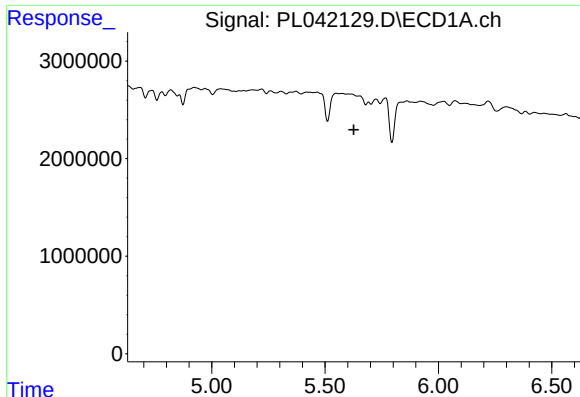

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.627 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

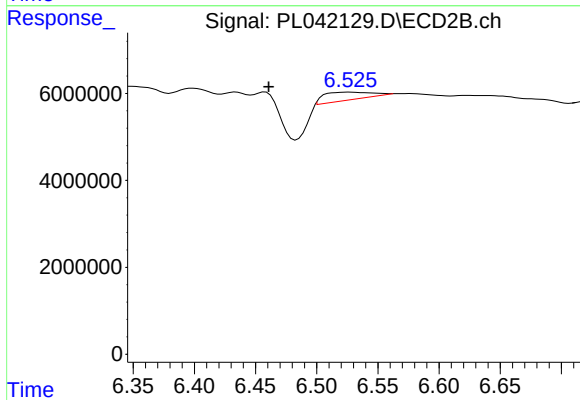


#12 4,4'-DDE

R.T.: 6.527 min
Delta R.T.: 0.066 min
Response: 4862428
Conc: 1.42 ng/ml

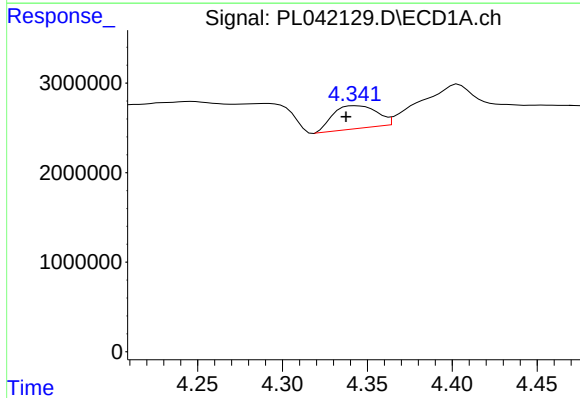


#23 Chlordane-1

R.T.: 4.343 min
Delta R.T.: 0.005 min
Response: 4591943
Conc: 15.39 ng/ml

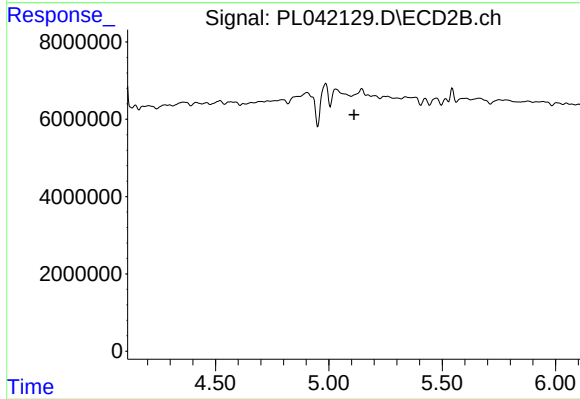

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.112 min
Response: 0
Conc: N.D.

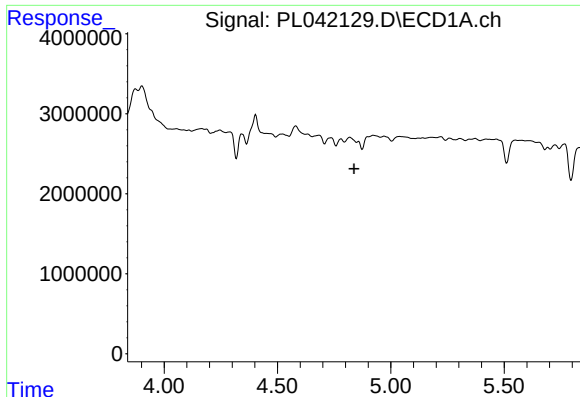

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

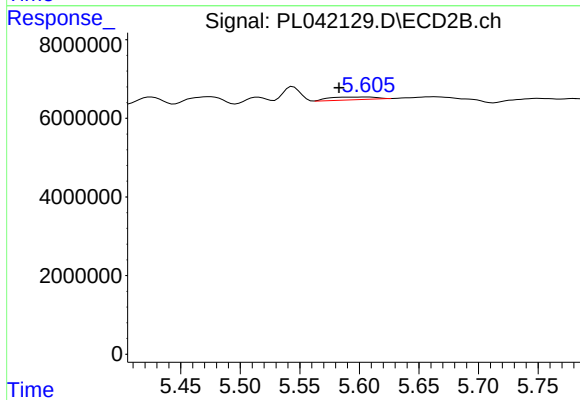


#24 Chlordane-2

R.T.: 5.607 min
Delta R.T.: 0.024 min
Response: 1947025
Conc: 13.37 ng/ml

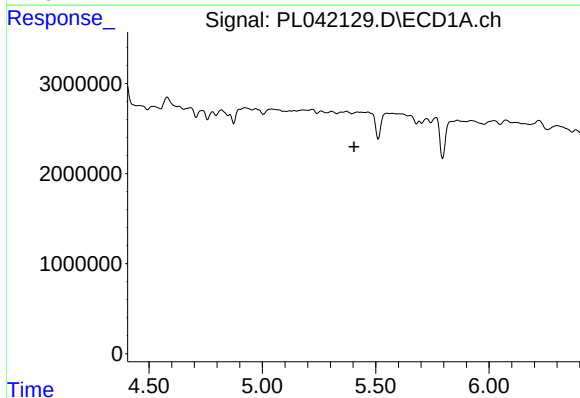


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.404 min
Response: 0
Conc: N.D.

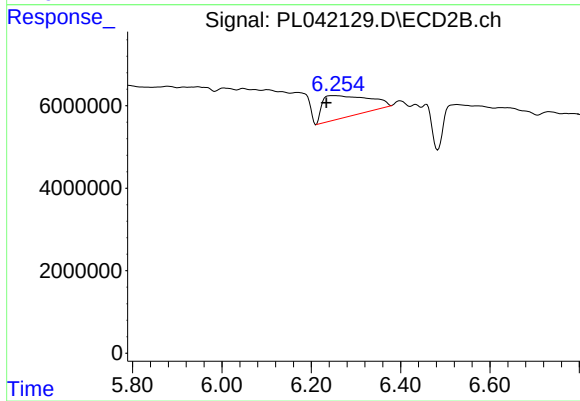

#25 Chlordane-3


R.T.: 6.245 min
Delta R.T.: 0.011 min
Response: 38240138
Conc: 74.88 ng/ml

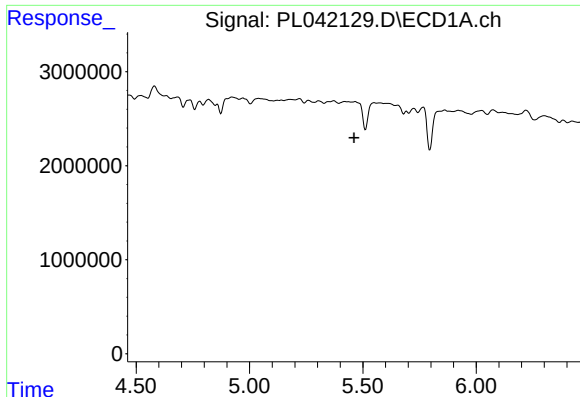

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.461 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

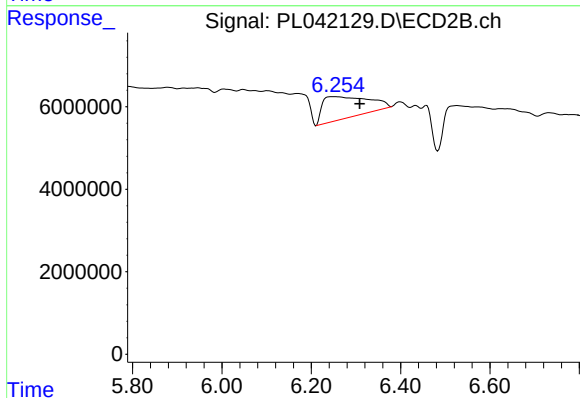


#26 Chlordane-4

R.T.: 6.245 min
Delta R.T.: -0.063 min
Response: 38240138
Conc: 64.04 ng/ml

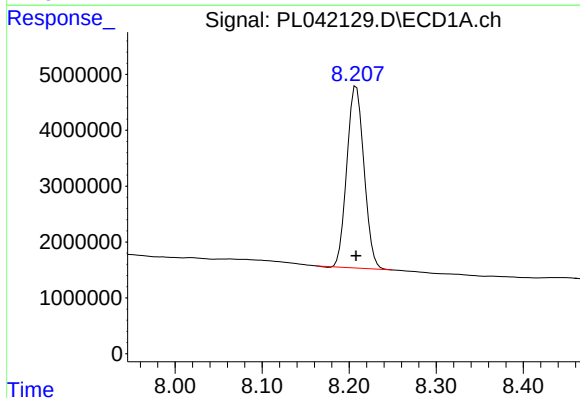

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 44560399
Conc: 6.50 ng/ml

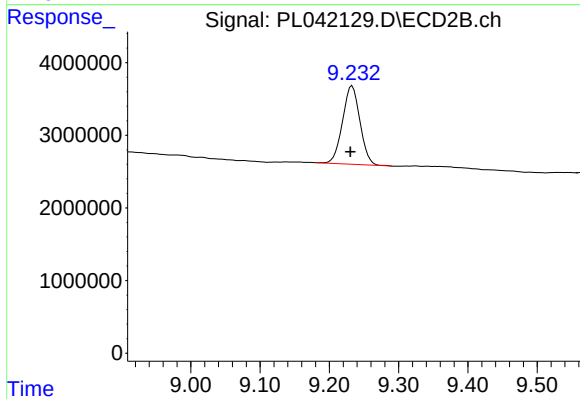

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.003 min
Response: 18846972
Conc: 7.39 ng/ml