

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 19:19
 Operator : AJ\SJ
 Sample : J5909-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:41:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	98362177	53525613	15.929	18.066
28)	SA Decachlor...	8.208	9.232	50382252	21083561	7.355	8.266
Target Compounds							
2)	A alpha-BHC	3.902	4.527f	4773346	-1829673	0.503	N.D. #
6)	B beta-BHC	4.404f	0.000	5222819	0	1.415	N.D. #
7)	B delta-BHC	0.000	5.162	0	2355445	N.D.	0.596 #
8)	B Heptachlo...	0.000	5.998	0	1592118	N.D.	0.443 #
15)	B Endosulfa...	6.220f	0.000	2118991	0	0.310	N.D. #
20)	A Methoxychlor	6.908	0.000	4177901	0	1.311	N.D. #
21)	B Endrin ke...	7.205f	7.923f	3725827	2197175	0.517	0.759 #
23)	Chlordane-1	4.359	5.162	2827838	2355445	9.475	16.359 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2018 19:19
Operator : AJ\SJ
Sample : J5909-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:41:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

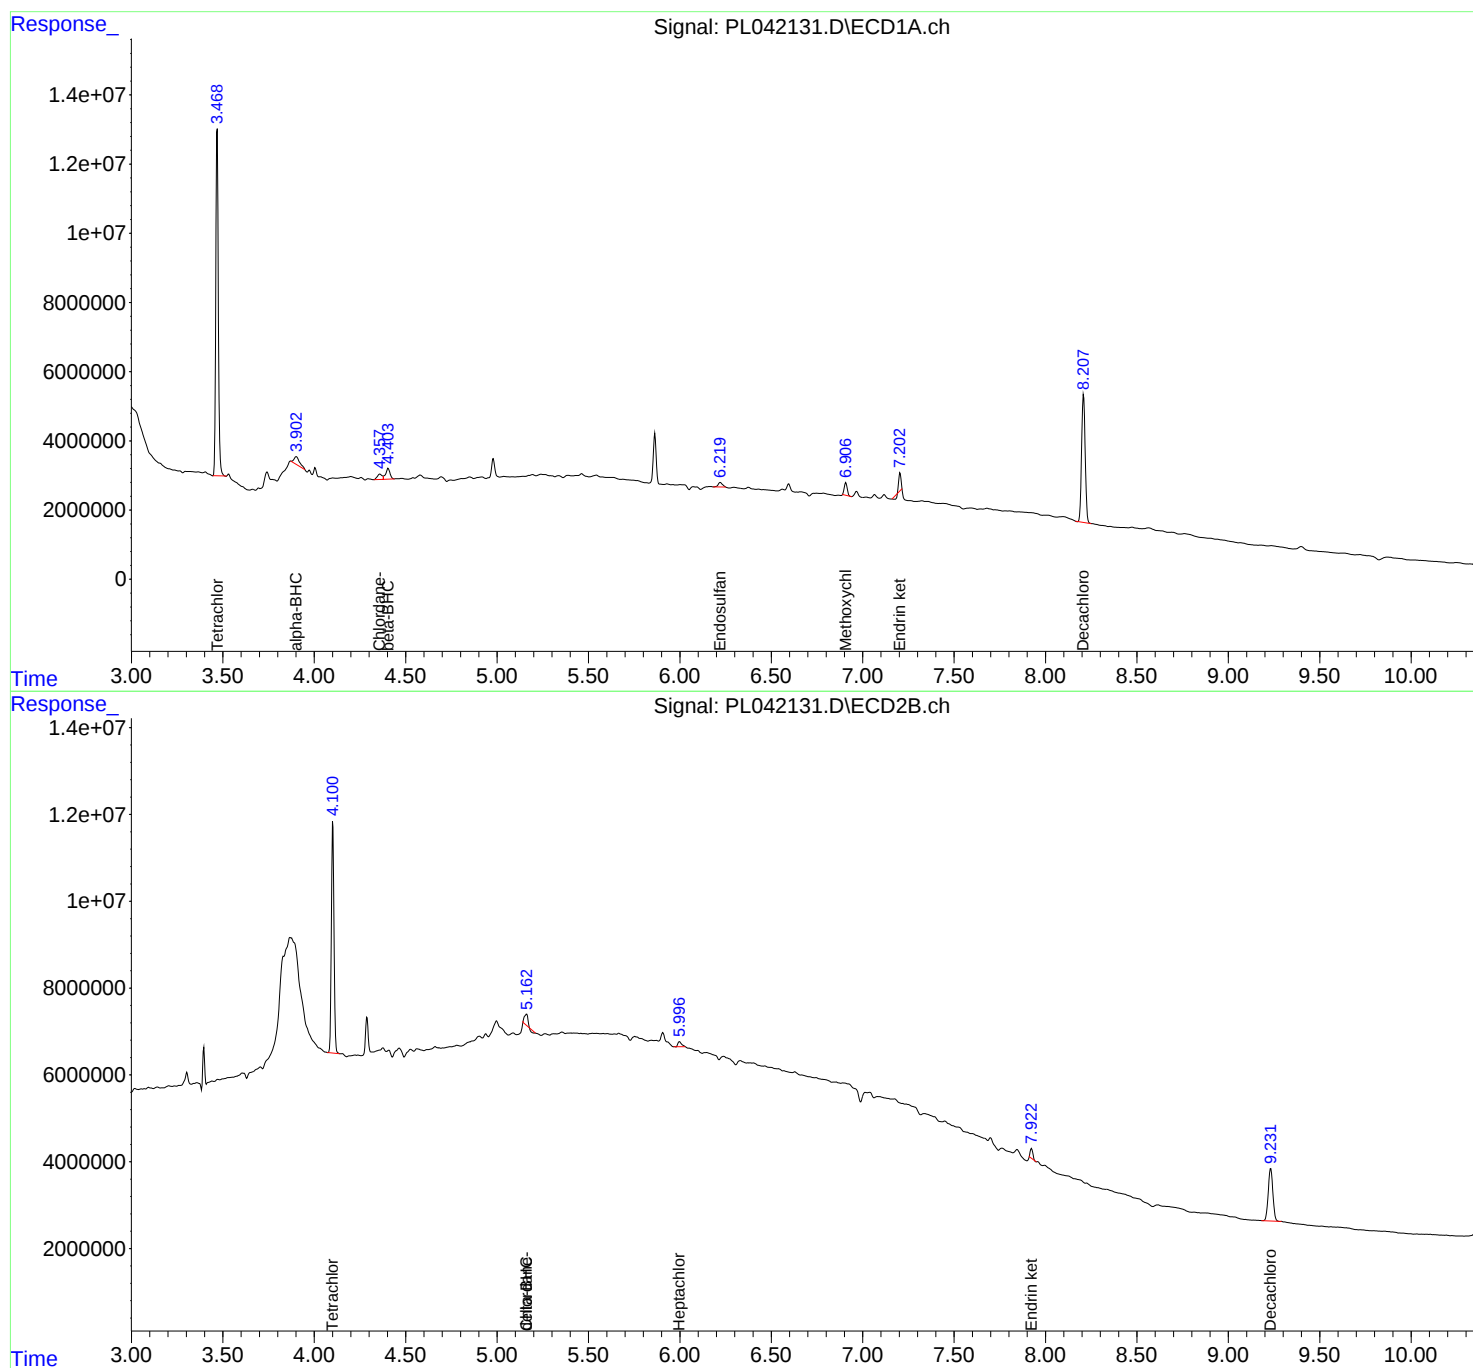


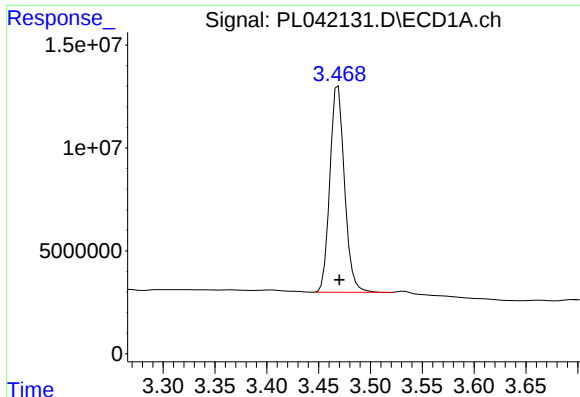

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 98362177
Conc: 15.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

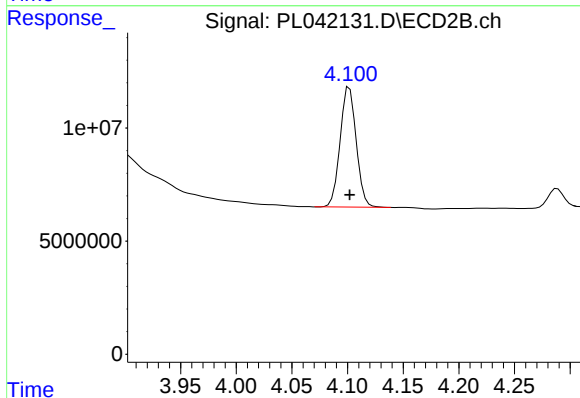


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 53525613
Conc: 18.07 ng/ml

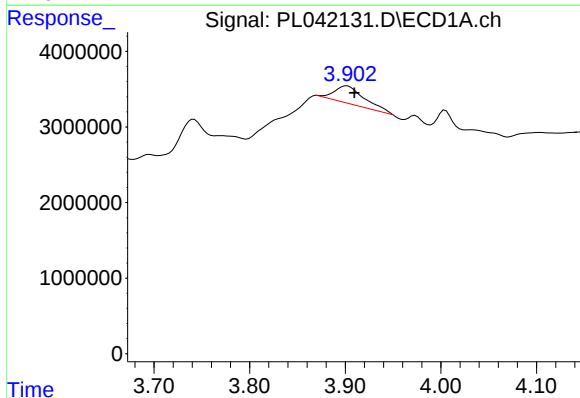


#2 alpha-BHC

R.T.: 3.902 min
Delta R.T.: -0.008 min
Response: 4773346
Conc: 0.50 ng/ml

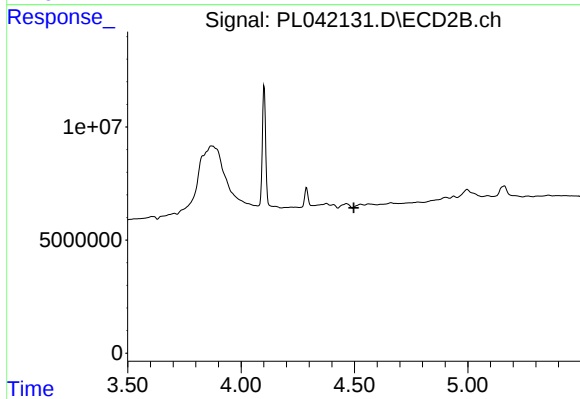

#2 alpha-BHC


R.T.: 4.527 min
Delta R.T.: 0.030 min
Response: -1829673
Conc: N.D.

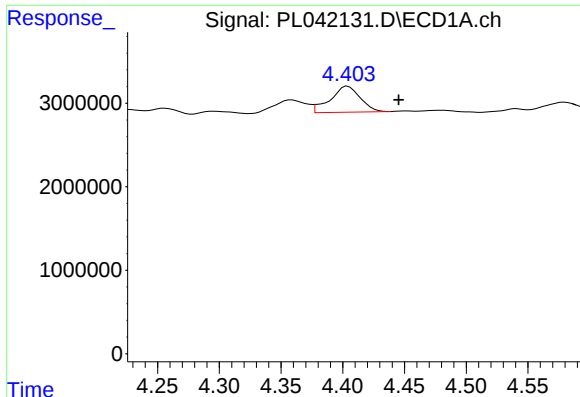

#6 beta-BHC


R.T.: 4.404 min
Delta R.T.: -0.041 min
Response: 5222819
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

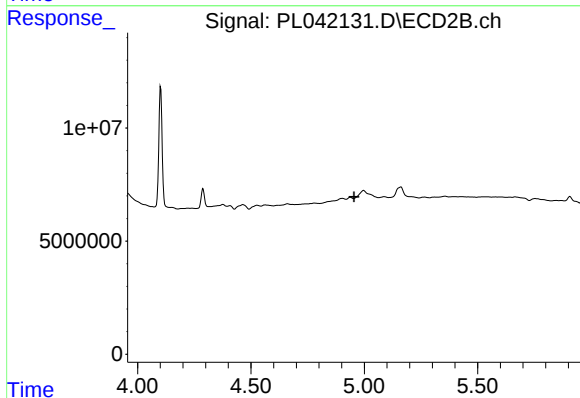


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

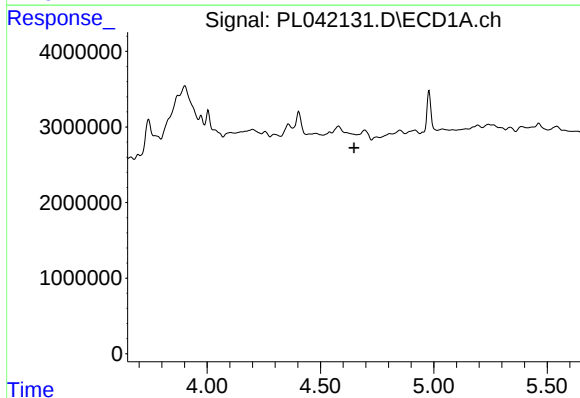


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

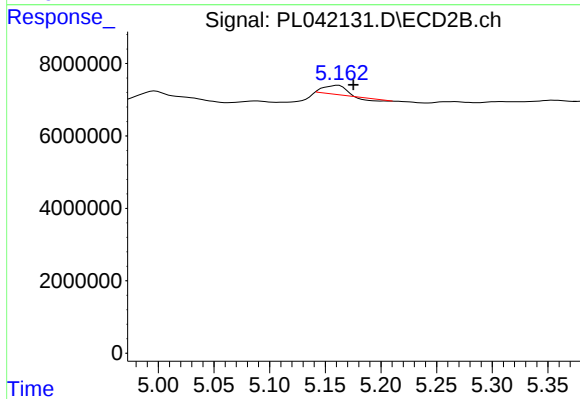

#7 delta-BHC


R.T.: 5.162 min
Delta R.T.: -0.014 min
Response: 2355445
Conc: 0.60 ng/ml

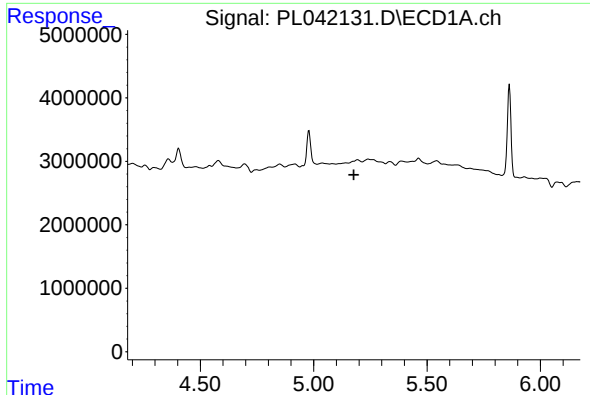

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

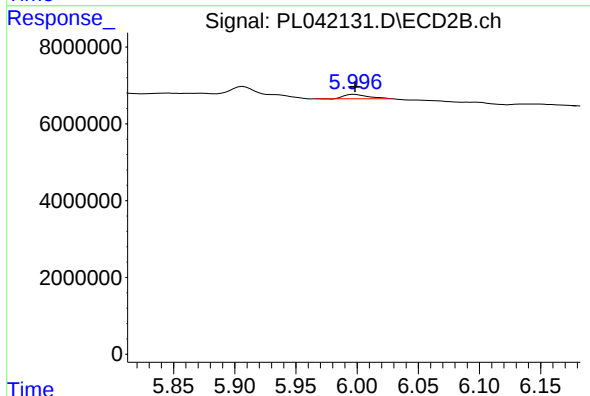


#8 Heptachlor epoxide

R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 1592118
Conc: 0.44 ng/ml

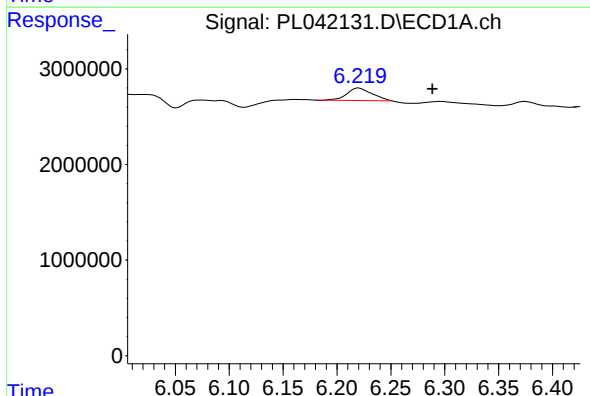


#15 Endosulfan II

R.T.: 6.220 min
Delta R.T.: -0.068 min
Response: 2118991
Conc: 0.31 ng/ml

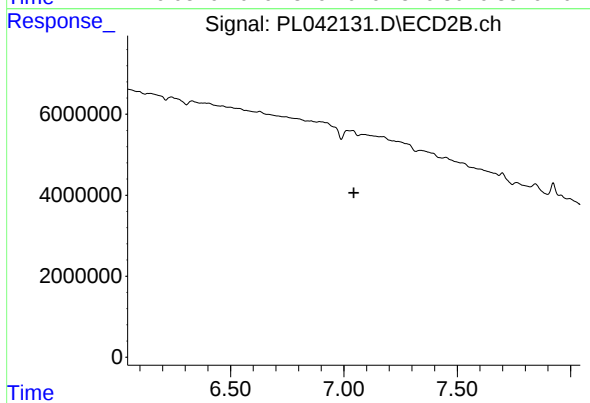

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.044 min
Response: 0
Conc: N.D.

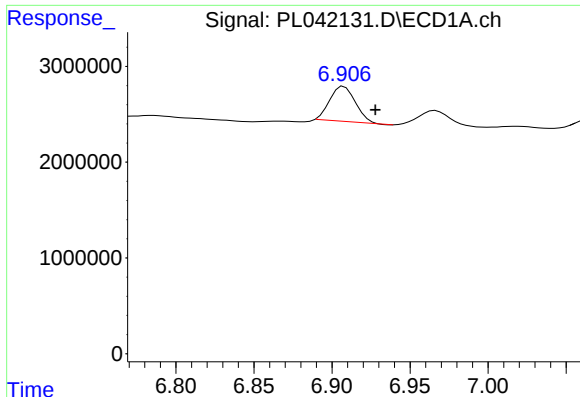

#20 Methoxychlor


R.T.: 6.908 min
Delta R.T.: -0.020 min
Response: 4177901
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

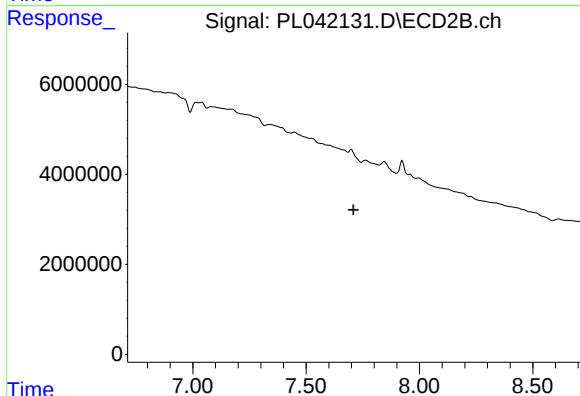


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

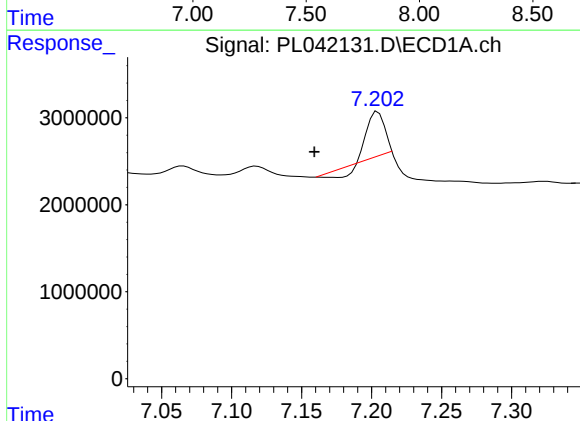


#21 Endrin ketone

R.T.: 7.205 min
Delta R.T.: 0.045 min
Response: 3725827
Conc: 0.52 ng/ml

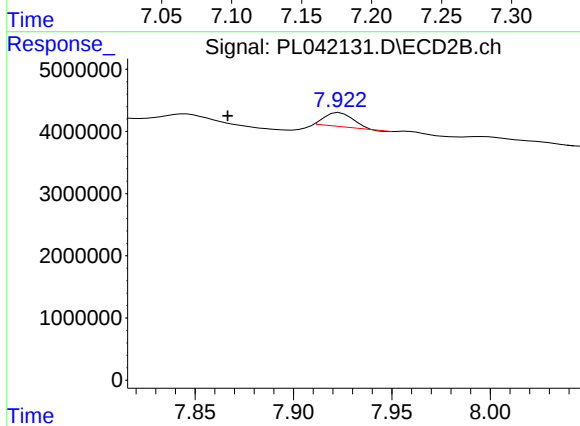

#21 Endrin ketone


R.T.: 7.923 min
Delta R.T.: 0.057 min
Response: 2197175
Conc: 0.76 ng/ml

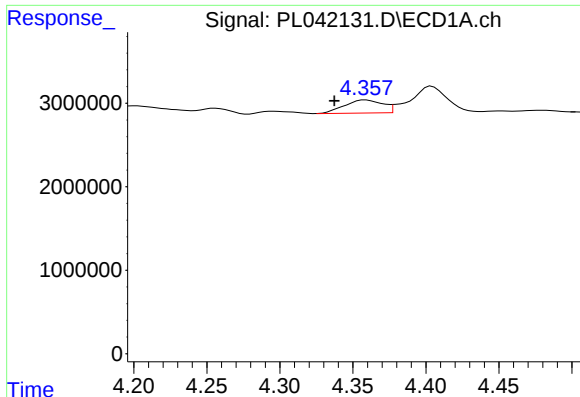

#23 Chlordane-1


R.T.: 4.359 min
Delta R.T.: 0.021 min
Response: 2827838
Conc: 9.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

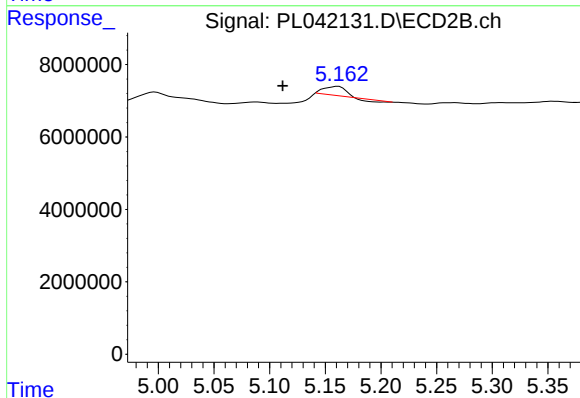


#23 Chlordane-1

R.T.: 5.162 min
Delta R.T.: 0.050 min
Response: 2355445
Conc: 16.36 ng/ml

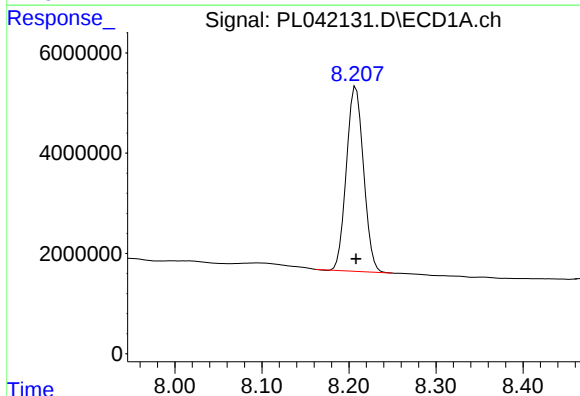

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 50382252
Conc: 7.35 ng/ml

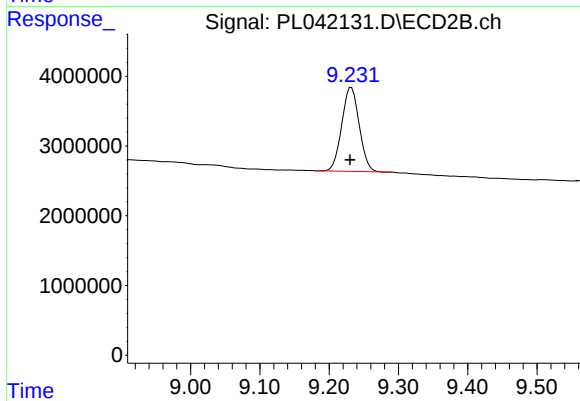

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.002 min
Response: 21083561
Conc: 8.27 ng/ml