

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 21:12
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:42:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	133.5E6	69701148	21.620	23.526
28)	SA Decachlor...	8.208	9.232	123.4E6	55141023	18.018	21.619
Target Compounds							
6)	B beta-BHC	4.402f	0.000	3212920	0	0.871	N.D. #
7)	B delta-BHC	0.000	5.163	0	6549246	N.D.	1.657 #
8)	B Heptachlo...	0.000	5.995	0	7533591	N.D.	2.097 #
9)	A Endosulfan I	5.519	0.000	3365461	0	0.462	N.D. #
10)	B gamma-Chl...	5.391	0.000	1151734	0	0.143	N.D. #
11)	B alpha-Chl...	5.489	0.000	4555651	0	0.572	N.D. #
23)	Chlordane-1	4.365	5.163	1676921	6549246	5.619	45.487 #
25)	Chlordane-3	5.391	0.000	1151734	0	1.232	N.D. #
26)	Chlordane-4	5.489	0.000	4555651	0	5.453	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2018 21:12
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:42:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

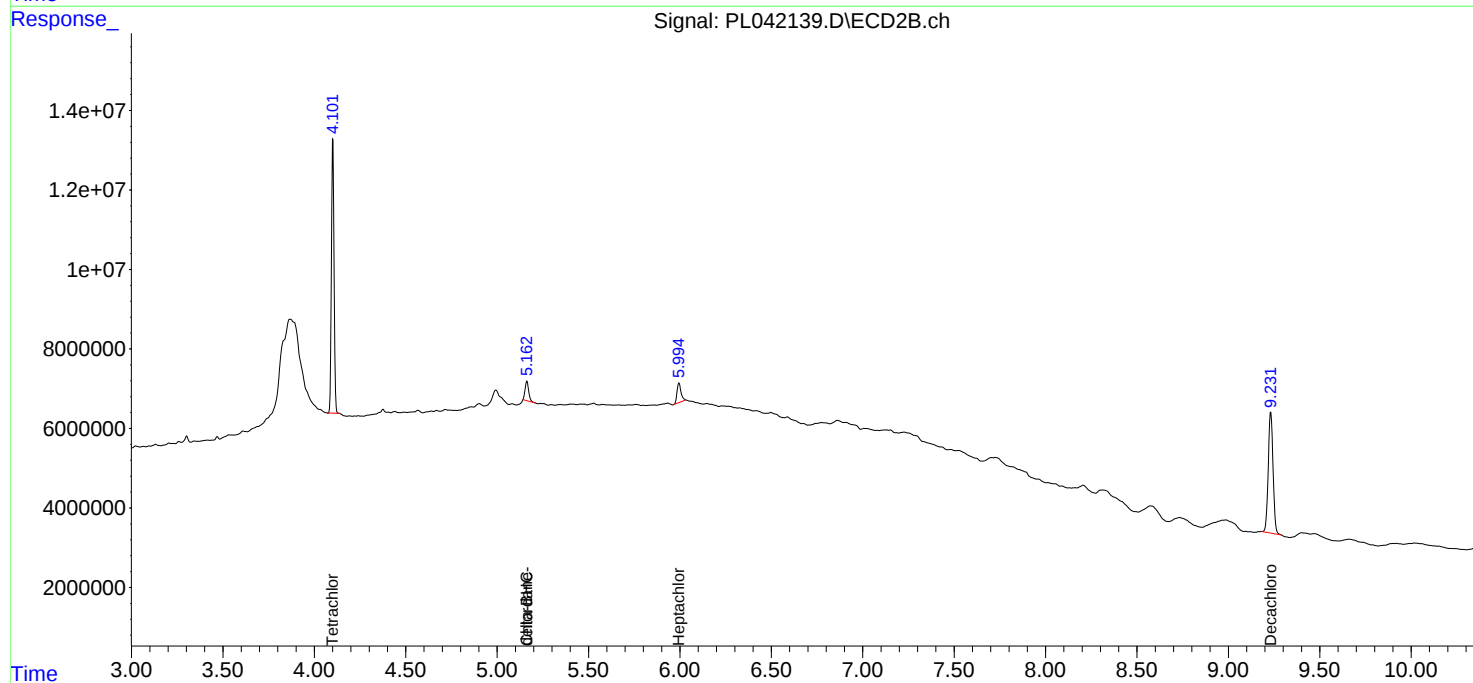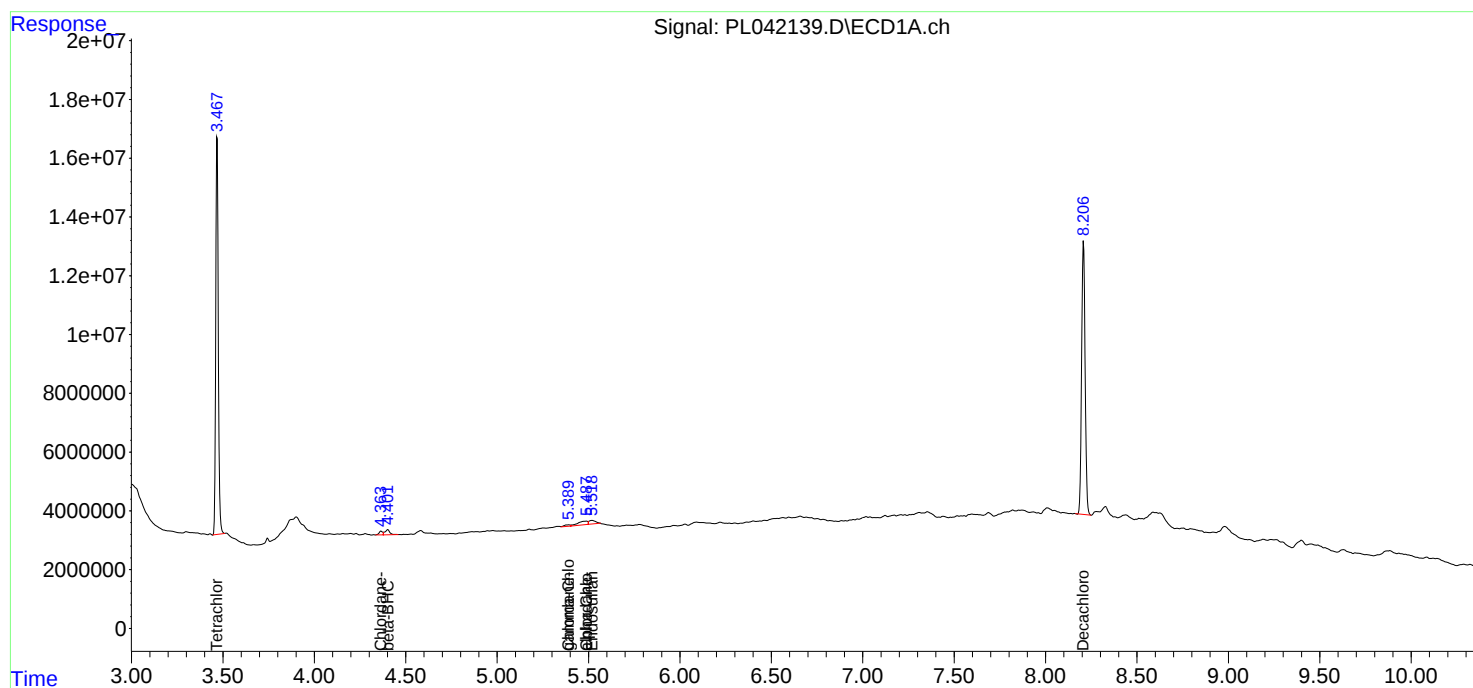


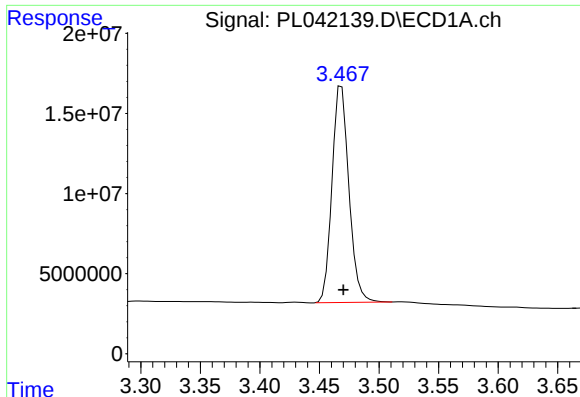

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 133499880
Conc: 21.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

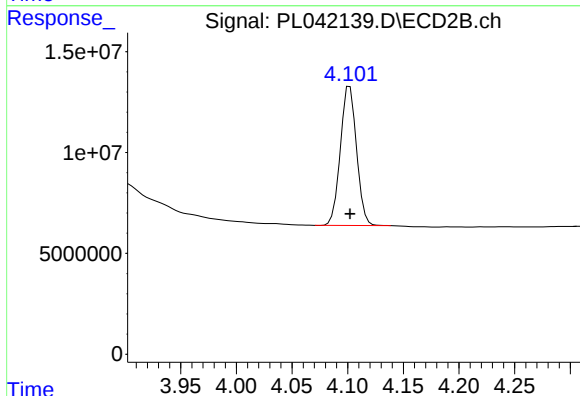


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 69701148
Conc: 23.53 ng/ml

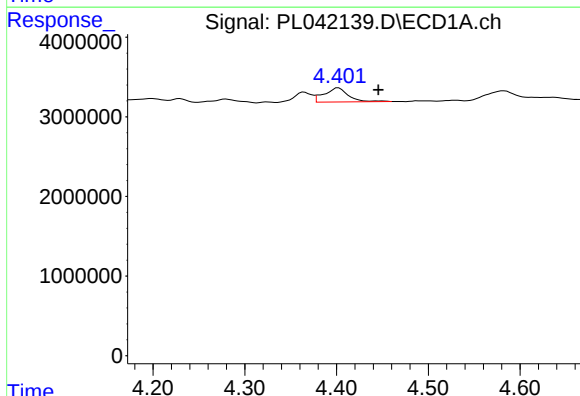


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.043 min
Response: 3212920
Conc: 0.87 ng/ml

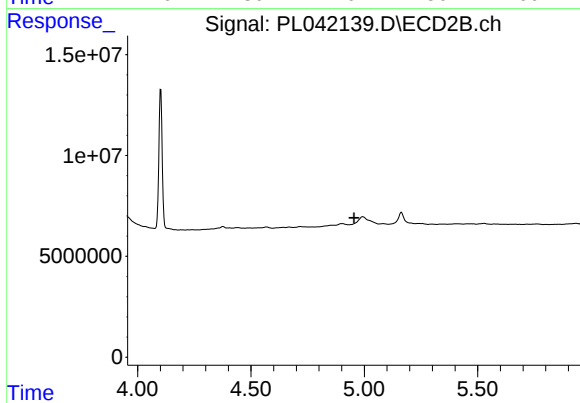

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

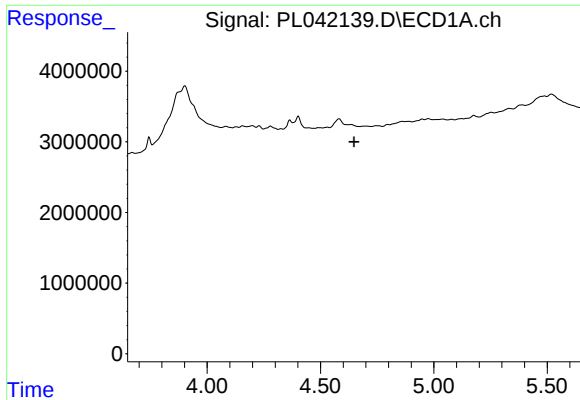

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

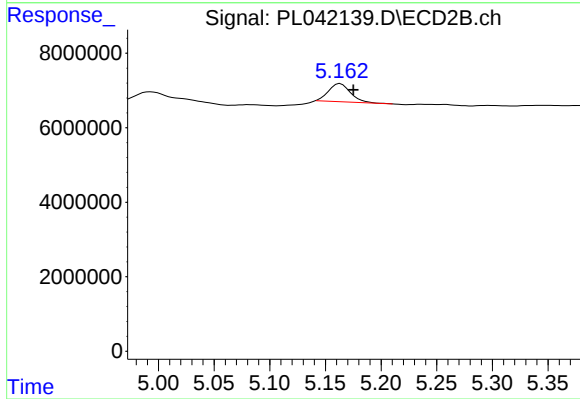


#7 delta-BHC

R.T.: 5.163 min
Delta R.T.: -0.012 min
Response: 6549246
Conc: 1.66 ng/ml

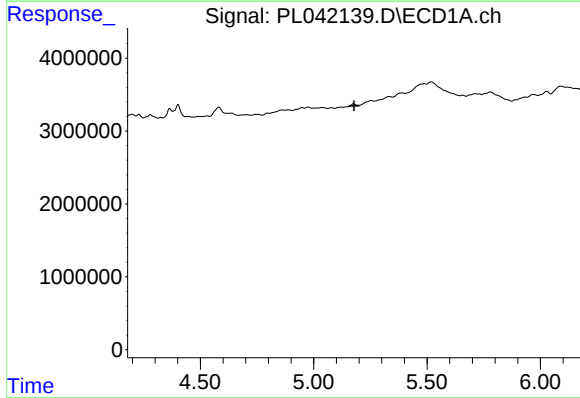


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

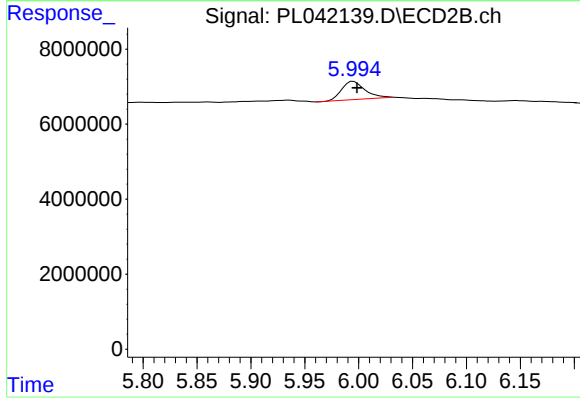

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 7533591
Conc: 2.10 ng/ml

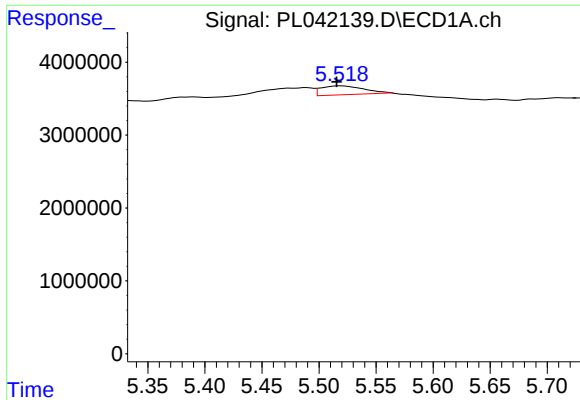

#9 Endosulfan I


R.T.: 5.519 min
Delta R.T.: 0.004 min
Response: 3365461
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

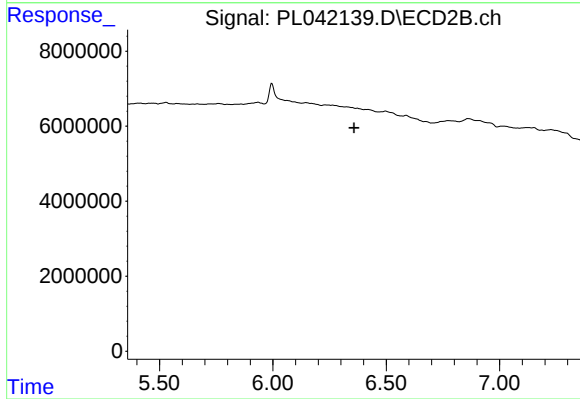


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

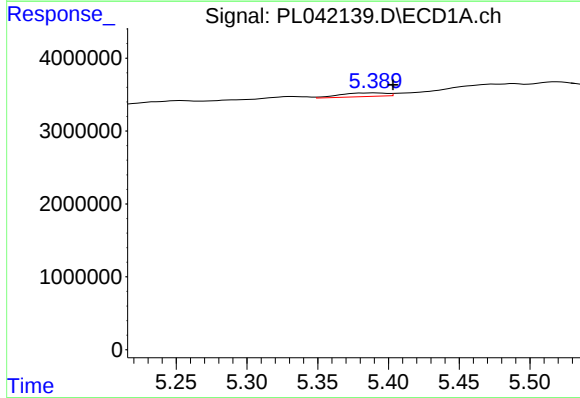


#10 gamma-Chlordane

R.T.: 5.391 min
Delta R.T.: -0.013 min
Response: 1151734
Conc: 0.14 ng/ml

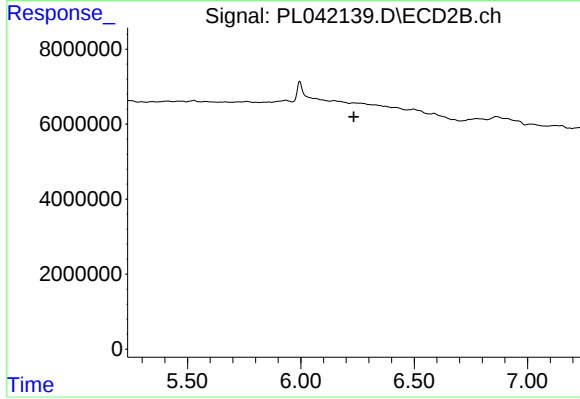

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

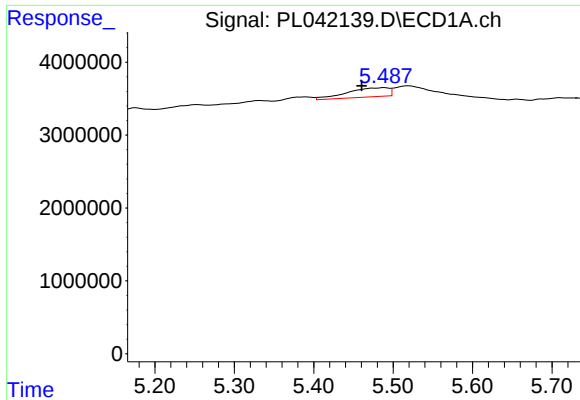

#11 alpha-Chlordane


R.T.: 5.489 min
Delta R.T.: 0.028 min
Response: 4555651
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

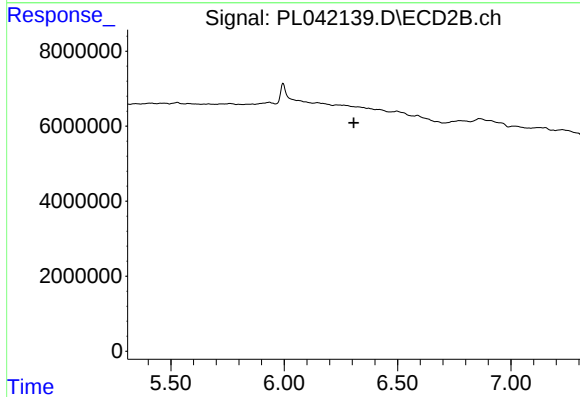


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

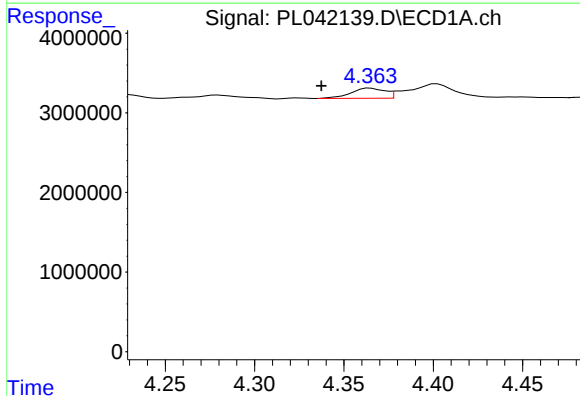


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.027 min
Response: 1676921
Conc: 5.62 ng/ml

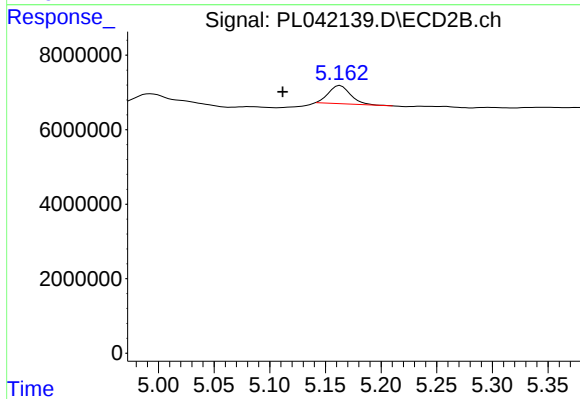

#23 Chlordane-1


R.T.: 5.163 min
Delta R.T.: 0.052 min
Response: 6549246
Conc: 45.49 ng/ml

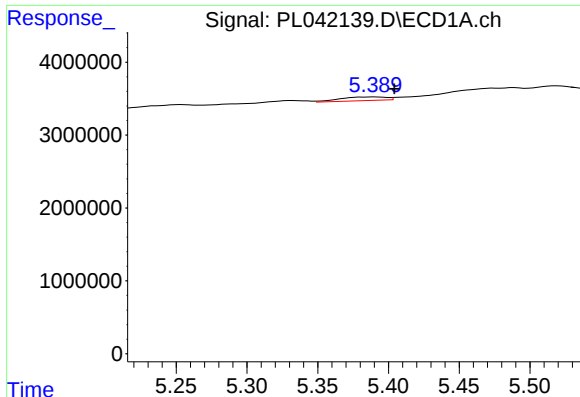

#25 Chlordane-3


R.T.: 5.391 min
Delta R.T.: -0.014 min
Response: 1151734
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

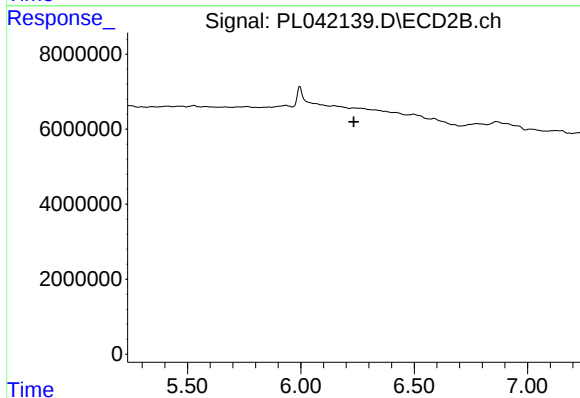


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

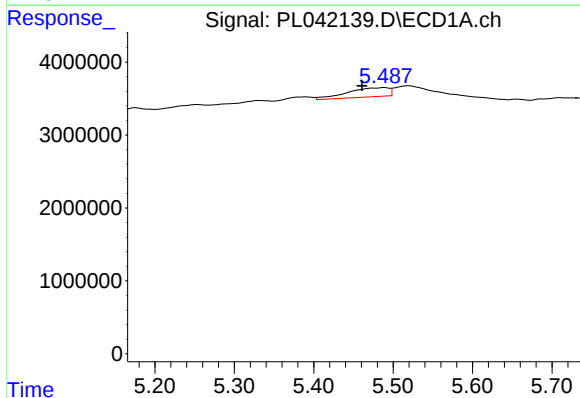


#26 Chlordane-4

R.T.: 5.489 min
Delta R.T.: 0.028 min
Response: 4555651
Conc: 5.45 ng/ml

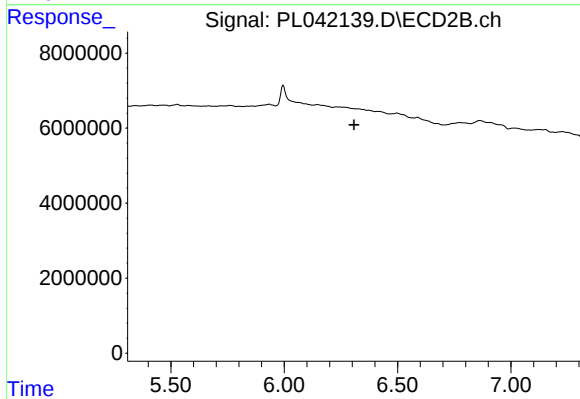

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

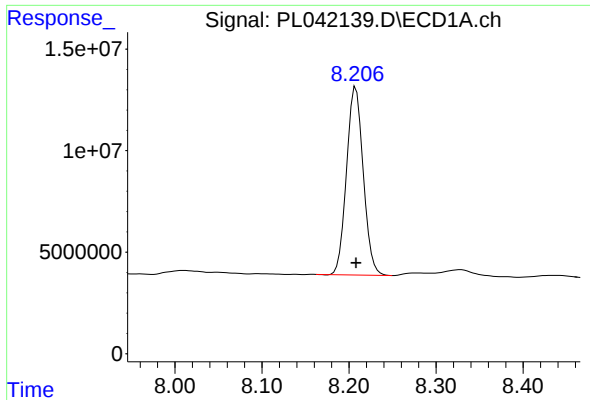

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 123429251
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

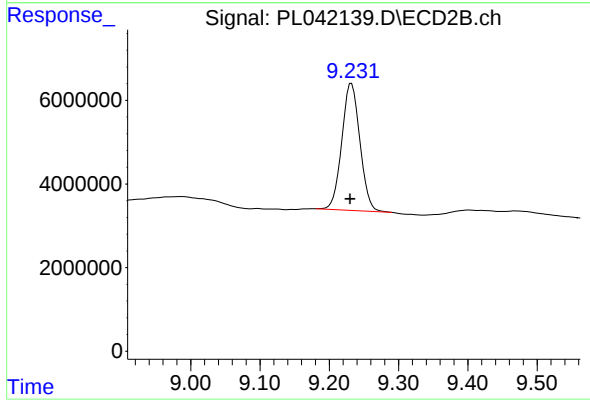

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.002 min
Response: 55141023
Conc: 21.62 ng/ml