

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 21:40
 Operator : AJ\SJ
 Sample : J5925-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:42:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	67860379	33221357	10.990	11.213
28)	SA Decachlor...	8.208	9.232	76113778	32136303	11.111	12.600
Target Compounds							
4)	MA Heptachlor	4.460	0.000	389942	0	0.044	N.D. #
6)	B beta-BHC	4.460	0.000	389942	0	0.106	N.D. #
8)	B Heptachlo...	0.000	5.997	0	2009947	N.D.	0.559 #
14)	MA Endrin	0.000	6.864	0	398304	N.D.	0.135 #
23)	Chlordane-1	4.404	0.000	10737894	0	35.980	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2018 21:40
Operator : AJ\SJ
Sample : J5925-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:42:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

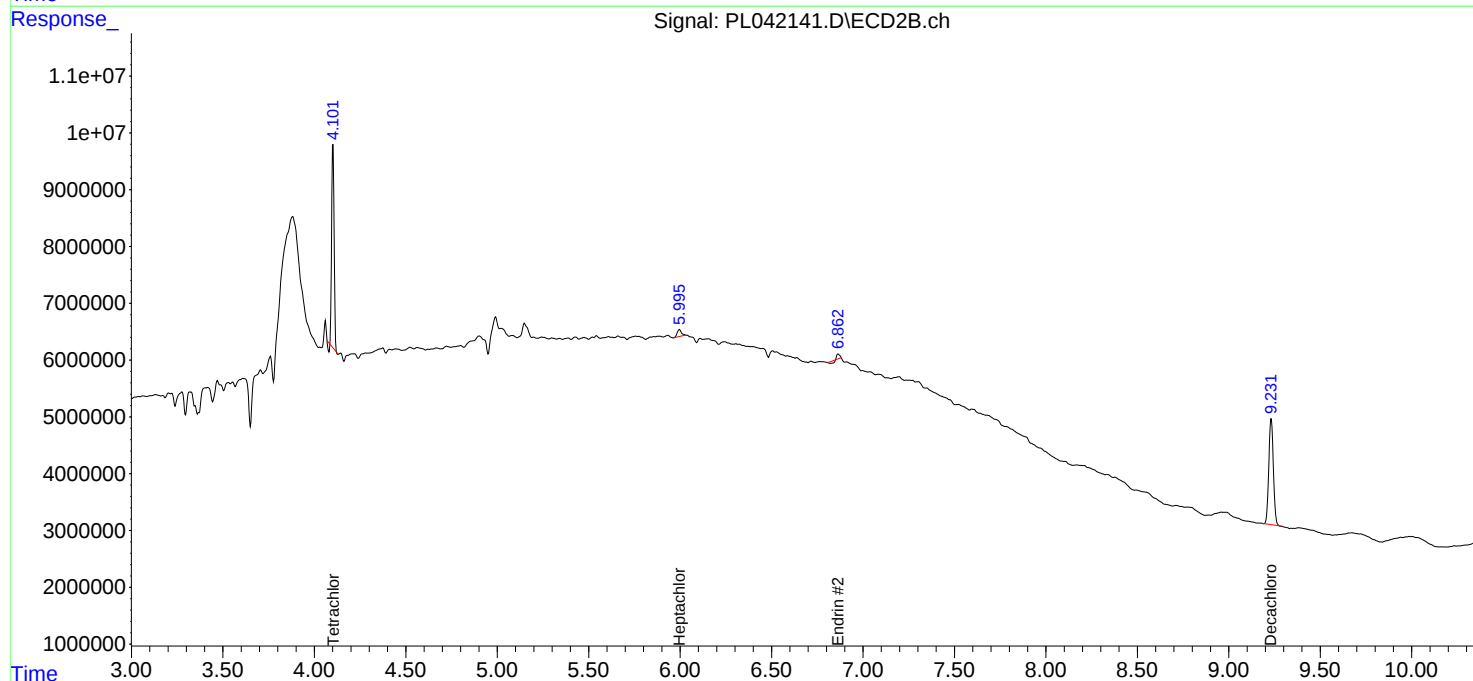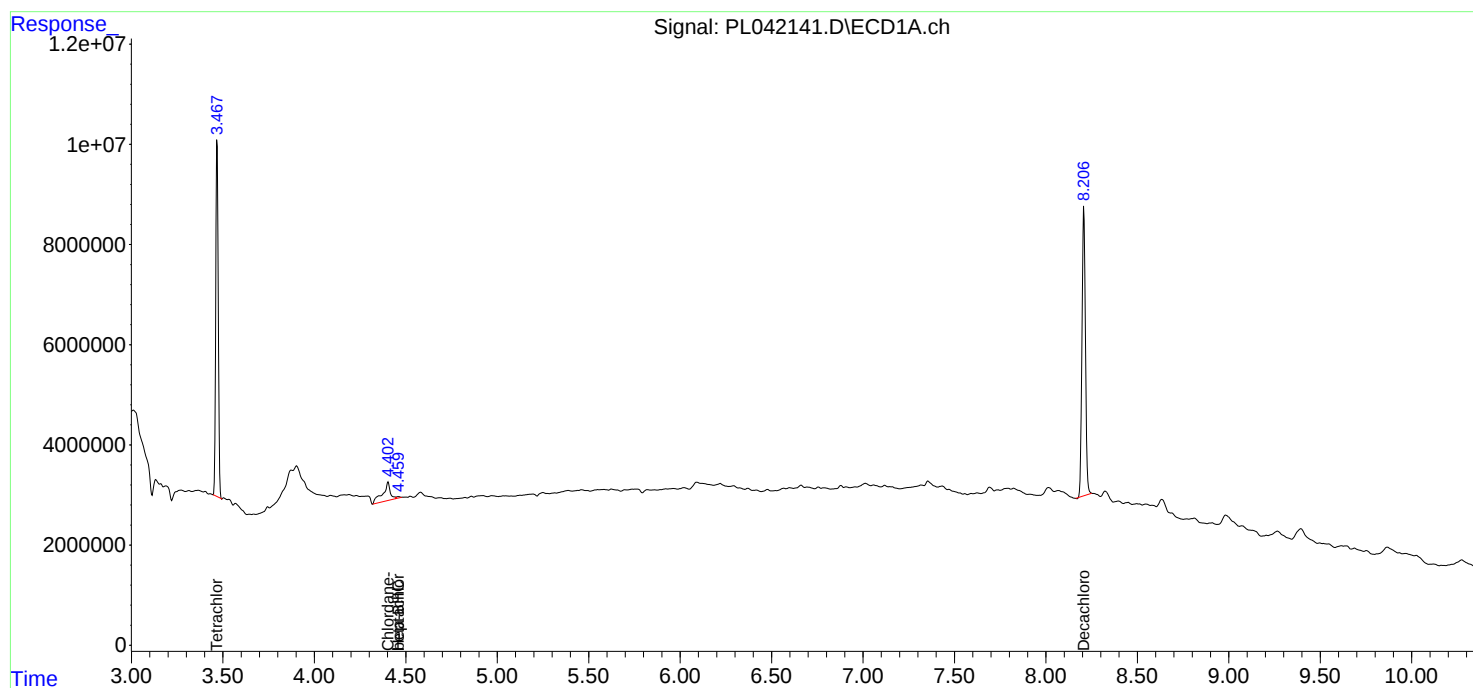


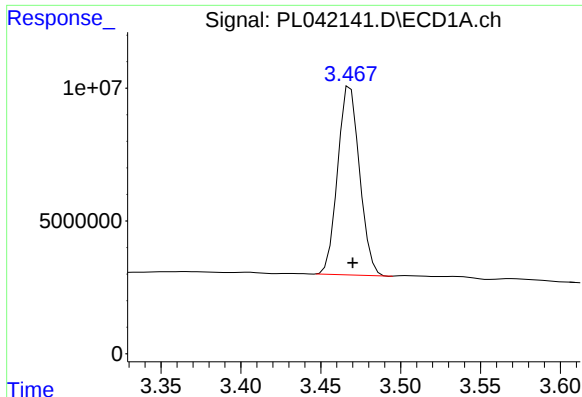

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 67860379
Conc: 10.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

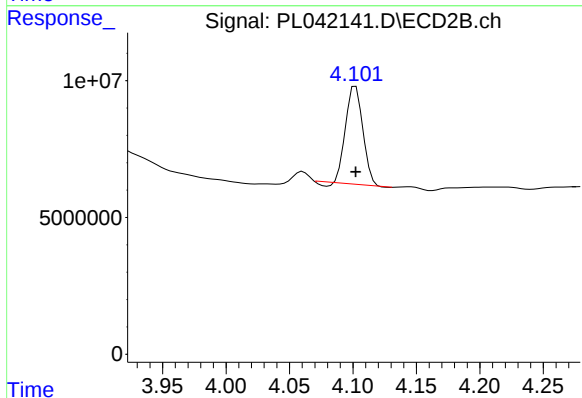


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 33221357
Conc: 11.21 ng/ml

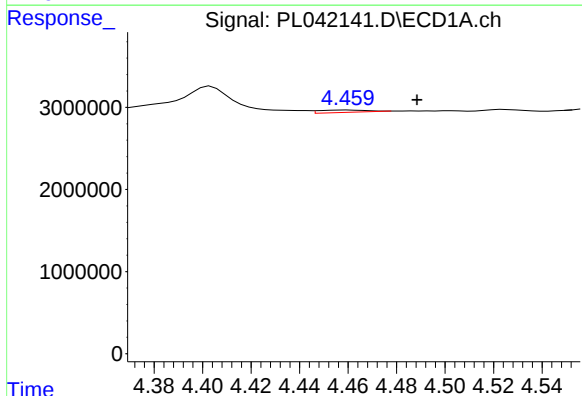


#4 Heptachlor

R.T.: 4.460 min
Delta R.T.: -0.028 min
Response: 389942
Conc: 0.04 ng/ml

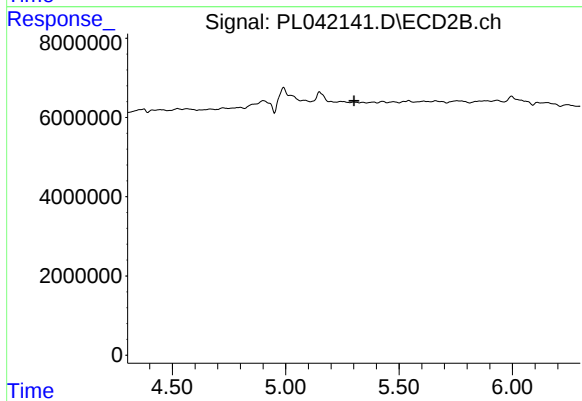

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.302 min
Response: 0
Conc: N.D.

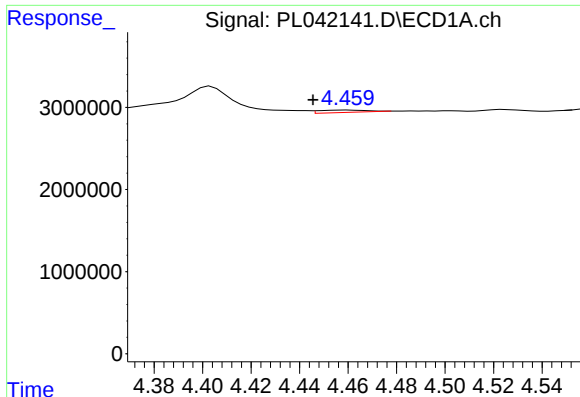

#6 beta-BHC


R.T.: 4.460 min
Delta R.T.: 0.015 min
Response: 389942
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

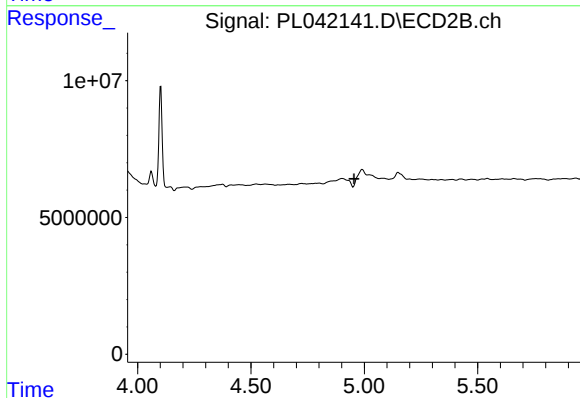


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

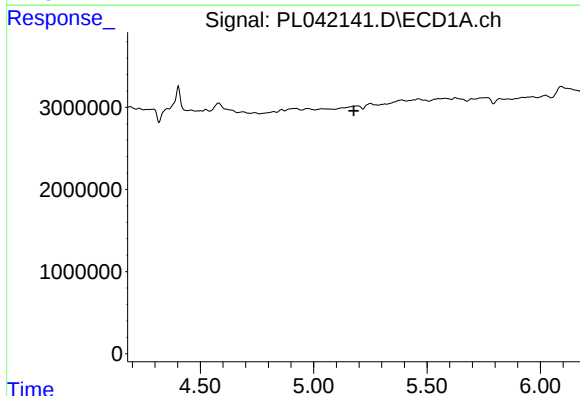


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.178 min
Response: 0
Conc: N.D.

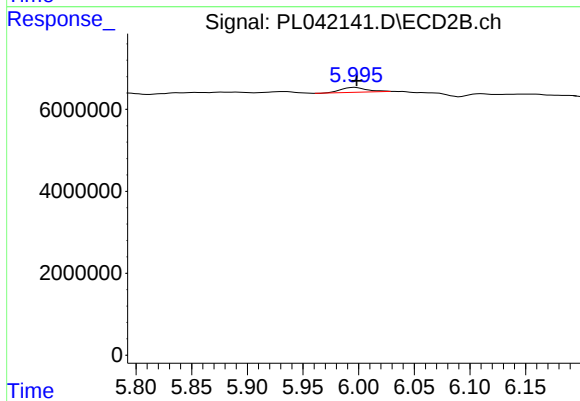

#8 Heptachlor epoxide


R.T.: 5.997 min
Delta R.T.: -0.002 min
Response: 2009947
Conc: 0.56 ng/ml

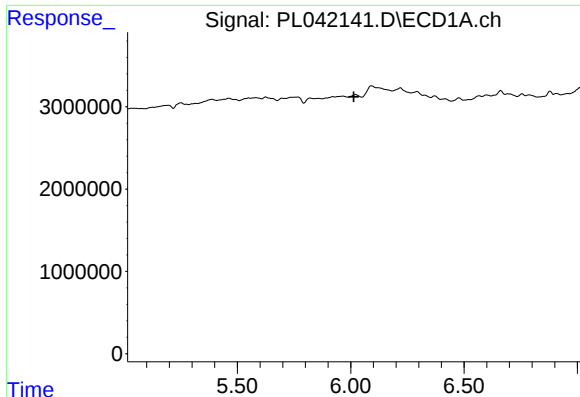

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

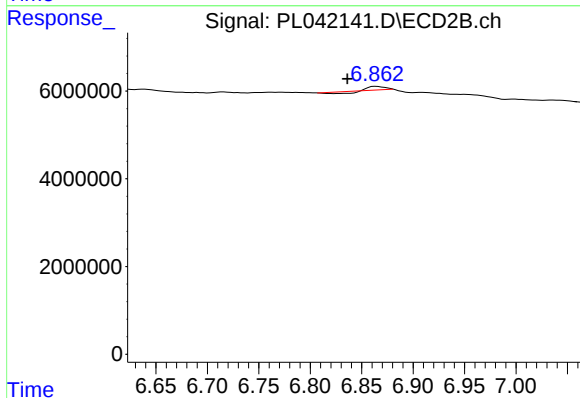


#14 Endrin

R.T.: 6.864 min
Delta R.T.: 0.028 min
Response: 398304
Conc: 0.14 ng/ml

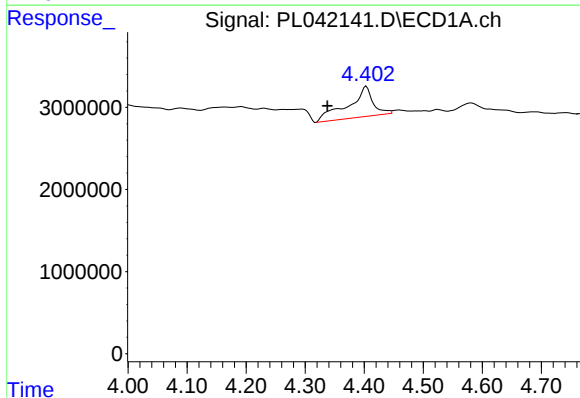


#23 Chlordane-1

R.T.: 4.404 min
Delta R.T.: 0.066 min
Response: 10737894
Conc: 35.98 ng/ml

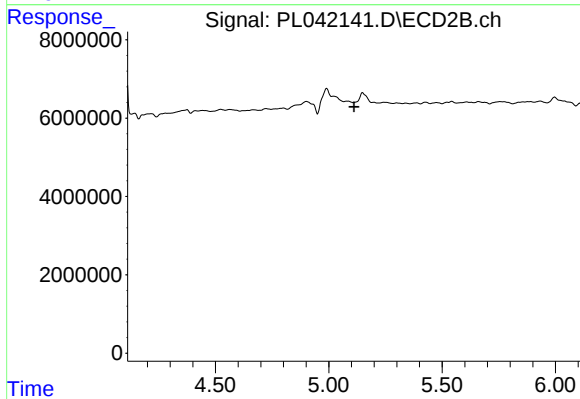

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.112 min
Response: 0
Conc: N.D.

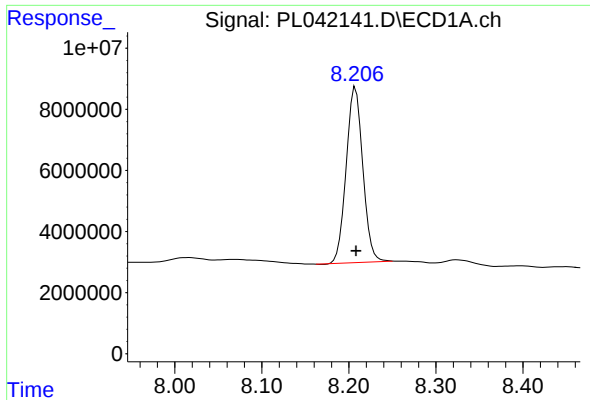

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 76113778
Conc: 11.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

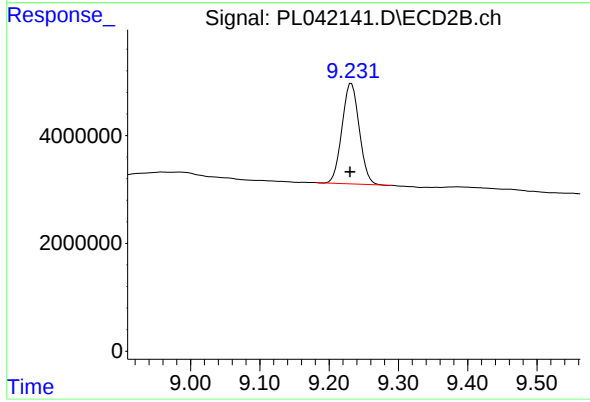

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.002 min
Response: 32136303
Conc: 12.60 ng/ml