

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 22:51
 Operator : AJ\SJ
 Sample : PB114776BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:43:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.469	4.102	147.6E6	79417840	23.908	26.806
28) SA Decachlor...	8.208	9.233	148.8E6	64109798	21.717	25.135
Target Compounds						
2) A alpha-BHC	3.901	4.504	3575533	713711	0.377	0.161 #
6) B beta-BHC	4.404f	0.000	5133382	0	1.391	N.D. #
8) B Heptachlo...	0.000	5.997	0	1840054	N.D.	0.512 #
19) B Endosulfa...	0.000	7.386	0	2375042	N.D.	0.873 #
20) A Methoxychlor	0.000	7.648f	0	2835355	N.D.	2.063 #
23) Chlordane-1	4.367	0.000	1566504	0	5.249	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2018 22:51
Operator : AJ\SJ
Sample : PB114776BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:43:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

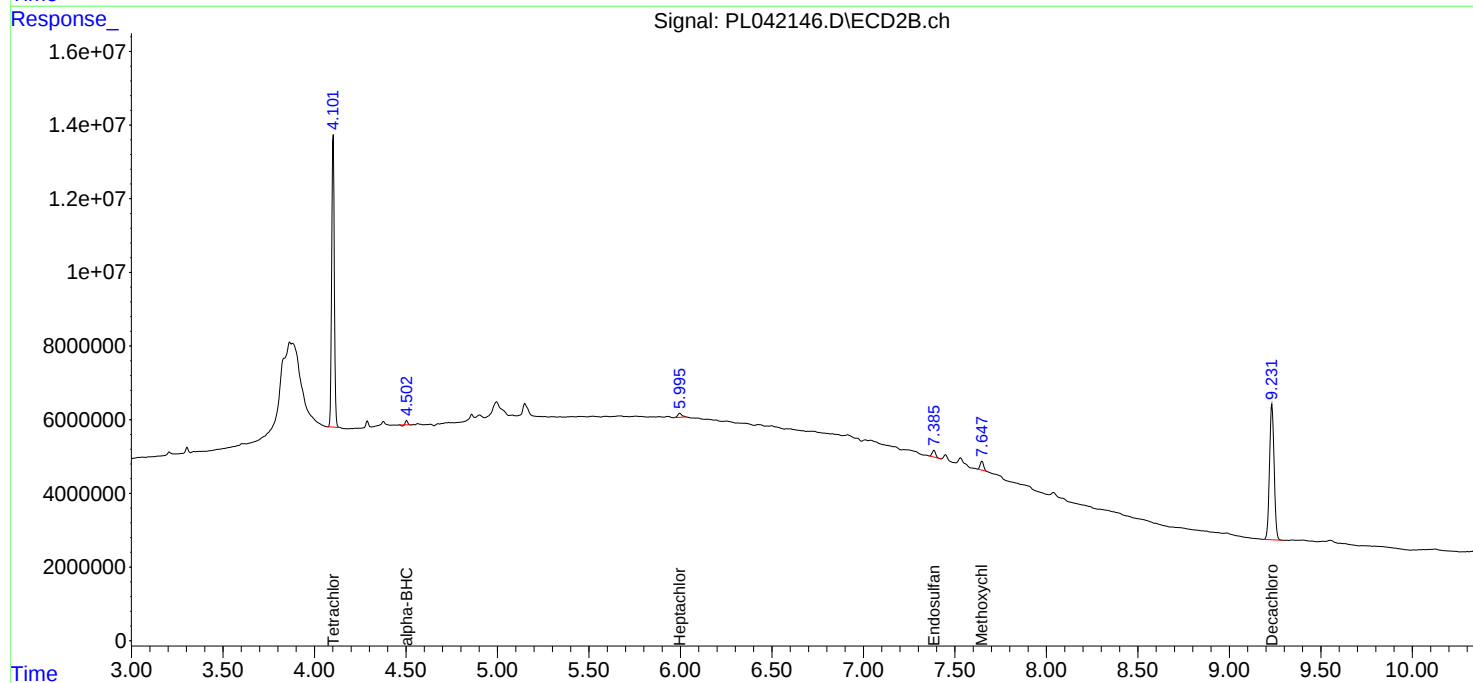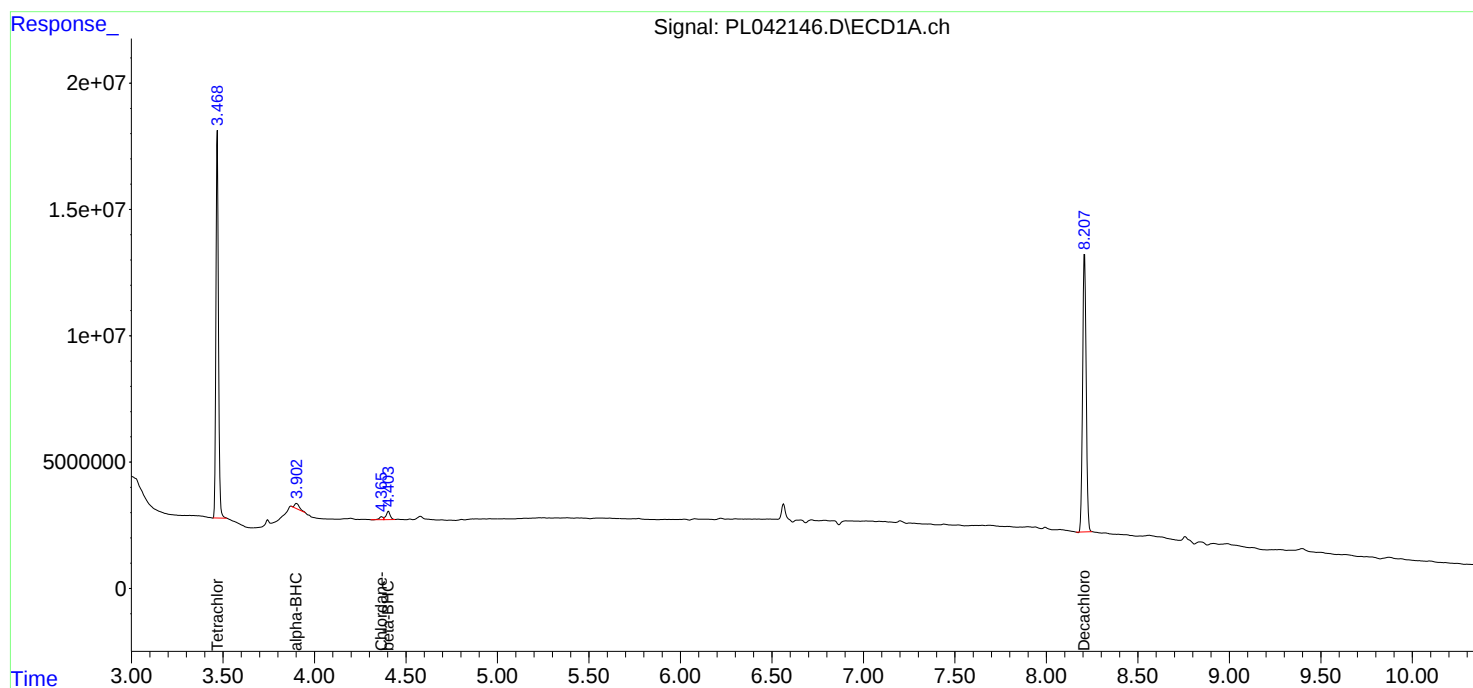


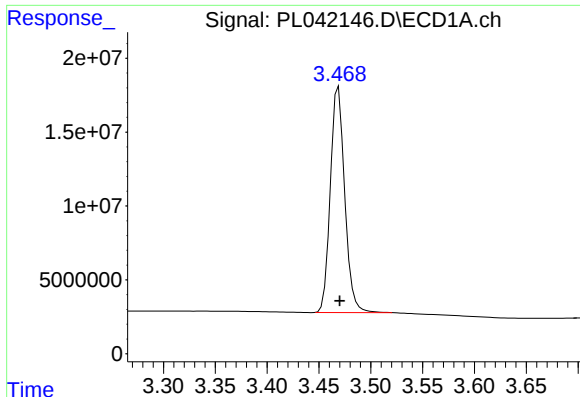

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 147632351
Conc: 23.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

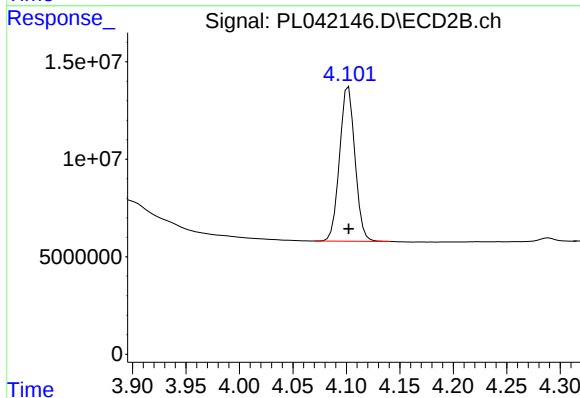


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 79417840
Conc: 26.81 ng/ml

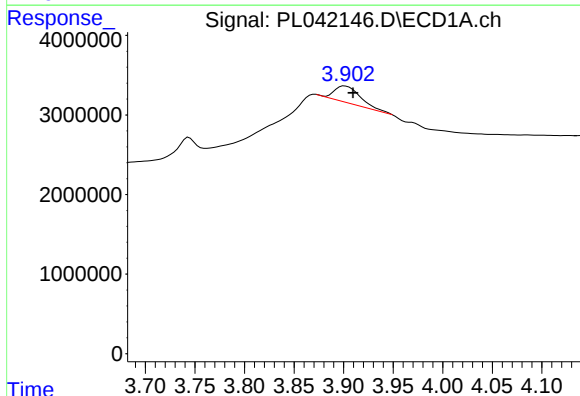


#2 alpha-BHC

R.T.: 3.901 min
Delta R.T.: -0.008 min
Response: 3575533
Conc: 0.38 ng/ml

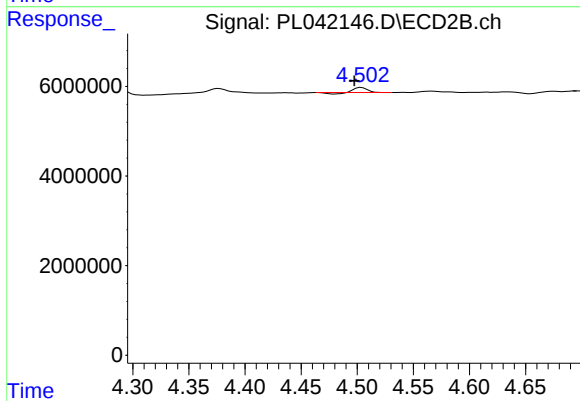

#2 alpha-BHC


R.T.: 4.504 min
Delta R.T.: 0.006 min
Response: 713711
Conc: 0.16 ng/ml

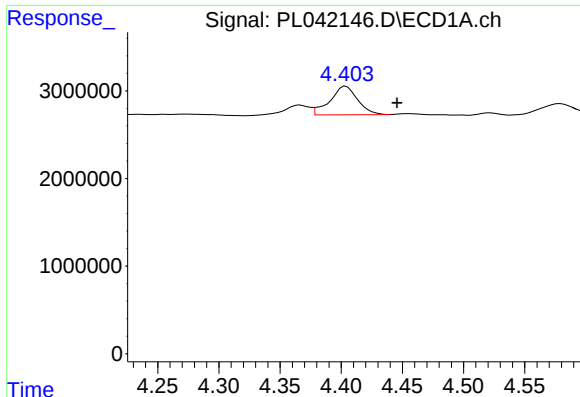

#6 beta-BHC


R.T.: 4.404 min
Delta R.T.: -0.041 min
Response: 5133382
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

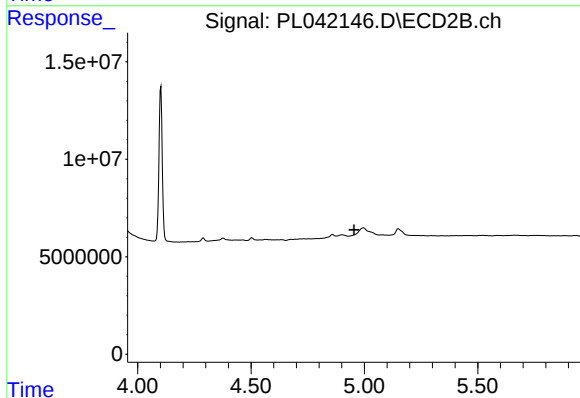


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

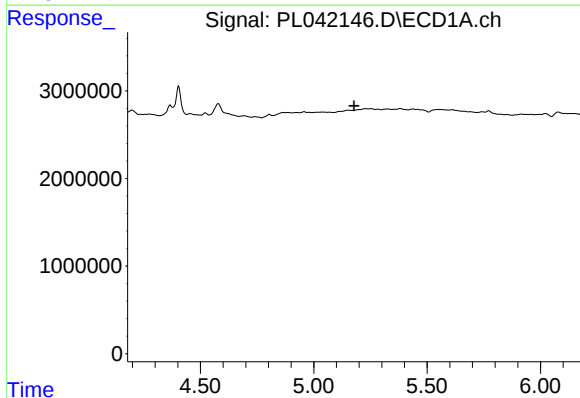


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.178 min
Response: 0
Conc: N.D.

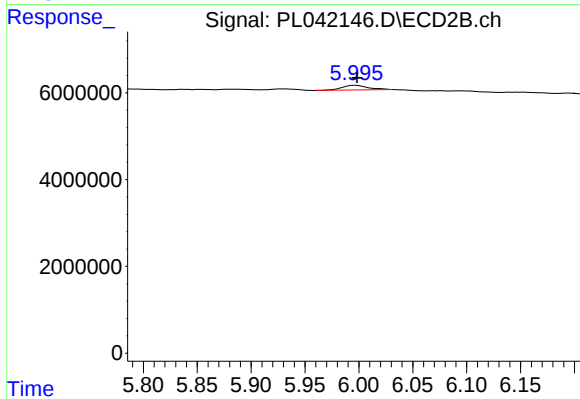

#8 Heptachlor epoxide


R.T.: 5.997 min
Delta R.T.: -0.002 min
Response: 1840054
Conc: 0.51 ng/ml

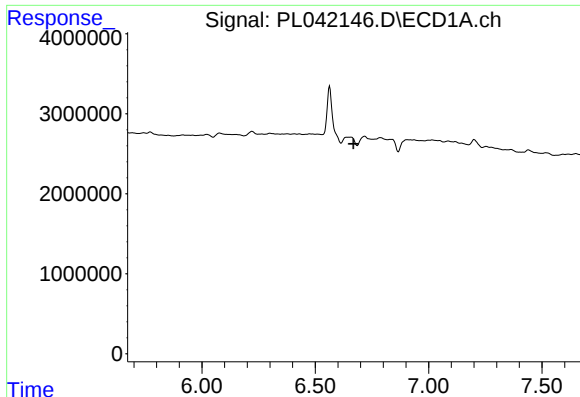

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

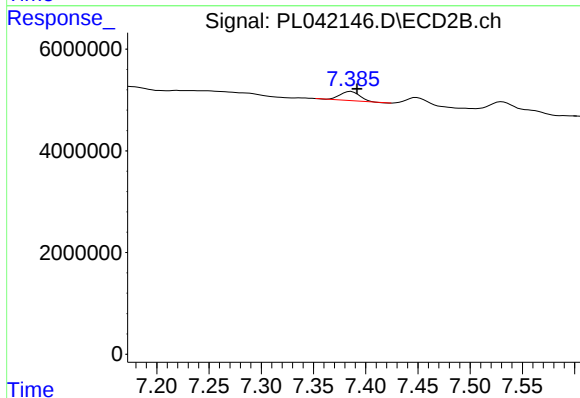


#19 Endosulfan Sulfate

R.T.: 7.386 min
Delta R.T.: -0.006 min
Response: 2375042
Conc: 0.87 ng/ml

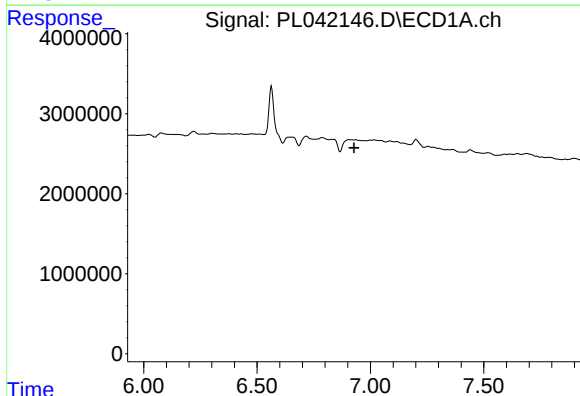


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.928 min
Response: 0
Conc: N.D.

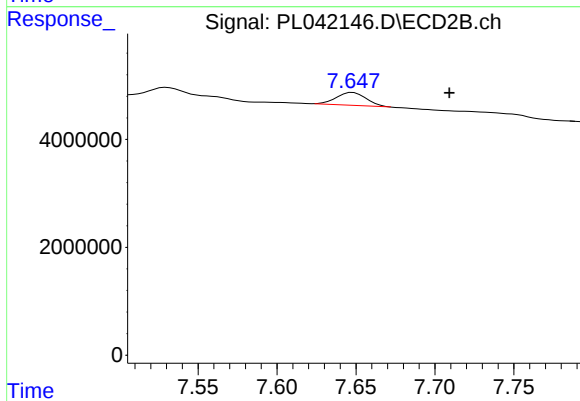

#20 Methoxychlor


R.T.: 7.648 min
Delta R.T.: -0.061 min
Response: 2835355
Conc: 2.06 ng/ml

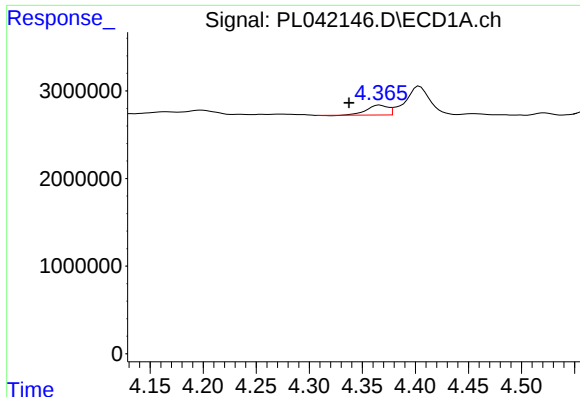

#23 Chlordane-1


R.T.: 4.367 min
Delta R.T.: 0.029 min
Response: 1566504
Conc: 5.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

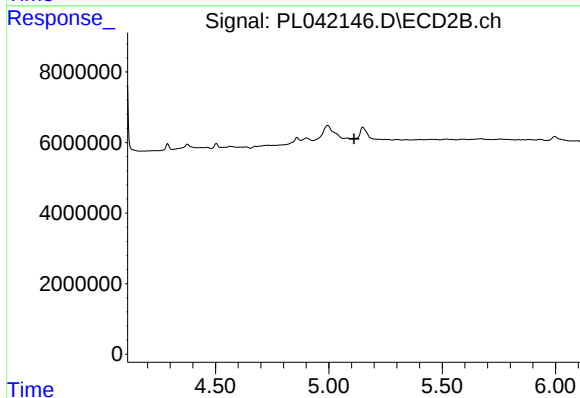


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

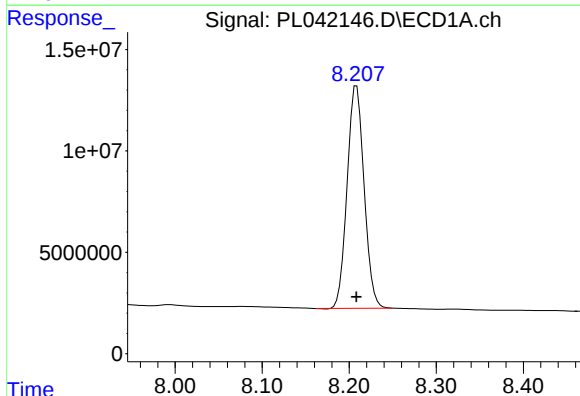

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 148771635
Conc: 21.72 ng/ml

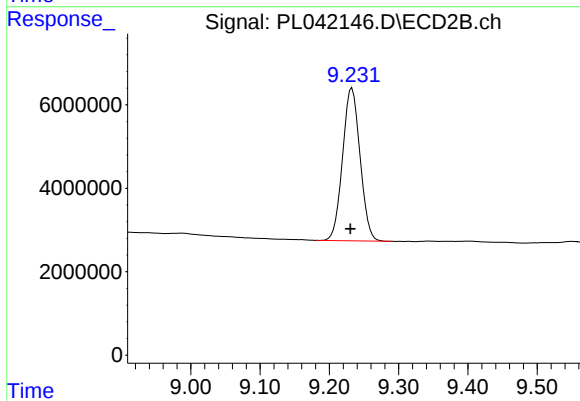

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 64109798
Conc: 25.14 ng/ml