

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2018 23:19
 Operator : AJ\SJ
 Sample : PB114776TB
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:43:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	128.9E6	69907444	20.876	23.596
28)	SA Decachlor...	8.208	9.233	133.3E6	56857111	19.463	22.292
Target Compounds							
2)	A alpha-BHC	3.904	4.503	3465543	6005543	0.365	1.353 #
6)	B beta-BHC	4.407f	0.000	7344625	0	1.990	N.D. #
8)	B Heptachlo...	0.000	5.995	0	1612160	N.D.	0.449 #
19)	B Endosulfa...	6.659	7.386	8536625	10347681	1.339	3.804 #
20)	A Methoxychlor	0.000	7.648f	0	11635263	N.D.	8.468 #
21)	B Endrin ke...	7.200f	0.000	5288288	0	0.734	N.D. #
23)	Chlordane-1	4.366	0.000	1775625	0	5.950	N.D. #
24)	Chlordane-2	4.803	0.000	1273031	0	4.013	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2018 23:19
Operator : AJ\SJ
Sample : PB114776TB
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:43:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

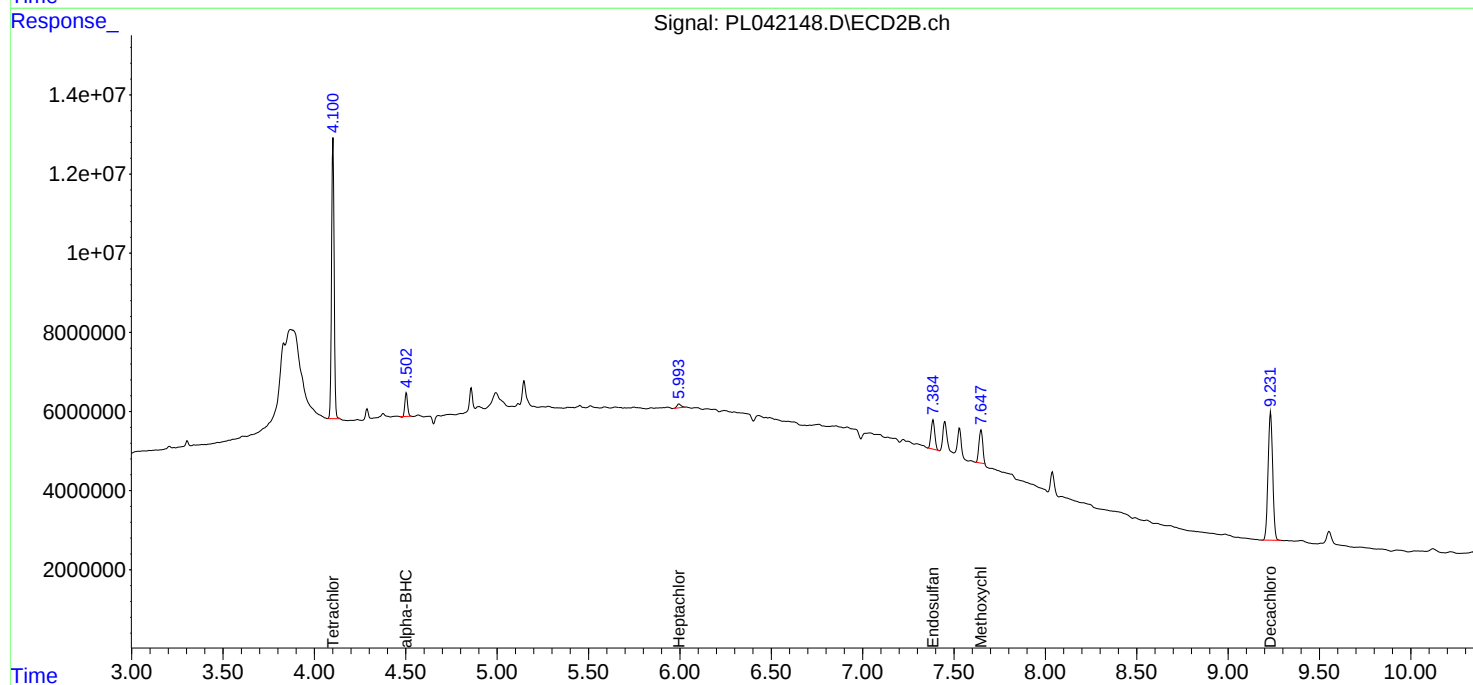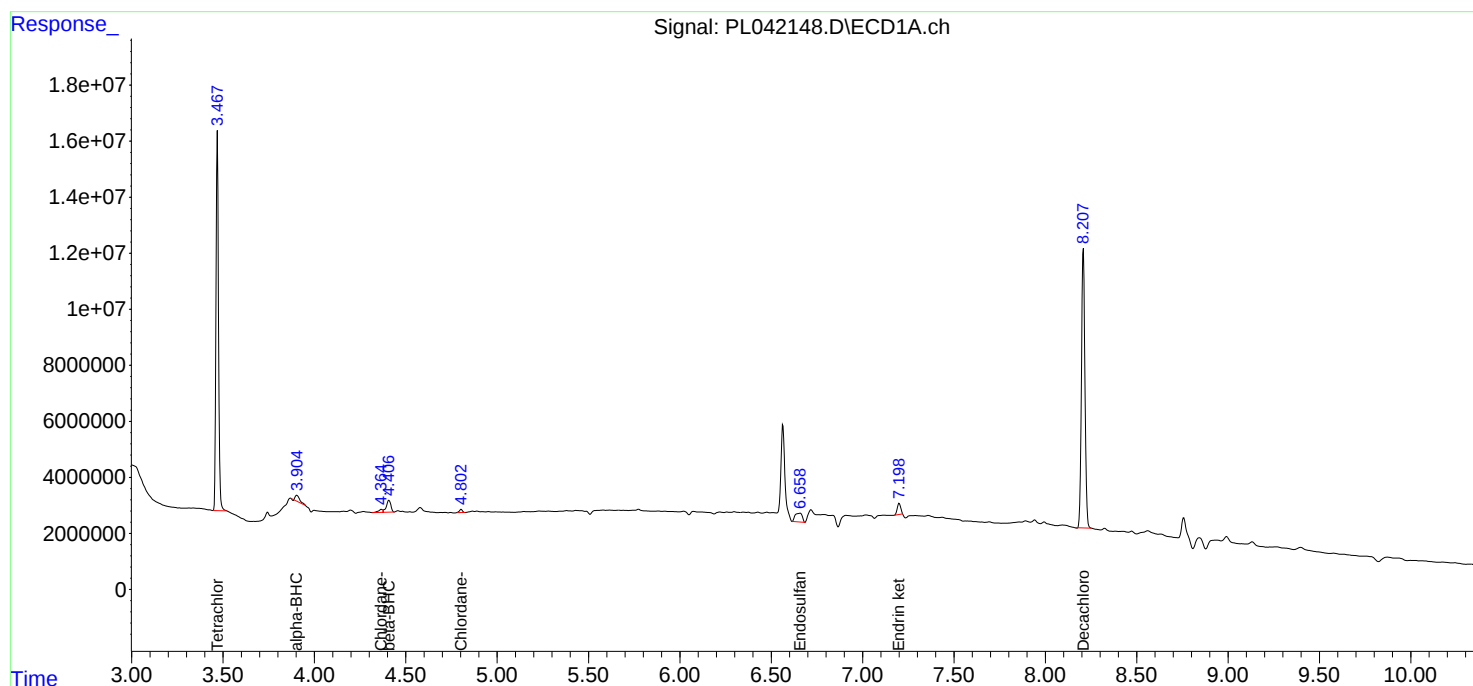


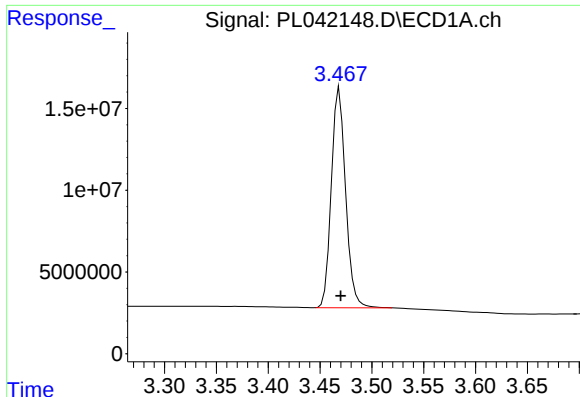

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 128907621
Conc: 20.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

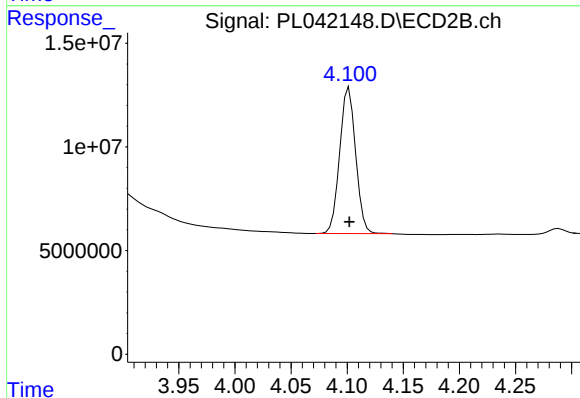


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 69907444
Conc: 23.60 ng/ml

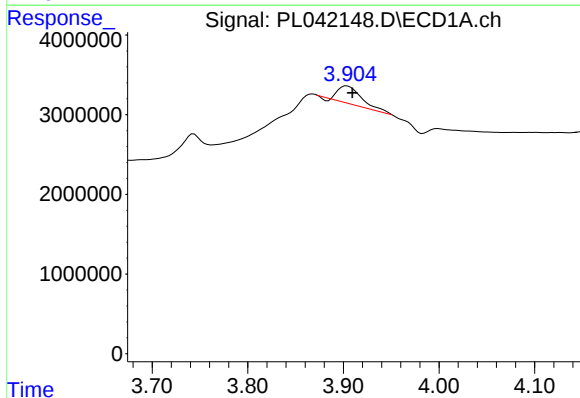


#2 alpha-BHC

R.T.: 3.904 min
Delta R.T.: -0.006 min
Response: 3465543
Conc: 0.37 ng/ml

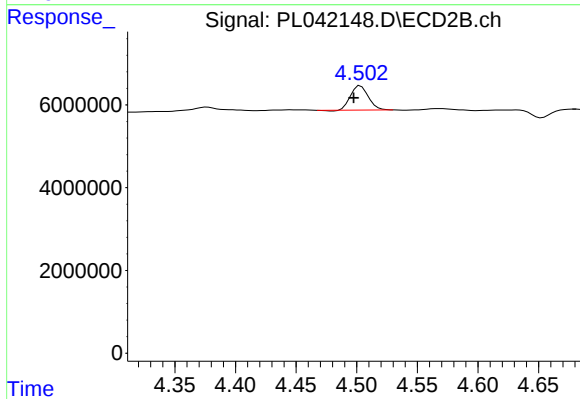

#2 alpha-BHC


R.T.: 4.503 min
Delta R.T.: 0.006 min
Response: 6005543
Conc: 1.35 ng/ml

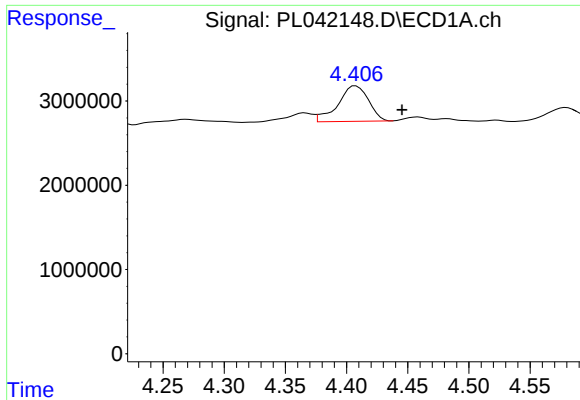

#6 beta-BHC


R.T.: 4.407 min
Delta R.T.: -0.038 min
Response: 7344625
Conc: 1.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

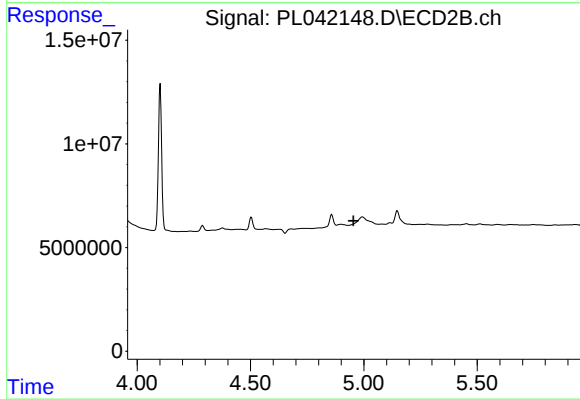


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

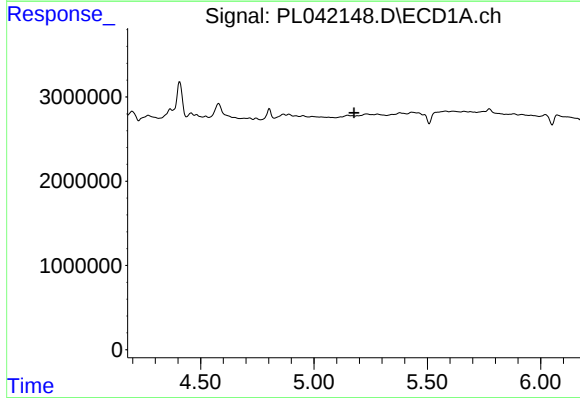


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.178 min
Response: 0
Conc: N.D.

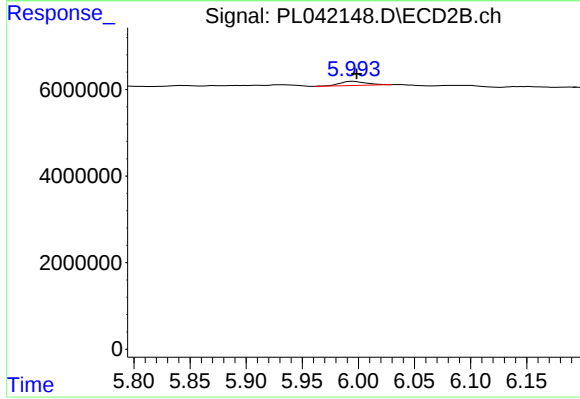

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: -0.004 min
Response: 1612160
Conc: 0.45 ng/ml

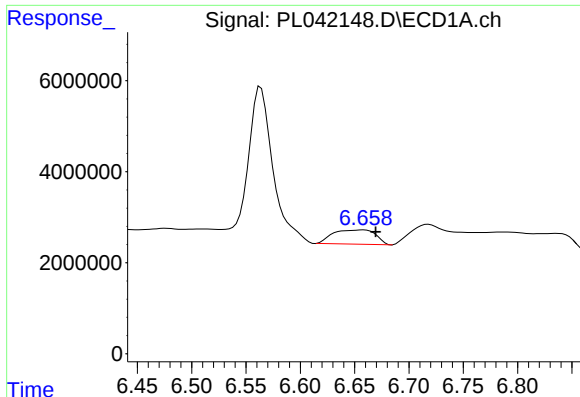

#19 Endosulfan Sulfate


R.T.: 6.659 min
Delta R.T.: -0.011 min
Response: 8536625
Conc: 1.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

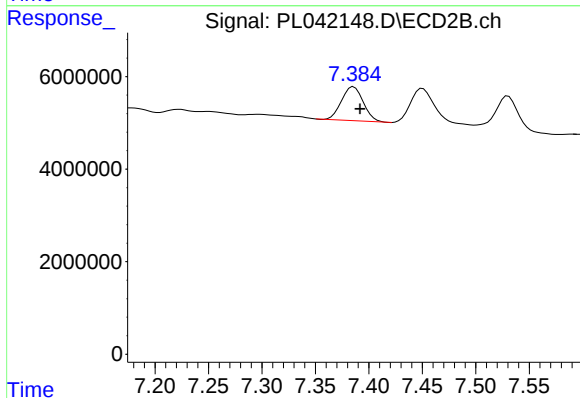


#19 Endosulfan Sulfate

R.T.: 7.386 min
Delta R.T.: -0.006 min
Response: 10347681
Conc: 3.80 ng/ml

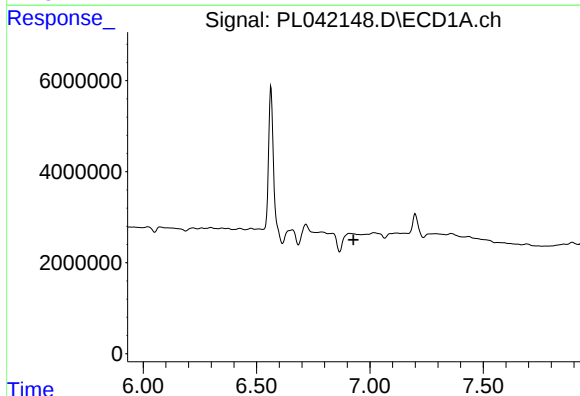


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

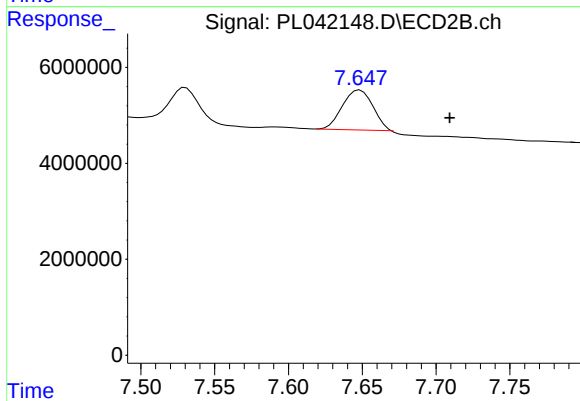

#20 Methoxychlor


R.T.: 7.648 min
Delta R.T.: -0.061 min
Response: 11635263
Conc: 8.47 ng/ml

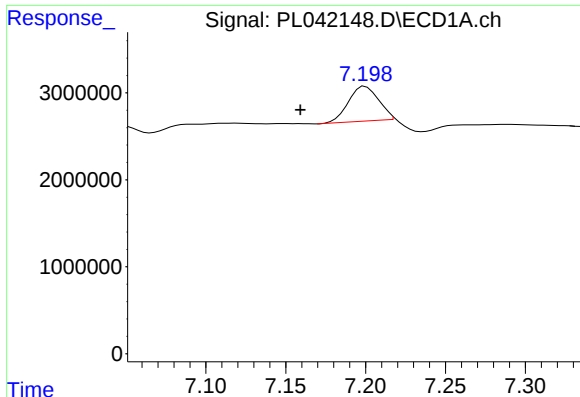

#21 Endrin ketone


R.T.: 7.200 min
Delta R.T.: 0.041 min
Response: 5288288
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

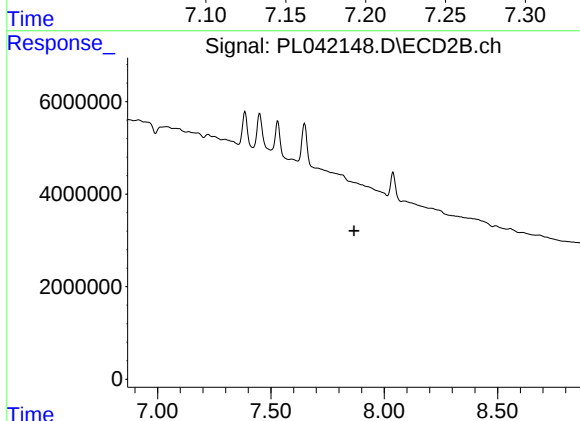


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.867 min
Response: 0
Conc: N.D.

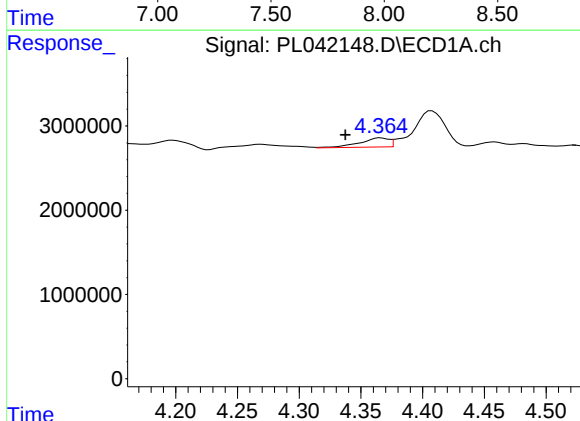


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.028 min
Response: 1775625
Conc: 5.95 ng/ml

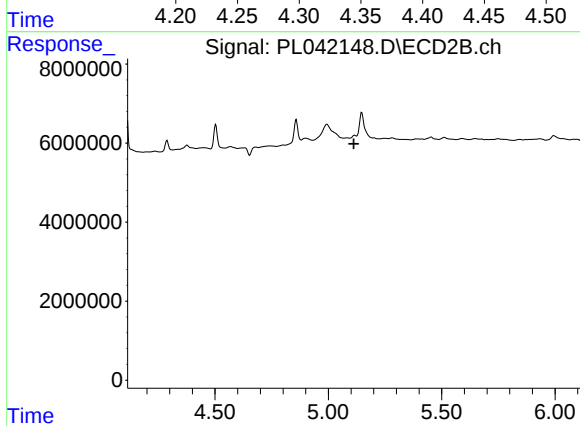

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

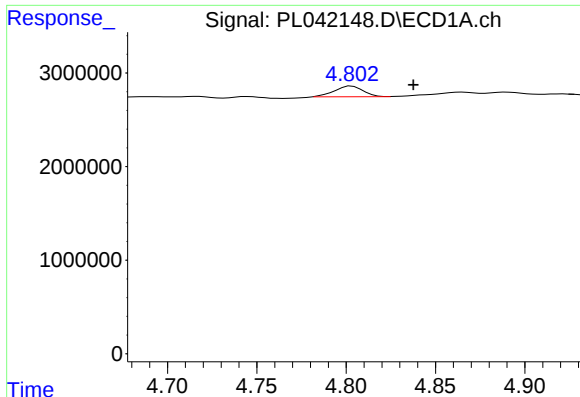

#24 Chlordane-2


R.T.: 4.803 min
Delta R.T.: -0.034 min
Response: 1273031
Conc: 4.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

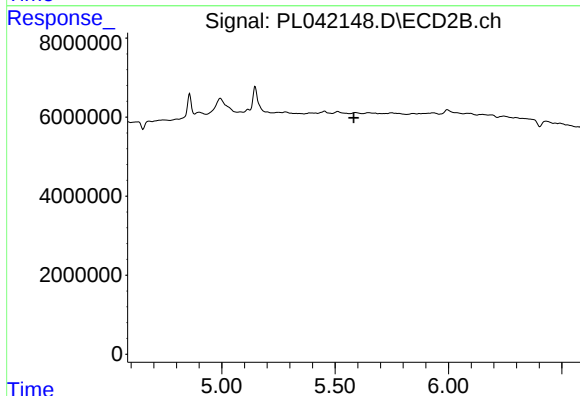


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.583 min
Response: 0
Conc: N.D.

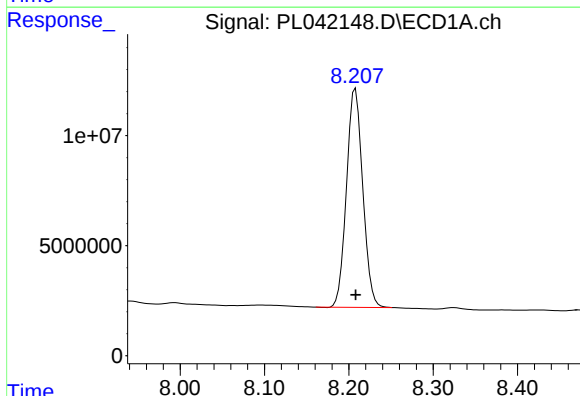

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 133331635
Conc: 19.46 ng/ml

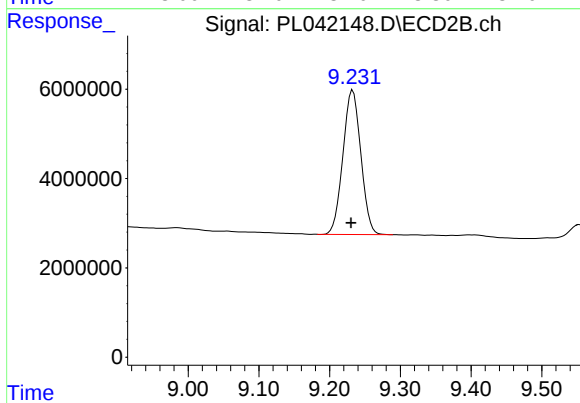

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 56857111
Conc: 22.29 ng/ml