

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 02:08
 Operator : AJ\SJ
 Sample : J5908-20
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:45:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	110.4E6	60194783	17.879	20.318
28)	SA Decachlor...	8.208	9.232	113.4E6	47826010	16.547	18.751
Target Compounds							
6)	B beta-BHC	4.404f	0.000	15939094	0	4.319	N.D. #
8)	B Heptachlo...	0.000	6.026	0	673218	N.D.	0.187 #
9)	A Endosulfan I	5.461f	0.000	3622658	0	0.497	N.D. #
10)	B gamma-Chl...	5.461f	0.000	3622658	0	0.449	N.D. #
11)	B alpha-Chl...	5.461	0.000	3622658	0	0.455	N.D. #
23)	Chlordane-1	4.404	0.000	15939094	0	53.408	N.D. #
25)	Chlordane-3	5.461	0.000	3622658	0	3.875	N.D. #
26)	Chlordane-4	5.461	0.000	3622658	0	4.336	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 02:08
Operator : AJ\SJ
Sample : J5908-20
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:45:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

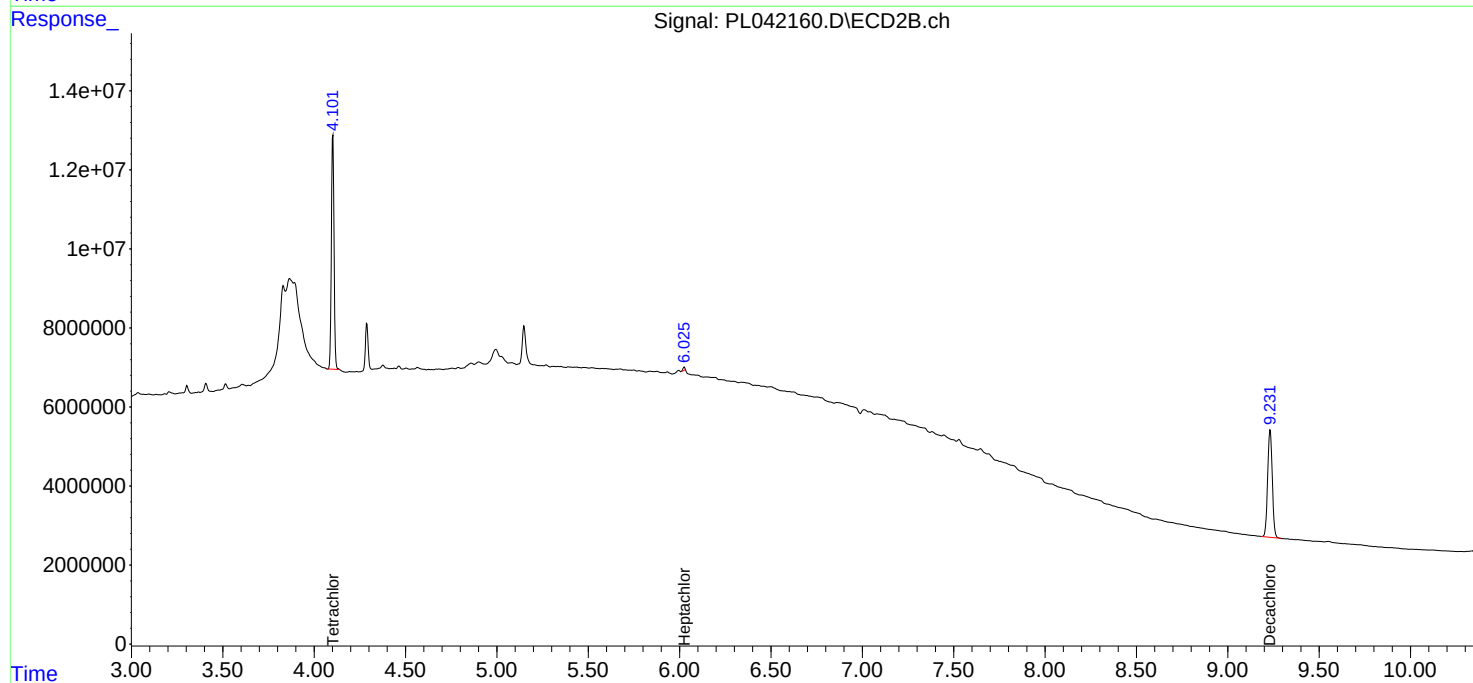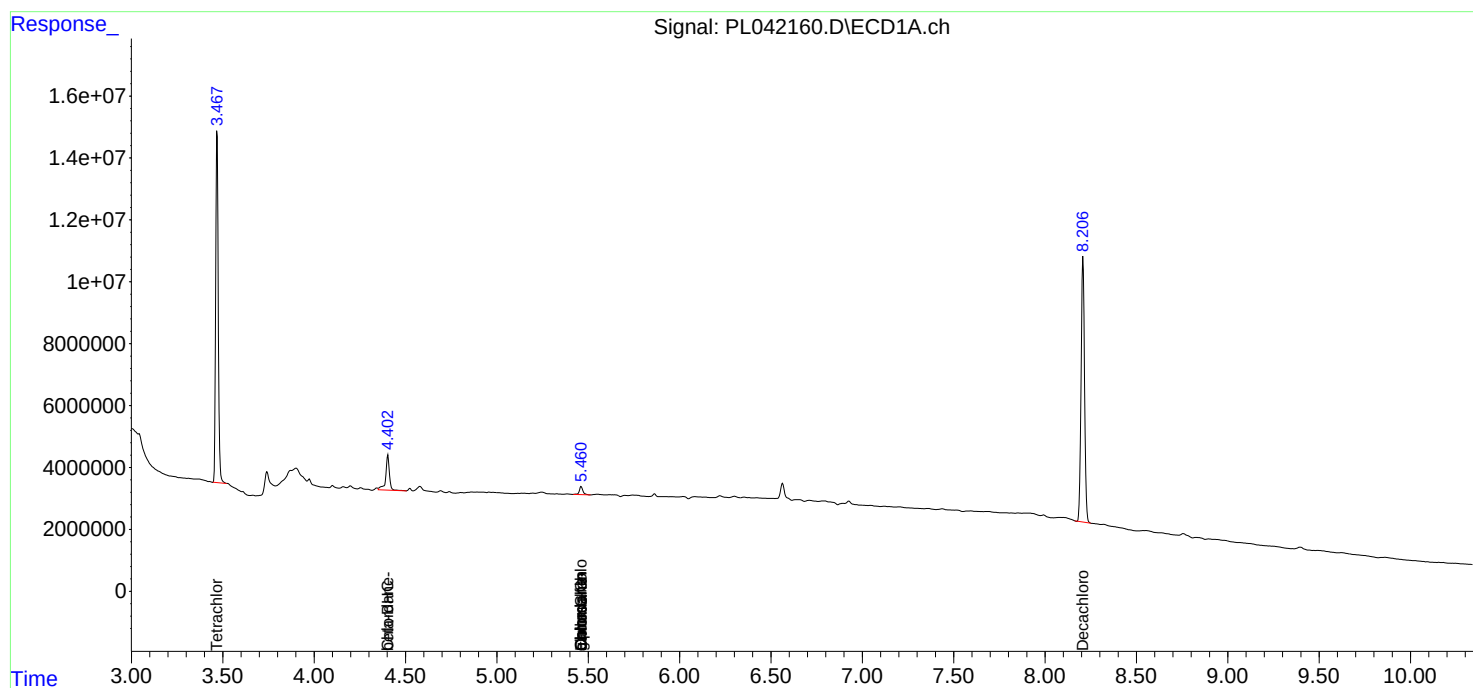


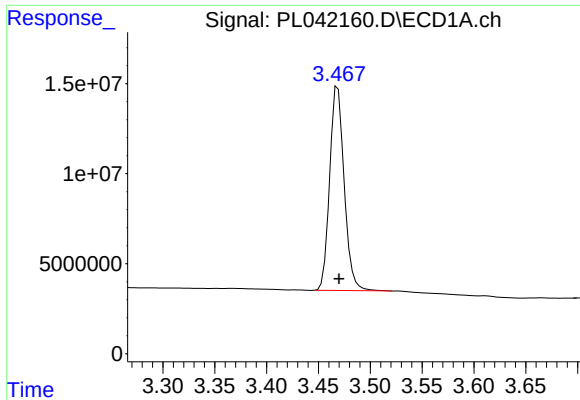

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 110404379
Conc: 17.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

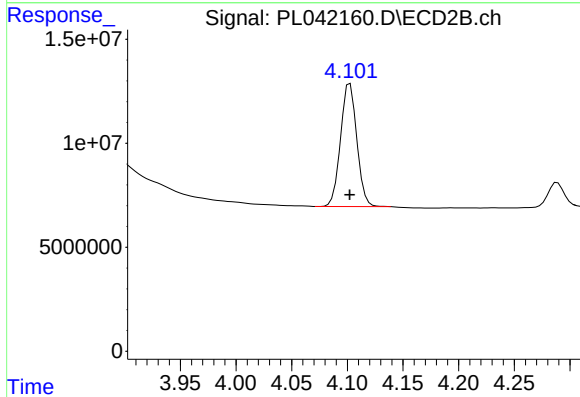


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 60194783
Conc: 20.32 ng/ml

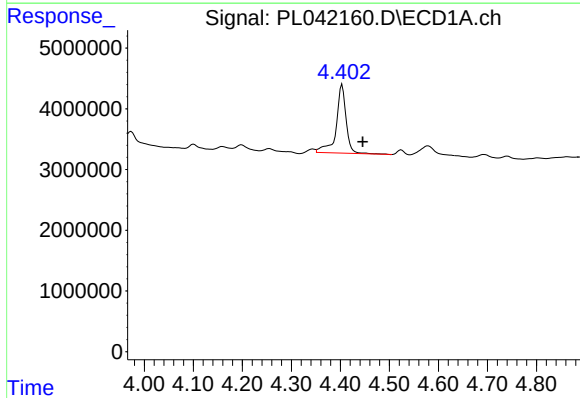


#6 beta-BHC

R.T.: 4.404 min
Delta R.T.: -0.042 min
Response: 15939094
Conc: 4.32 ng/ml

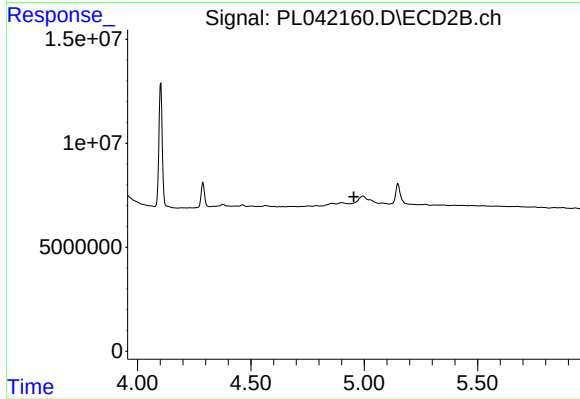

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

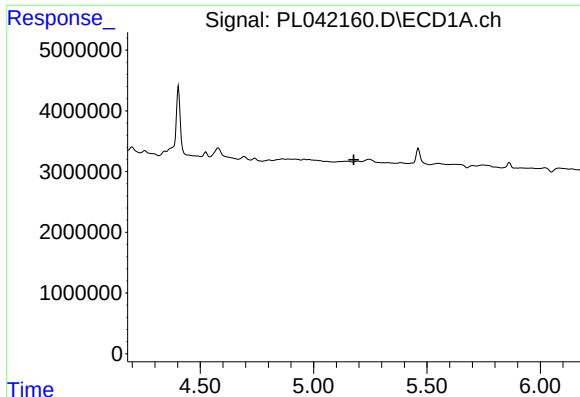

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

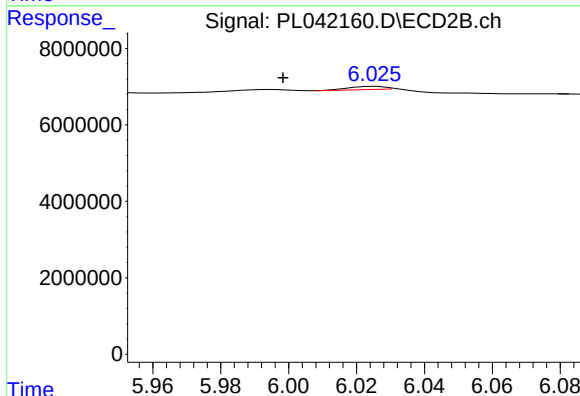


#8 Heptachlor epoxide

R.T.: 6.026 min
Delta R.T.: 0.027 min
Response: 673218
Conc: 0.19 ng/ml

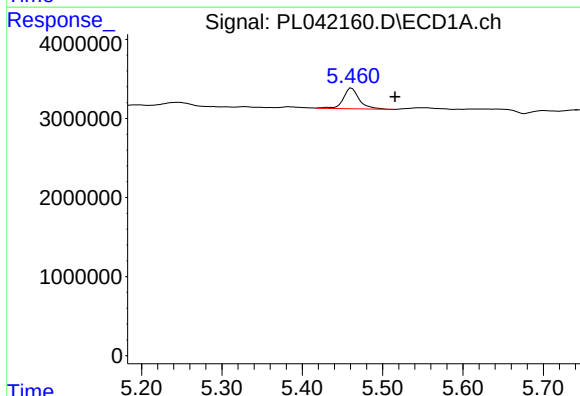


#9 Endosulfan I

R.T.: 5.461 min
Delta R.T.: -0.054 min
Response: 3622658
Conc: 0.50 ng/ml

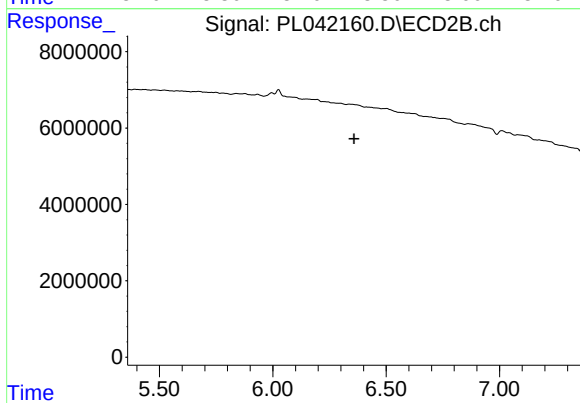

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

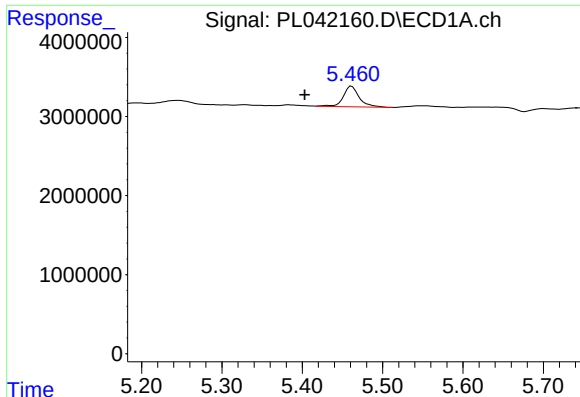

#10 gamma-Chlordane


R.T.: 5.461 min
Delta R.T.: 0.058 min
Response: 3622658
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

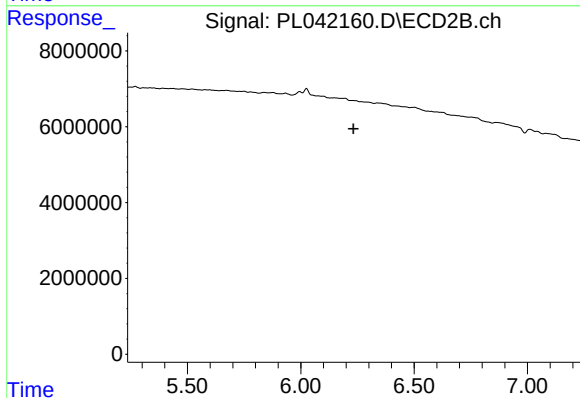


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

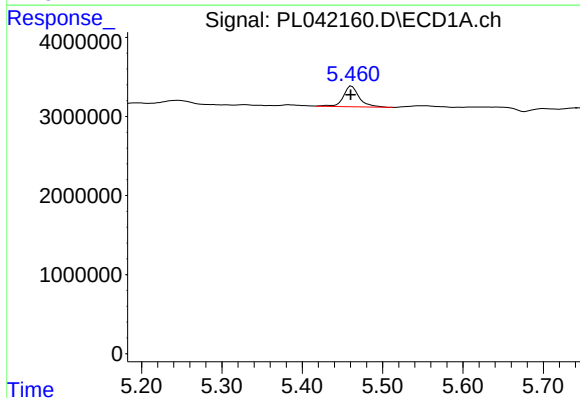


#11 alpha-Chlordane

R.T.: 5.461 min
Delta R.T.: 0.001 min
Response: 3622658
Conc: 0.45 ng/ml

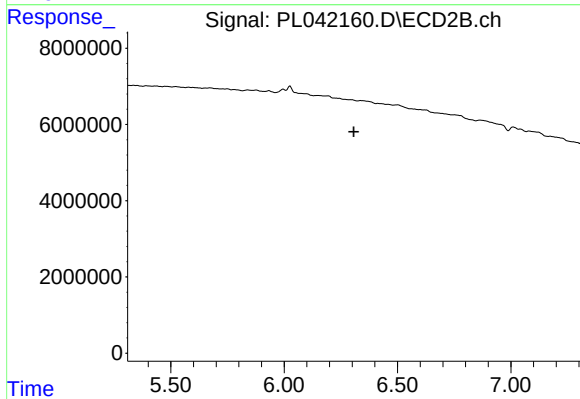

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

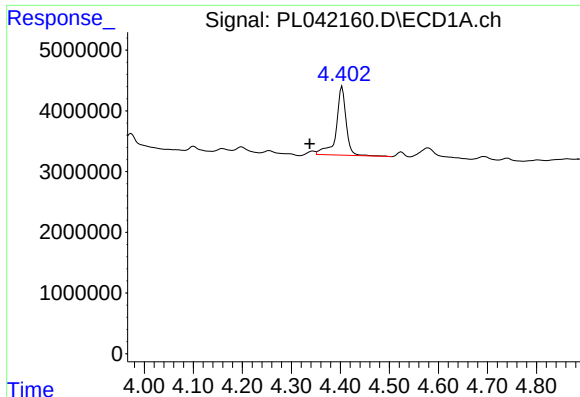

#23 Chlordane-1


R.T.: 4.404 min
Delta R.T.: 0.066 min
Response: 15939094
Conc: 53.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

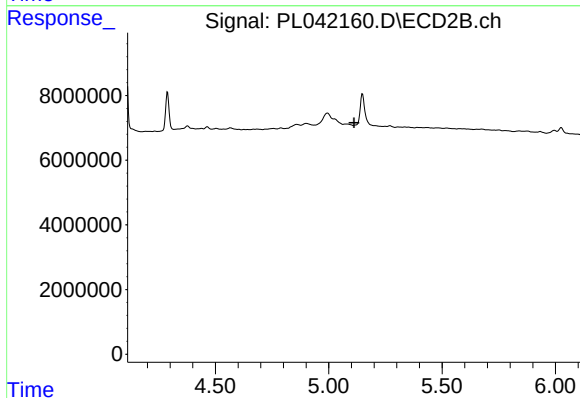


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

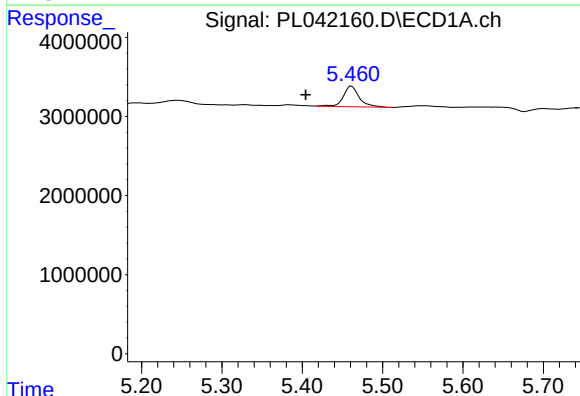


#25 Chlordane-3

R.T.: 5.461 min
Delta R.T.: 0.057 min
Response: 3622658
Conc: 3.87 ng/ml

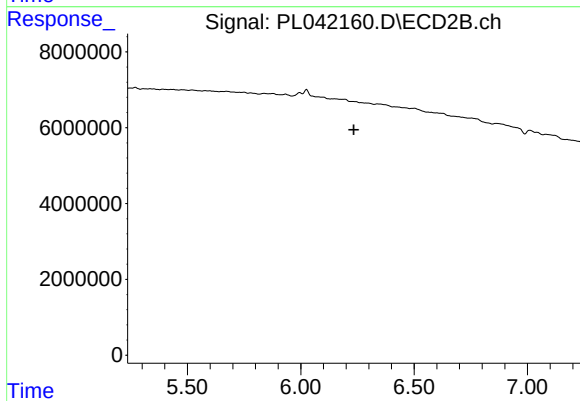

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

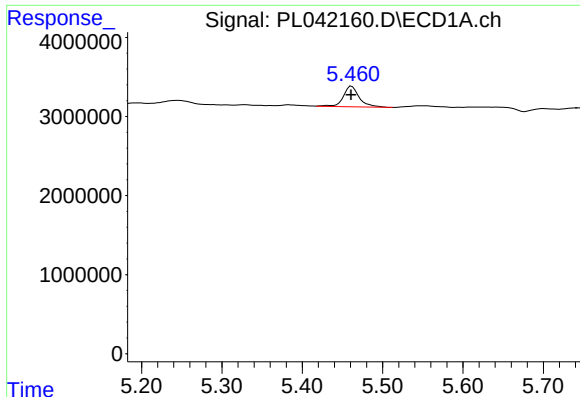

#26 Chlordane-4


R.T.: 5.461 min
Delta R.T.: 0.000 min
Response: 3622658
Conc: 4.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

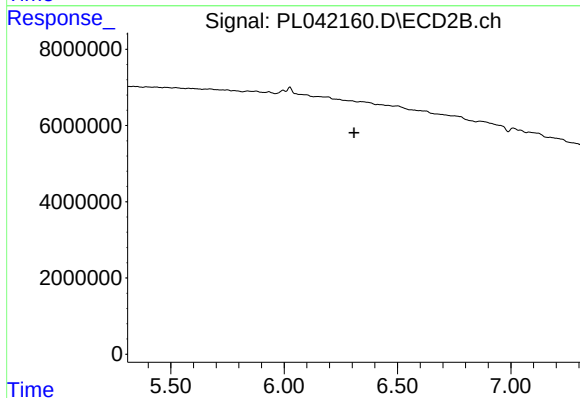


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

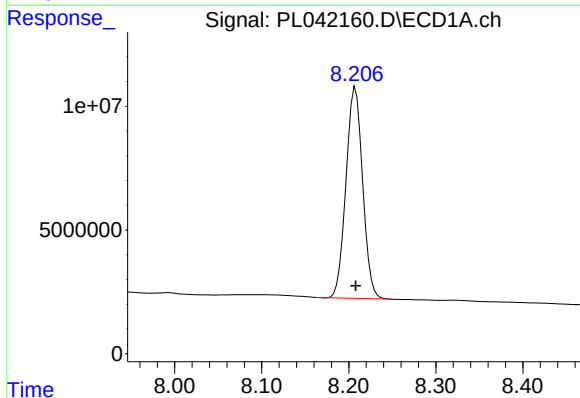

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 113352669
Conc: 16.55 ng/ml

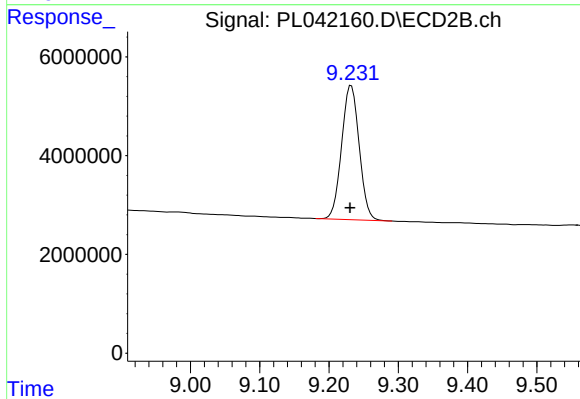

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.002 min
Response: 47826010
Conc: 18.75 ng/ml