

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 02:23
 Operator : AJ\SJ
 Sample : J5908-24
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:45:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	125.4E6	67540584	20.307	22.797
28)	SA Decachlor...	8.207	9.232	135.0E6	57477241	19.702	22.535
Target Compounds							
6)	B beta-BHC	4.404f	0.000	14241266	0	3.859	N.D. #
23)	Chlordane-1	4.404	0.000	14241266	0	47.719	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 02:23
Operator : AJ\SJ
Sample : J5908-24
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:45:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

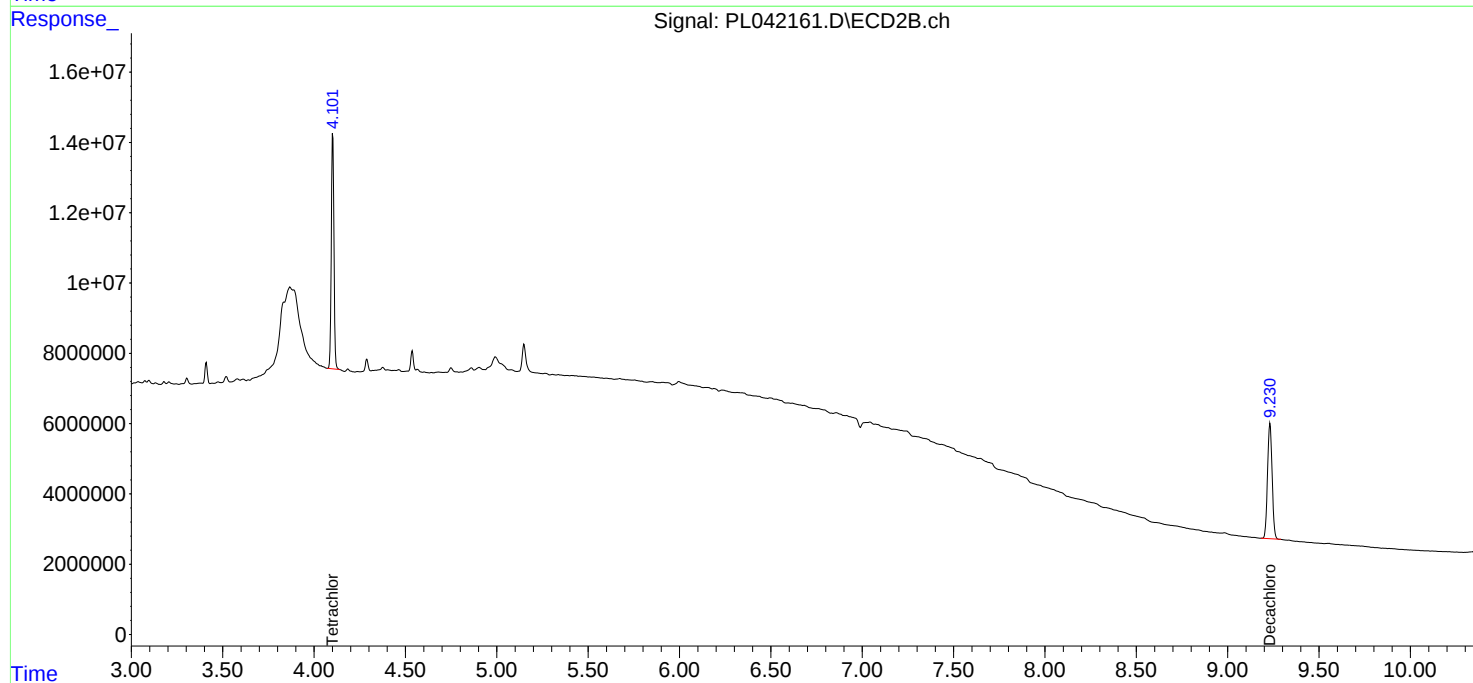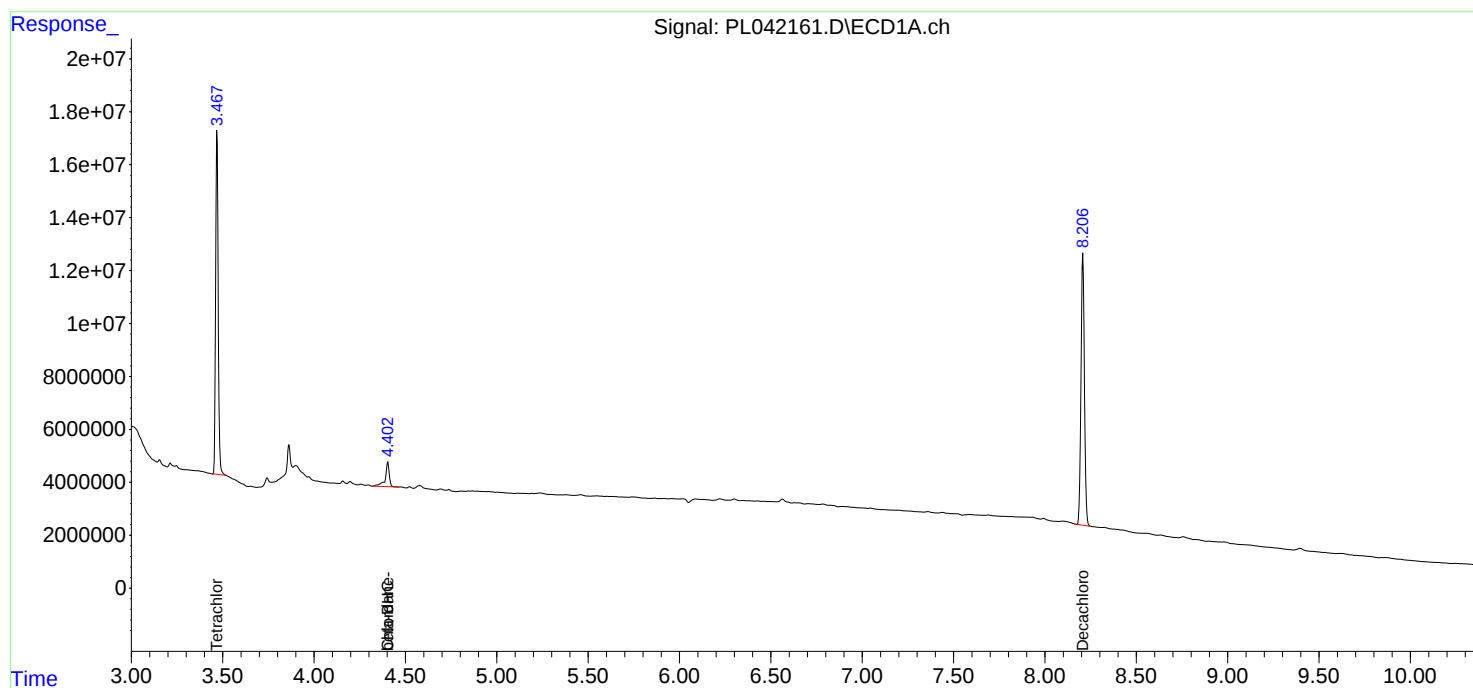


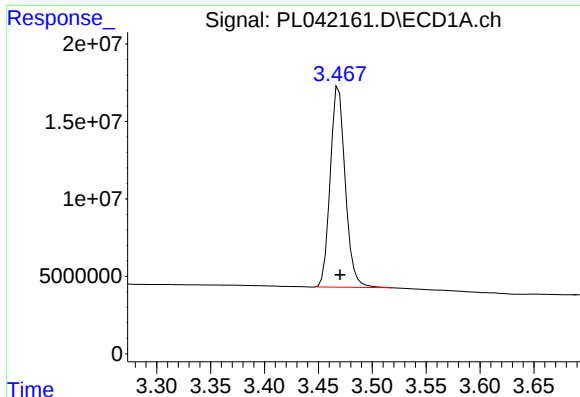

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 125392095
Conc: 20.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

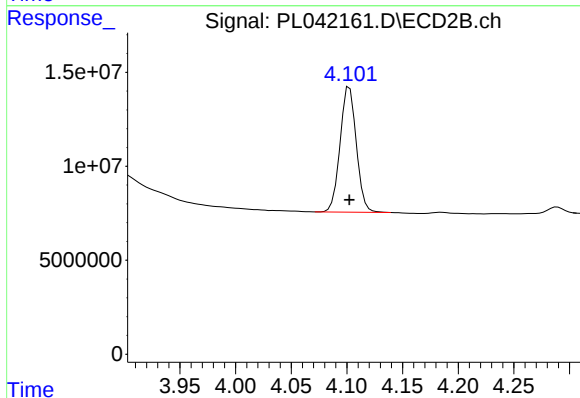


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 67540584
Conc: 22.80 ng/ml

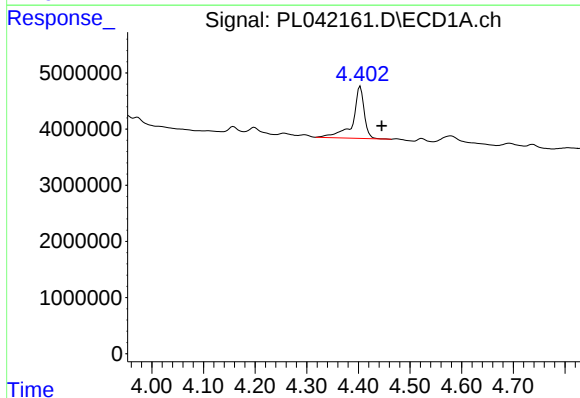


#6 beta-BHC

R.T.: 4.404 min
Delta R.T.: -0.042 min
Response: 14241266
Conc: 3.86 ng/ml

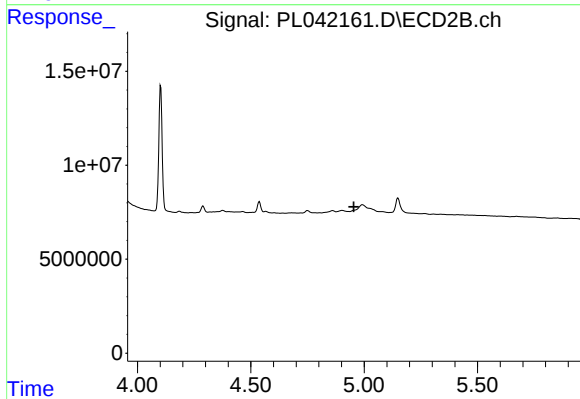

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.954 min
Response: 0
Conc: N.D.

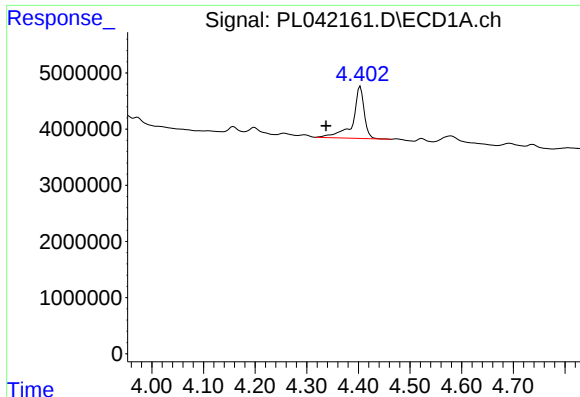

#23 Chlordane-1


R.T.: 4.404 min
Delta R.T.: 0.066 min
Response: 14241266
Conc: 47.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

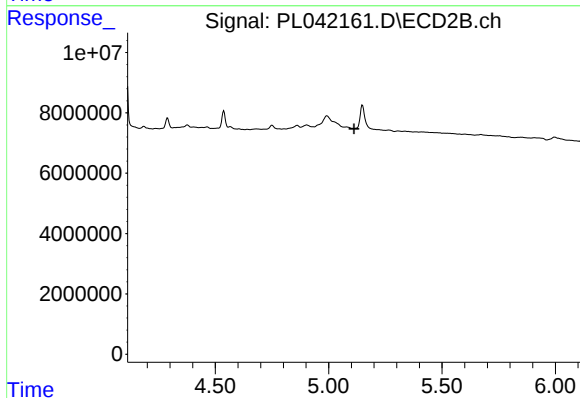


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

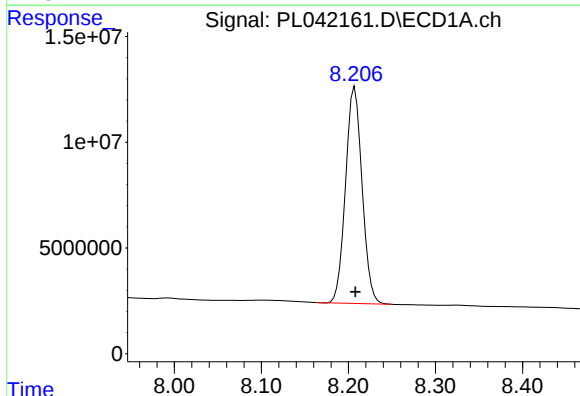

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 134964052
Conc: 19.70 ng/ml

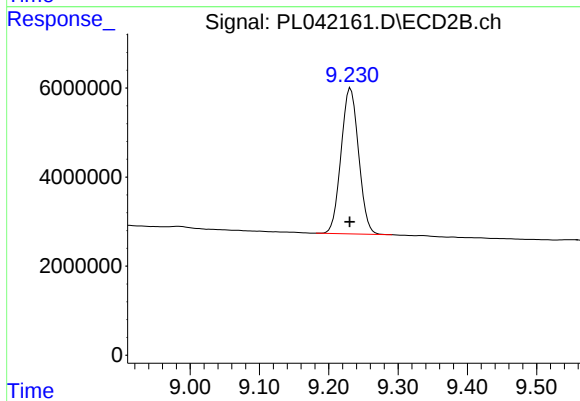

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.001 min
Response: 57477241
Conc: 22.53 ng/ml