

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 02:37
 Operator : AJ\SJ
 Sample : J5908-28
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:45:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	116.1E6	62713146	18.796	21.168
2)	SA Decachlor...	8.208	9.232	121.8E6	50906240	17.779	19.959
Target Compounds							
3)	MA gamma-BHC...	4.200	4.767	9728500	1973679	1.127	0.479 #
6)	B beta-BHC	4.404f	0.000	13493649	0	3.656	N.D. #
8)	B Heptachlo...	5.245f	0.000	16985958	0	2.153	N.D. #
9)	A Endosulfan I	5.544	0.000	8196281	0	1.125	N.D. #
10)	B gamma-Chl...	5.461f	6.165f	5415406	3908172	0.672	1.103 #
11)	B alpha-Chl...	5.461	0.000	5415406	0	0.680	N.D. #
13)	MA Dieldrin	5.765	0.000	4420486	0	0.568	N.D. #
16)	A 4,4'-DDD	6.101f	0.000	825180	0	0.149	N.D. #
20)	A Methoxychlor	0.000	7.646f	0	2225426	N.D.	1.620 #
23)	Chlordane-1	4.343	0.000	1252816	0	4.198	N.D. #
25)	Chlordane-3	5.461	6.165	5415406	3908172	5.792	7.653 #
26)	Chlordane-4	5.461	0.000	5415406	0	6.482	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 02:37
Operator : AJ\SJ
Sample : J5908-28
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:45:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

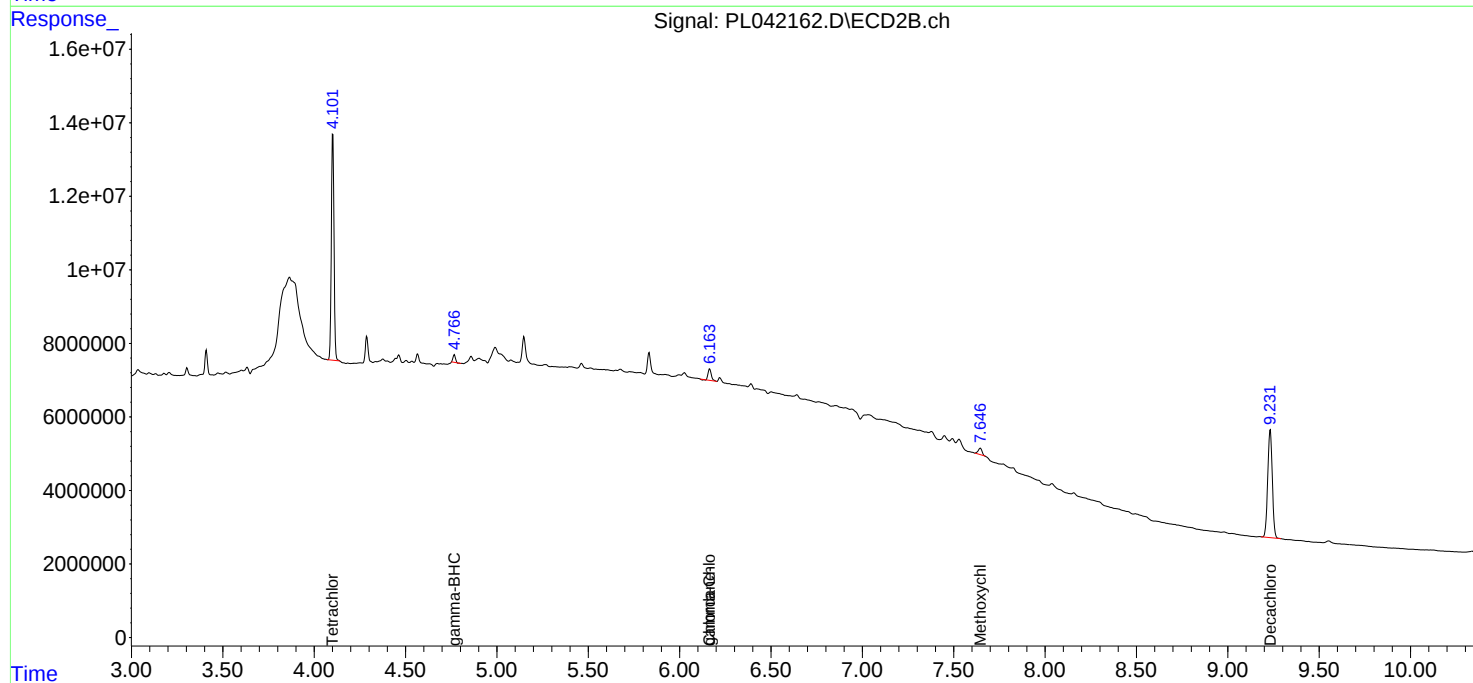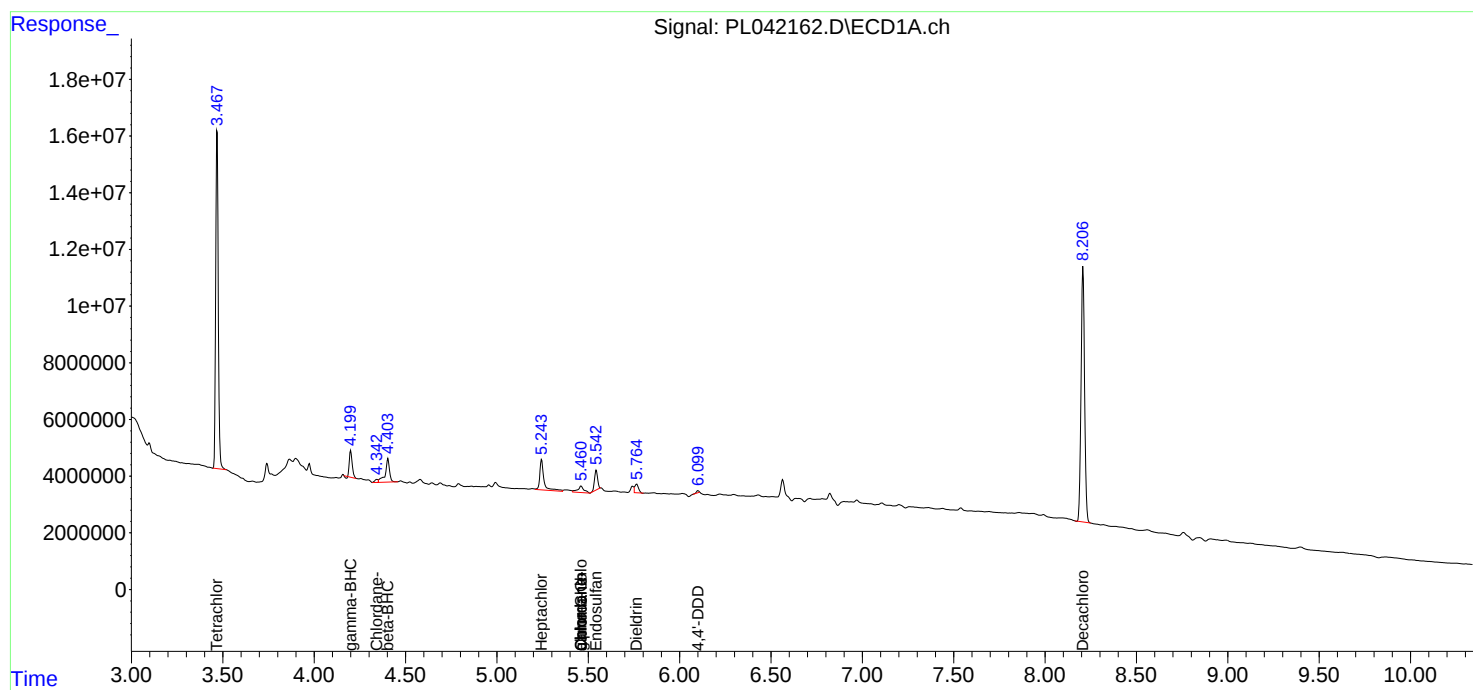


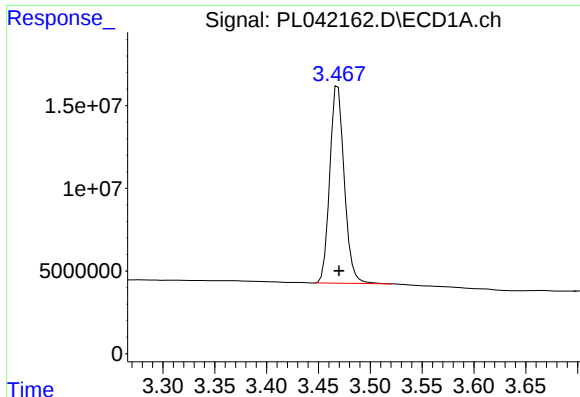

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 116065212
Conc: 18.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

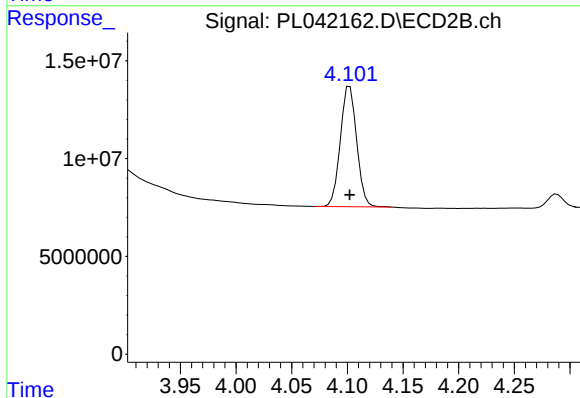


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 62713146
Conc: 21.17 ng/ml

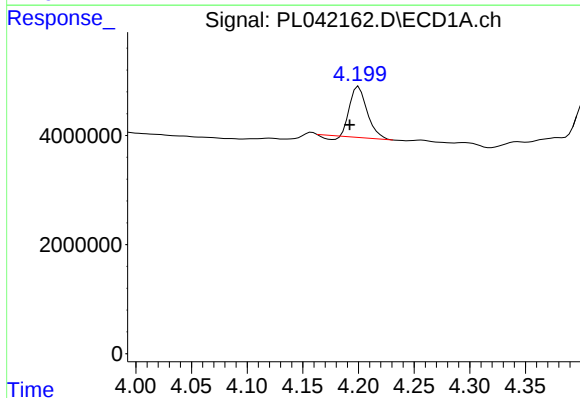


#3 gamma-BHC (Lindane)

R.T.: 4.200 min
Delta R.T.: 0.008 min
Response: 9728500
Conc: 1.13 ng/ml

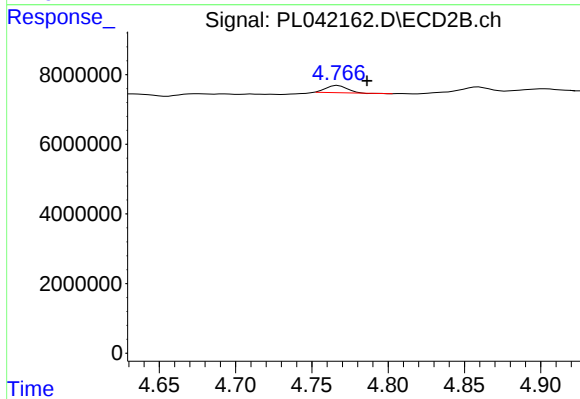

#3 gamma-BHC (Lindane)


R.T.: 4.767 min
Delta R.T.: -0.019 min
Response: 1973679
Conc: 0.48 ng/ml

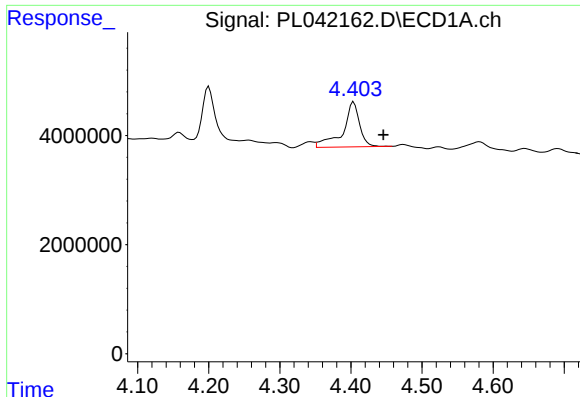

#6 beta-BHC


R.T.: 4.404 min
Delta R.T.: -0.041 min
Response: 13493649
Conc: 3.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

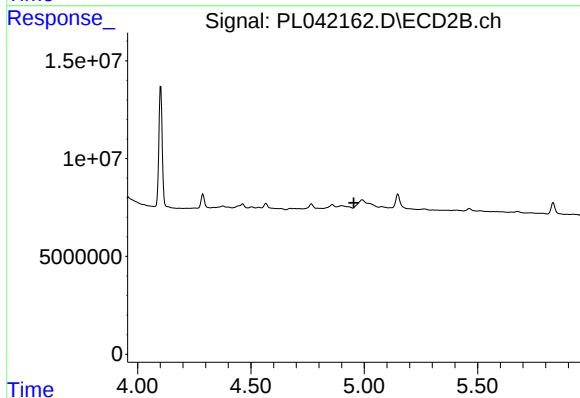


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

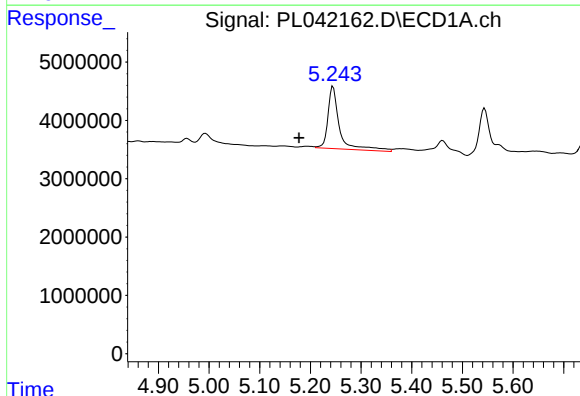


#8 Heptachlor epoxide

R.T.: 5.245 min
Delta R.T.: 0.067 min
Response: 16985958
Conc: 2.15 ng/ml

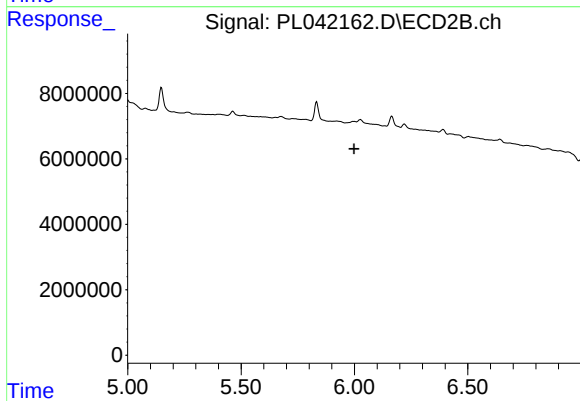

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.998 min
Response: 0
Conc: N.D.

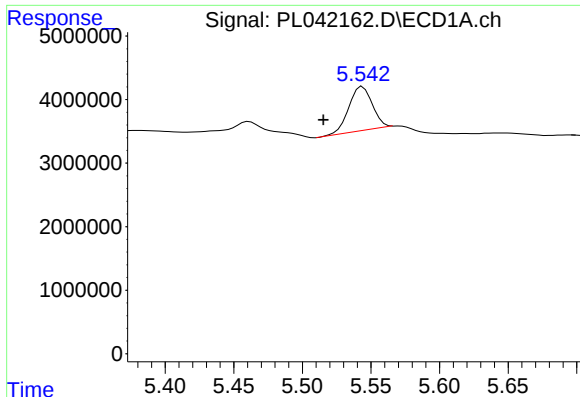

#9 Endosulfan I


R.T.: 5.544 min
Delta R.T.: 0.028 min
Response: 8196281
Conc: 1.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

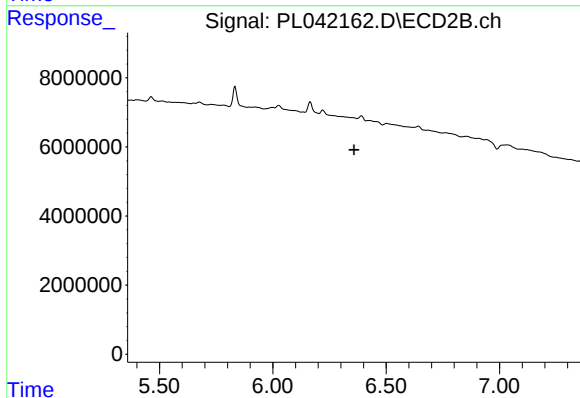


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

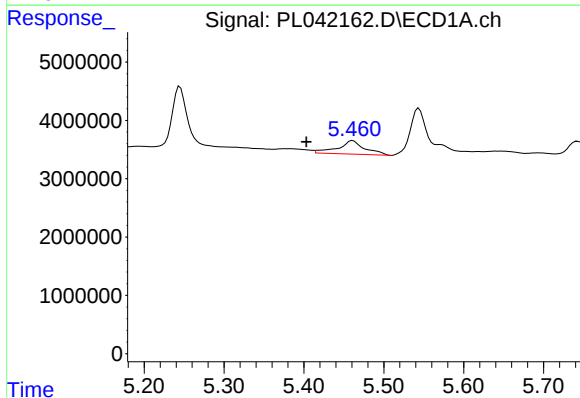


#10 gamma-Chlordane

R.T.: 5.461 min
Delta R.T.: 0.058 min
Response: 5415406
Conc: 0.67 ng/ml

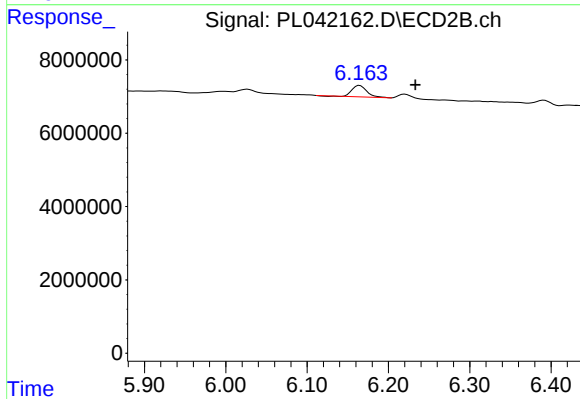

#10 gamma-Chlordane


R.T.: 6.165 min
Delta R.T.: -0.068 min
Response: 3908172
Conc: 1.10 ng/ml

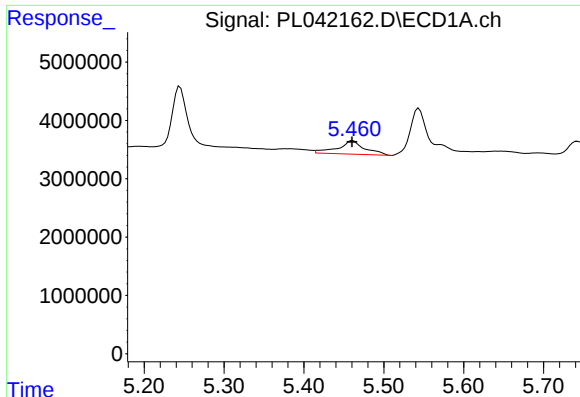

#11 alpha-Chlordane


R.T.: 5.461 min
Delta R.T.: 0.000 min
Response: 5415406
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

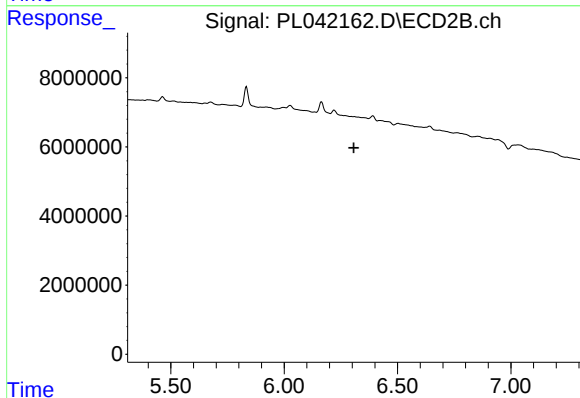


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

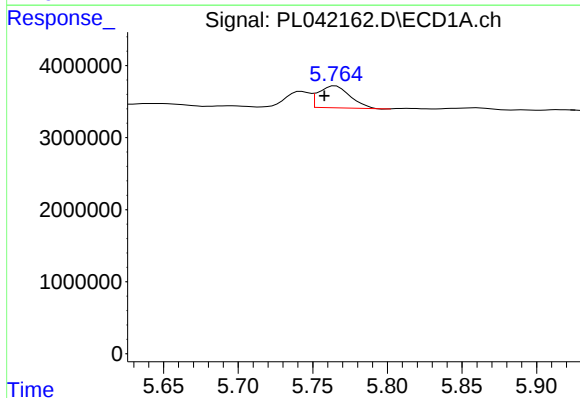


#13 Dieldrin

R.T.: 5.765 min
Delta R.T.: 0.007 min
Response: 4420486
Conc: 0.57 ng/ml

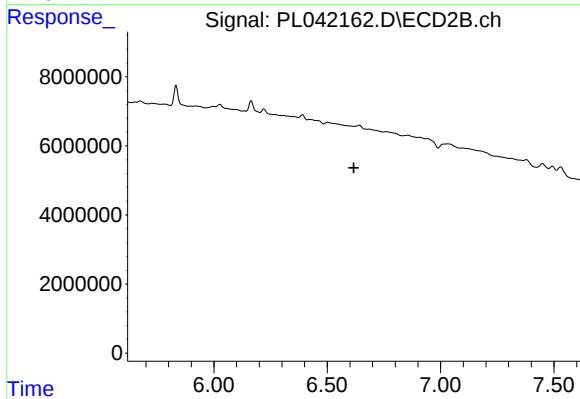

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.617 min
Response: 0
Conc: N.D.

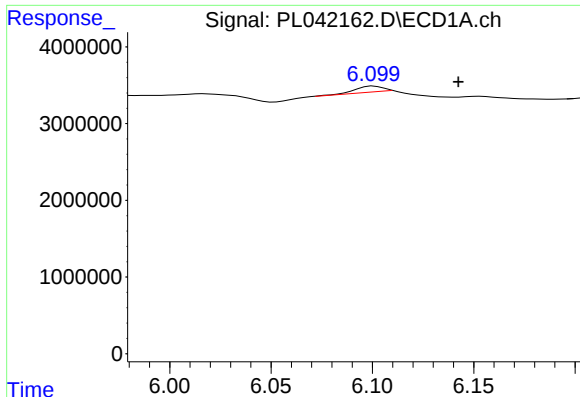

#16 4,4'-DDD


R.T.: 6.101 min
Delta R.T.: -0.042 min
Response: 825180
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

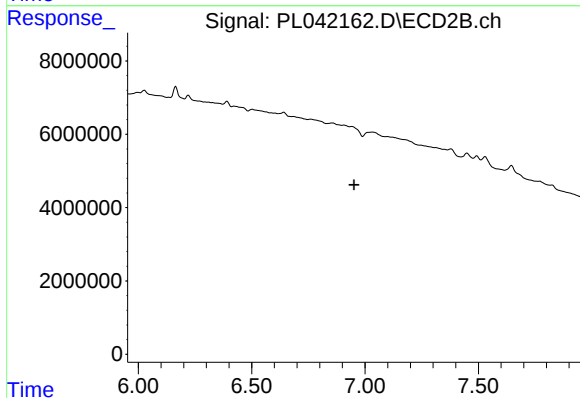


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

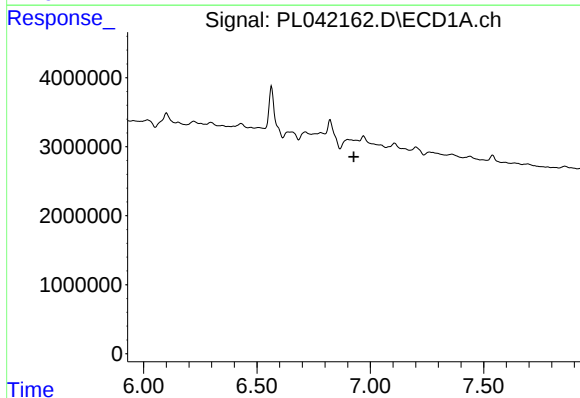


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

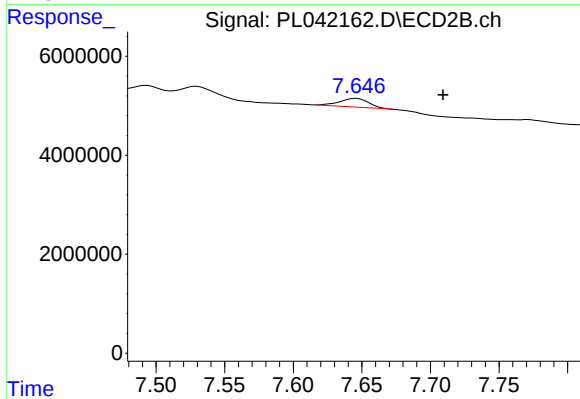

#20 Methoxychlor


R.T.: 7.646 min
Delta R.T.: -0.063 min
Response: 2225426
Conc: 1.62 ng/ml

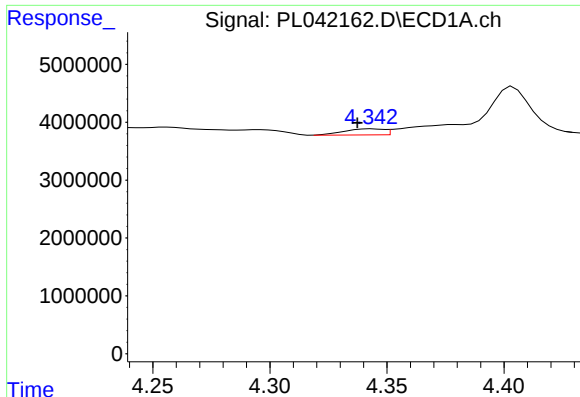

#23 Chlordane-1


R.T.: 4.343 min
Delta R.T.: 0.006 min
Response: 1252816
Conc: 4.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

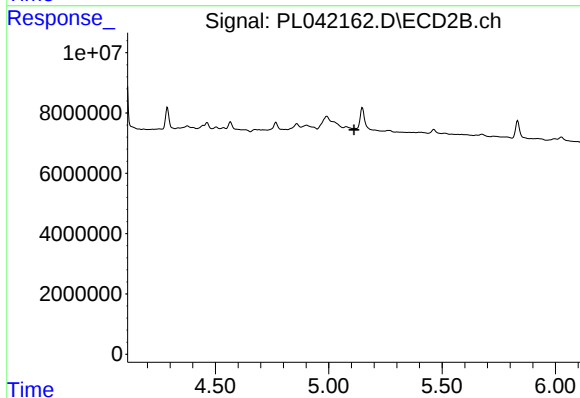


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

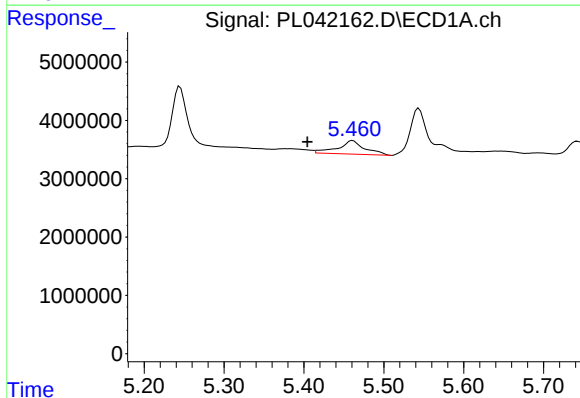


#25 Chlordane-3

R.T.: 5.461 min
Delta R.T.: 0.057 min
Response: 5415406
Conc: 5.79 ng/ml

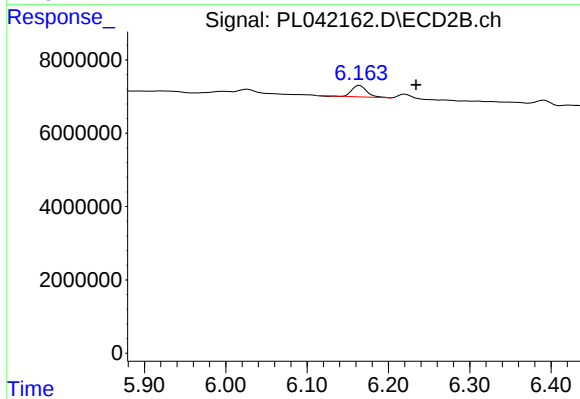

#25 Chlordane-3


R.T.: 6.165 min
Delta R.T.: -0.069 min
Response: 3908172
Conc: 7.65 ng/ml

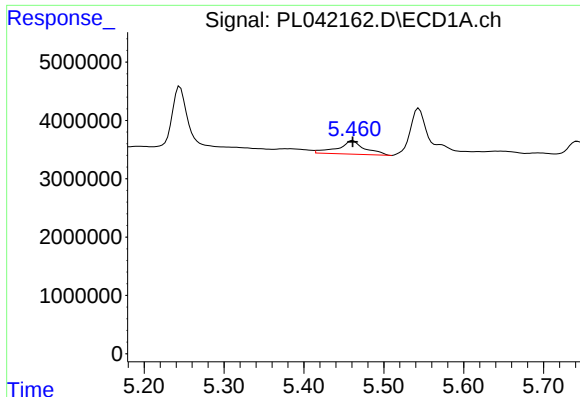

#26 Chlordane-4


R.T.: 5.461 min
Delta R.T.: 0.000 min
Response: 5415406
Conc: 6.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

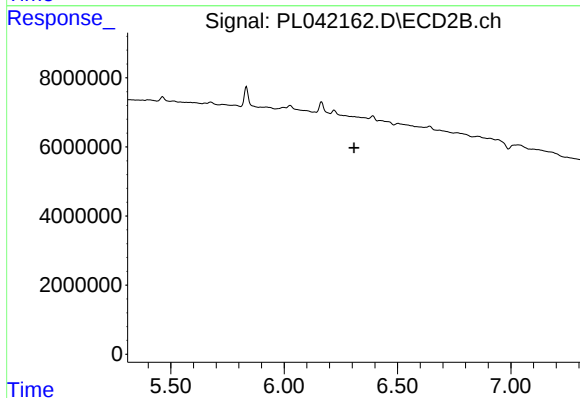


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

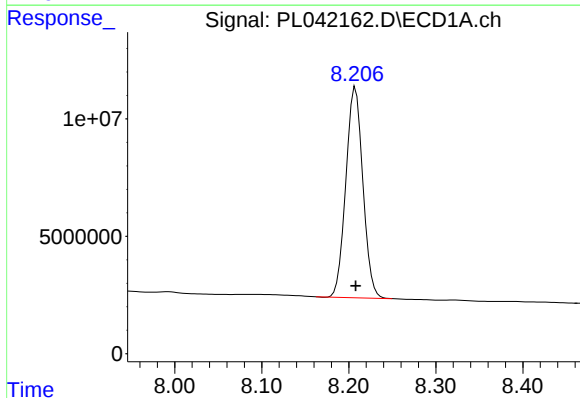

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 121794932
Conc: 17.78 ng/ml

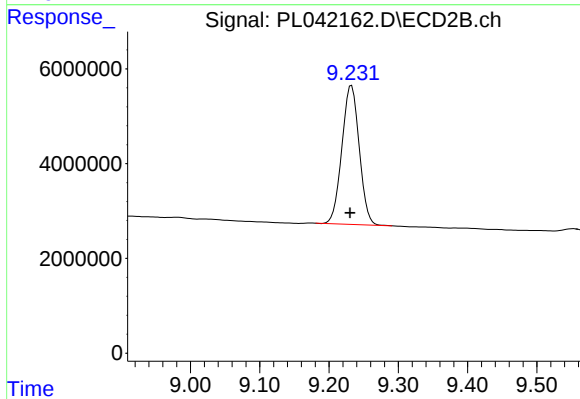

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.002 min
Response: 50906240
Conc: 19.96 ng/ml