

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 03:47
 Operator : AJ\SJ
 Sample : J5910-08
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:45:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	117.1E6	62092564	18.961	20.958
28)	SA Decachlor...	8.207	9.232	130.9E6	54923473	19.116	21.534
Target Compounds							
2)	A alpha-BHC	3.903	4.504	2902384	1207582	0.306	0.272
6)	B beta-BHC	4.405f	0.000	12318167	0	3.338	N.D. #
8)	B Heptachlo...	0.000	5.997	0	2998339	N.D.	0.835 #
9)	A Endosulfan I	5.555f	0.000	4365364	0	0.599	N.D. #
19)	B Endosulfa...	6.655	7.385	9605482	7257170	1.506	2.668 #
20)	A Methoxychlor	0.000	7.648f	0	7454651	N.D.	5.425 #
21)	B Endrin ke...	7.200f	0.000	2493184	0	0.346	N.D. #
23)	Chlordane-1	4.405	0.000	12318167	0	41.275	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 03:47
Operator : AJ\SJ
Sample : J5910-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:45:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

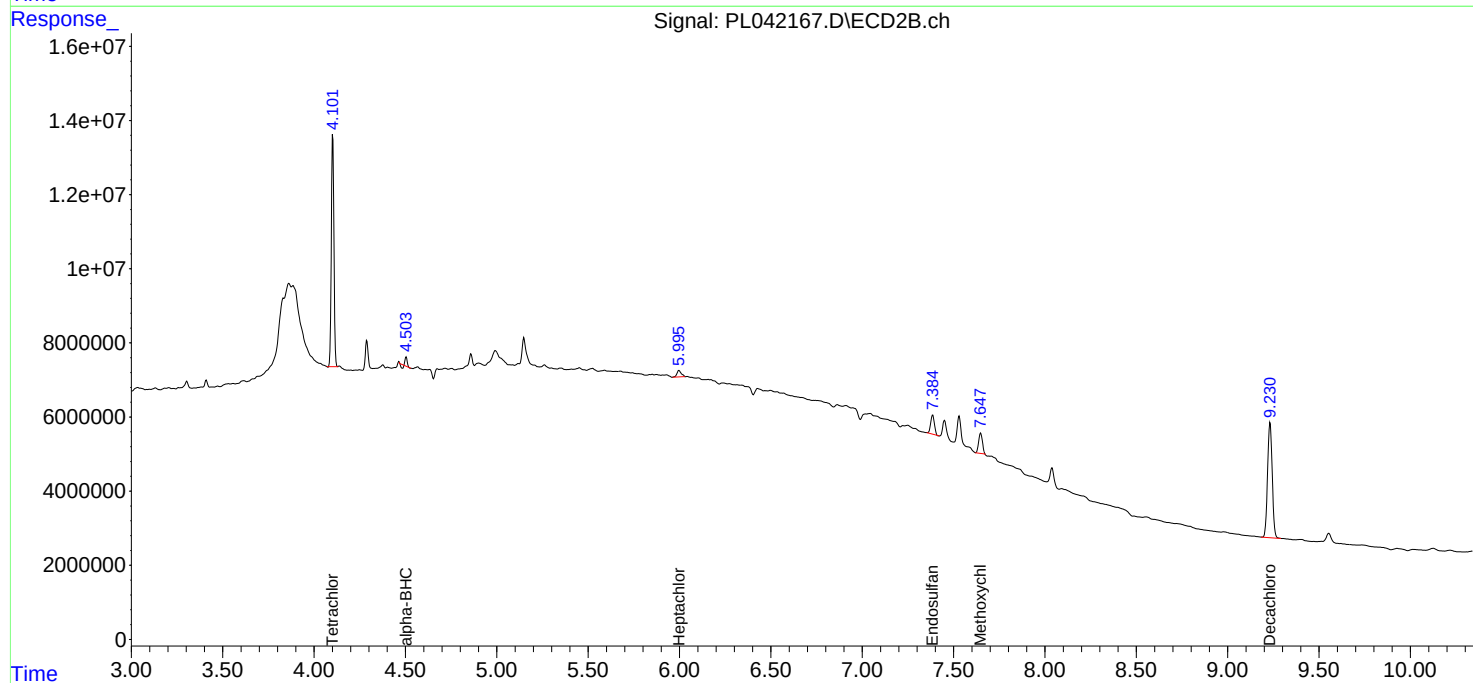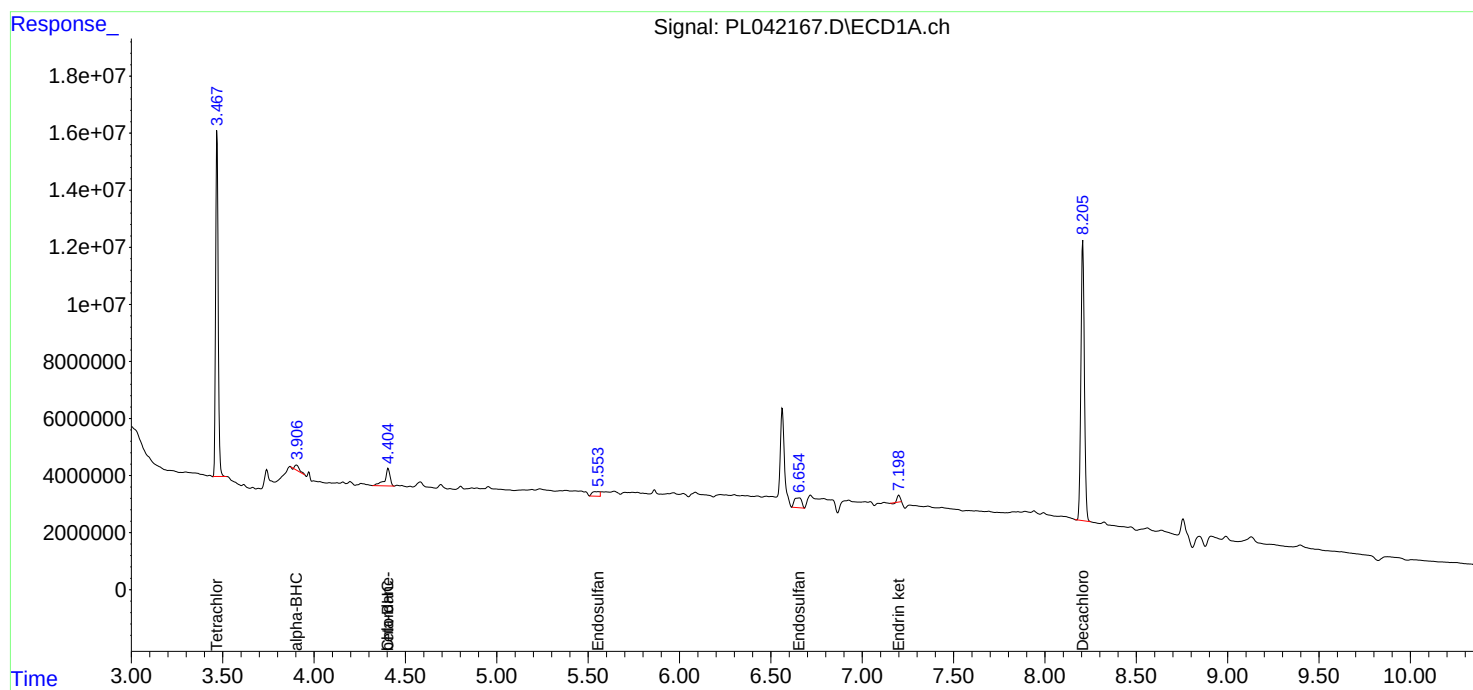


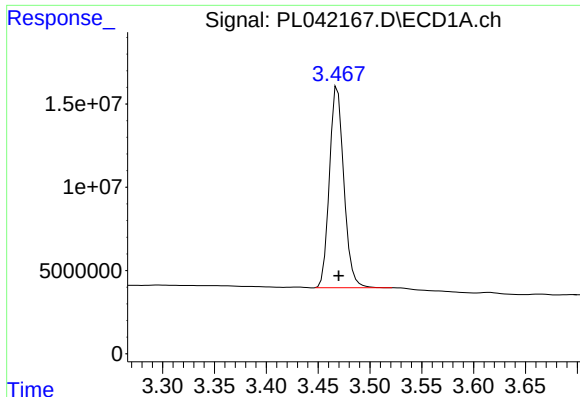

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 117085662
Conc: 18.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

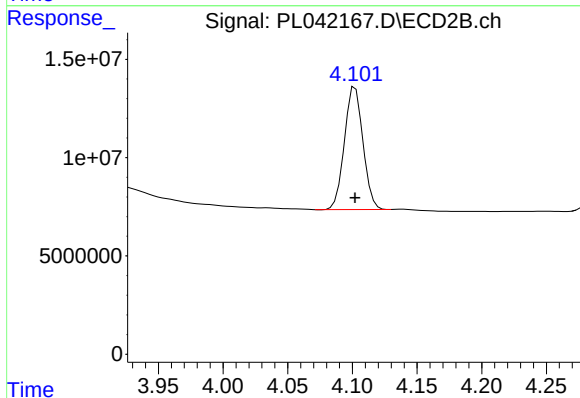


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 62092564
Conc: 20.96 ng/ml

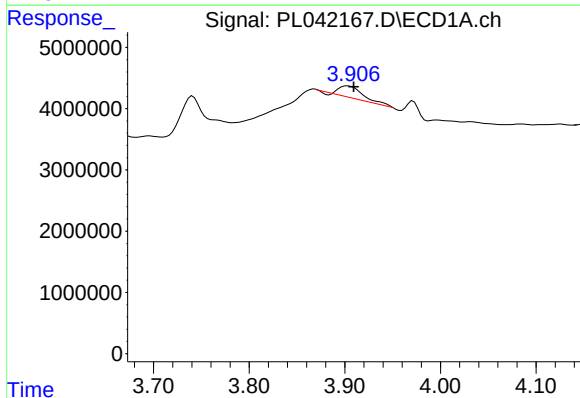


#2 alpha-BHC

R.T.: 3.903 min
Delta R.T.: -0.006 min
Response: 2902384
Conc: 0.31 ng/ml

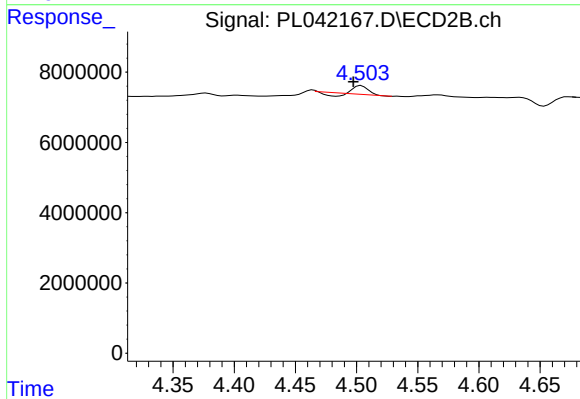

#2 alpha-BHC


R.T.: 4.504 min
Delta R.T.: 0.006 min
Response: 1207582
Conc: 0.27 ng/ml

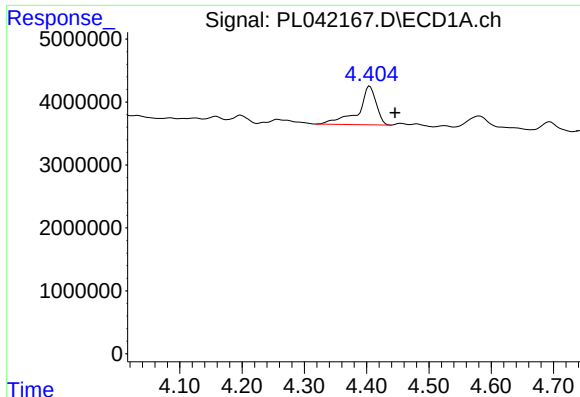

#6 beta-BHC


R.T.: 4.405 min
Delta R.T.: -0.040 min
Response: 12318167
Conc: 3.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

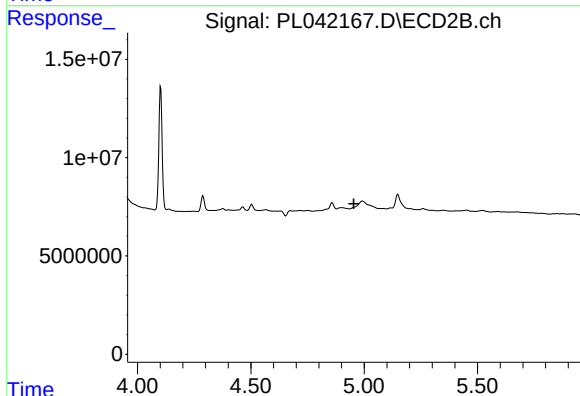


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

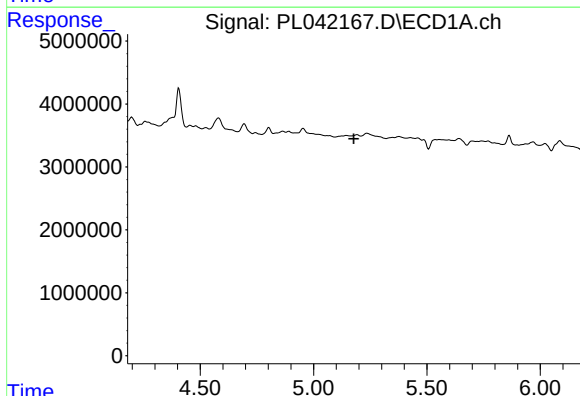


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.178 min
Response: 0
Conc: N.D.

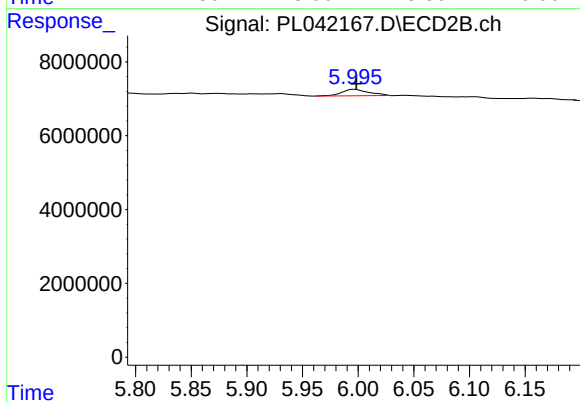

#8 Heptachlor epoxide


R.T.: 5.997 min
Delta R.T.: -0.002 min
Response: 2998339
Conc: 0.83 ng/ml

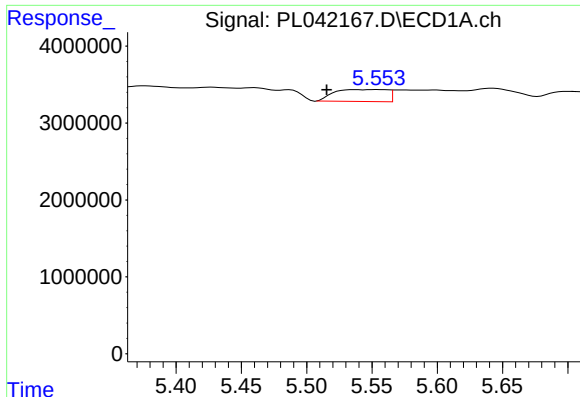

#9 Endosulfan I


R.T.: 5.555 min
Delta R.T.: 0.039 min
Response: 4365364
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

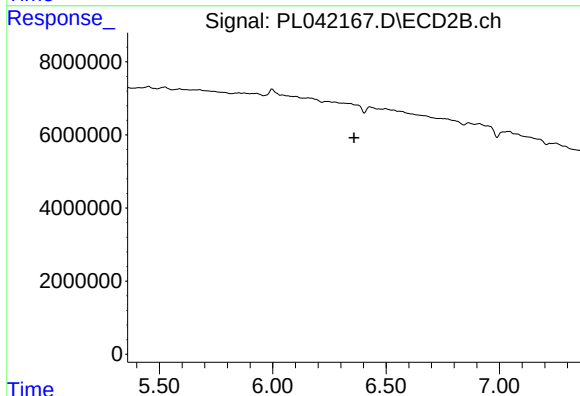


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

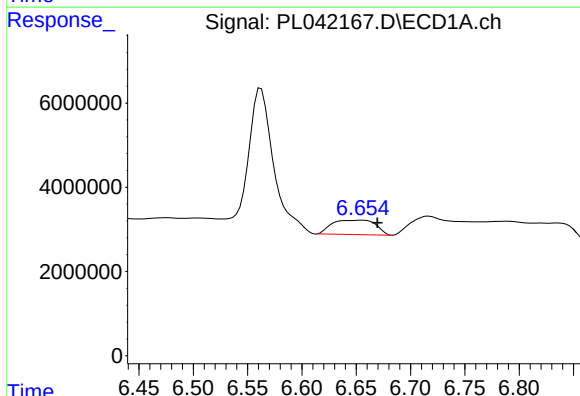


#19 Endosulfan Sulfate

R.T.: 6.655 min
Delta R.T.: -0.014 min
Response: 9605482
Conc: 1.51 ng/ml

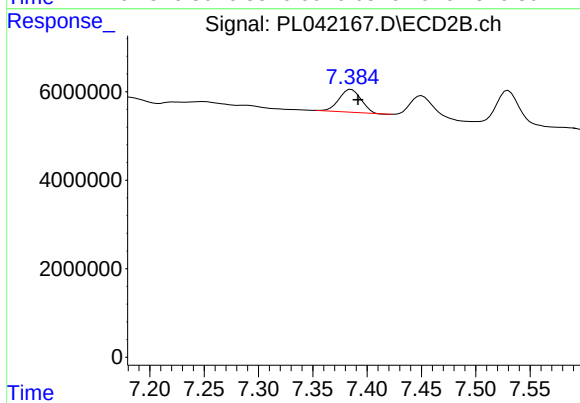

#19 Endosulfan Sulfate


R.T.: 7.385 min
Delta R.T.: -0.006 min
Response: 7257170
Conc: 2.67 ng/ml

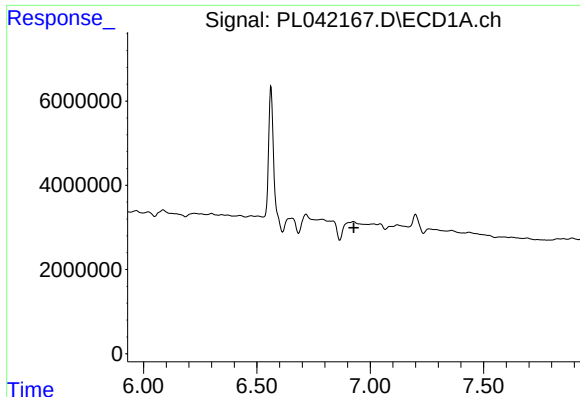

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.928 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

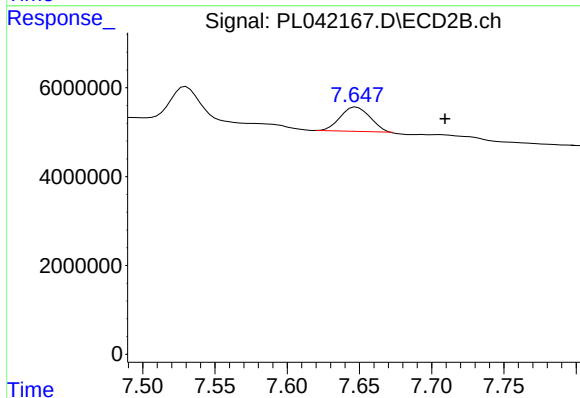


#20 Methoxychlor

R.T.: 7.648 min
Delta R.T.: -0.061 min
Response: 7454651
Conc: 5.43 ng/ml

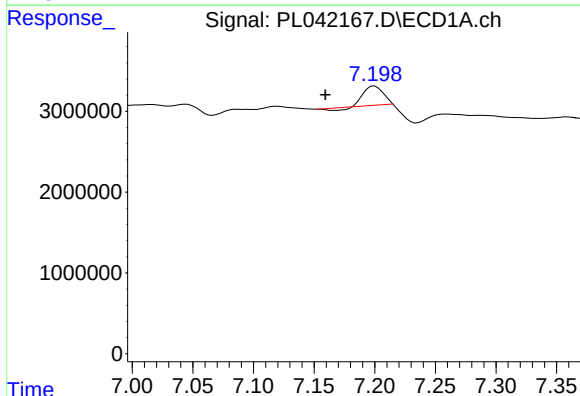


#21 Endrin ketone

R.T.: 7.200 min
Delta R.T.: 0.041 min
Response: 2493184
Conc: 0.35 ng/ml

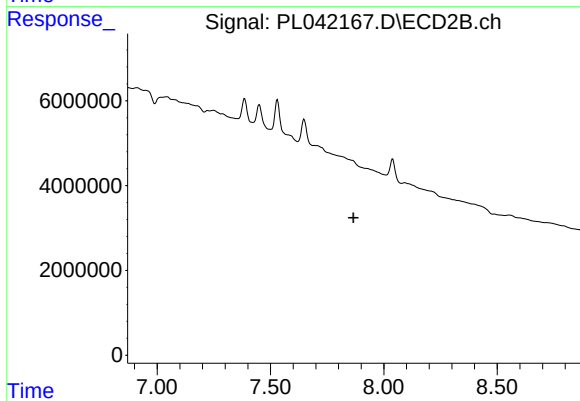

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.867 min
Response: 0
Conc: N.D.

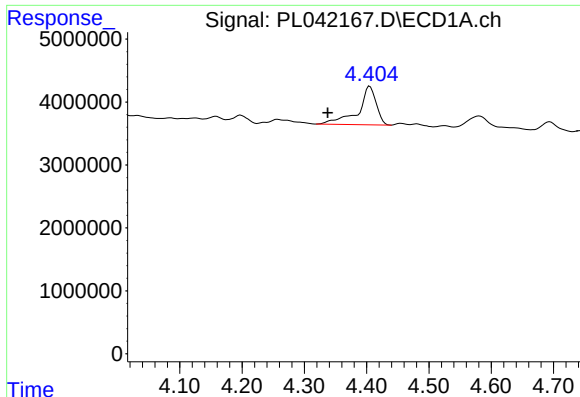

#23 Chlordane-1


R.T.: 4.405 min
Delta R.T.: 0.068 min
Response: 12318167
Conc: 41.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

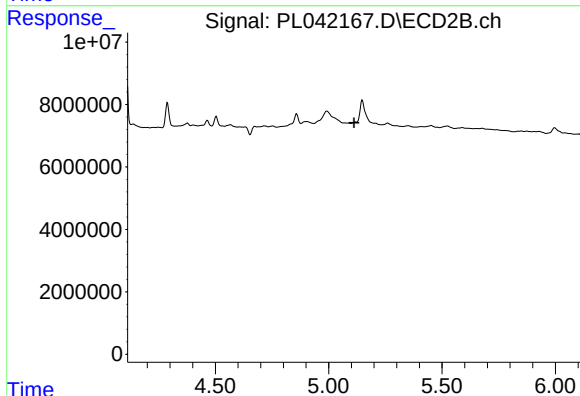


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

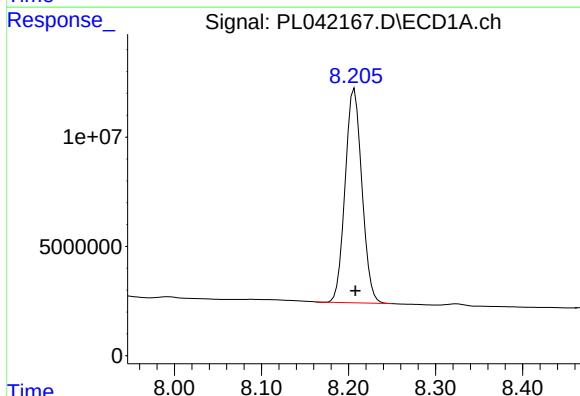

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.001 min
Response: 130948675
Conc: 19.12 ng/ml

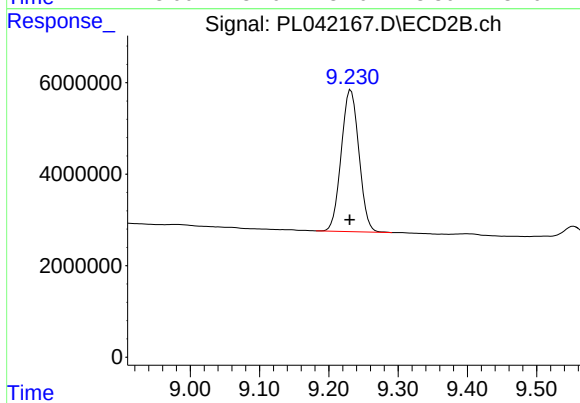

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.001 min
Response: 54923473
Conc: 21.53 ng/ml