

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 04:30
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:47:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	132.3E6	68921313	21.420	23.263
28)	SA Decachlor...	8.207	9.233	139.4E6	57675191	20.356	22.613
Target Compounds							
6)	B beta-BHC	4.402f	0.000	3167558	0	0.858	N.D. #
8)	B Heptachlo...	0.000	5.996	0	2063980	N.D.	0.575 #
23)	Chlordane-1	4.365	0.000	1471053	0	4.929	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 04:30
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:47:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

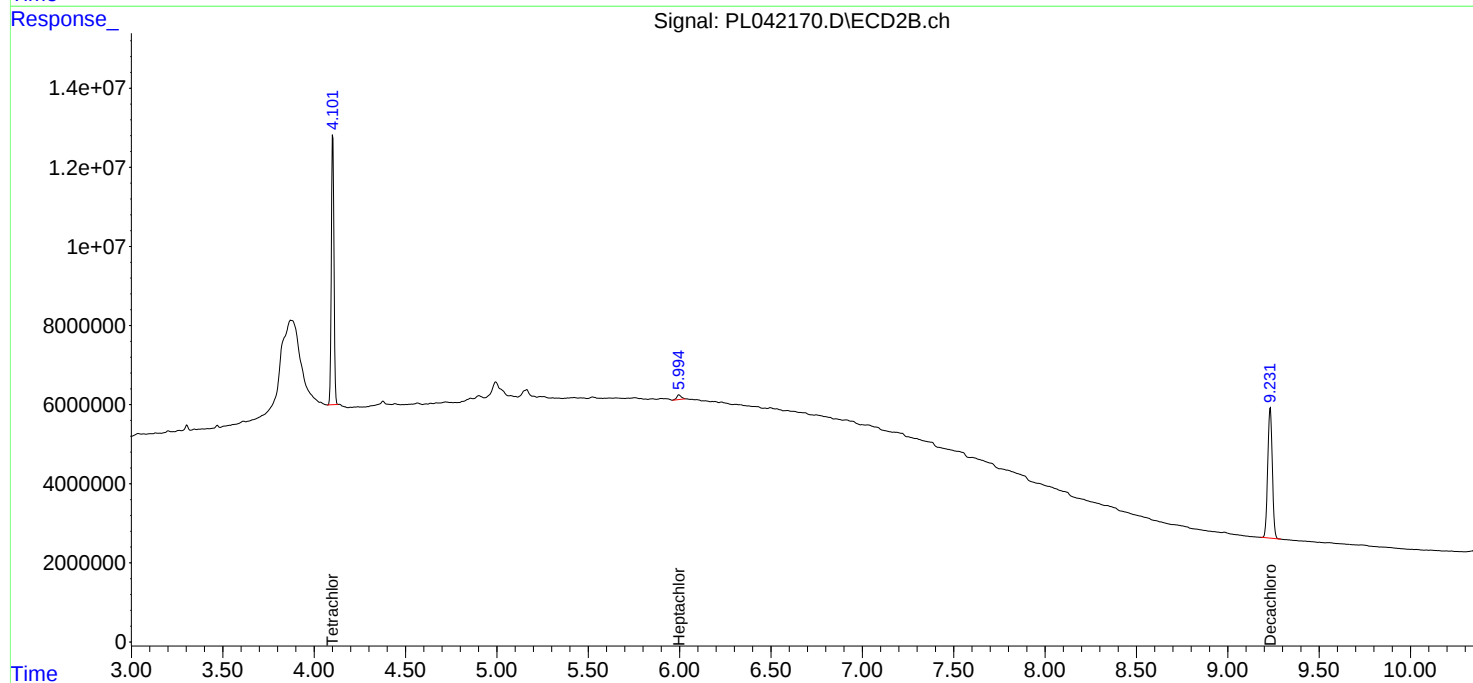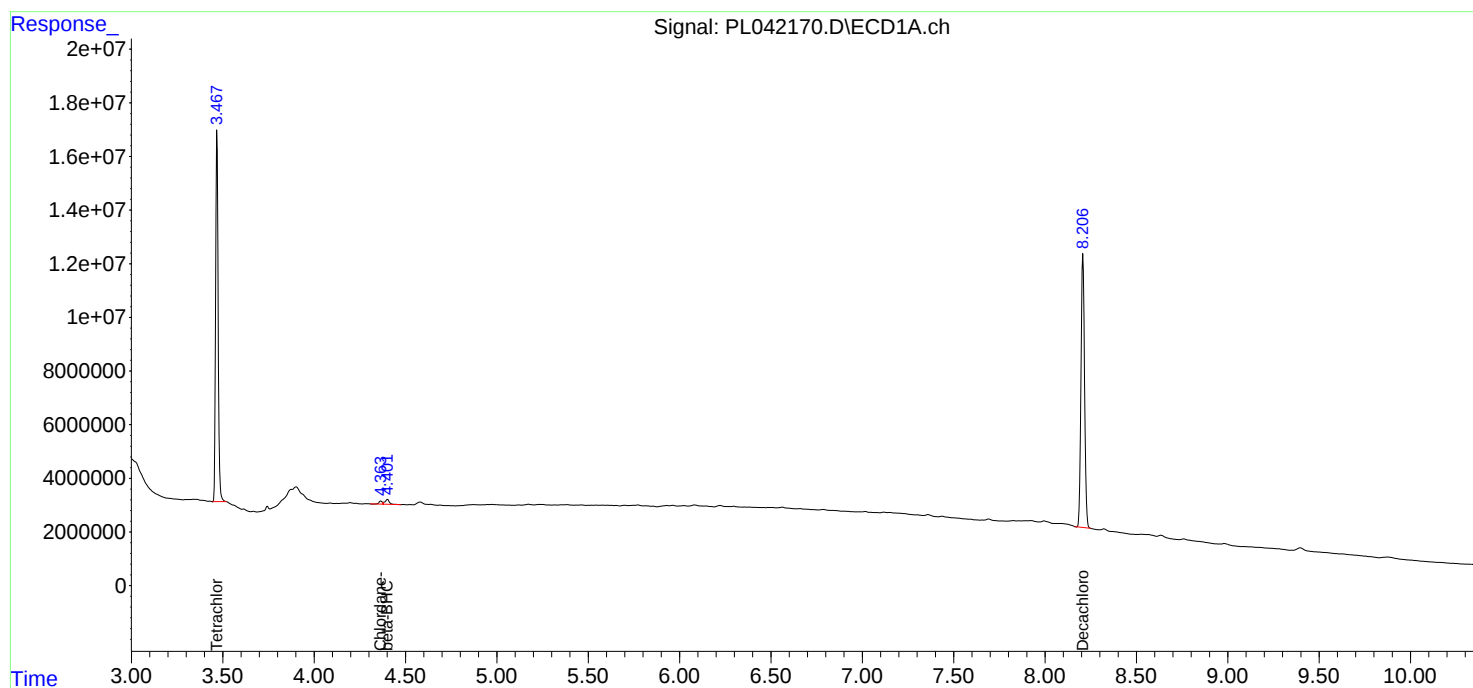


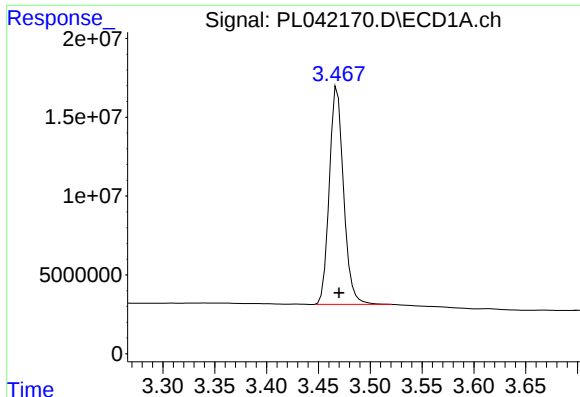

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: -0.002 min
Response: 132269521
Conc: 21.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

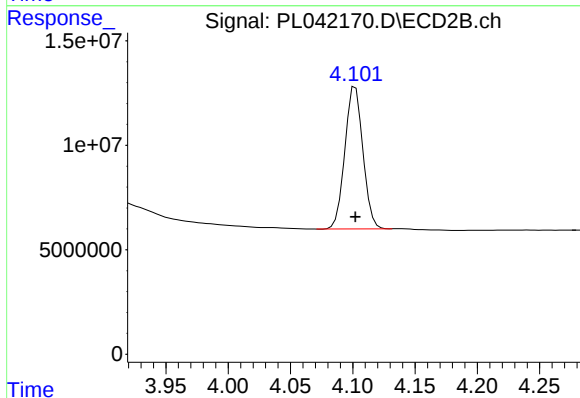


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 68921313
Conc: 23.26 ng/ml

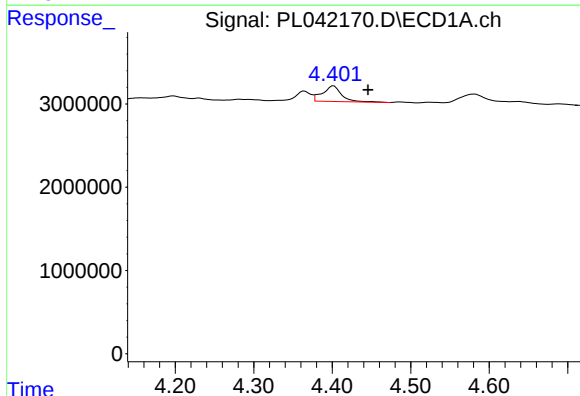


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.044 min
Response: 3167558
Conc: 0.86 ng/ml

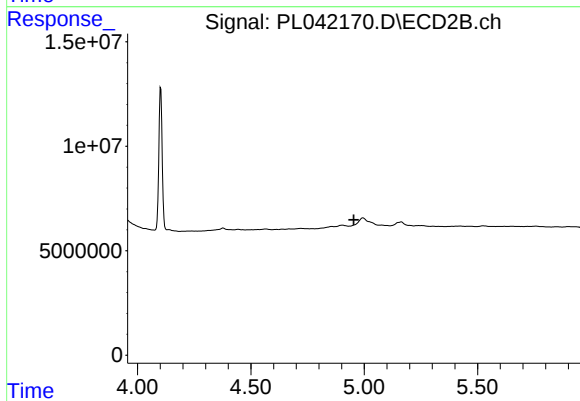

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

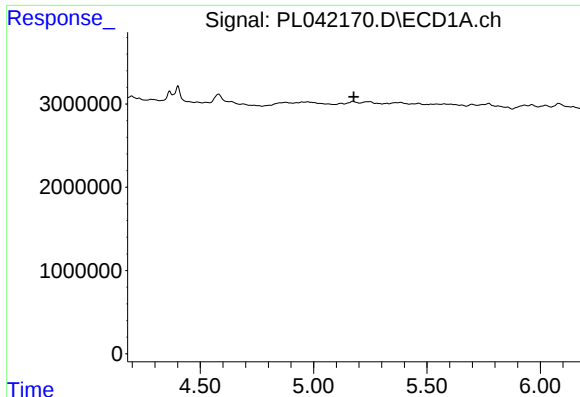

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

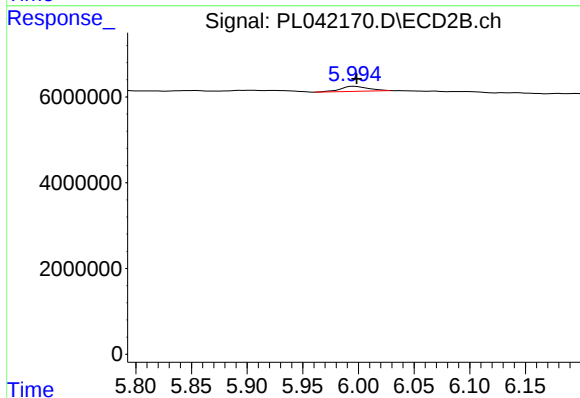


#8 Heptachlor epoxide

R.T.: 5.996 min
Delta R.T.: -0.002 min
Response: 2063980
Conc: 0.57 ng/ml

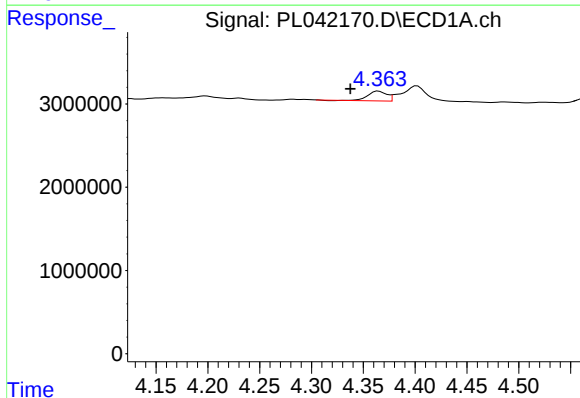


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.027 min
Response: 1471053
Conc: 4.93 ng/ml

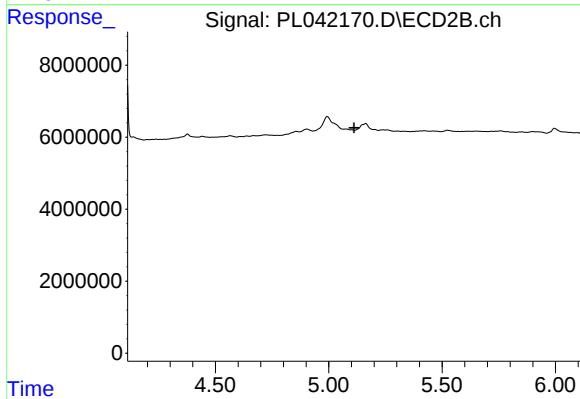

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.112 min
Response: 0
Conc: N.D.

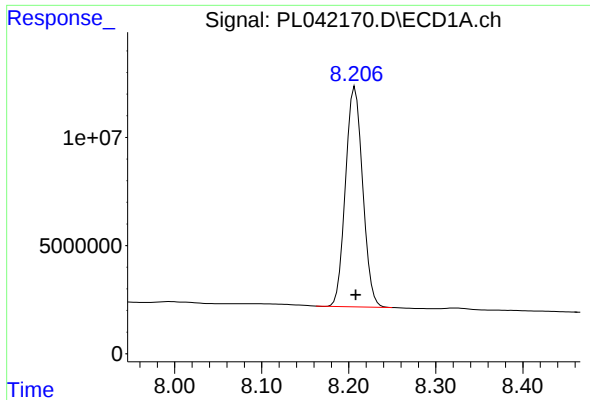

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 139446635
Conc: 20.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

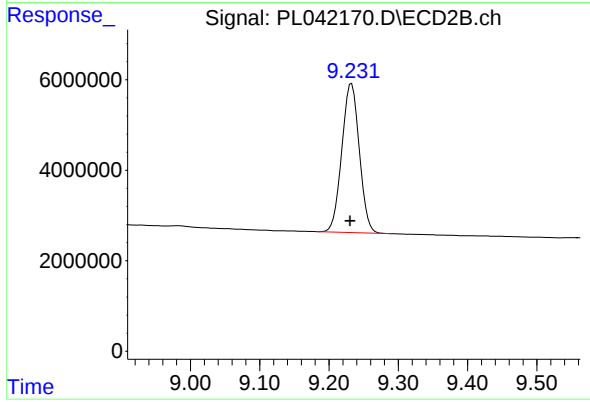

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 57675191
Conc: 22.61 ng/ml