

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
 Data File : PL042172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 04:58
 Operator : AJ\SJ
 Sample : PB114780BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 05:47:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	129.6E6	68373290	20.980	23.078
28)	SA Decachlor...	8.206	9.232	142.0E6	59176284	20.722	23.201
Target Compounds							
2)	A alpha-BHC	3.904	4.504	3145563	10986518	0.332	2.475 #
3)	MA gamma-BHC...	0.000	4.742f	0	16606127	N.D.	4.027 #
6)	B beta-BHC	4.413f	0.000	8223851	0	2.228	N.D. #
19)	B Endosulfa...	6.656	7.386	11143141	18239131	1.747	6.706 #
20)	A Methoxychlor	0.000	7.648f	0	18698372	N.D.	13.608 #
21)	B Endrin ke...	7.198f	0.000	8476614	0	1.176	N.D. #
23)	Chlordane-1	4.365	5.115	1760830	390381	5.900	2.711 #
24)	Chlordane-2	4.803	0.000	2702855	0	8.520	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111418\
Data File : PL042172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 04:58
Operator : AJ\SJ
Sample : PB114780BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 05:47:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

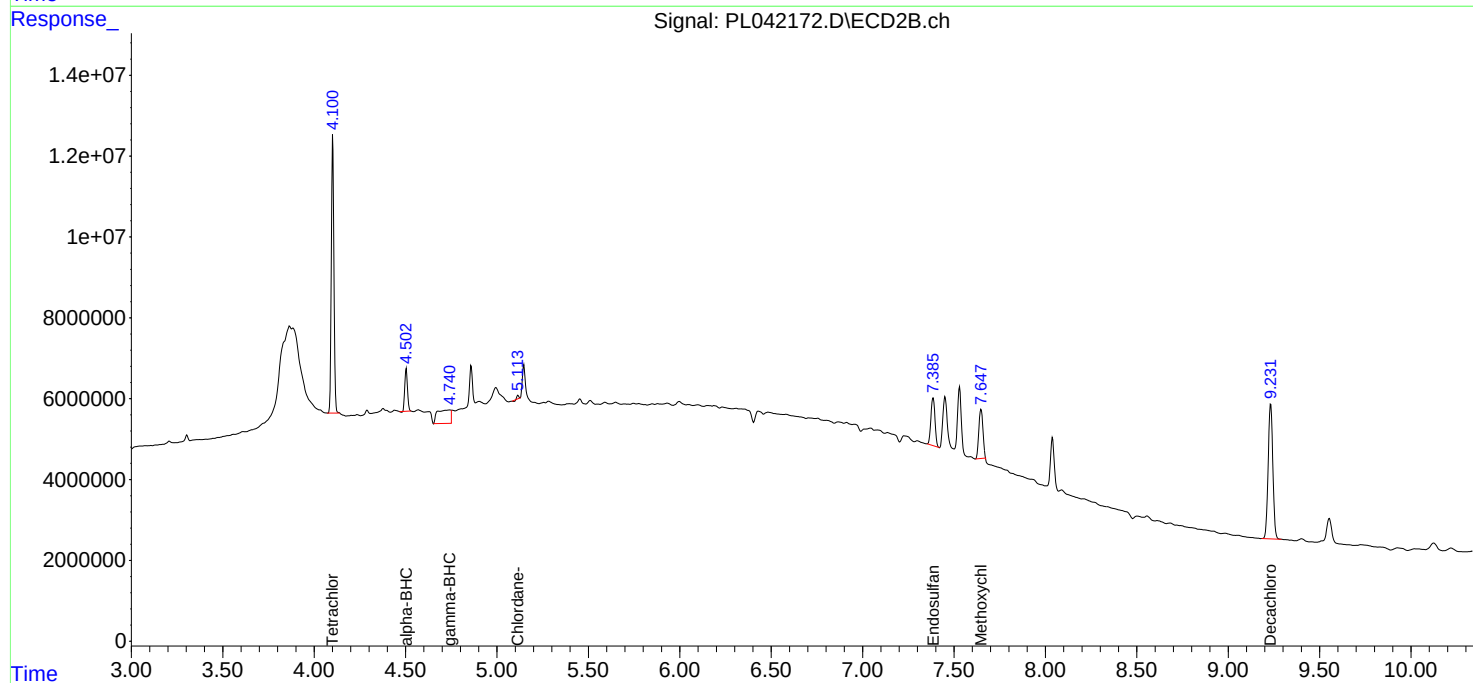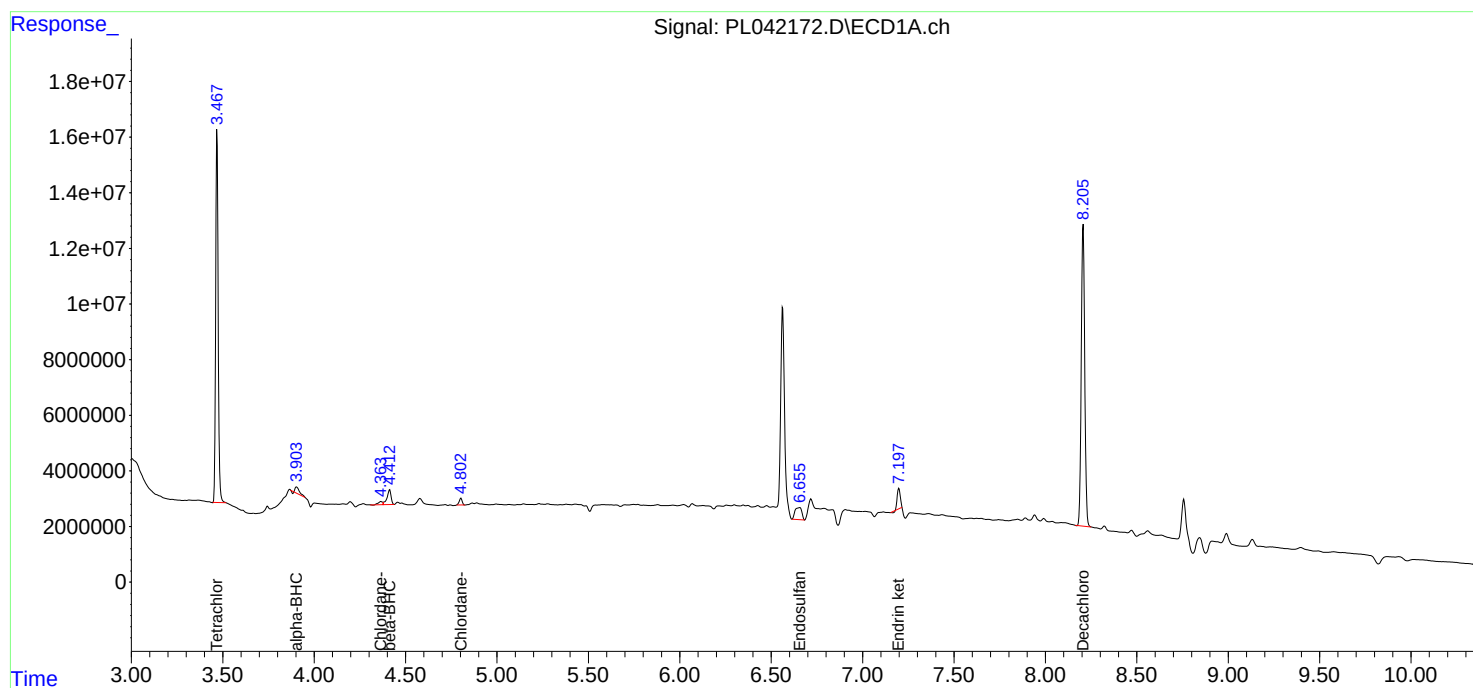


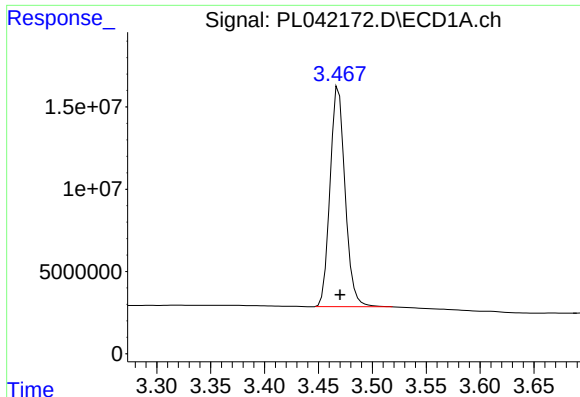

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 129550895
Conc: 20.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

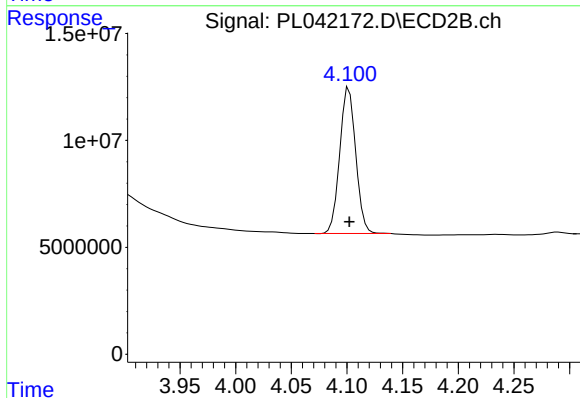


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 68373290
Conc: 23.08 ng/ml

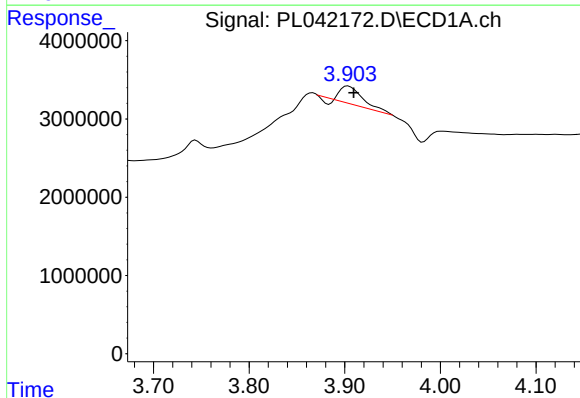


#2 alpha-BHC

R.T.: 3.904 min
Delta R.T.: -0.006 min
Response: 3145563
Conc: 0.33 ng/ml

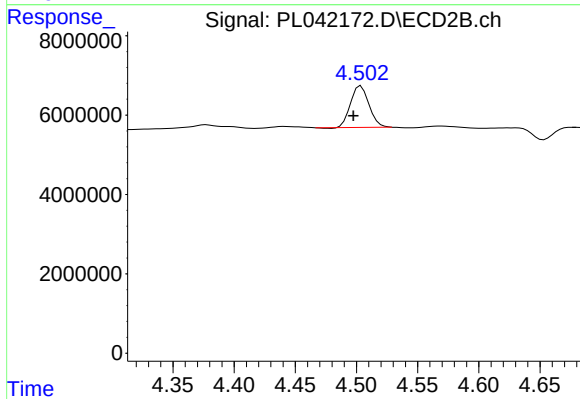

#2 alpha-BHC


R.T.: 4.504 min
Delta R.T.: 0.006 min
Response: 10986518
Conc: 2.47 ng/ml

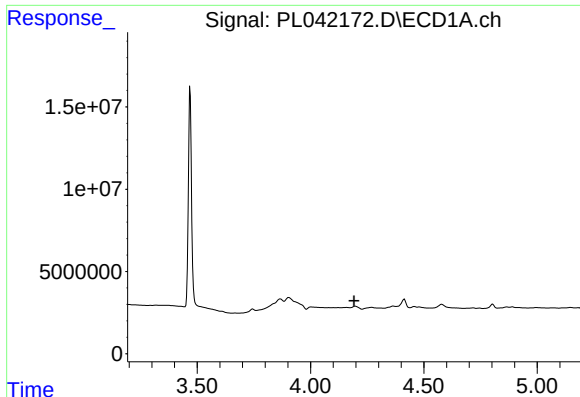

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

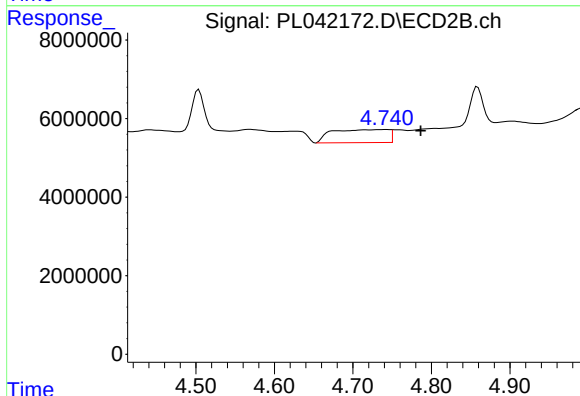


#3 gamma-BHC (Lindane)

R.T.: 4.742 min
Delta R.T.: -0.045 min
Response: 16606127
Conc: 4.03 ng/ml

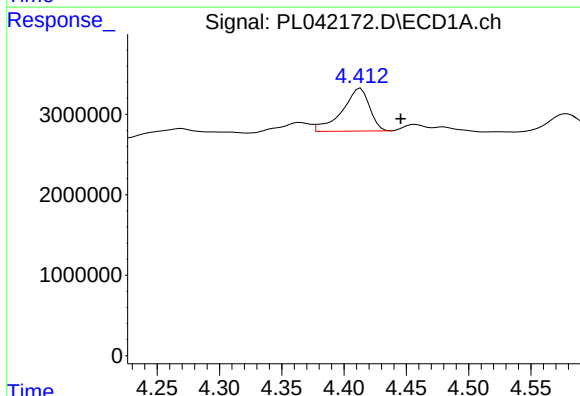


#6 beta-BHC

R.T.: 4.413 min
Delta R.T.: -0.032 min
Response: 8223851
Conc: 2.23 ng/ml

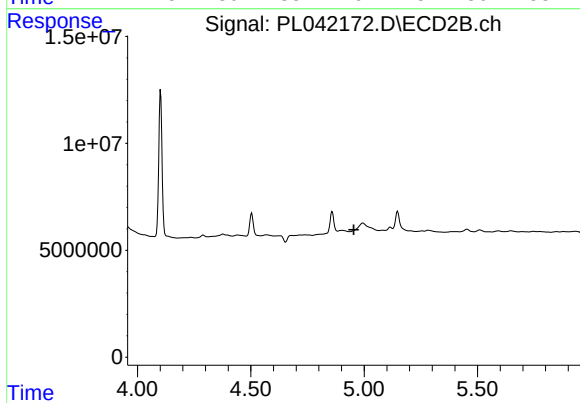

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.954 min
Response: 0
Conc: N.D.

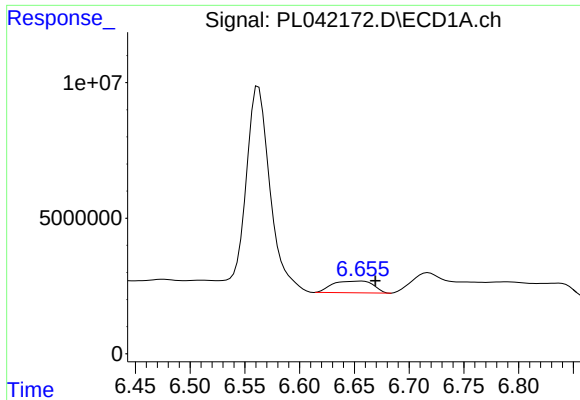

#19 Endosulfan Sulfate


R.T.: 6.656 min
Delta R.T.: -0.013 min
Response: 11143141
Conc: 1.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

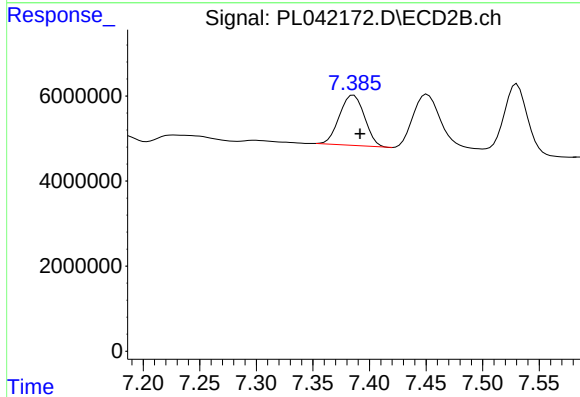


#19 Endosulfan Sulfate

R.T.: 7.386 min
Delta R.T.: -0.006 min
Response: 18239131
Conc: 6.71 ng/ml

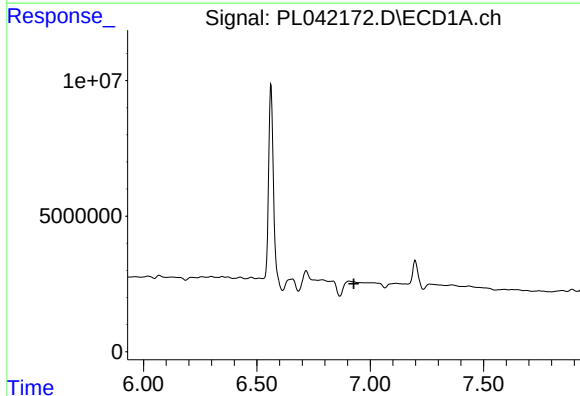


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

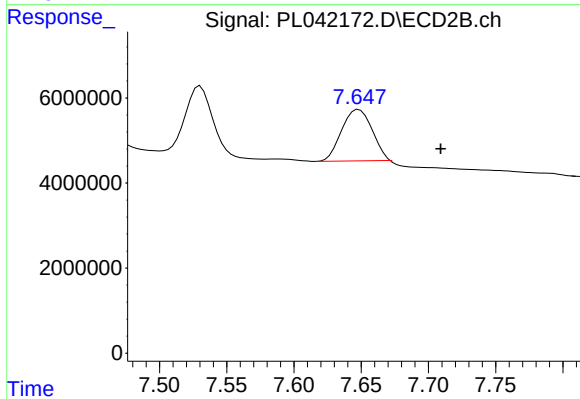

#20 Methoxychlor


R.T.: 7.648 min
Delta R.T.: -0.061 min
Response: 18698372
Conc: 13.61 ng/ml

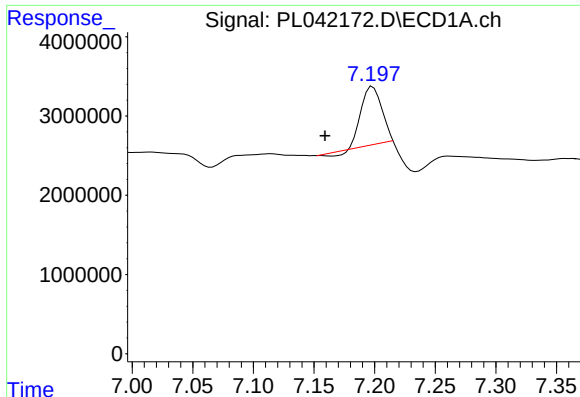

#21 Endrin ketone


R.T.: 7.198 min
Delta R.T.: 0.039 min
Response: 8476614
Conc: 1.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

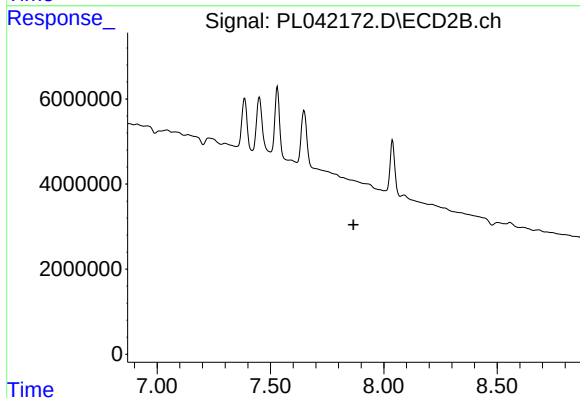


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.867 min
Response: 0
Conc: N.D.

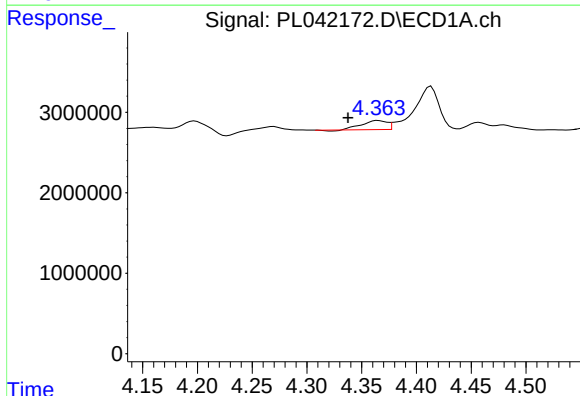


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.027 min
Response: 1760830
Conc: 5.90 ng/ml

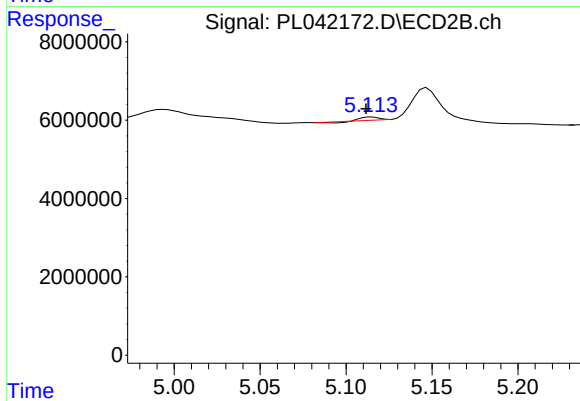

#23 Chlordane-1


R.T.: 5.115 min
Delta R.T.: 0.003 min
Response: 390381
Conc: 2.71 ng/ml

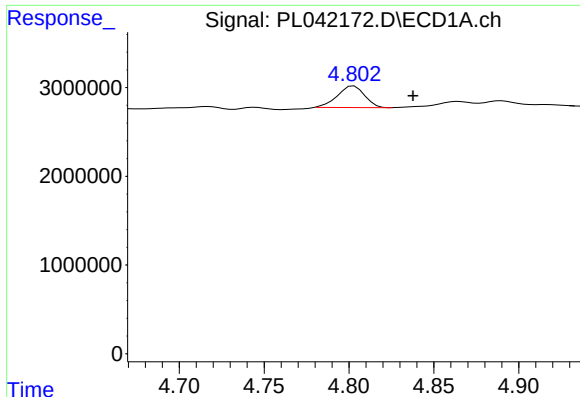

#24 Chlordane-2


R.T.: 4.803 min
Delta R.T.: -0.035 min
Response: 2702855
Conc: 8.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

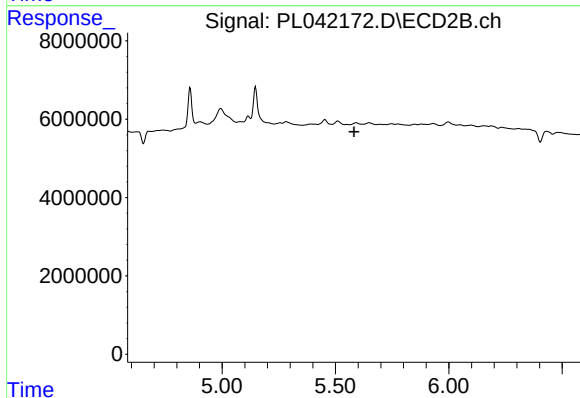


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.583 min
Response: 0
Conc: N.D.

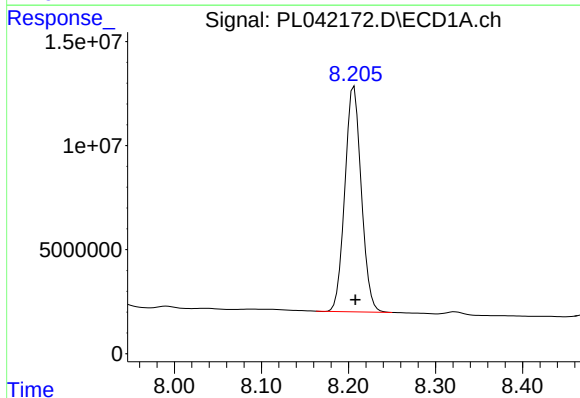

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.002 min
Response: 141952992
Conc: 20.72 ng/ml

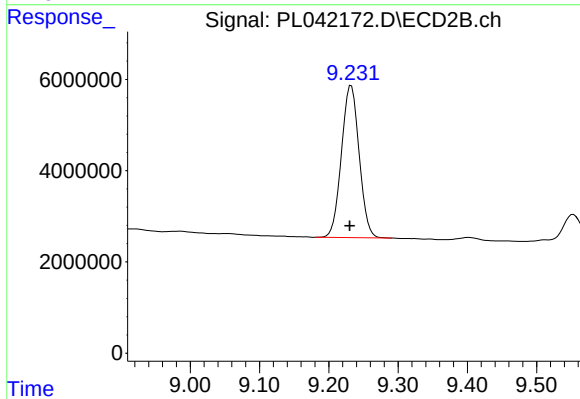

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.002 min
Response: 59176284
Conc: 23.20 ng/ml