

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111419\
 Data File : PL054233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2019 08:47
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:33:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	9.128	0	4780628	N.D.	1.698 #
Target Compounds							
6)	B beta-BHC	4.549f	0.000	7534570	0	1.143	N.D. #
7)	B delta-BHC	4.735	0.000	996257	0	0.065	N.D. #
8)	B Heptachlo...	5.255f	0.000	79123369	0	5.861	N.D. #
9)	A Endosulfan I	5.628	0.000	16155487	0	1.314	N.D. #
11)	B alpha-Chl...	5.543f	0.000	26796661	0	2.014	N.D. #
12)	B 4,4'-DDE	5.746f	0.000	4810109	0	0.405	N.D. #
14)	MA Endrin	6.129	0.000	20833576	0	1.797	N.D. #
17)	MA 4,4'-DDT	6.518f	0.000	14543421	0	1.468	N.D. #
24)	Chlordane-2	4.923	0.000	4464661	0	11.587	N.D. #
26)	Chlordane-4	5.543f	0.000	26796661	0	28.585	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111419\
Data File : PL054233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2019 08:47
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:33:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

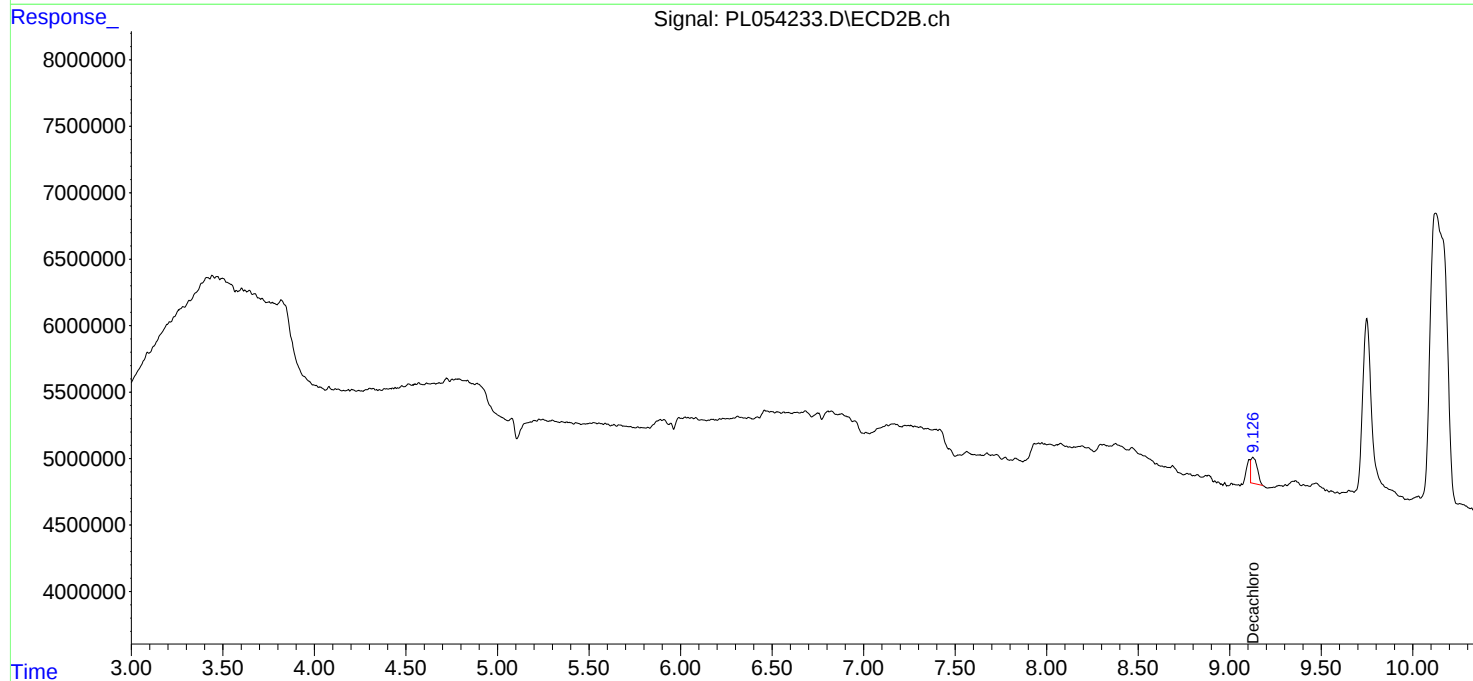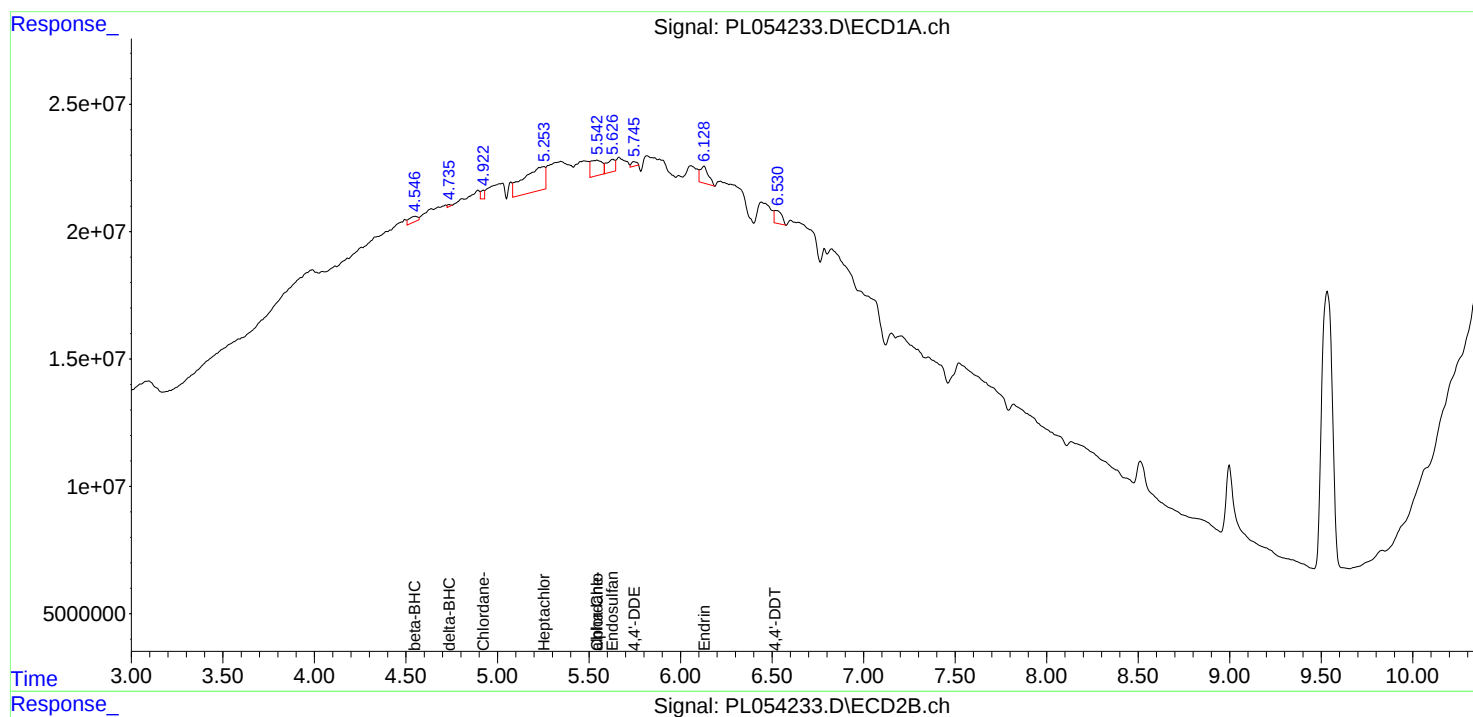


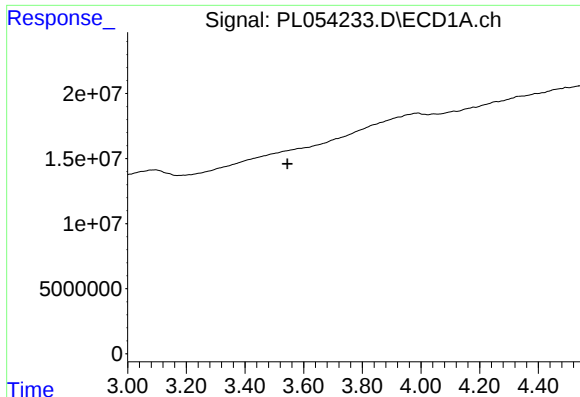

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.544 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

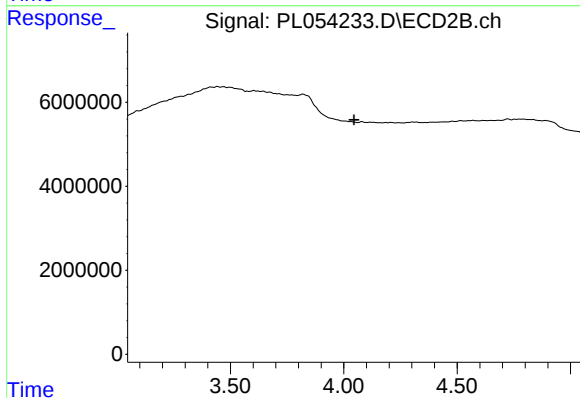


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.046 min
Response: 0
Conc: N.D.

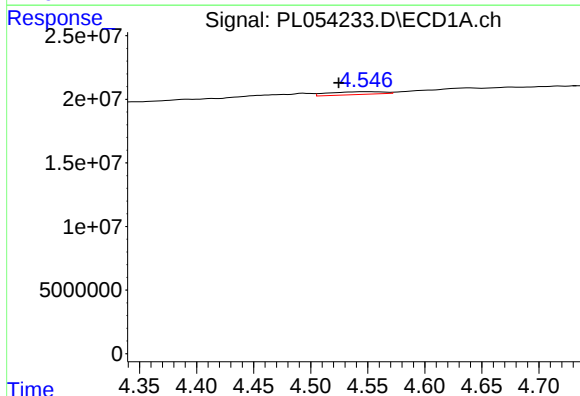


#6 beta-BHC

R.T.: 4.549 min
Delta R.T.: 0.025 min
Response: 7534570
Conc: 1.14 ng/ml

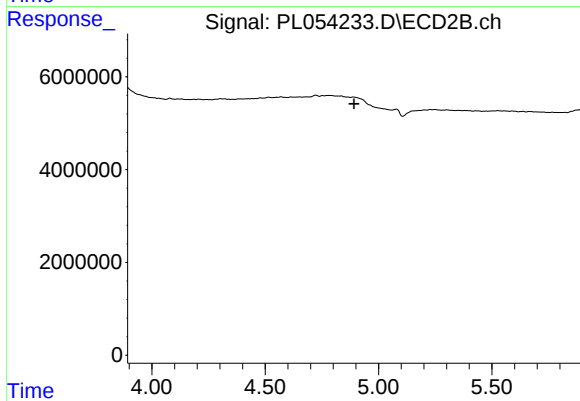

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

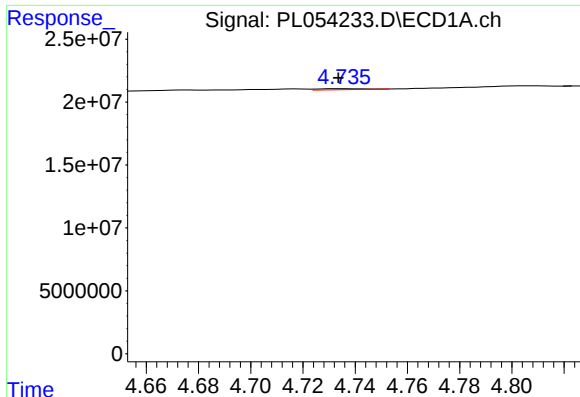

#7 delta-BHC


R.T.: 4.735 min
Delta R.T.: 0.002 min
Response: 996257
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

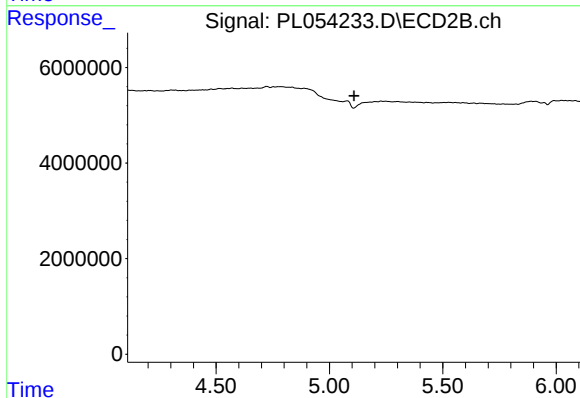


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

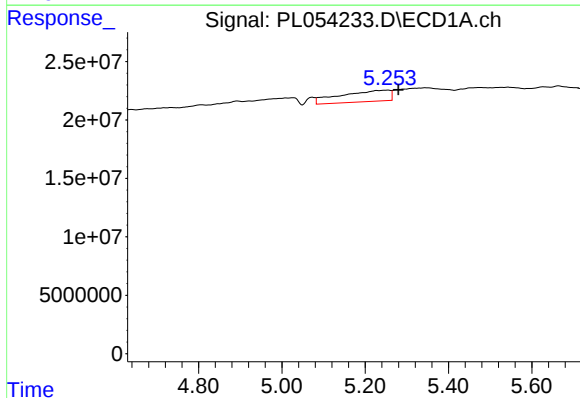


#8 Heptachlor epoxide

R.T.: 5.255 min
Delta R.T.: -0.025 min
Response: 79123369
Conc: 5.86 ng/ml

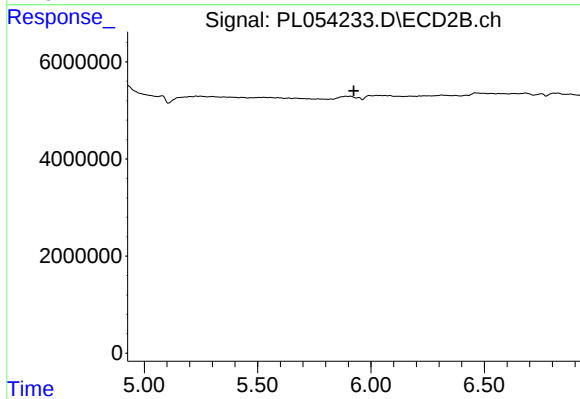

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

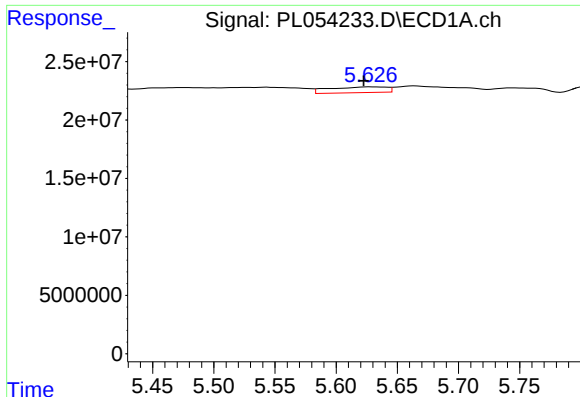

#9 Endosulfan I


R.T.: 5.628 min
Delta R.T.: 0.005 min
Response: 16155487
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

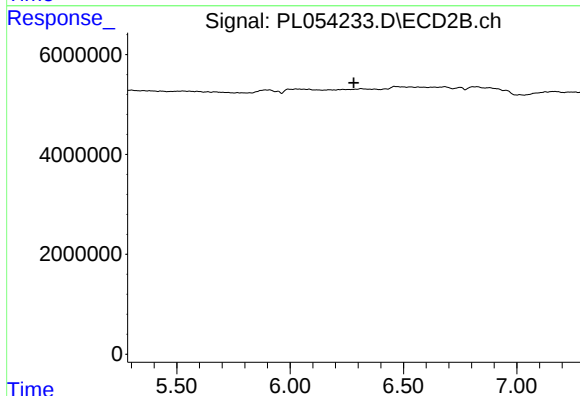


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

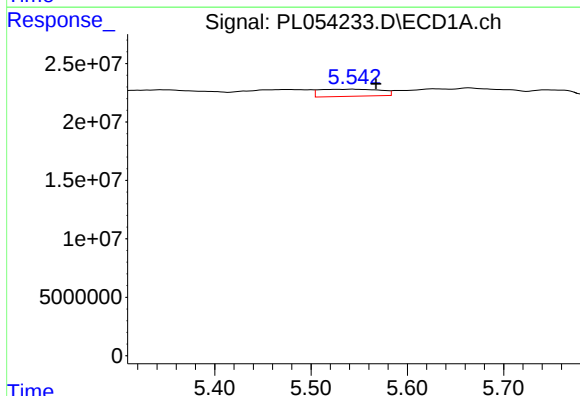


#11 alpha-Chlordane

R.T.: 5.543 min
Delta R.T.: -0.024 min
Response: 26796661
Conc: 2.01 ng/ml

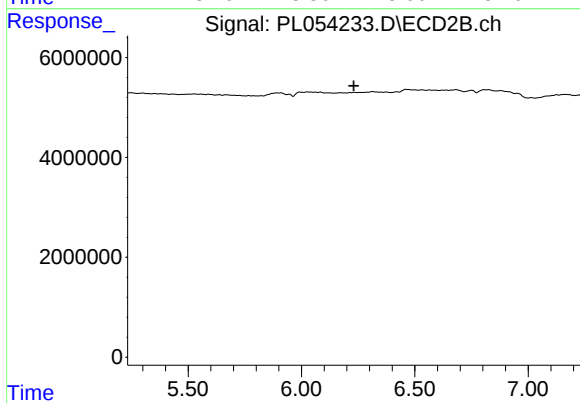

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

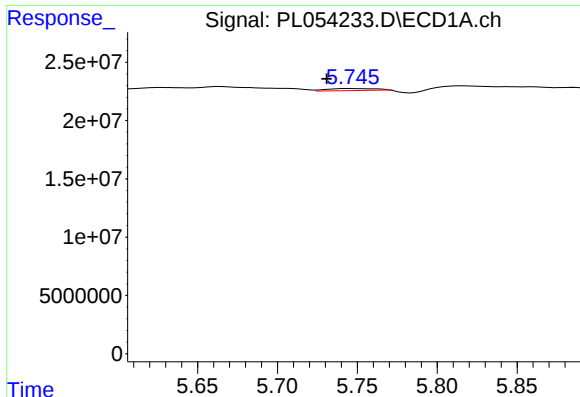

#12 4,4'-DDE


R.T.: 5.746 min
Delta R.T.: 0.015 min
Response: 4810109
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

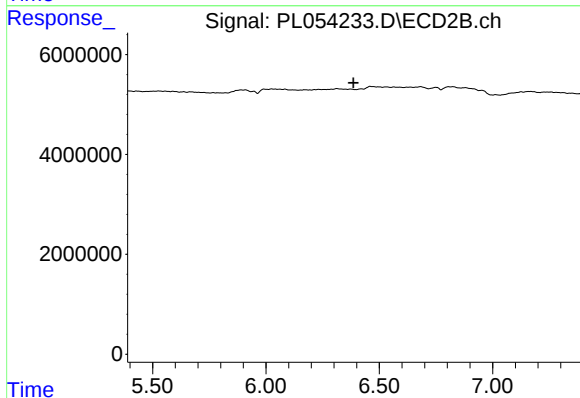


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

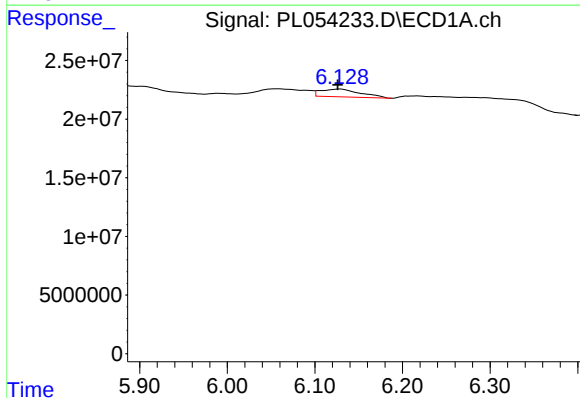


#14 Endrin

R.T.: 6.129 min
Delta R.T.: 0.003 min
Response: 20833576
Conc: 1.80 ng/ml

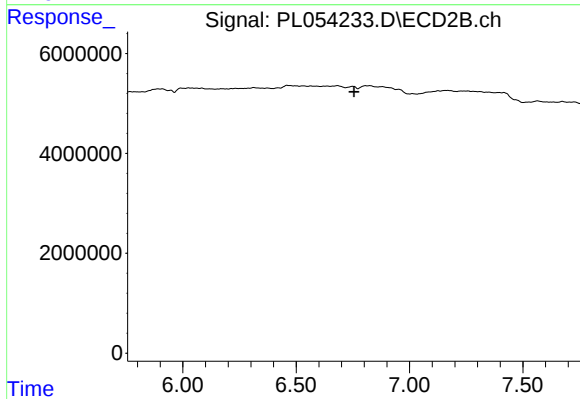

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.756 min
Response: 0
Conc: N.D.

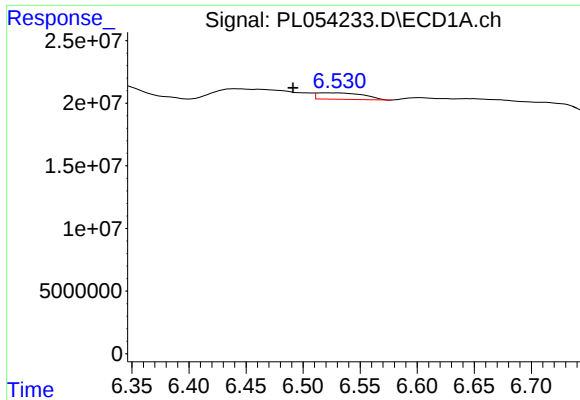

#17 4,4'-DDT


R.T.: 6.518 min
Delta R.T.: 0.027 min
Response: 14543421
Conc: 1.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

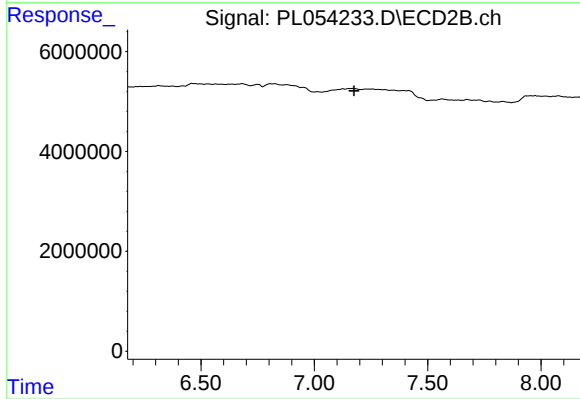


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.176 min
Response: 0
Conc: N.D.

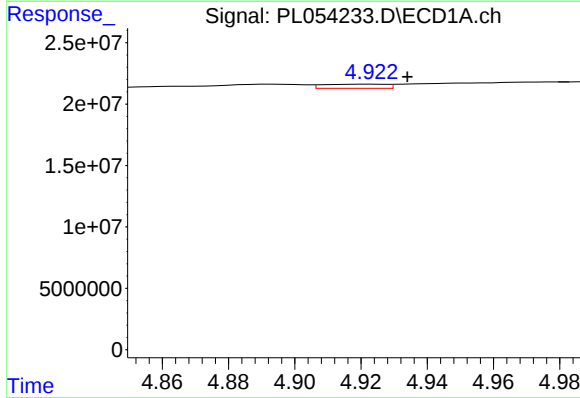


#24 Chlordane-2

R.T.: 4.923 min
Delta R.T.: -0.011 min
Response: 4464661
Conc: 11.59 ng/ml

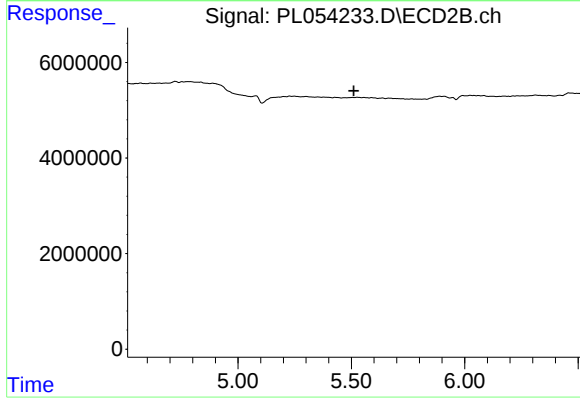

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.510 min
Response: 0
Conc: N.D.

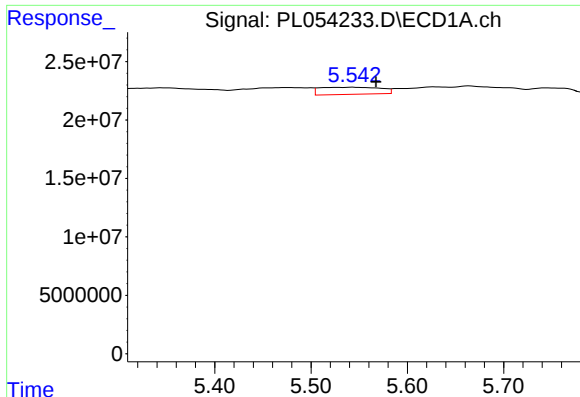

#26 Chlordane-4


R.T.: 5.543 min
Delta R.T.: -0.024 min
Response: 26796661
Conc: 28.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

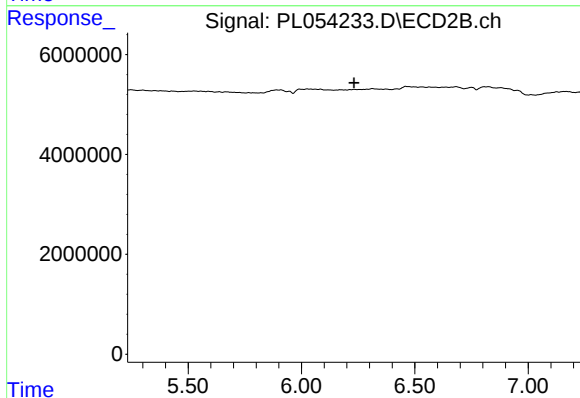


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

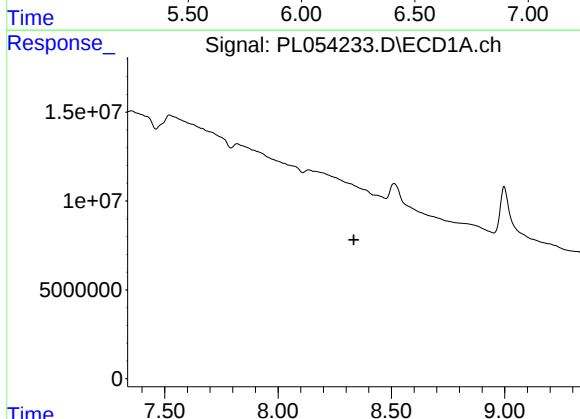

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.334 min
Response: 0
Conc: N.D.

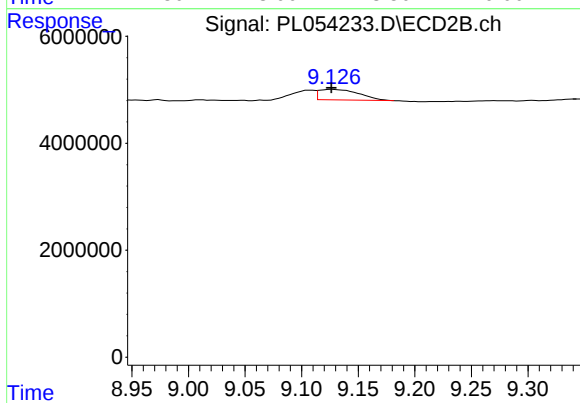

#28 Decachlorobiphenyl

R.T.: 9.128 min
Delta R.T.: 0.001 min
Response: 4780628
Conc: 1.70 ng/ml