

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111419\
 Data File : PL054244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2019 14:13
 Operator : SG\AJ
 Sample : K5826-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:35:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	4.042	237.4E6	52975723	21.904	21.170
28)	SA Decachlor...	8.320	9.119	179.5E6	52201430	18.297	18.537
Target Compounds							
16)	A 4,4'-DDD	6.238	0.000	1319213	0	0.148	N.D. #
17)	MA 4,4'-DDT	6.476	0.000	3376271	0	0.341	N.D. #
20)	A Methoxychlor	7.011f	0.000	4456493	0	0.904	N.D. #
23)	Chlordane-1	4.441	0.000	5492460	0	15.486	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111419\
Data File : PL054244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2019 14:13
Operator : SG\AJ
Sample : K5826-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:35:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

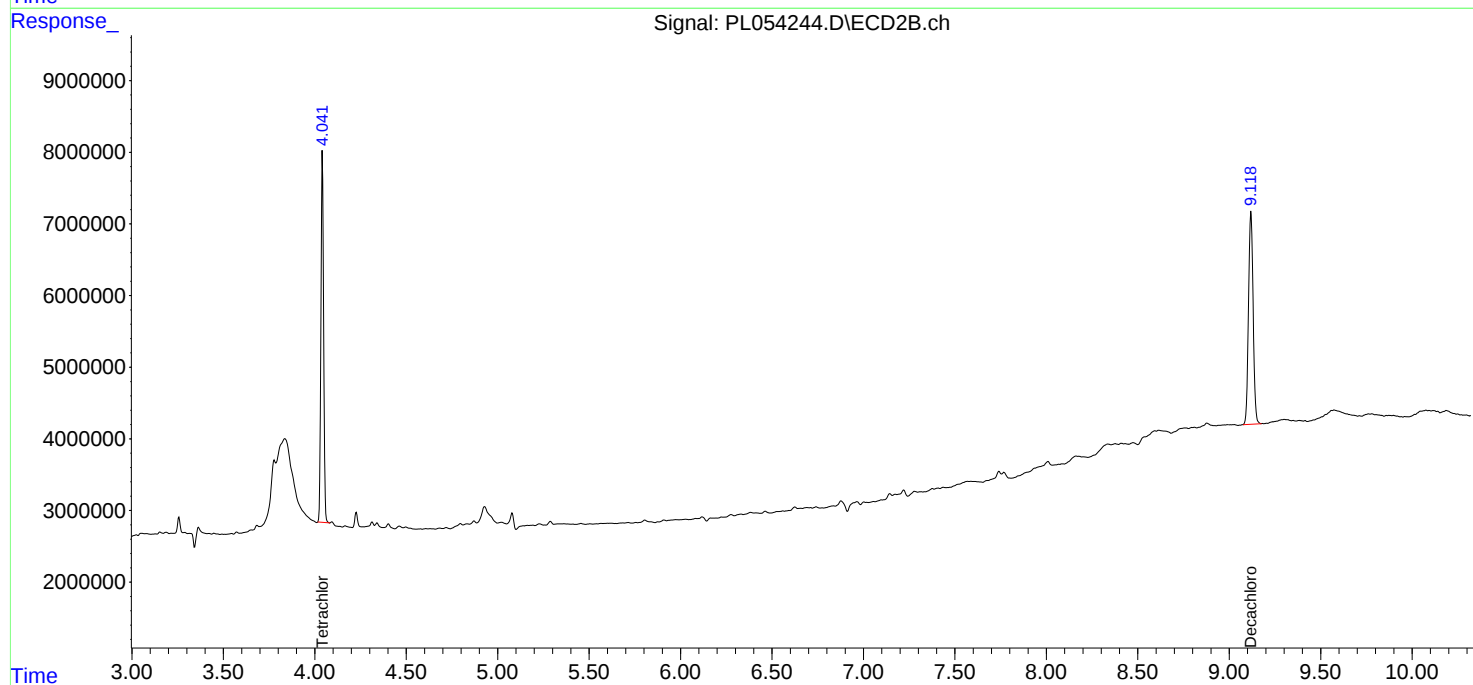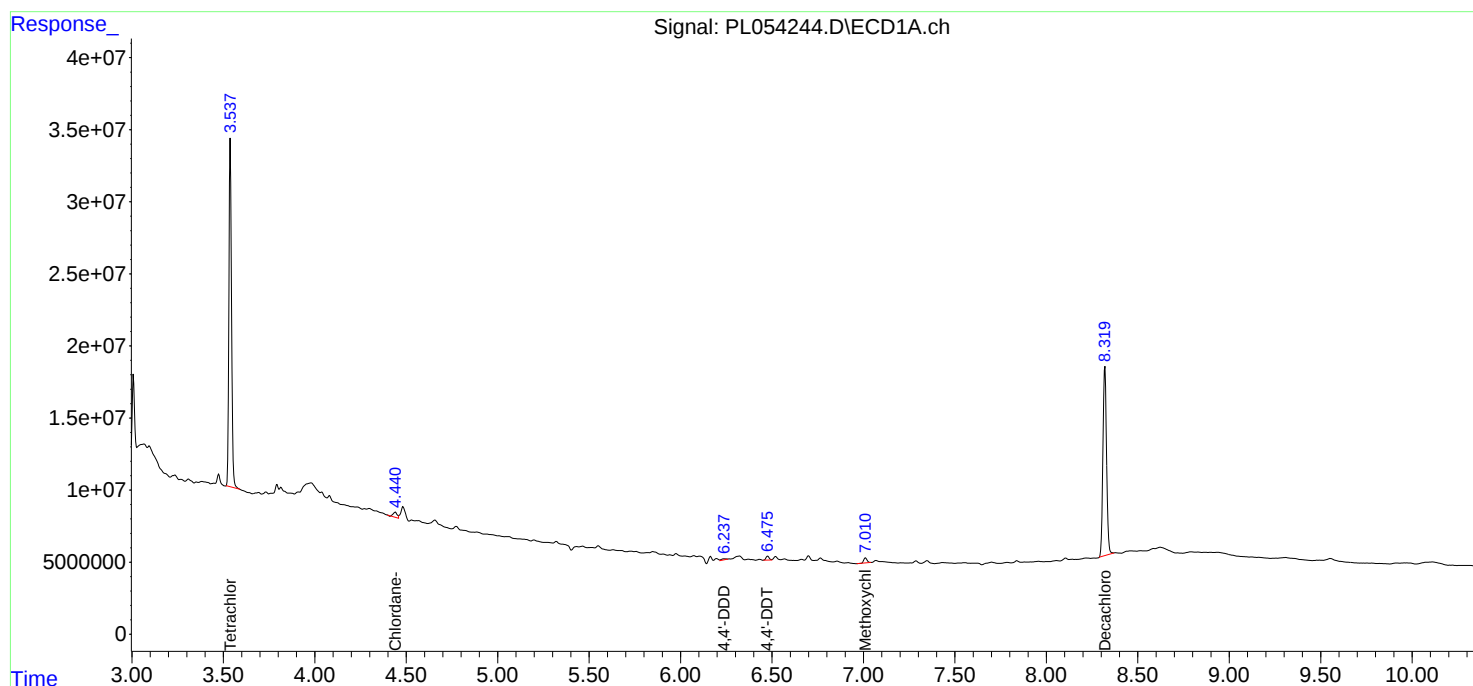


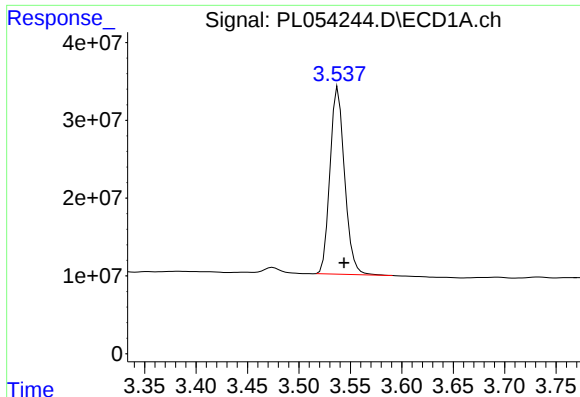

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: -0.006 min
Response: 237428237
Conc: 21.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

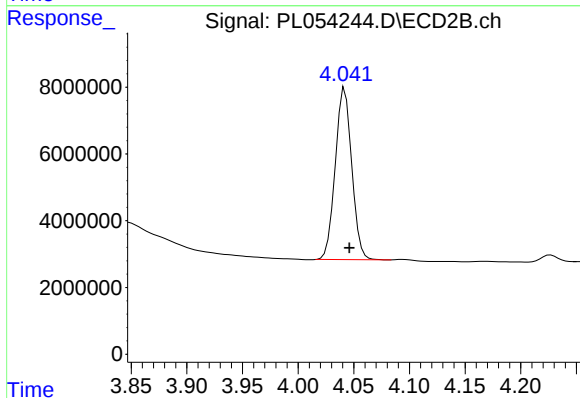


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.004 min
Response: 52975723
Conc: 21.17 ng/ml

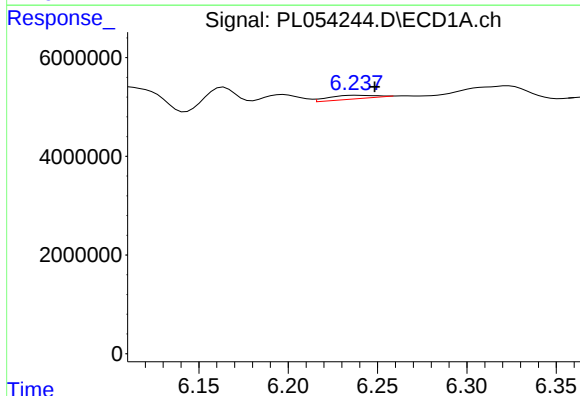


#16 4,4'-DDD

R.T.: 6.238 min
Delta R.T.: -0.010 min
Response: 1319213
Conc: 0.15 ng/ml

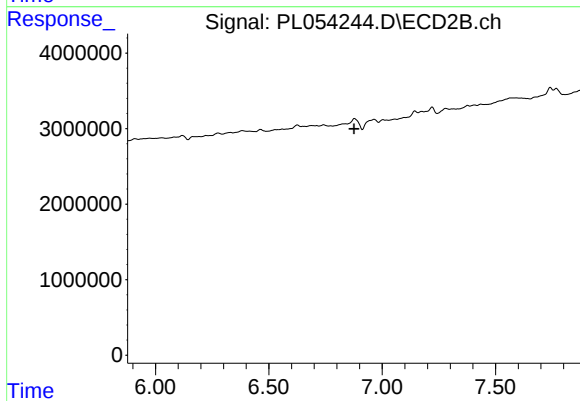

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.877 min
Response: 0
Conc: N.D.

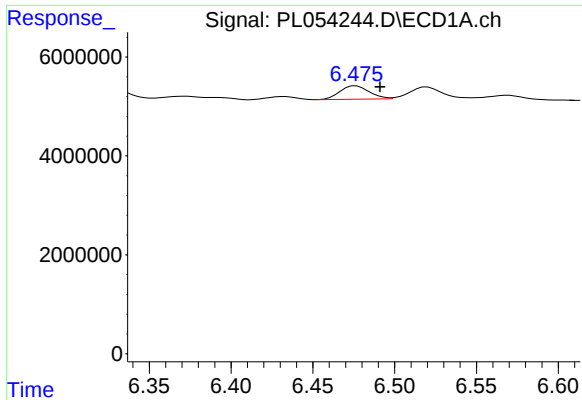

#17 4,4'-DDT


R.T.: 6.476 min
Delta R.T.: -0.015 min
Response: 3376271
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

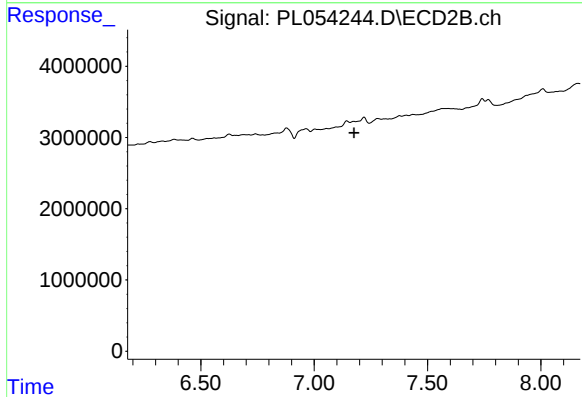


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.176 min
Response: 0
Conc: N.D.

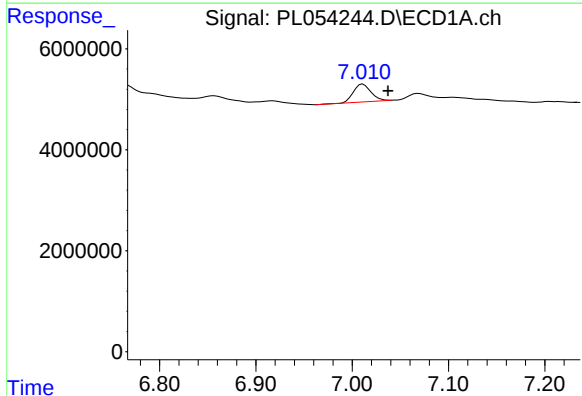


#20 Methoxychlor

R.T.: 7.011 min
Delta R.T.: -0.026 min
Response: 4456493
Conc: 0.90 ng/ml

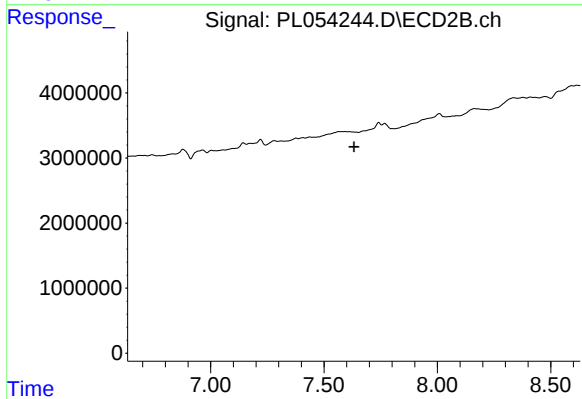

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.633 min
Response: 0
Conc: N.D.

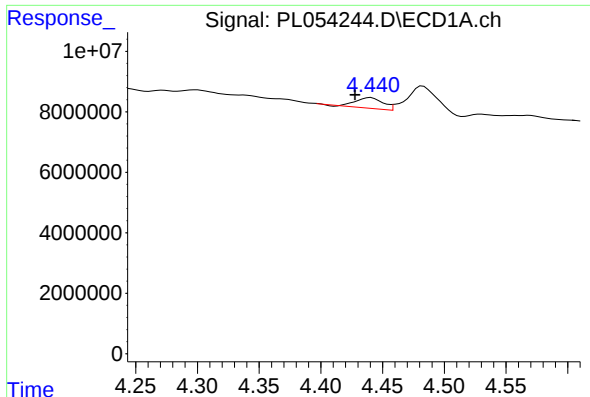

#23 Chlordane-1


R.T.: 4.441 min
Delta R.T.: 0.013 min
Response: 5492460
Conc: 15.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

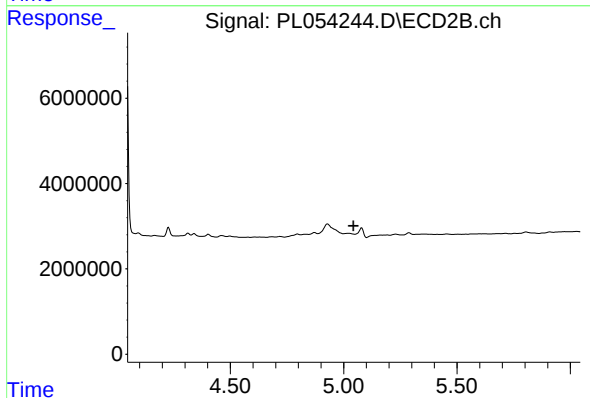


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

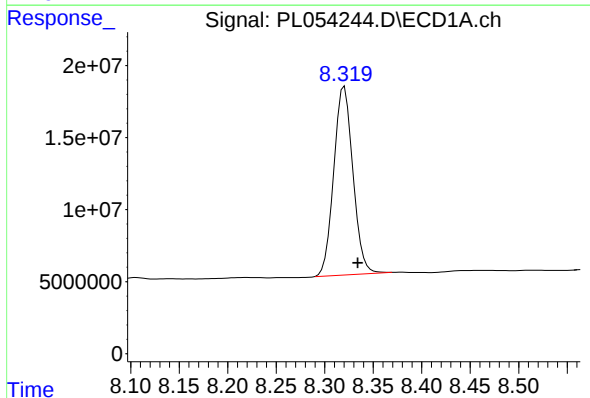

#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.014 min
Response: 179524841
Conc: 18.30 ng/ml

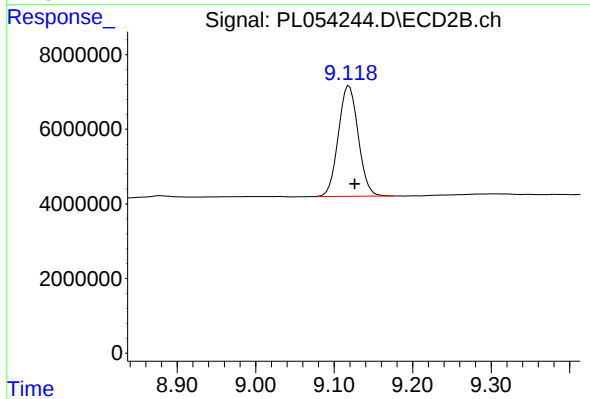

#28 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: -0.007 min
Response: 52201430
Conc: 18.54 ng/ml