

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111419\
 Data File : PS007695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2019 13:00
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:40:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
10) T	Pentachlo...	0.000	6.461	0	6277466	N.D. <MDL
12) T	2,4,5-T	7.421	0.000	56315494	0	6.879 N.D. #
15) T	Picloram	8.969	8.917	253.9E6	166.9E6	22.872 28.485



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111419\
Data File : PS007695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2019 13:00
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:40:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

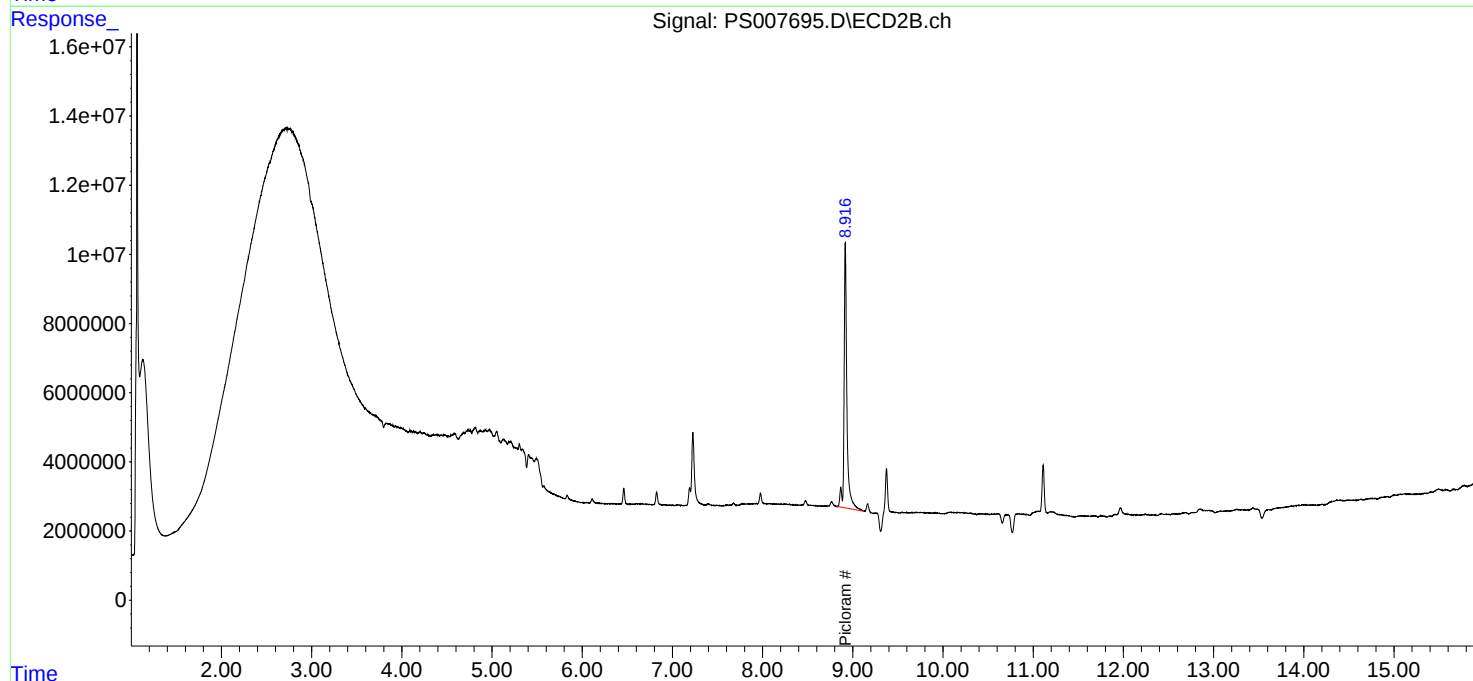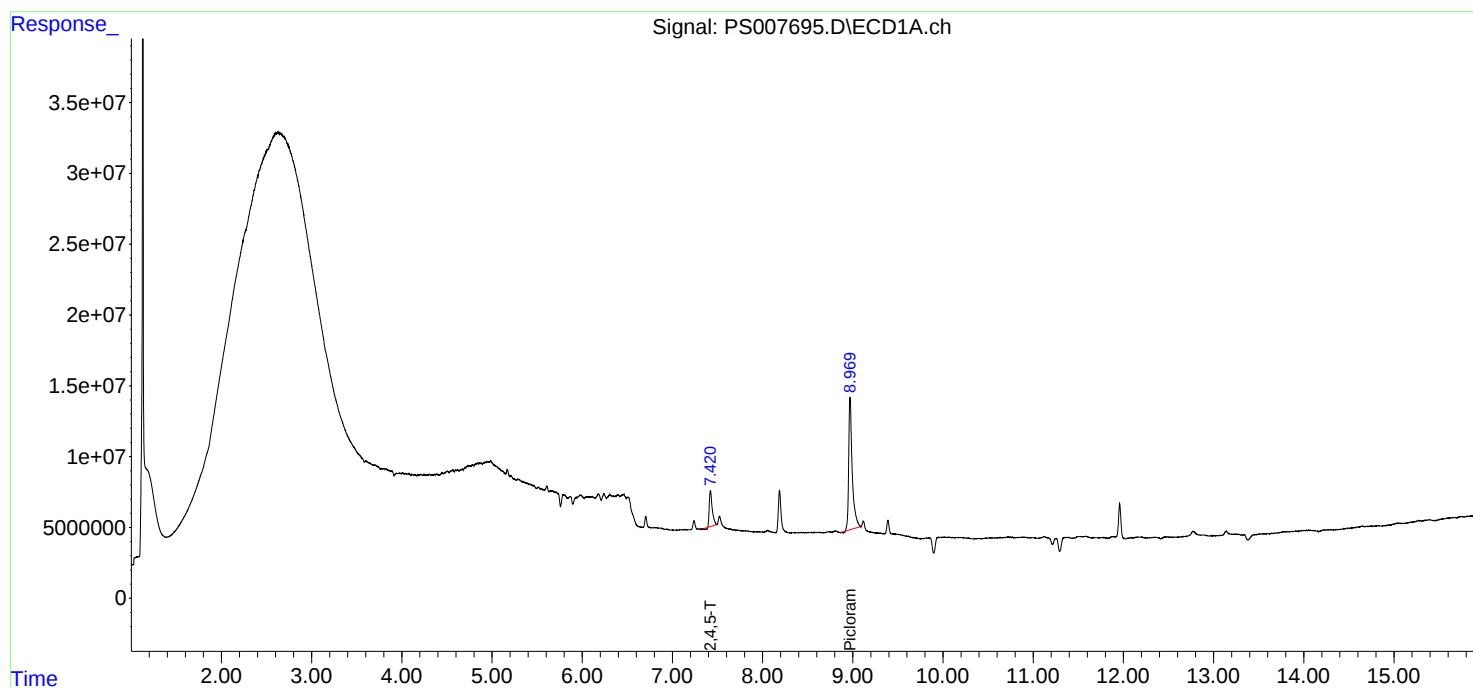


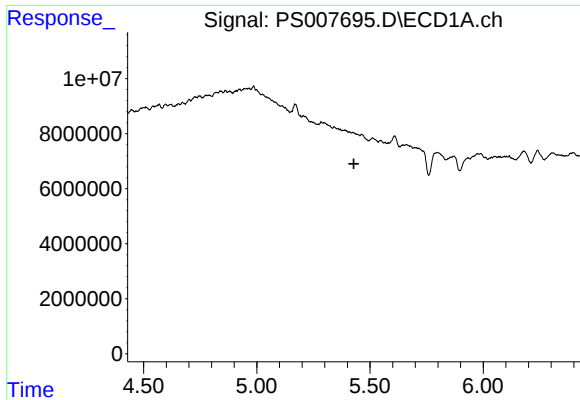

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

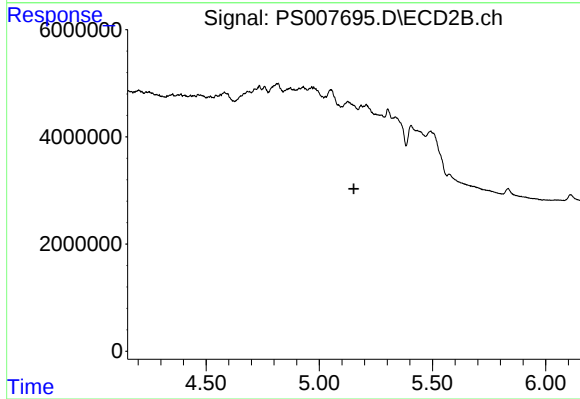


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 5.153 min
Response: 0
Conc: N.D.

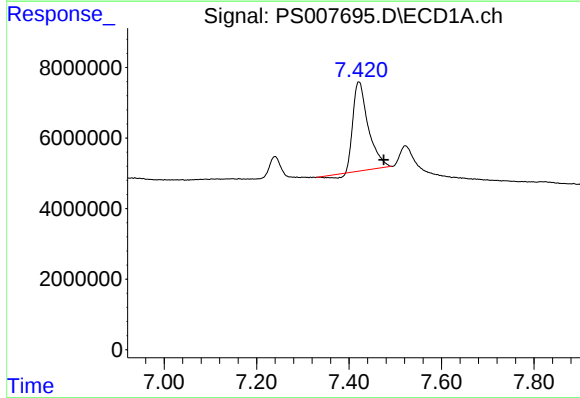


#12 2,4,5-T

R.T.: 7.421 min
Delta R.T.: -0.054 min
Response: 56315494
Conc: 6.88 ng/ml

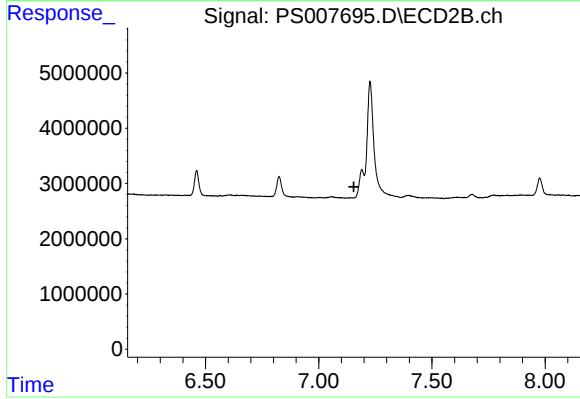

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

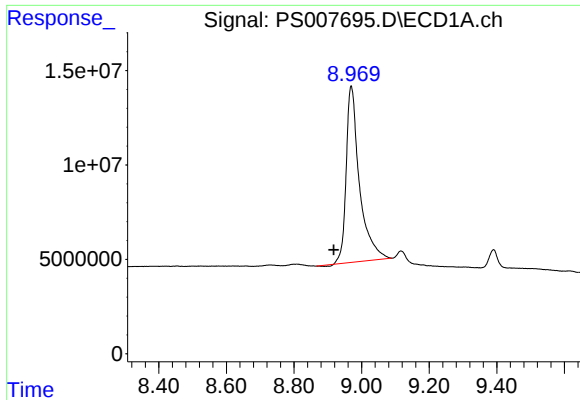

#15 Picloram

R.T.: 8.969 min
Delta R.T.: 0.051 min
Response: 253945970
Conc: 22.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

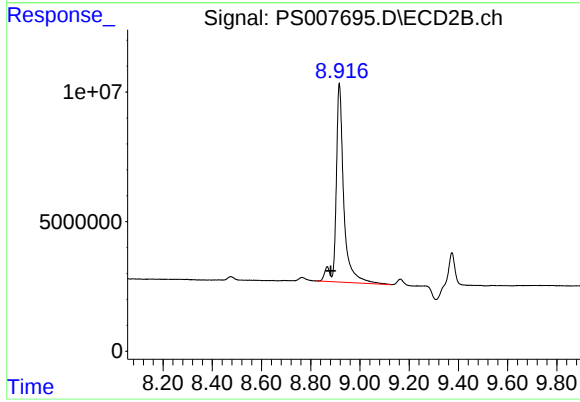

#15 Picloram

R.T.: 8.917 min
Delta R.T.: 0.035 min
Response: 166893285
Conc: 28.49 ng/ml