

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111419\
 Data File : PS007702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2019 17:49
 Operator : SM\AJ
 Sample : K5670-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:42:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.442	5.167	716.0E6	336.6E6	519.932	479.169
Target Compounds							
1) T	Dalapon	2.007	1.714	114.3E6	180.0E6	63.165	151.560 #
2) T	3,5-DICHL...	0.000	4.461	0	10550692	N.D.	11.678
3) T	4-Nitroph...	0.000	4.845	0	11069108	N.D.	26.900
5) T	DICAMBA	5.534	0.000	47141324	0	9.266	N.D. #
7) T	MCPA	0.000	5.479	0	54334108	N.D.	18.077
9) T	2,4-D	0.000	6.007	0	10229773	N.D.	12.686
10) T	Pentachlo...	0.000	6.378	0	19743198	N.D.	2.016
11) T	2,4,5-TP ...	0.000	6.765	0	73015945	N.D.	18.646
12) T	2,4,5-T	7.413	0.000	165.4E6	0	20.205	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111419\
Data File : PS007702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2019 17:49
Operator : SM\AJ
Sample : K5670-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:42:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

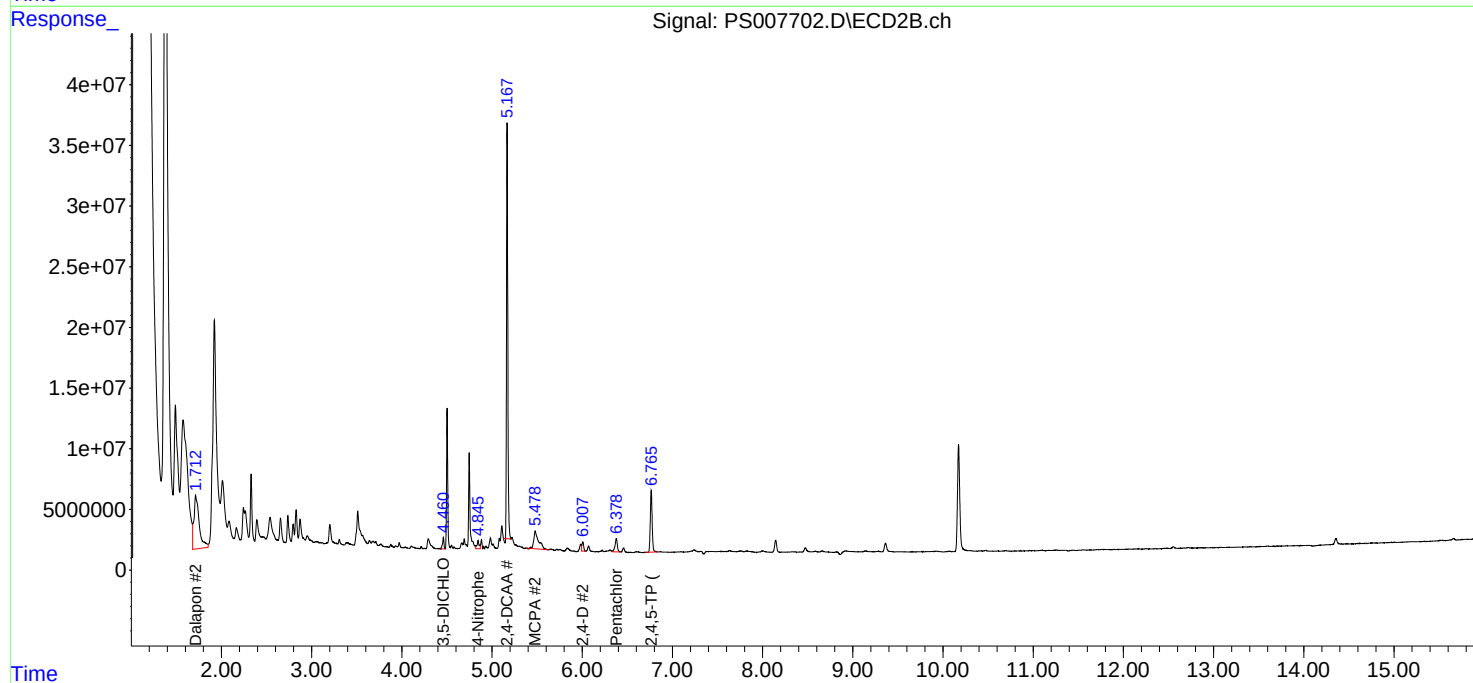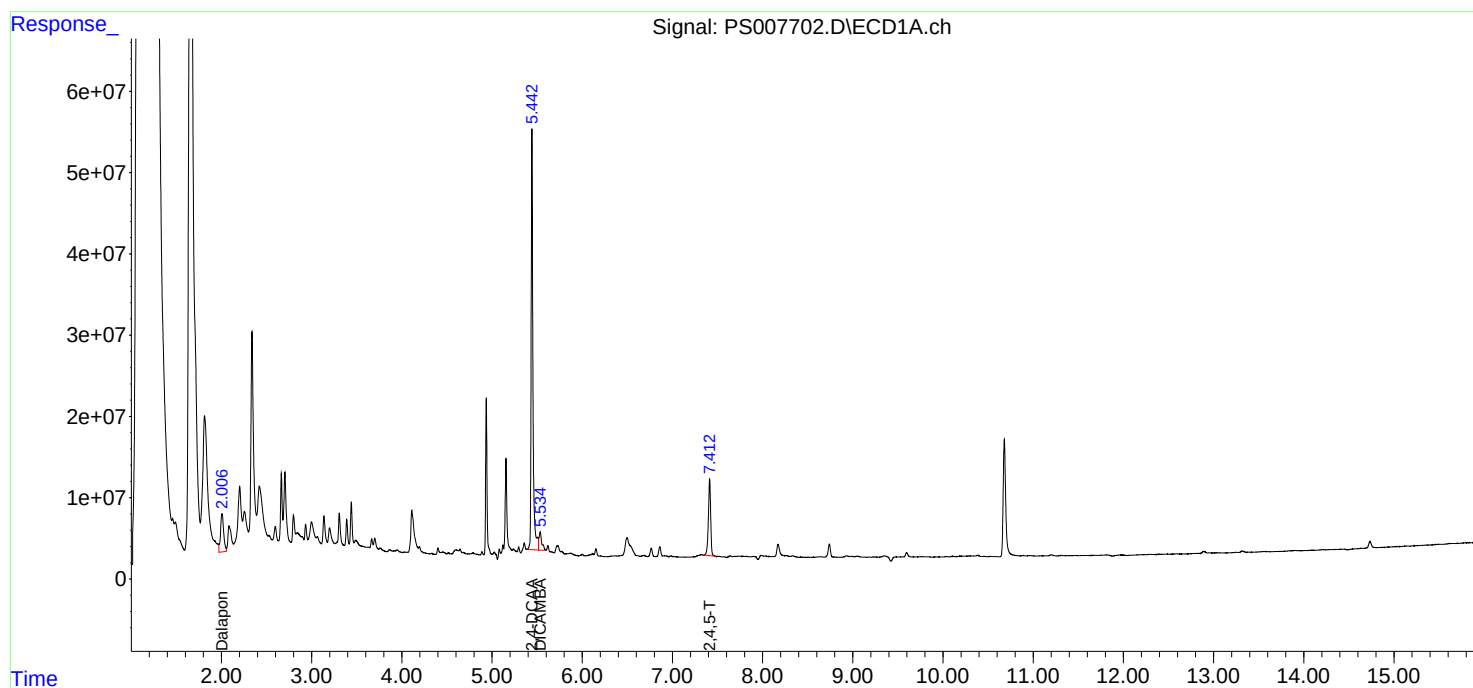


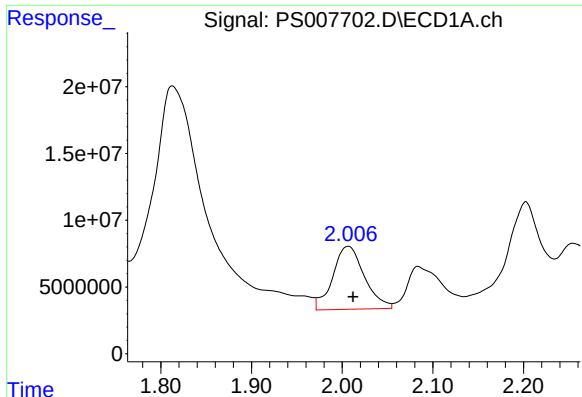

#1 Dalapon


R.T.: 2.007 min
Delta R.T.: -0.005 min
Response: 114277104
Conc: 63.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

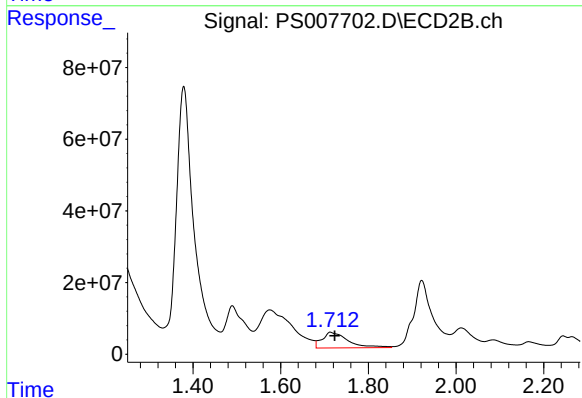


#1 Dalapon

R.T.: 1.714 min
Delta R.T.: -0.010 min
Response: 179963136
Conc: 151.56 ng/ml

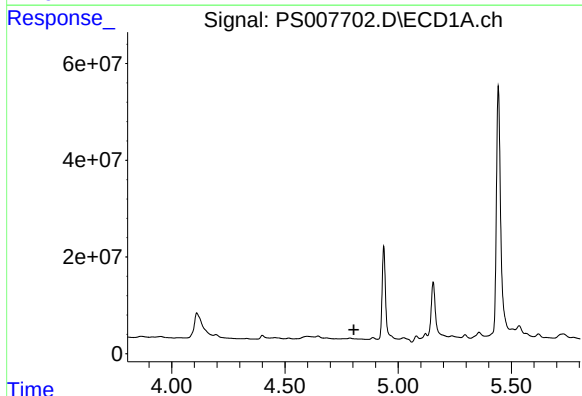


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

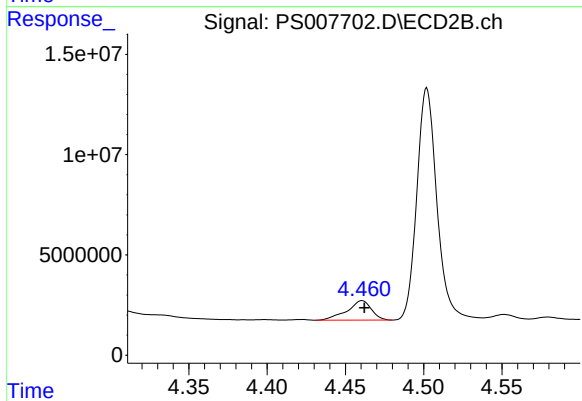

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.461 min
Delta R.T.: -0.002 min
Response: 10550692
Conc: 11.68 ng/ml

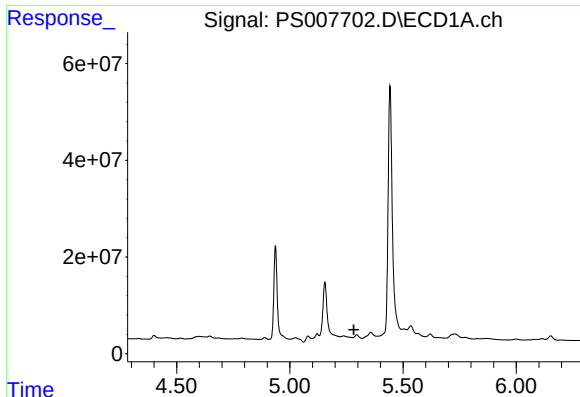

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

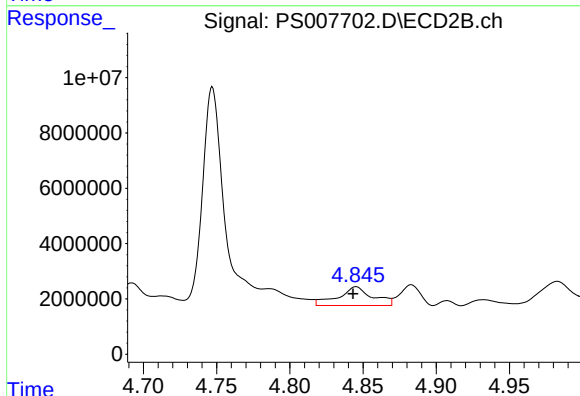


#3 4-Nitrophenol

R.T.: 4.845 min
Delta R.T.: 0.002 min
Response: 11069108
Conc: 26.90 ng/ml

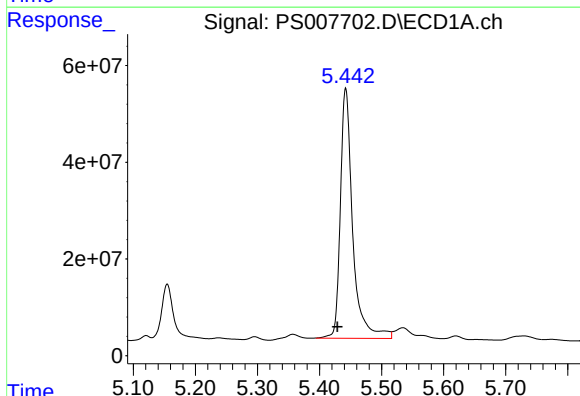


#4 2,4-DCAA

R.T.: 5.442 min
Delta R.T.: 0.014 min
Response: 716042523
Conc: 519.93 ng/ml

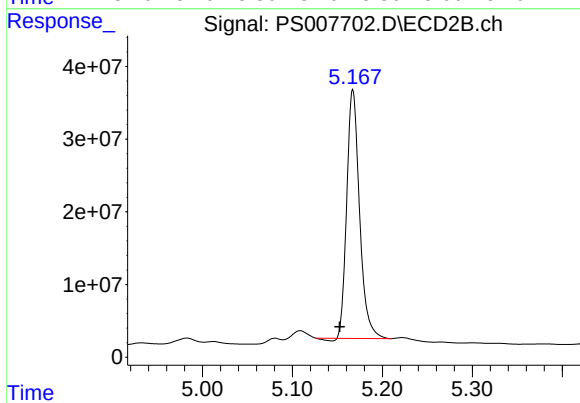

#4 2,4-DCAA


R.T.: 5.167 min
Delta R.T.: 0.015 min
Response: 336646893
Conc: 479.17 ng/ml

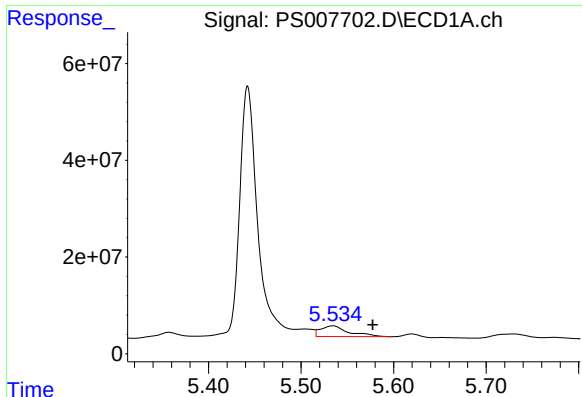

#5 DICAMBA


R.T.: 5.534 min
Delta R.T.: -0.043 min
Response: 47141324
Conc: 9.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

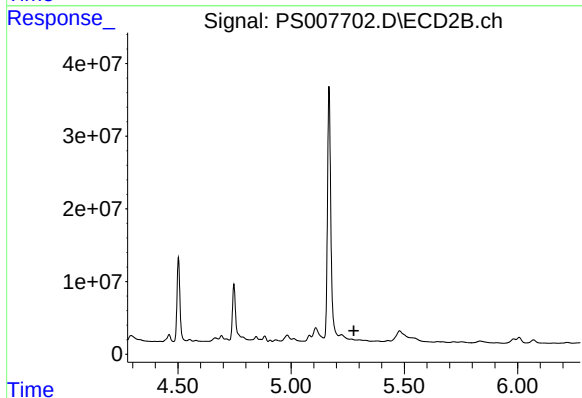


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

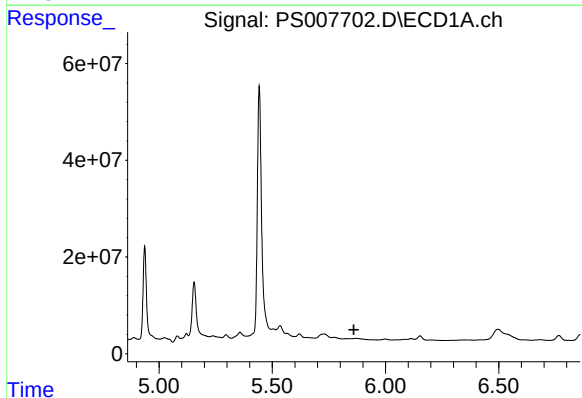


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

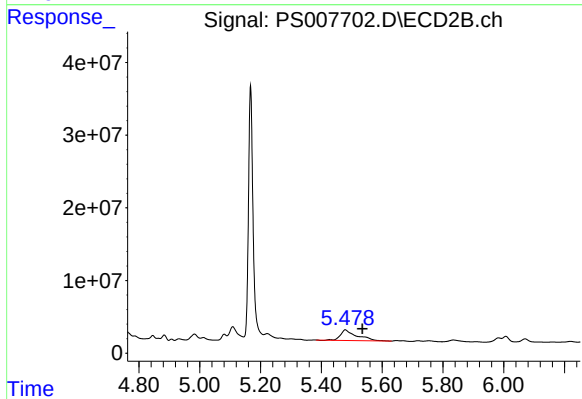

#7 MCPA


R.T.: 5.479 min
Delta R.T.: -0.057 min
Response: 54334108
Conc: 18.08 ug/ml

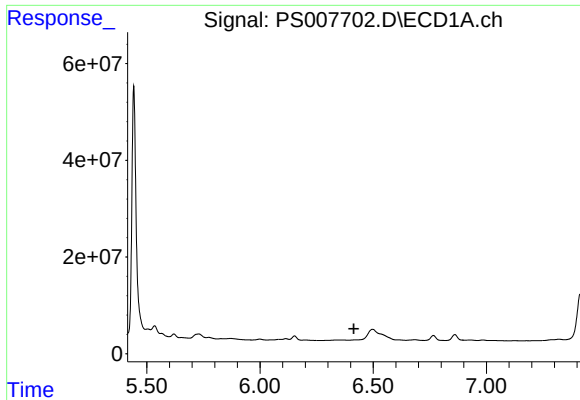

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

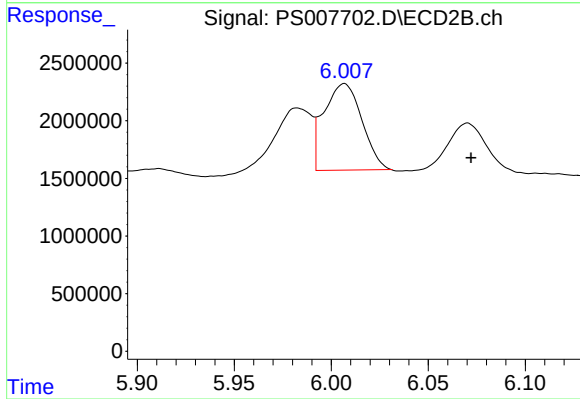


#9 2,4-D

R.T.: 6.007 min
Delta R.T.: -0.066 min
Response: 10229773
Conc: 12.69 ng/ml

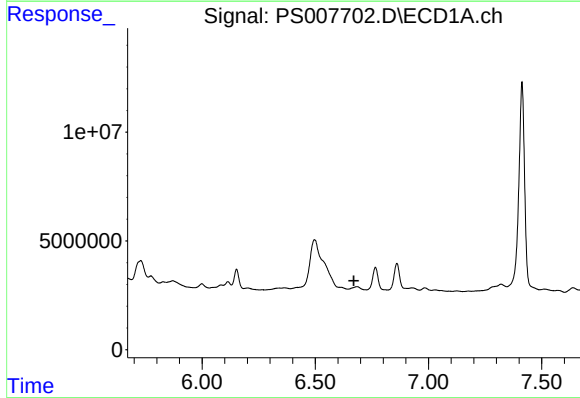


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

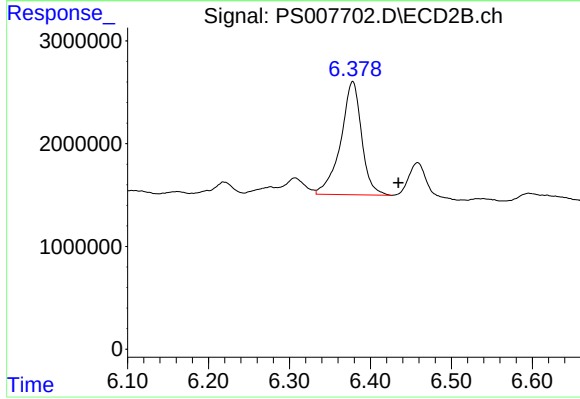

#10 Pentachlorophenol


R.T.: 6.378 min
Delta R.T.: -0.057 min
Response: 19743198
Conc: 2.02 ng/ml

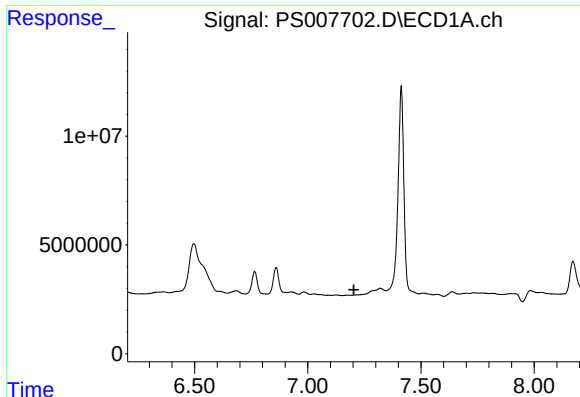

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

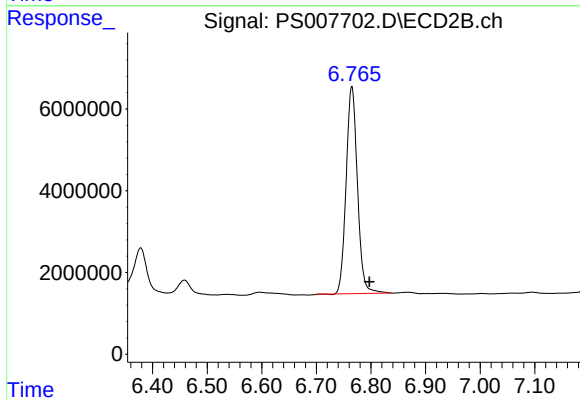


#11 2,4,5-TP (SILVEX)

R.T.: 6.765 min
Delta R.T.: -0.032 min
Response: 73015945
Conc: 18.65 ng/ml

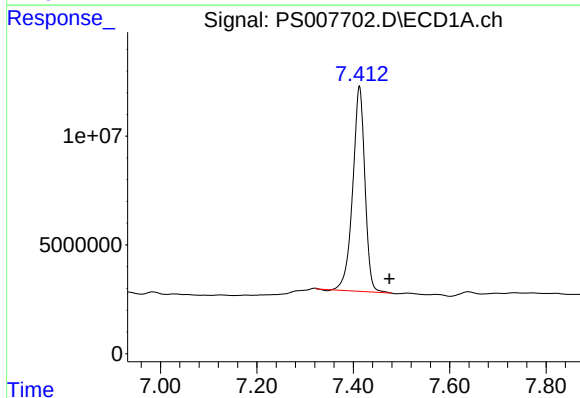

#12 2,4,5-T

R.T.: 7.413 min
Delta R.T.: -0.062 min
Response: 165400784
Conc: 20.21 ng/ml

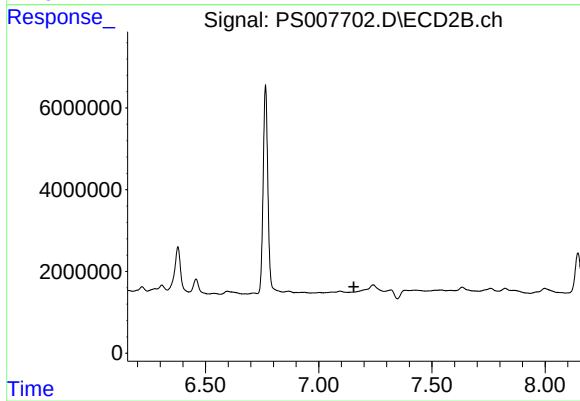

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.