

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111422\
 Data File : PL079104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2022 18:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 20:25:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	2.567	41211415	51628006	21.610	20.221
28)	SA Decachlor...	8.768	7.633	29918334	36698562	19.888	19.375
Target Compounds							
3)	MA gamma-BHC...	4.135f	0.000	194349	0	0.073	N.D. #
5)	MB Aldrin	0.000	3.991	0	3146673	N.D.	0.899 #
6)	B beta-BHC	4.315f	3.675	964915	450074	0.838	0.314 #
8)	B Heptachlo...	5.464	4.479	1177159	494966	0.554	0.164 #
9)	A Endosulfan I	5.859	0.000	249314	0	0.117	N.D. #
13)	MA Dieldrin	6.141f	5.089	147082	493396	0.068	0.167 #
14)	MA Endrin	6.376f	5.389f	579550	587507	0.305	0.226 #
20)	A Methoxychlor	7.314f	0.000	98274	0	0.107	N.D. #
22)	Mirex	7.913f	0.000	1256716	0	0.861	N.D. #
24)	Chlordane-2	0.000	4.090	0	2429862	N.D.	22.831 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111422\
Data File : PL079104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2022 18:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 20:25:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

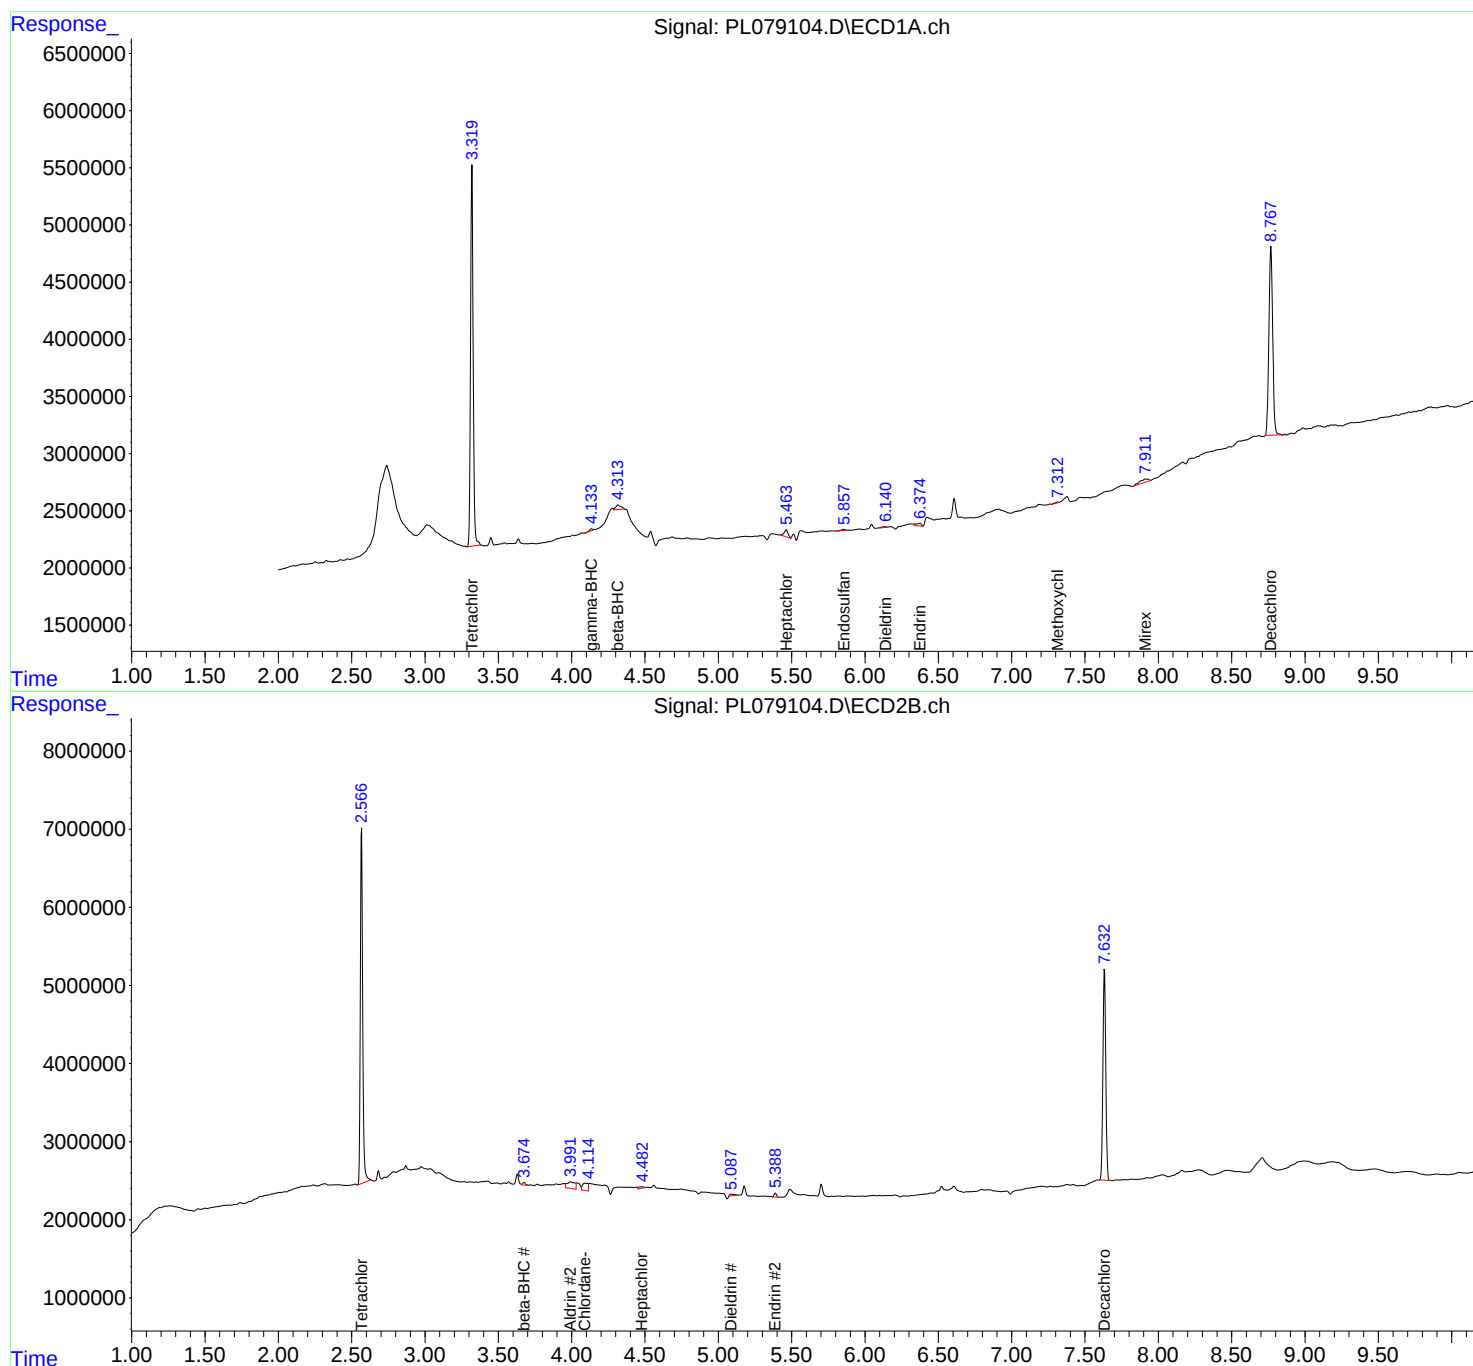


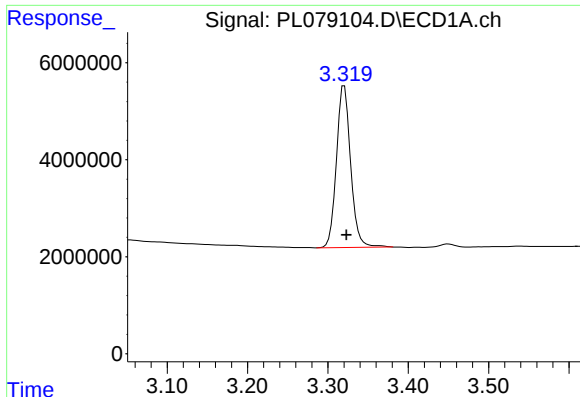

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.003 min
Response: 41211415
Conc: 21.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

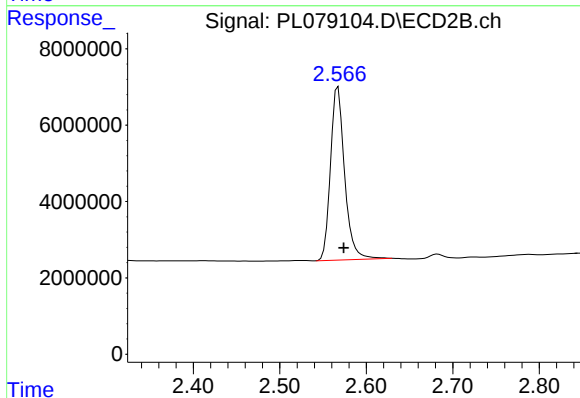


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: -0.006 min
Response: 51628006
Conc: 20.22 ng/ml

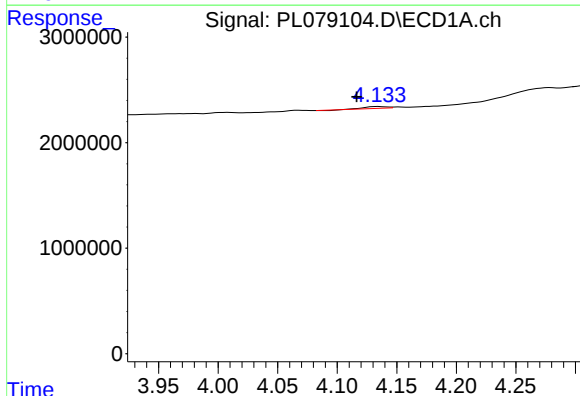


#3 gamma-BHC (Lindane)

R.T.: 4.135 min
Delta R.T.: 0.018 min
Response: 194349
Conc: 0.07 ng/ml

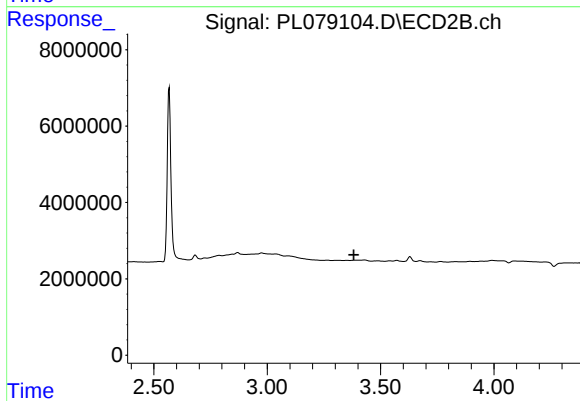

#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.382 min
Response: 0
Conc: N.D.

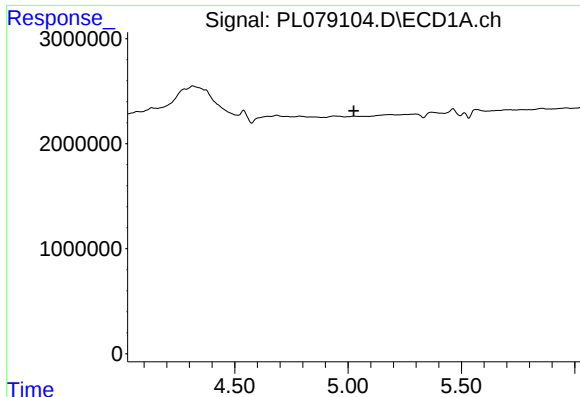

#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.025 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#5 Aldrin


R.T.: 3.991 min
Delta R.T.: 0.011 min
Response: 3146673
Conc: 0.90 ng/ml

#6 beta-BHC

R.T.: 4.315 min
Delta R.T.: -0.016 min
Response: 964915
Conc: 0.84 ng/ml

#6 beta-BHC


R.T.: 3.675 min
Delta R.T.: -0.006 min
Response: 450074
Conc: 0.31 ng/ml

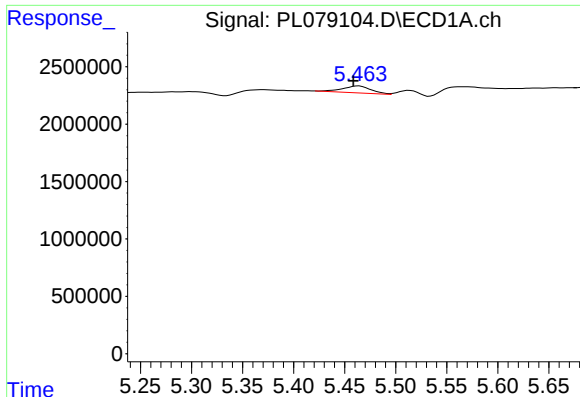

#8 Heptachlor epoxide


R.T.: 5.464 min
Delta R.T.: 0.005 min
Response: 1177159
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

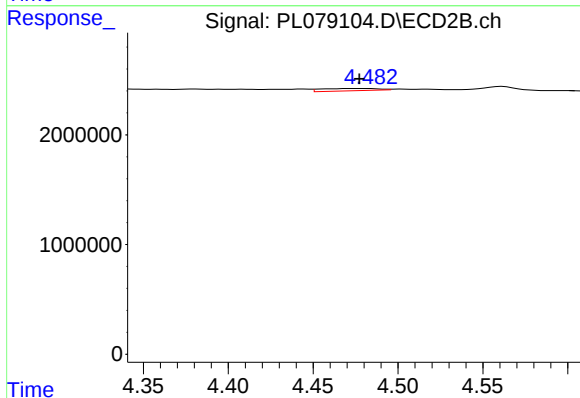


#8 Heptachlor epoxide

R.T.: 4.479 min
Delta R.T.: 0.002 min
Response: 494966
Conc: 0.16 ng/ml

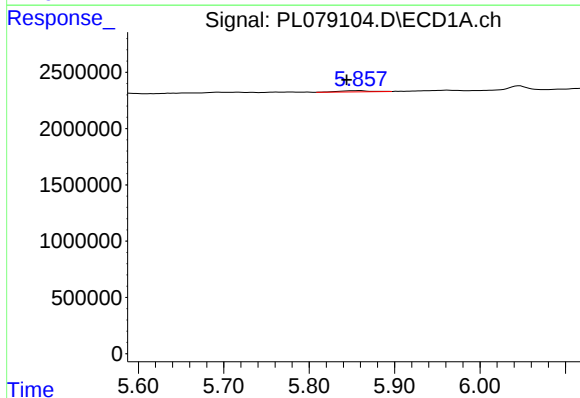


#9 Endosulfan I

R.T.: 5.859 min
Delta R.T.: 0.015 min
Response: 249314
Conc: 0.12 ng/ml

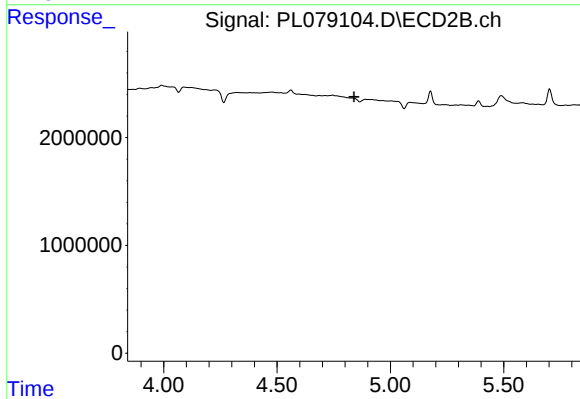

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 4.840 min
Response: 0
Conc: N.D.

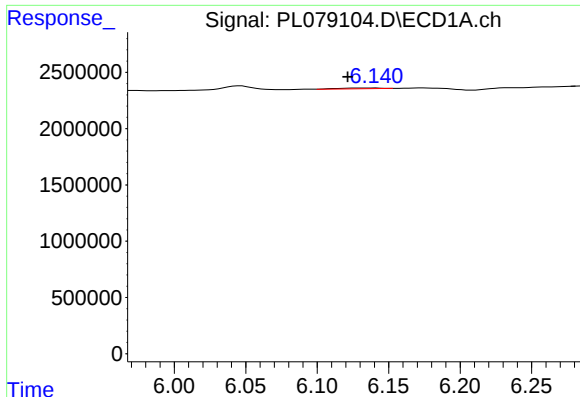

#13 Dieldrin


R.T.: 6.141 min
Delta R.T.: 0.019 min
Response: 147082
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

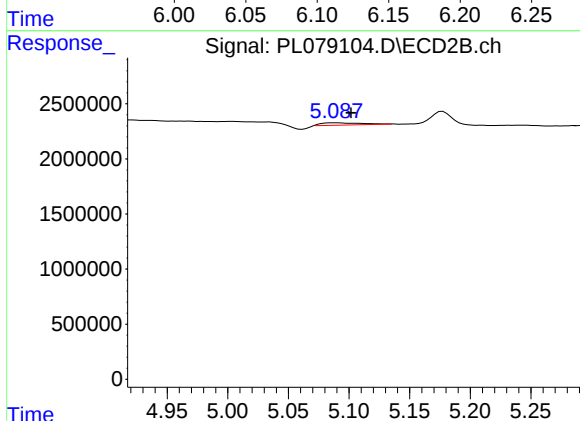


#13 Dieldrin

R.T.: 5.089 min
Delta R.T.: -0.013 min
Response: 493396
Conc: 0.17 ng/ml

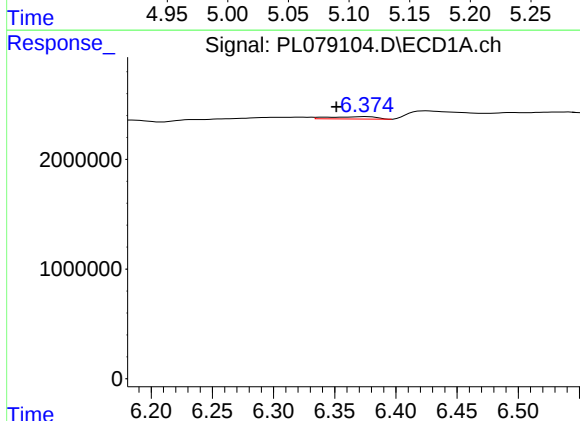


#14 Endrin

R.T.: 6.376 min
Delta R.T.: 0.024 min
Response: 579550
Conc: 0.31 ng/ml

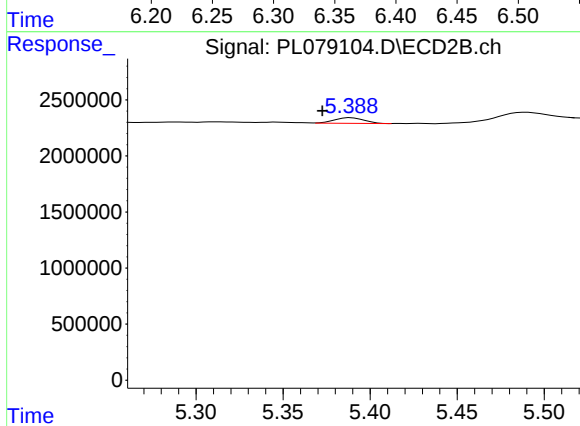

#14 Endrin


R.T.: 5.389 min
Delta R.T.: 0.017 min
Response: 587507
Conc: 0.23 ng/ml

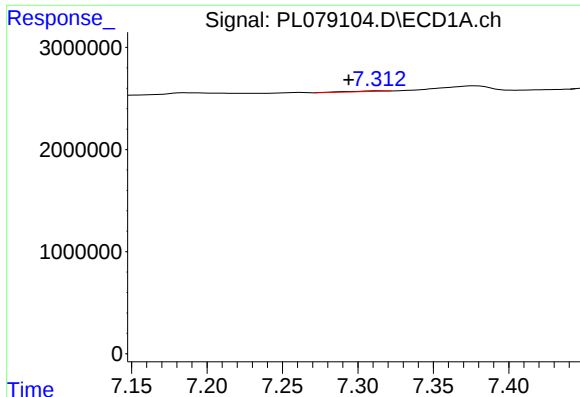

#20 Methoxychlor


R.T.: 7.314 min
Delta R.T.: 0.020 min
Response: 98274
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

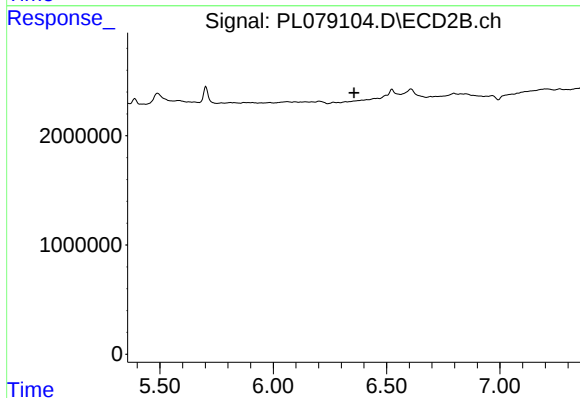


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

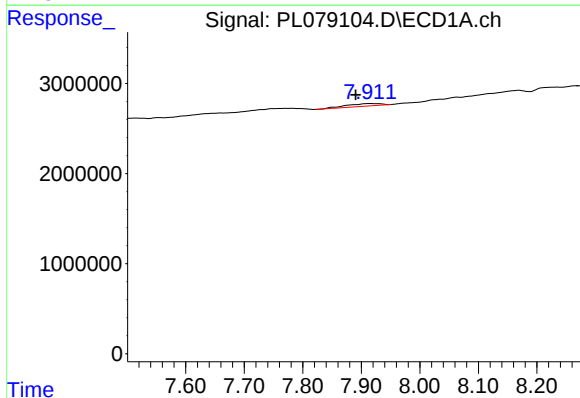


#22 Mirex

R.T.: 7.913 min
Delta R.T.: 0.023 min
Response: 1256716
Conc: 0.86 ng/ml

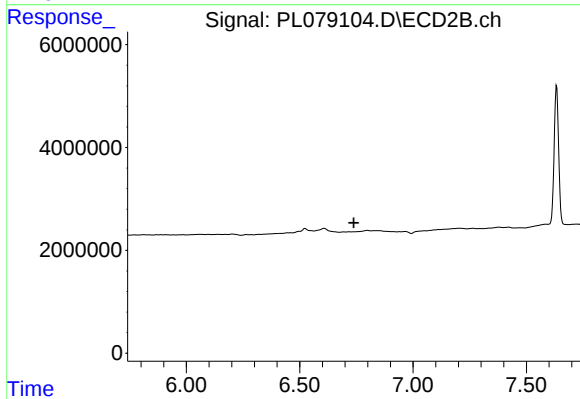

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 6.739 min
Response: 0
Conc: N.D.

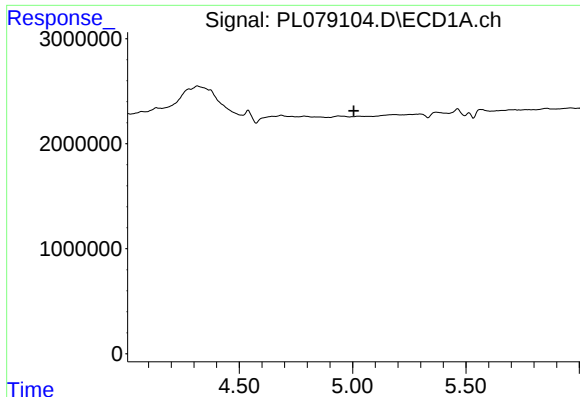

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

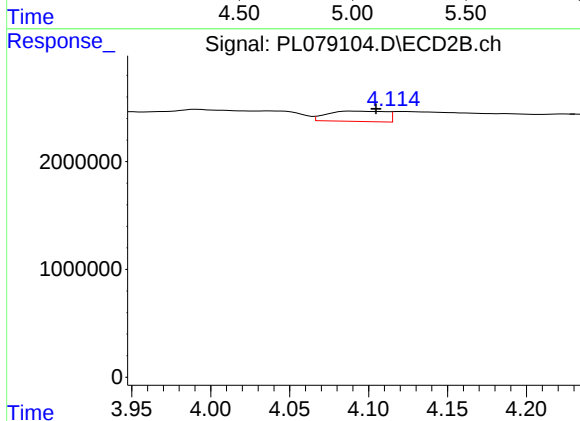


#24 Chlordane-2

R.T.: 4.090 min
Delta R.T.: -0.015 min
Response: 2429862
Conc: 22.83 ng/ml

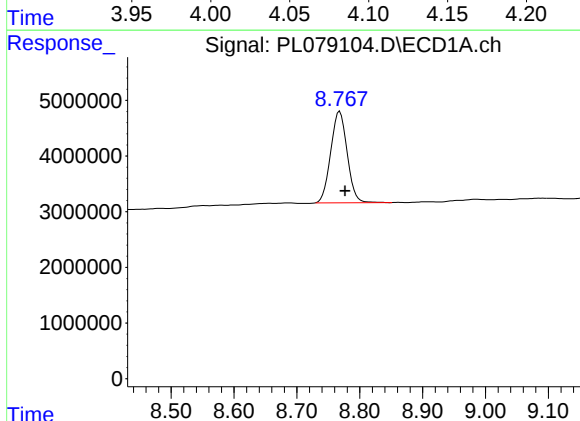

#28 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.008 min
Response: 29918334
Conc: 19.89 ng/ml

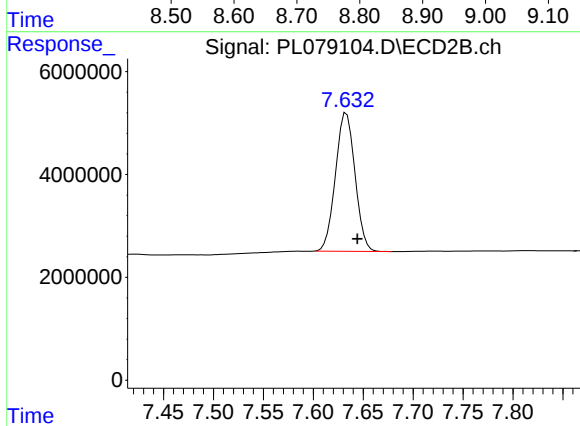

#28 Decachlorobiphenyl

R.T.: 7.633 min
Delta R.T.: -0.011 min
Response: 36698562
Conc: 19.38 ng/ml