

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111423\
 Data File : PL086646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2023 13:59
 Operator : AR\AJ
 Sample : 05384-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-11102023

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/15/2023
 Supervised By :Ankita Jodhani 11/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 19:47:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 13:04:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.616	35045259	10612780	10.793	10.778
28)	SA Decachlor...	8.850	7.767	33501822	12499379	11.445	10.351
Target Compounds							
12)	B 4,4'-DDE	6.014	5.073	2134714	757829	0.615m	0.738

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111423\
Data File : PL086646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2023 13:59
Operator : AR\AJ
Sample : 05384-03
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EO-02-11102023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/15/2023
Supervised By : Ankita Jodhani 11/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 19:47:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 13:04:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

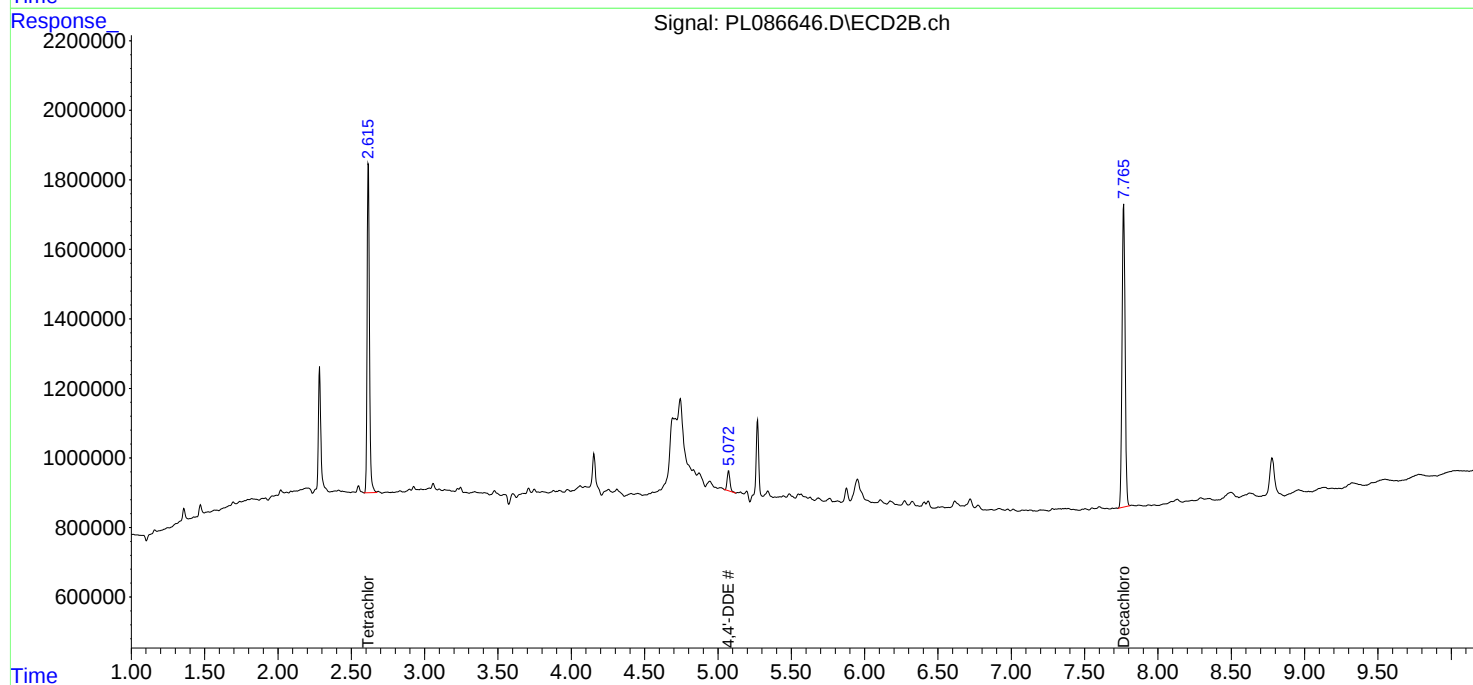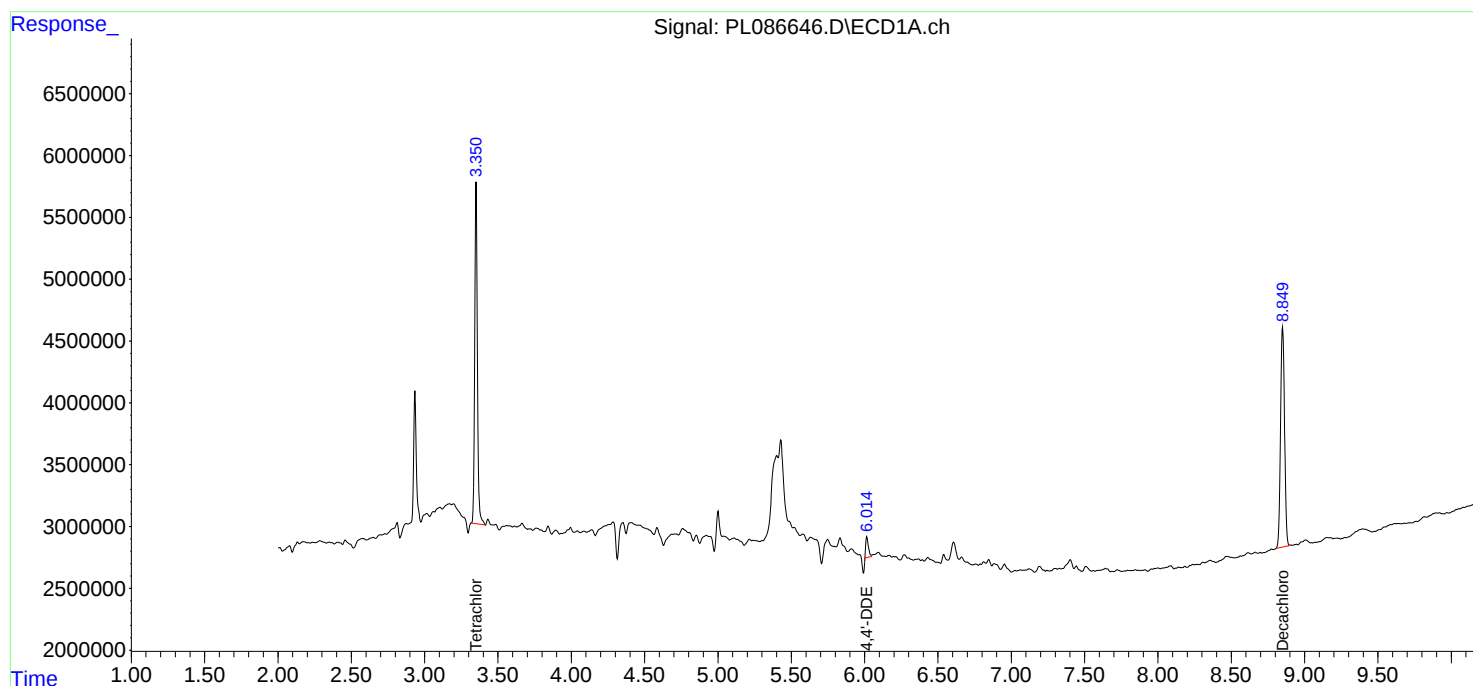

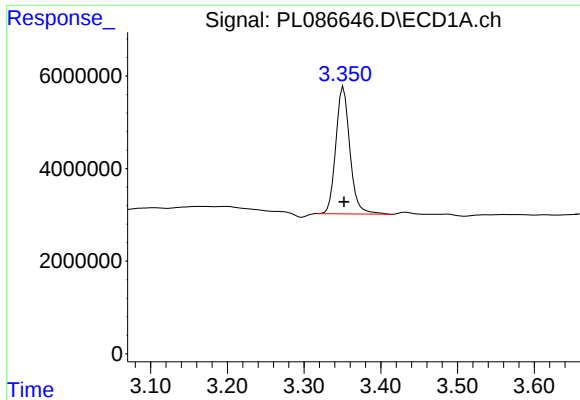


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 35045259
Conc: 10.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-11102023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/15/2023
Supervised By :Ankita Jodhani 11/15/2023

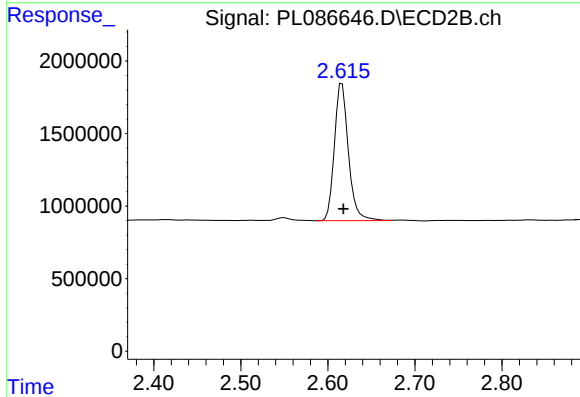


#1 Tetrachloro-m-xylene

R.T.: 2.616 min
Delta R.T.: -0.002 min
Response: 10612780
Conc: 10.78 ng/ml

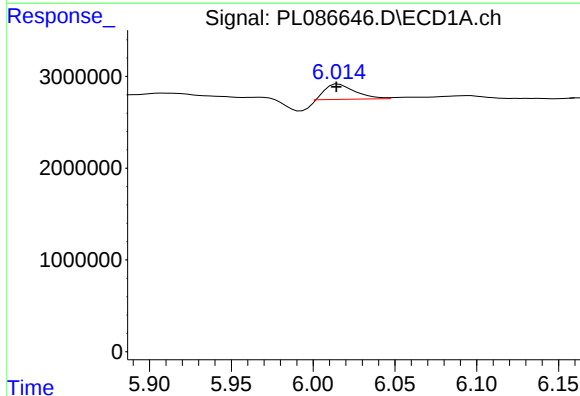


#12 4,4'-DDE

R.T.: 6.014 min
Delta R.T.: 0.000 min
Response: 2134714
Conc: 0.62 ng/ml m

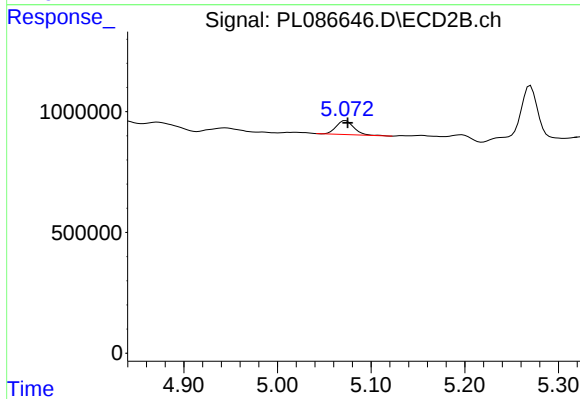

#12 4,4'-DDE

R.T.: 5.073 min
Delta R.T.: -0.002 min
Response: 757829
Conc: 0.74 ng/ml

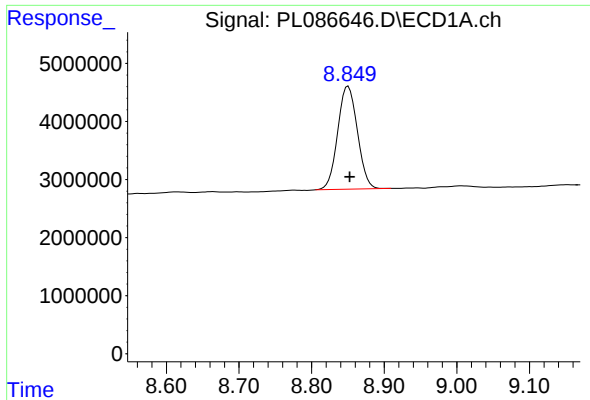


#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: -0.002 min
Response: 33501822
Conc: 11.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-11102023

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/15/2023
Supervised By :Ankita Jodhani 11/15/2023

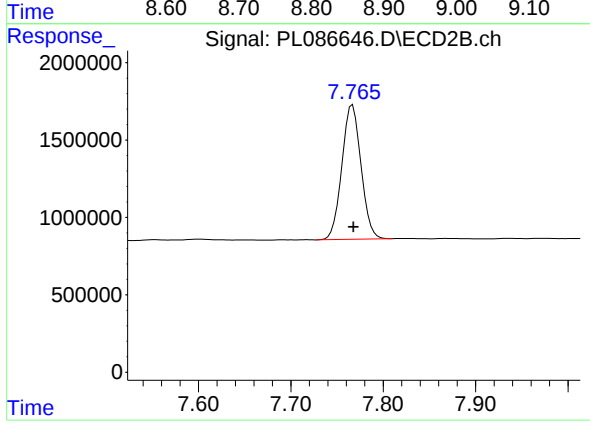

#28 Decachlorobiphenyl

R.T.: 7.767 min
Delta R.T.: -0.001 min
Response: 12499379
Conc: 10.35 ng/ml