

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111424\
 Data File : PL093064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 14:12
 Operator : AR\AJ
 Sample : P4834-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SLP-1-STONE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :Ankita Jodhani 11/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:45:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.776	61308777	69390604	25.022m	25.500
28) SA Decachlor...	9.053	7.914	45949393	64393735	23.875	23.594

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111424\
Data File : PL093064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 14:12
Operator : AR\AJ
Sample : P4834-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SLP-1-STONE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :Ankita Jodhani 11/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:45:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

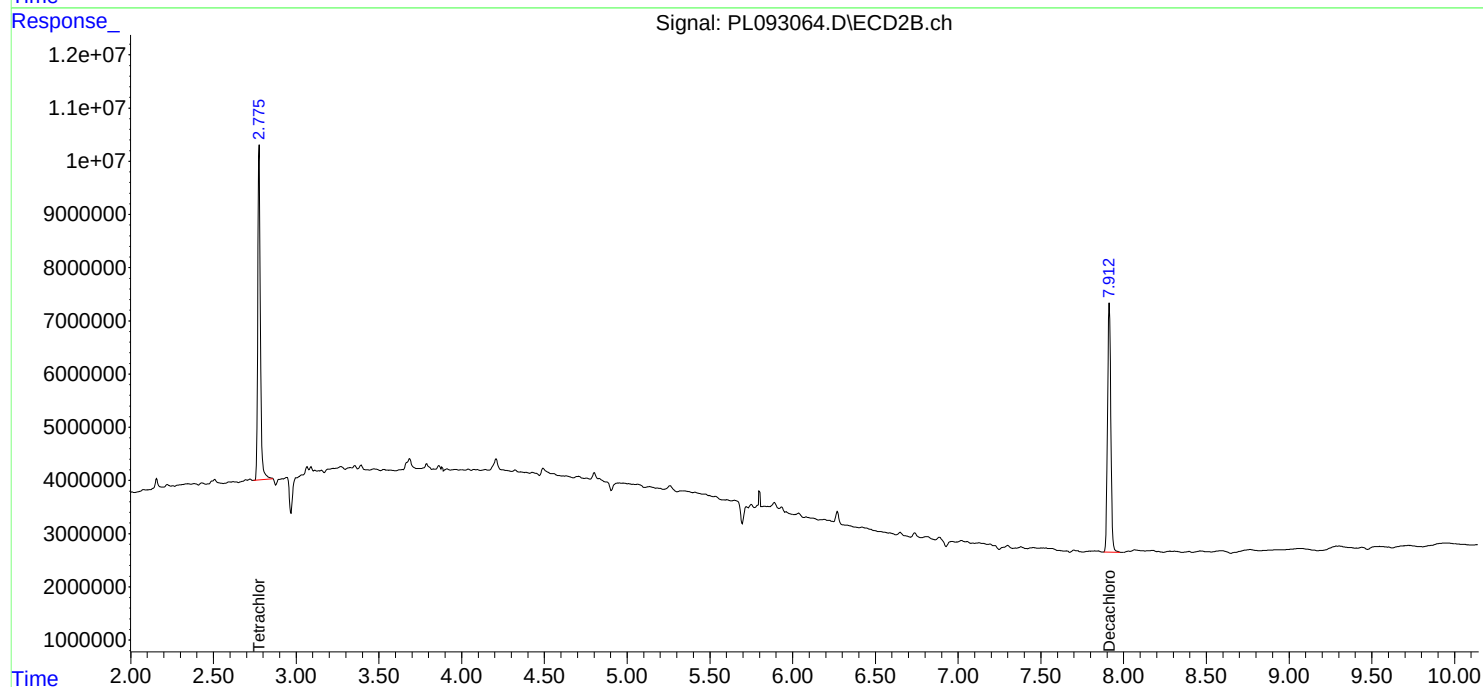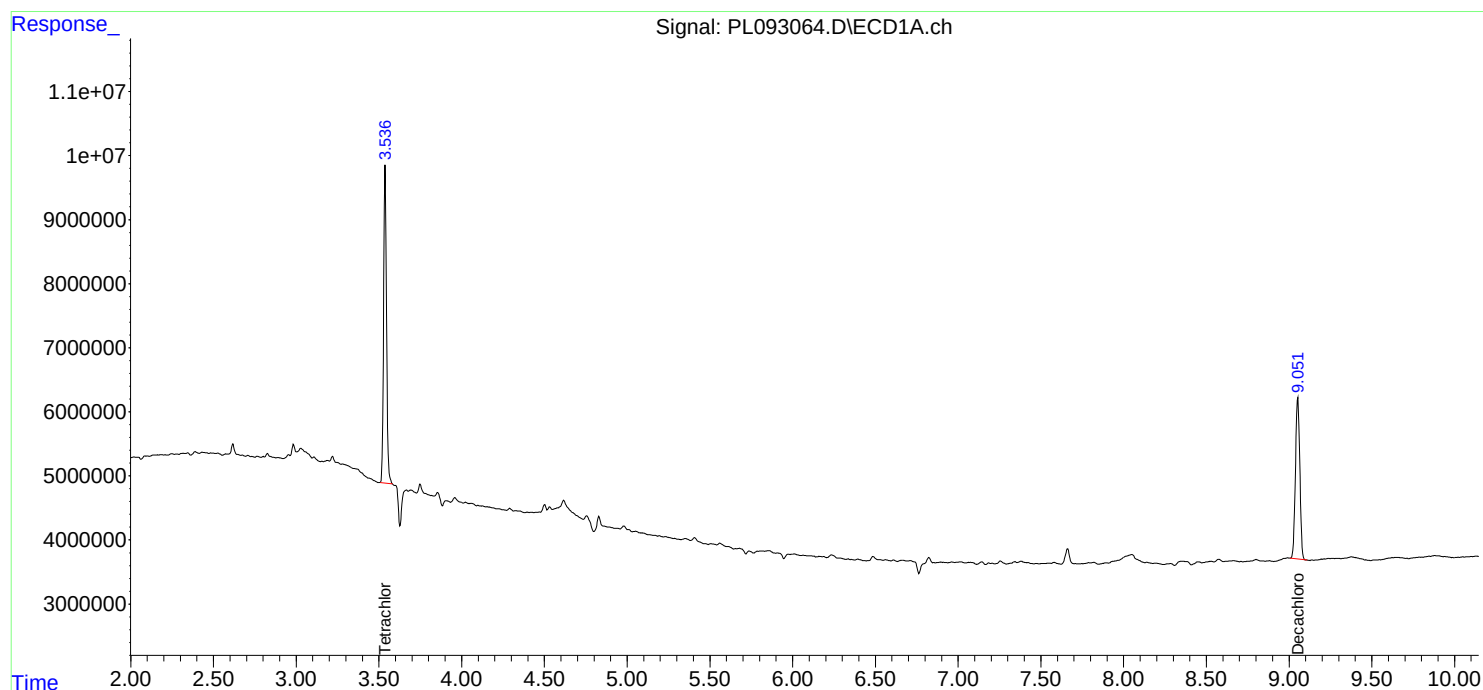

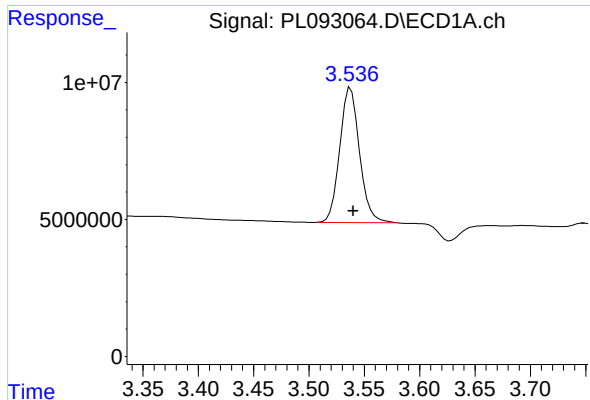


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.004 min
Response: 61308777
Conc: 25.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
SLP-1-STONE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :Ankita Jodhani 11/15/2024

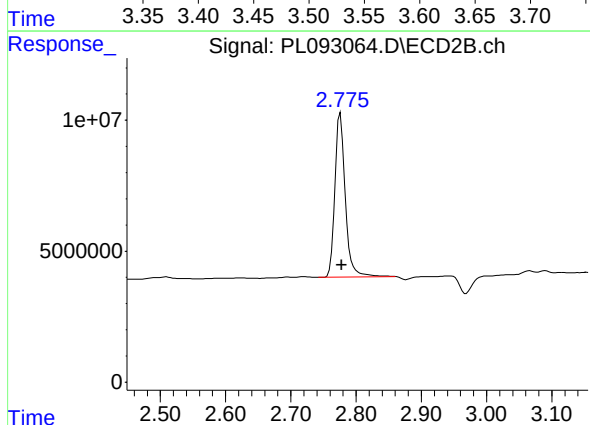


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: -0.002 min
Response: 69390604
Conc: 25.50 ng/ml

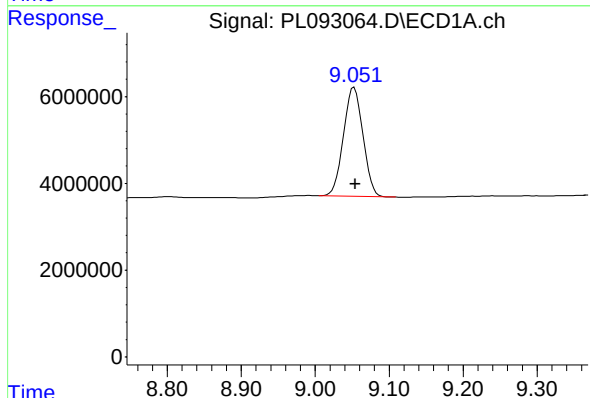

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.001 min
Response: 45949393
Conc: 23.88 ng/ml

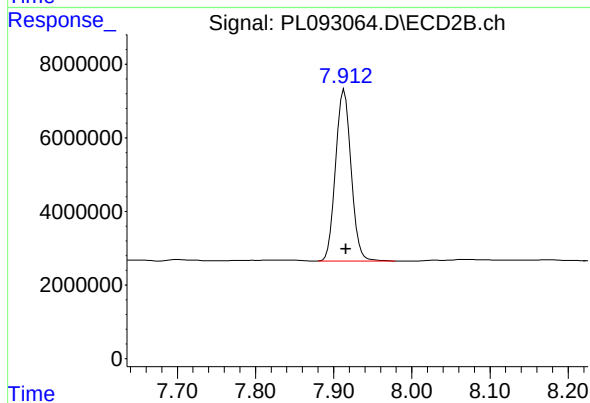

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: -0.002 min
Response: 64393735
Conc: 23.59 ng/ml