

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
 Data File : PL054260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2019 08:18
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 00:16:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	4.550f	0.000	6961579	0	1.056	N.D.	#
7) B	delta-BHC	4.714f	0.000	2408332	0	0.158	N.D.	#
10) B	gamma-Chl...	5.515	0.000	9868803	0	0.723	N.D.	#
12) B	4,4'-DDE	5.754f	0.000	5695692	0	0.479	N.D.	#
14) MA	Endrin	6.129	0.000	21870156	0	1.887	N.D.	#
18) B	Endrin al...	6.538f	0.000	21041037	0	2.295	N.D.	#
24)	Chlordane-2	4.948	0.000	9491807	0	24.634	N.D.	#
25)	Chlordane-3	5.515	0.000	9868803	0	8.562	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
Data File : PL054260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2019 08:18
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 00:16:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

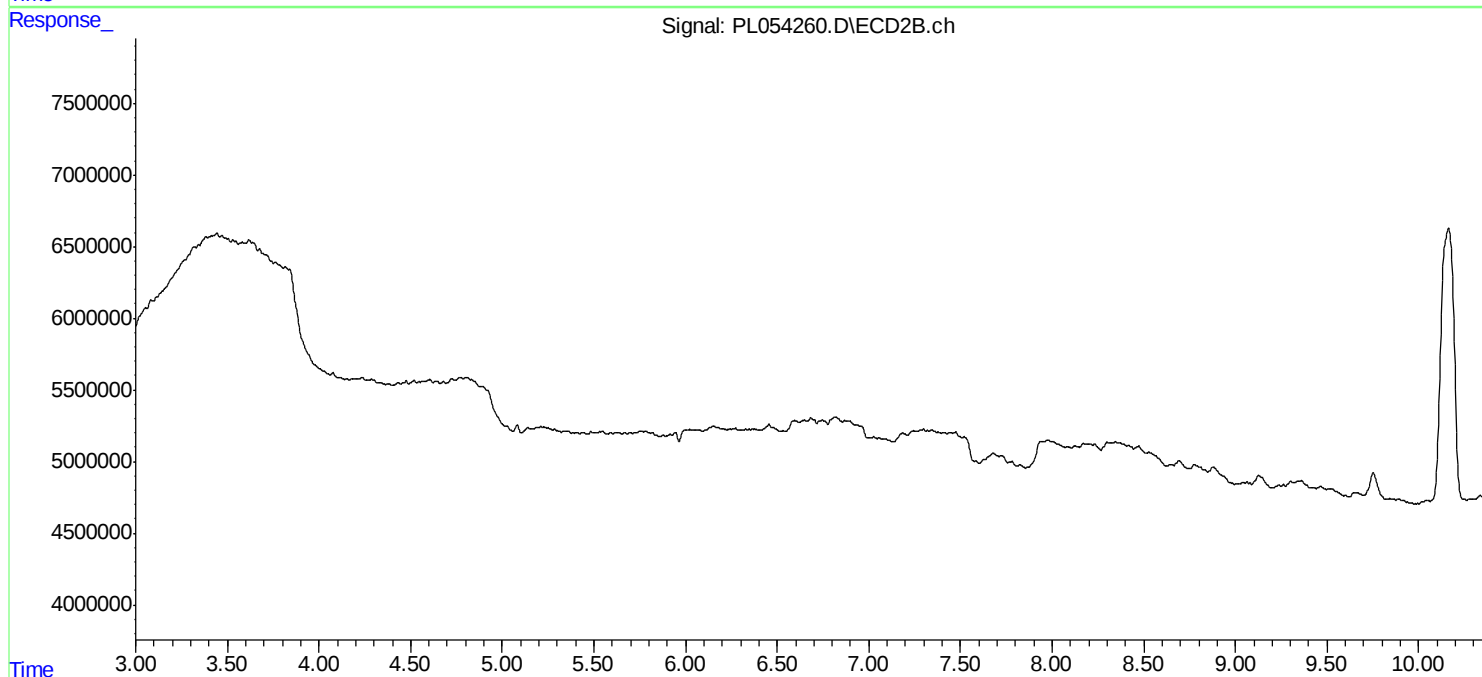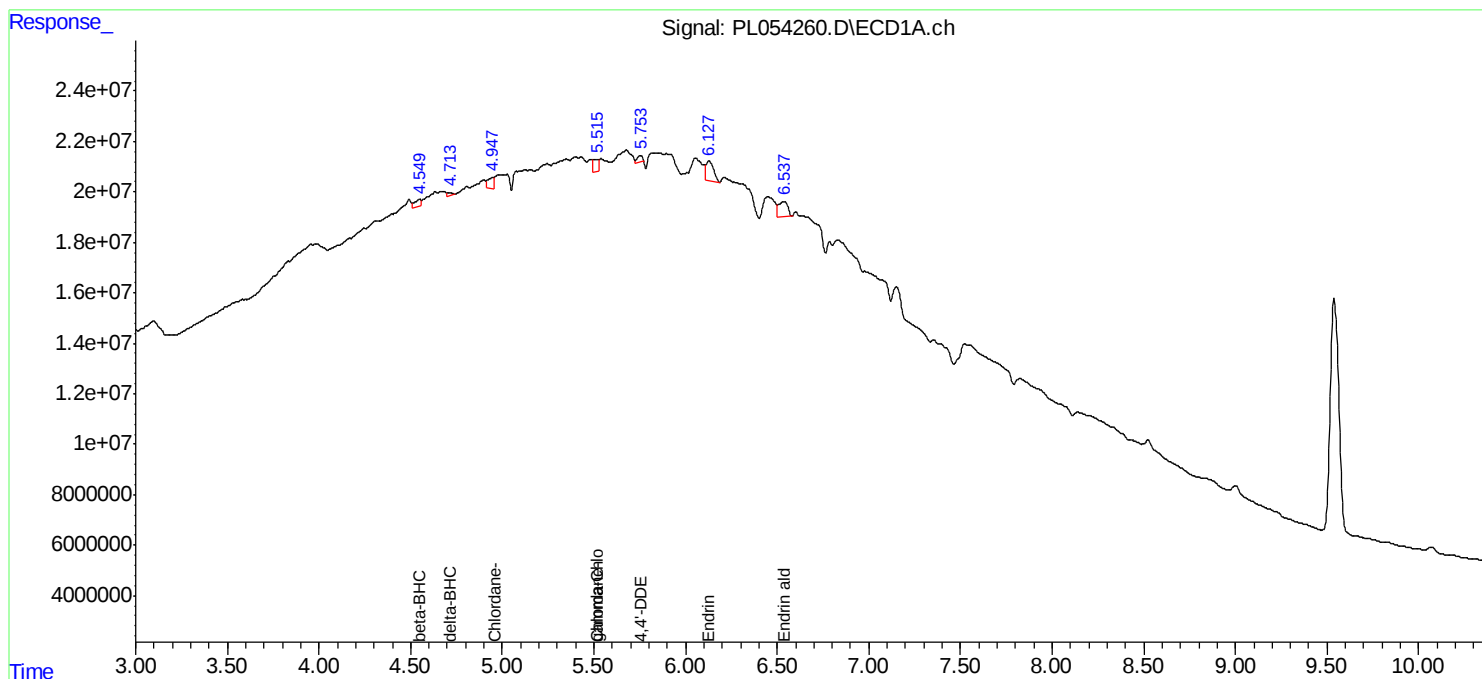


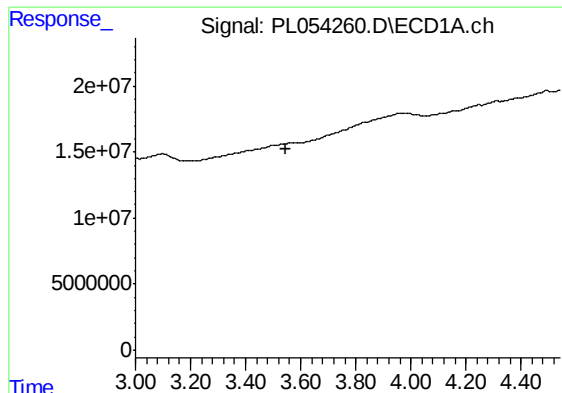

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.544 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

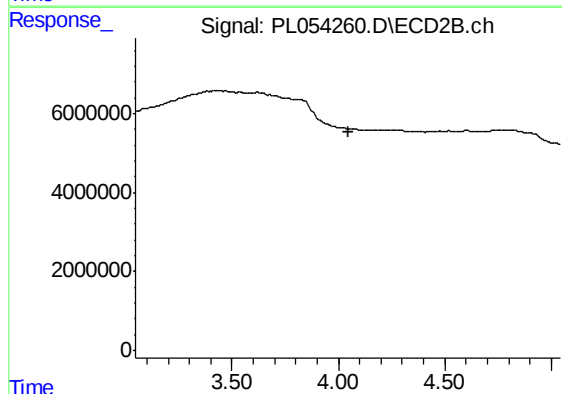


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.046 min
Response: 0
Conc: N.D.

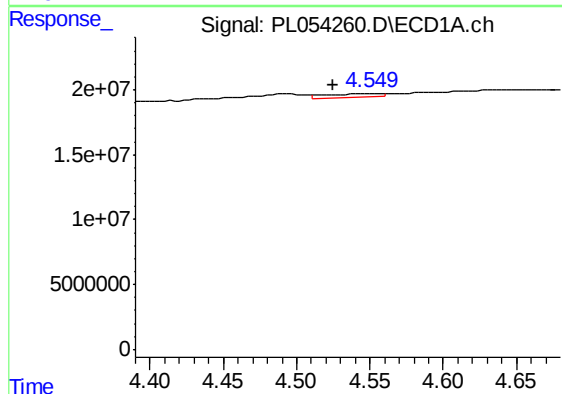


#6 beta-BHC

R.T.: 4.550 min
Delta R.T.: 0.026 min
Response: 6961579
Conc: 1.06 ng/ml

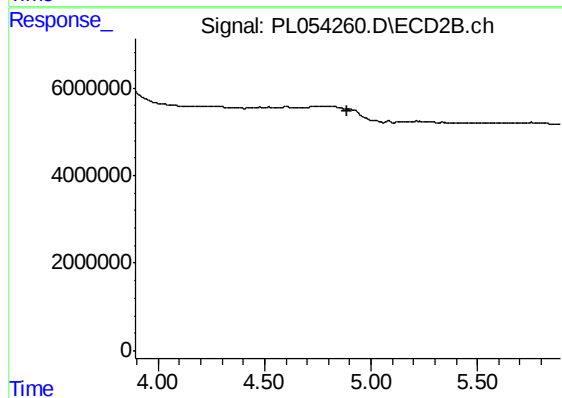

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

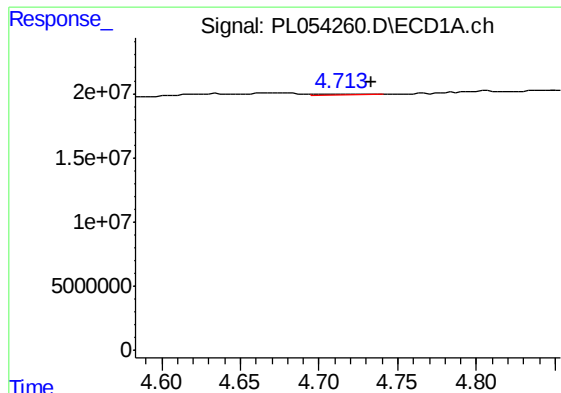

#7 delta-BHC


R.T.: 4.714 min
Delta R.T.: -0.020 min
Response: 2408332
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

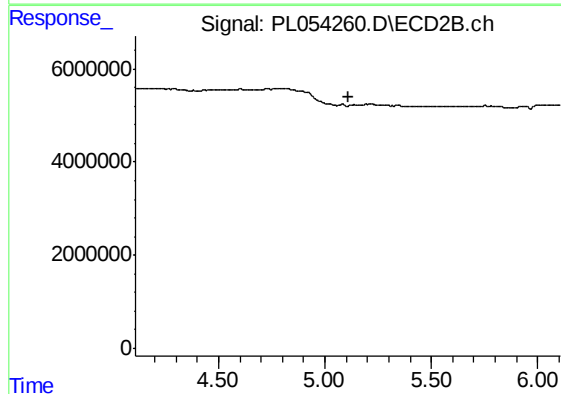


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

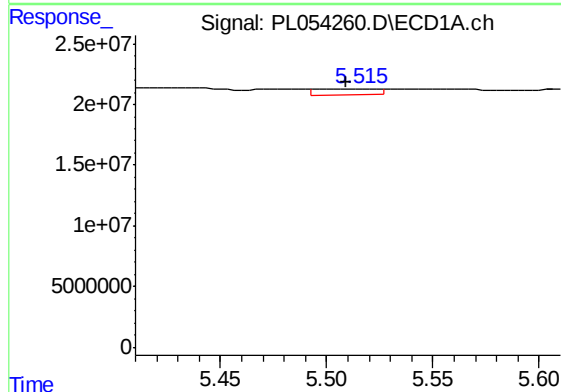


#10 gamma-Chlordane

R.T.: 5.515 min
Delta R.T.: 0.006 min
Response: 9868803
Conc: 0.72 ng/ml

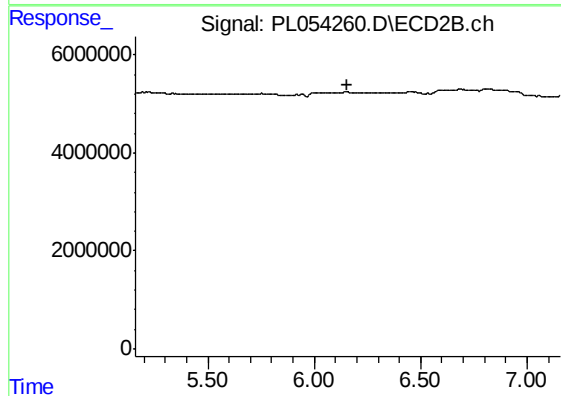

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

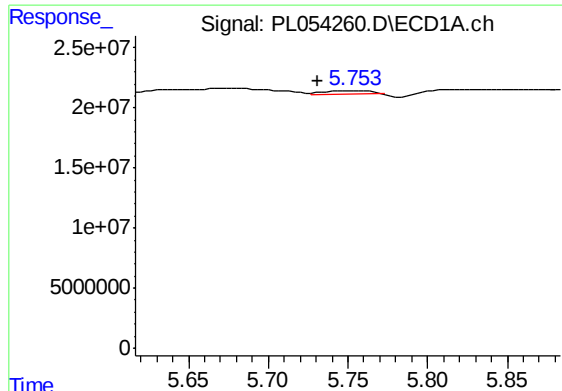

#12 4,4'-DDE


R.T.: 5.754 min
Delta R.T.: 0.023 min
Response: 5695692
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

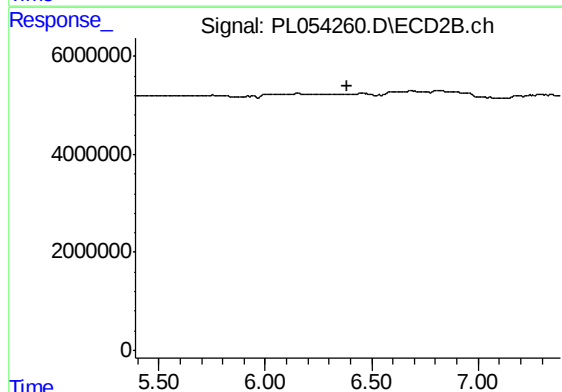


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

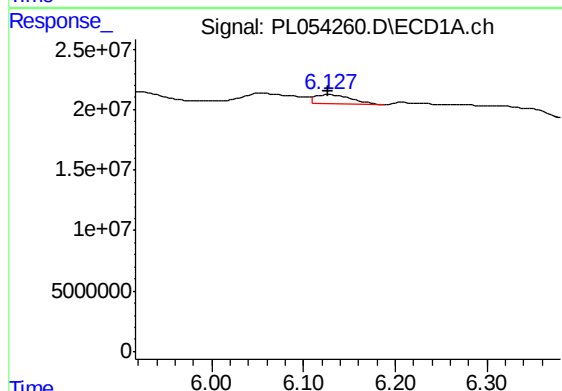


#14 Endrin

R.T.: 6.129 min
Delta R.T.: 0.003 min
Response: 21870156
Conc: 1.89 ng/ml

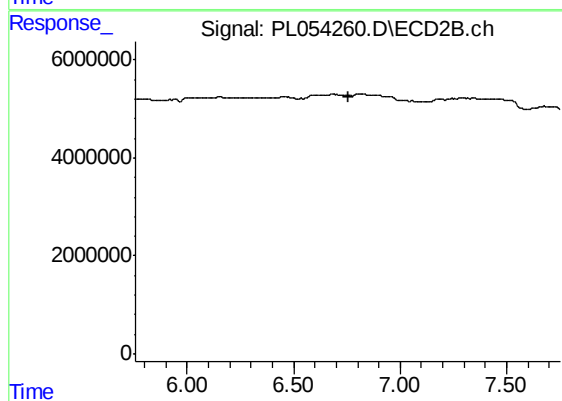

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.756 min
Response: 0
Conc: N.D.

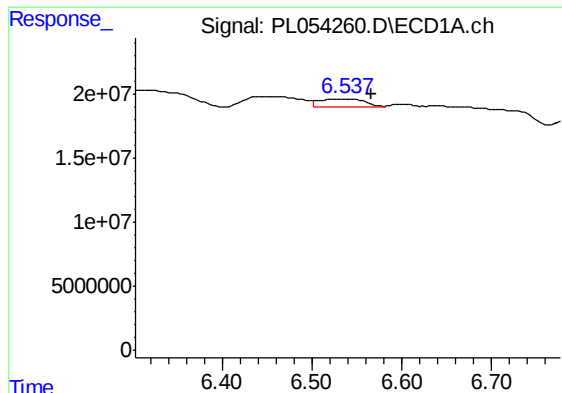

#18 Endrin aldehyde


R.T.: 6.538 min
Delta R.T.: -0.028 min
Response: 21041037
Conc: 2.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

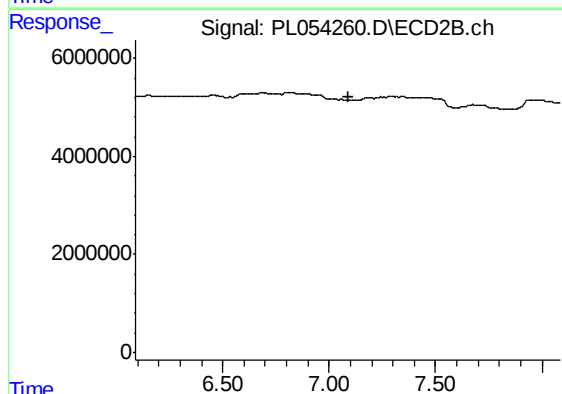


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

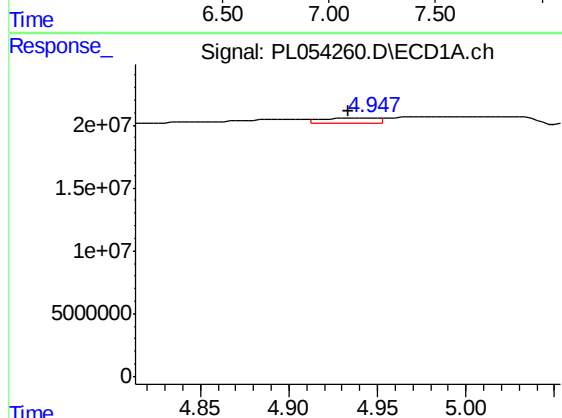


#24 Chlordane-2

R.T.: 4.948 min
Delta R.T.: 0.014 min
Response: 9491807
Conc: 24.63 ng/ml

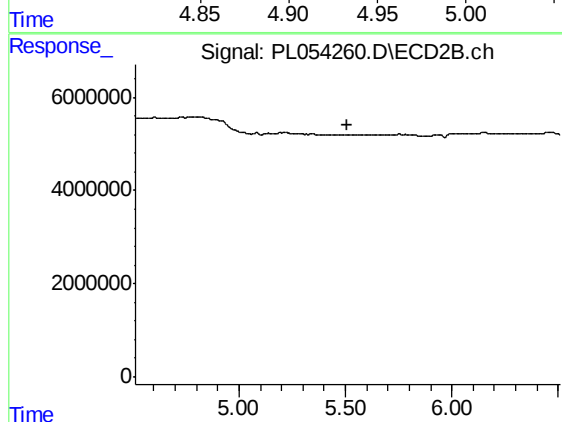

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.510 min
Response: 0
Conc: N.D.

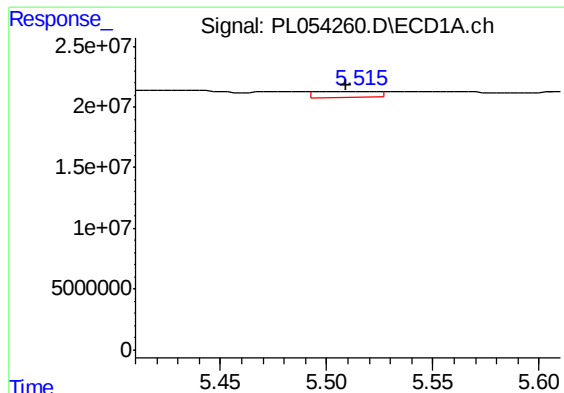

#25 Chlordane-3


R.T.: 5.515 min
Delta R.T.: 0.007 min
Response: 9868803
Conc: 8.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

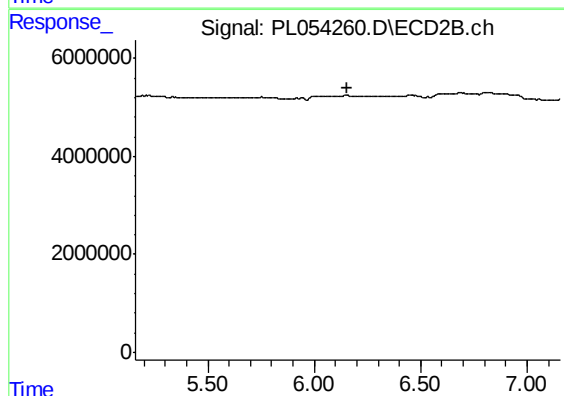


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

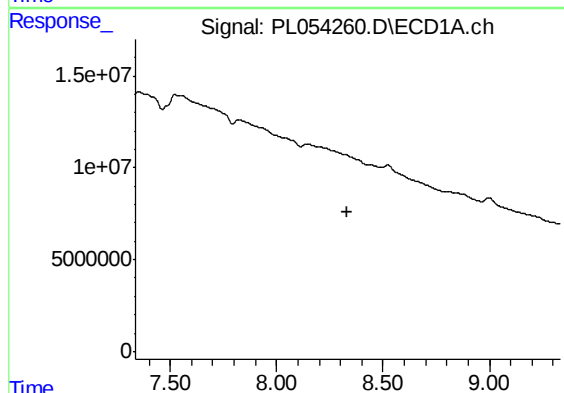

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.334 min
Response: 0
Conc: N.D.

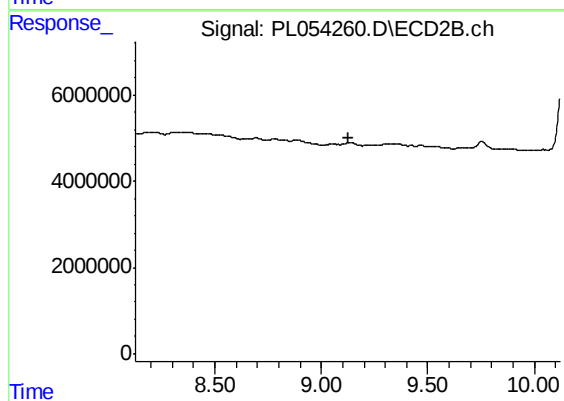

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.126 min
Response: 0
Conc: N.D.