

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
 Data File : PL054277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2019 12:26
 Operator : SG\AJ
 Sample : K5832-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 8-(6-8)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 00:21:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.043	225.0E6	51033790	20.761	20.394
28)	SA Decachlor...	8.322	9.121	182.8E6	50530484	18.633	17.944
Target Compounds							
2)	A alpha-BHC	3.985	0.000	8280961	0	0.475	N.D. #
8)	B Heptachlo...	0.000	5.913	0	5863449	N.D.	2.011 #
9)	A Endosulfan I	0.000	6.276	0	14725483	N.D.	5.431 #
11)	B alpha-Chl...	5.550f	0.000	82564211	0	6.206	N.D. #
12)	B 4,4'-DDE	5.736	0.000	4743312	0	0.399	N.D. #
15)	B Endosulfa...	0.000	6.975	0	4470676	N.D.	1.750 #
21)	B Endrin ke...	0.000	7.770	0	2003782	N.D.	0.777 #
26)	Chlordane-4	5.550f	0.000	82564211	0	88.073	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
Data File : PL054277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2019 12:26
Operator : SG\AJ
Sample : K5832-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
8-(6-8)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 00:21:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

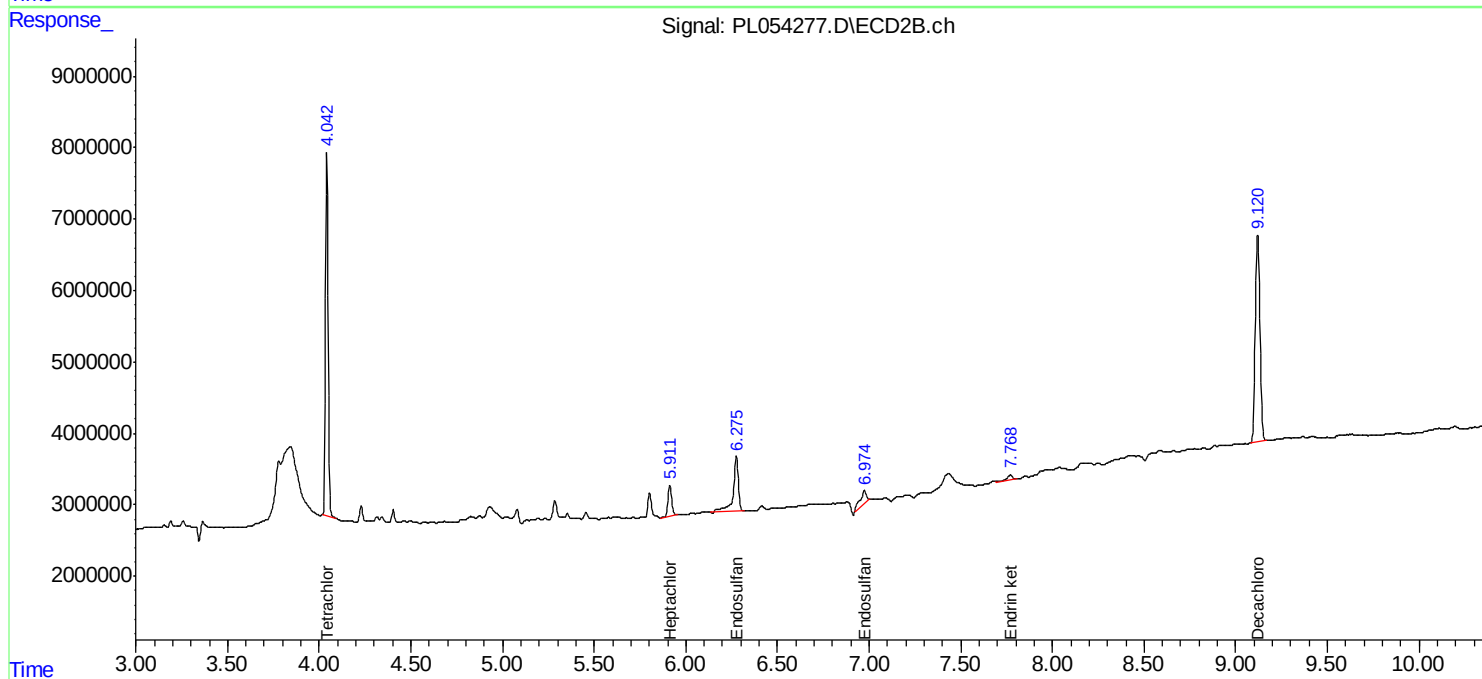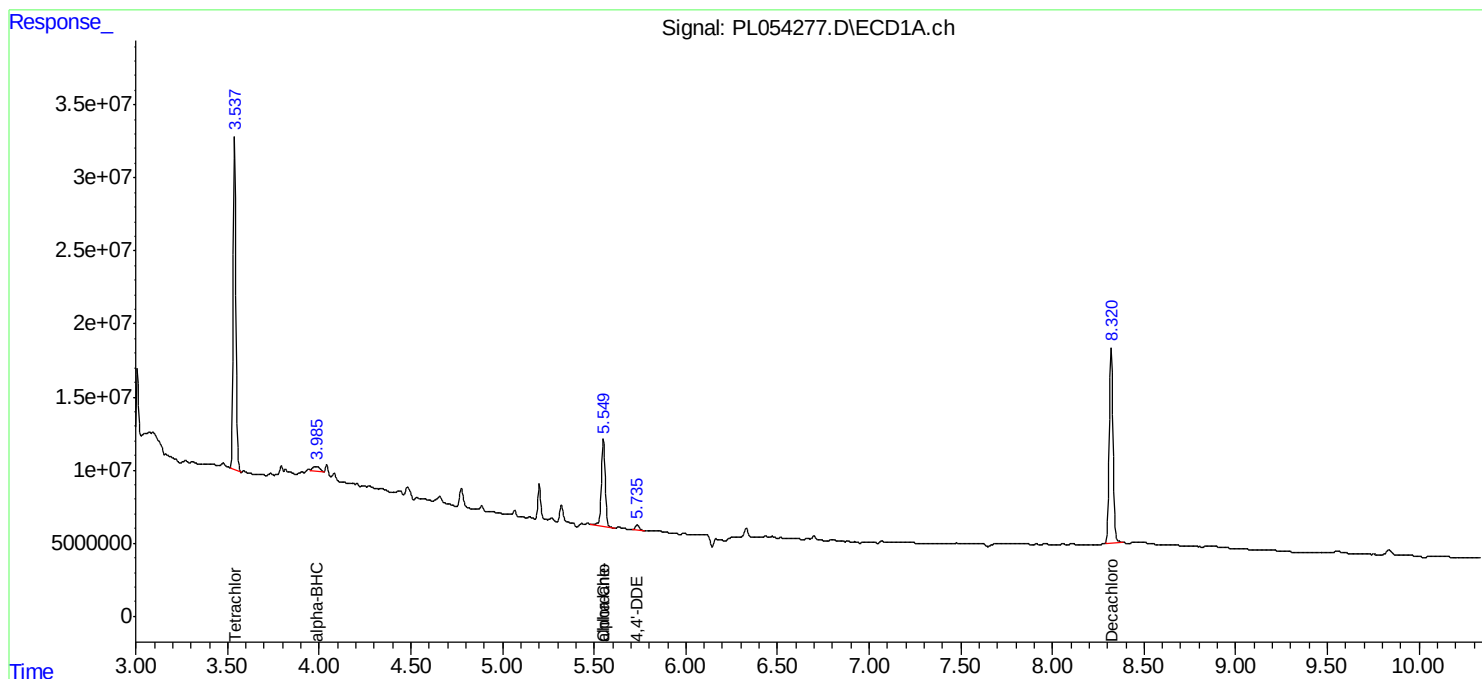


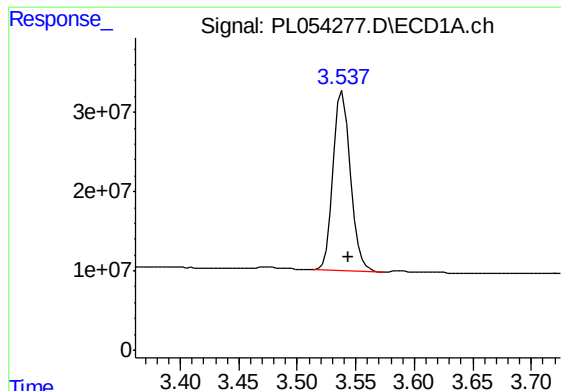

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: -0.005 min
Response: 225035936
Conc: 20.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
8-(6-8)

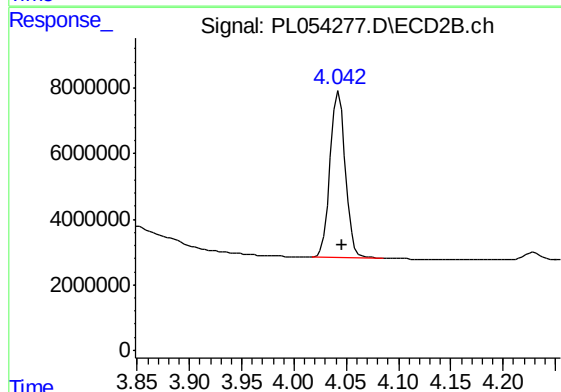


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 51033790
Conc: 20.39 ng/ml

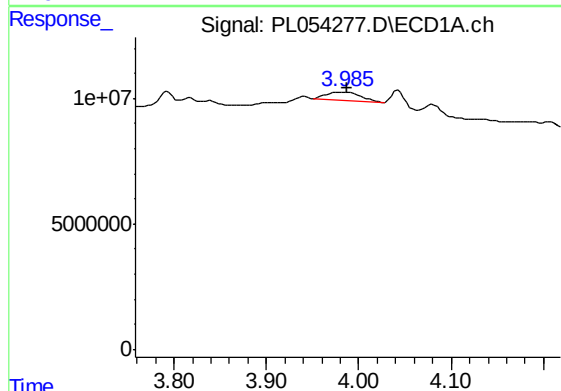


#2 alpha-BHC

R.T.: 3.985 min
Delta R.T.: -0.003 min
Response: 8280961
Conc: 0.47 ng/ml

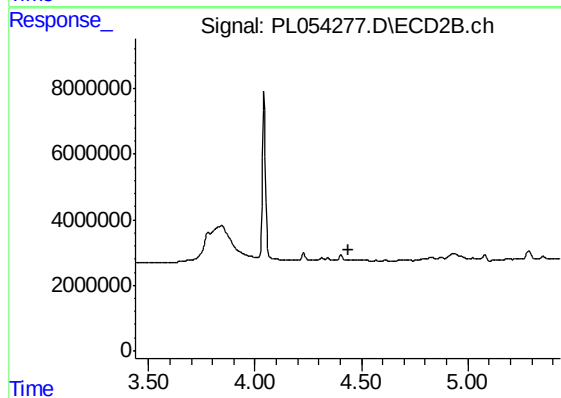

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.437 min
Response: 0
Conc: N.D.

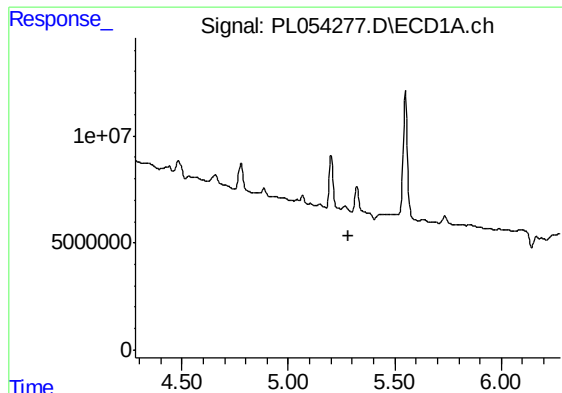

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.280 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
8-(6-8)

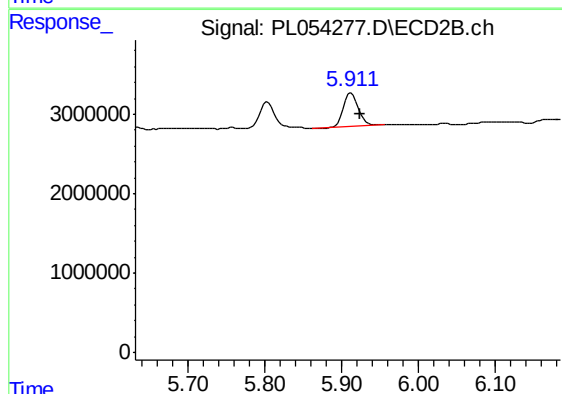


#8 Heptachlor epoxide

R.T.: 5.913 min
Delta R.T.: -0.012 min
Response: 5863449
Conc: 2.01 ng/ml

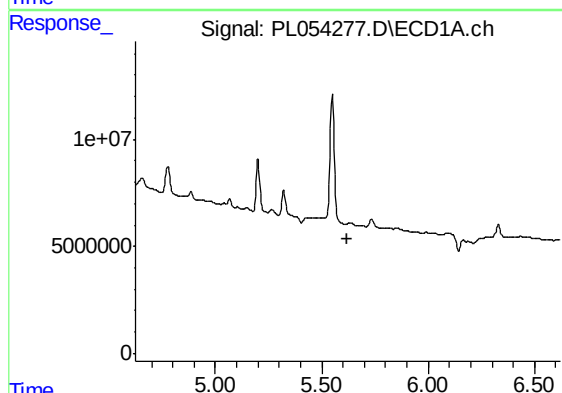


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.623 min
Response: 0
Conc: N.D.

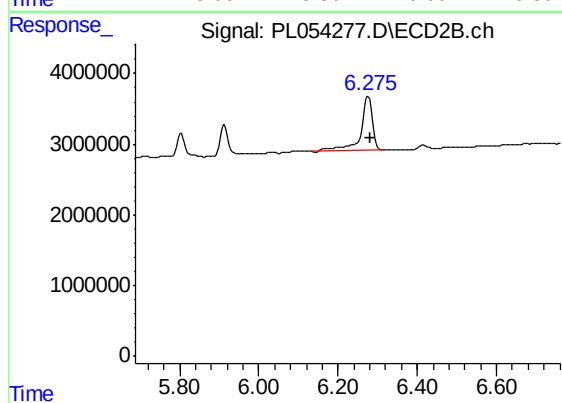

#9 Endosulfan I


R.T.: 6.276 min
Delta R.T.: -0.005 min
Response: 14725483
Conc: 5.43 ng/ml

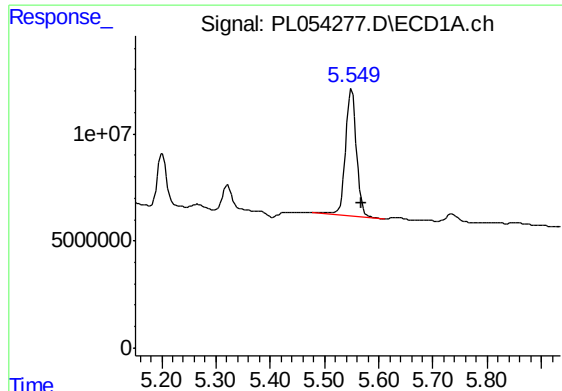

#11 alpha-Chlordane


R.T.: 5.550 min
Delta R.T.: -0.018 min
Response: 82564211
Conc: 6.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
8-(6-8)

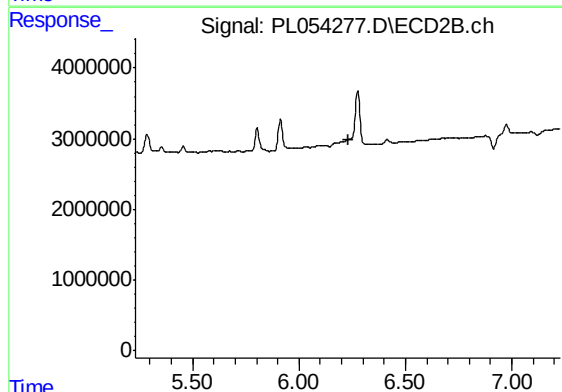


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

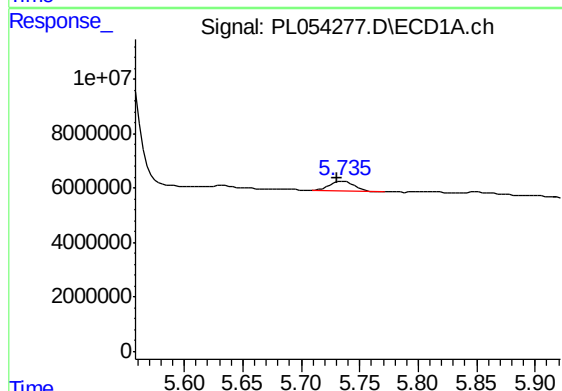


#12 4,4'-DDE

R.T.: 5.736 min
Delta R.T.: 0.005 min
Response: 4743312
Conc: 0.40 ng/ml

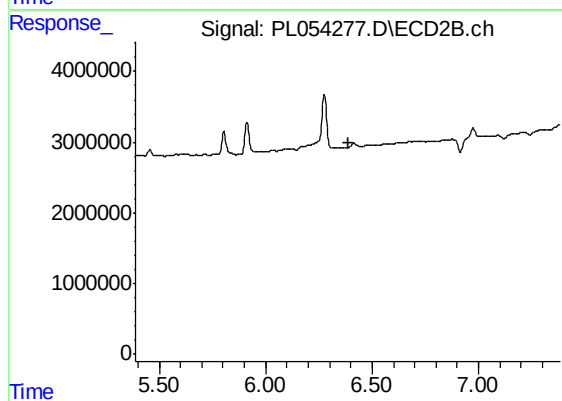

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

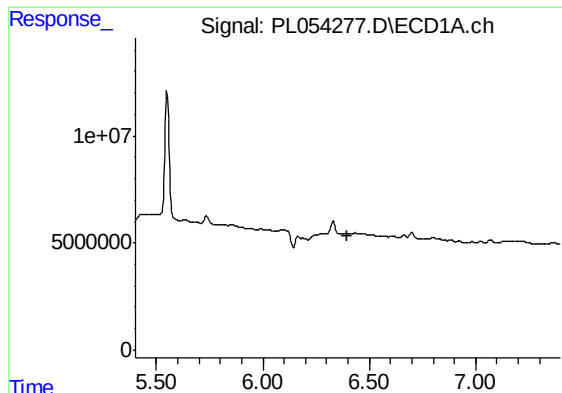

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
8-(6-8)

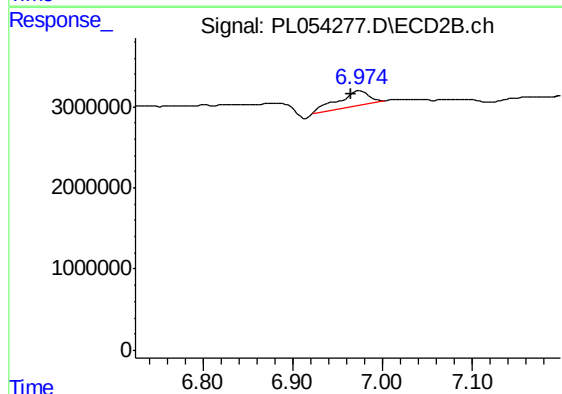


#15 Endosulfan II

R.T.: 6.975 min
Delta R.T.: 0.010 min
Response: 4470676
Conc: 1.75 ng/ml

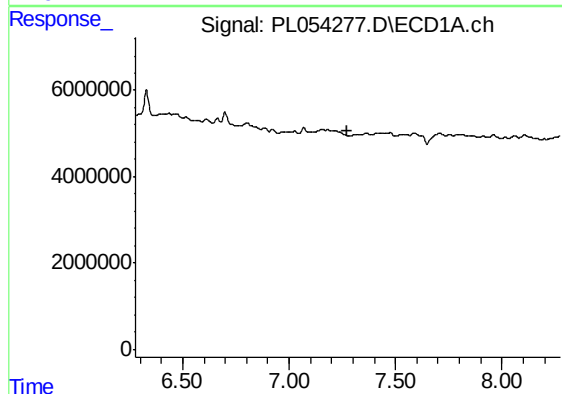


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.275 min
Response: 0
Conc: N.D.

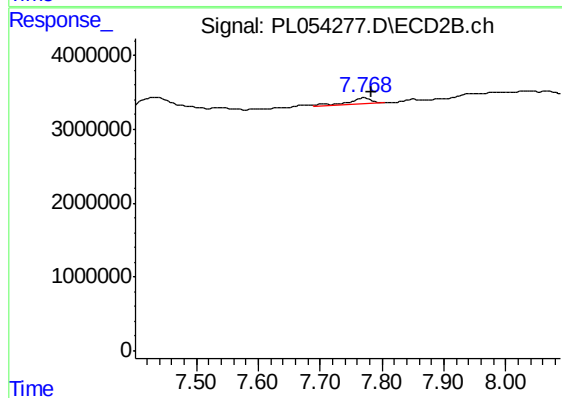

#21 Endrin ketone


R.T.: 7.770 min
Delta R.T.: -0.013 min
Response: 2003782
Conc: 0.78 ng/ml

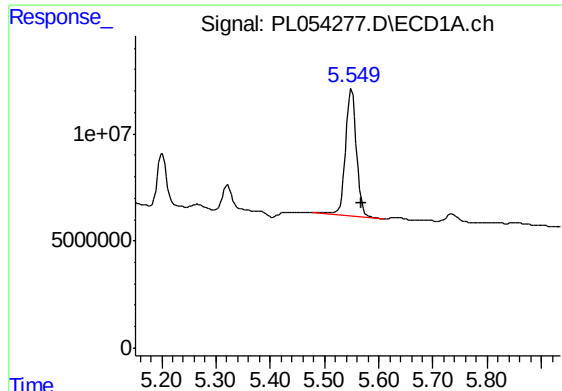

#26 Chlordane-4


R.T.: 5.550 min
Delta R.T.: -0.018 min
Response: 82564211
Conc: 88.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
8-(6-8)

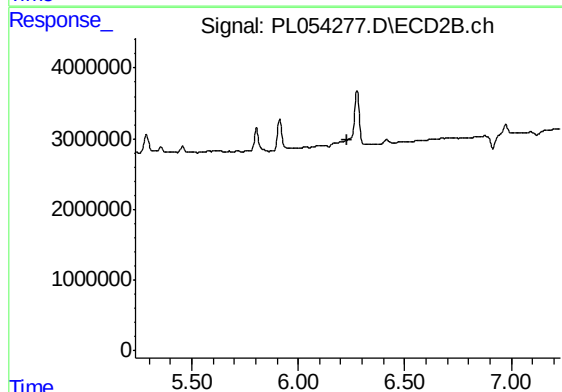


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

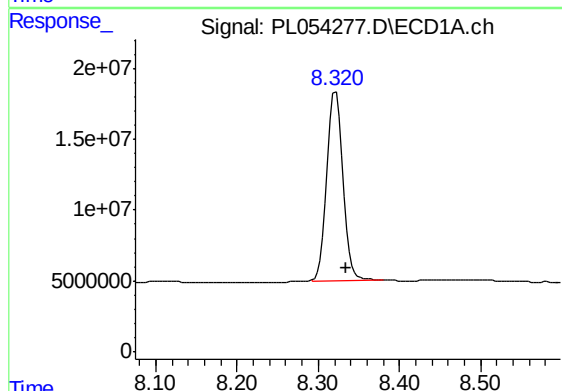

#28 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: -0.012 min
Response: 182817516
Conc: 18.63 ng/ml

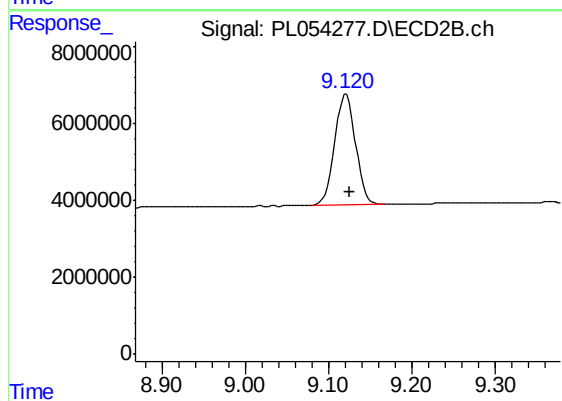

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 50530484
Conc: 17.94 ng/ml