

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
 Data File : PL054325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2019 00:09
 Operator : SG\AJ
 Sample : K5863-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 02:43:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.043	226.8E6	53818047	20.924	21.507
28)	SA Decachlor...	8.322	9.121	174.5E6	51458661	17.782	18.274
Target Compounds							
9)	A Endosulfan I	5.636	0.000	13660014	0	1.111	N.D. #
12)	B 4,4'-DDE	5.722	6.382	17876162	3378482	1.504	1.200
13)	MA Dieldrin	5.857	0.000	7187503	0	0.551	N.D. #
15)	B Endosulfa...	0.000	6.968	0	4912225	N.D.	1.923 #
16)	A 4,4'-DDD	6.239	0.000	6141607	0	0.690	N.D. #
17)	MA 4,4'-DDT	6.481	7.173	4491302	6301821	0.453	2.725 #
23)	Chlordane-1	4.426	0.000	9213857	0	25.979	N.D. #
27)	Chlordane-5	0.000	7.046	0	4692752	N.D.	61.385 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
Data File : PL054325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2019 00:09
Operator : SG\AJ
Sample : K5863-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 02:43:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

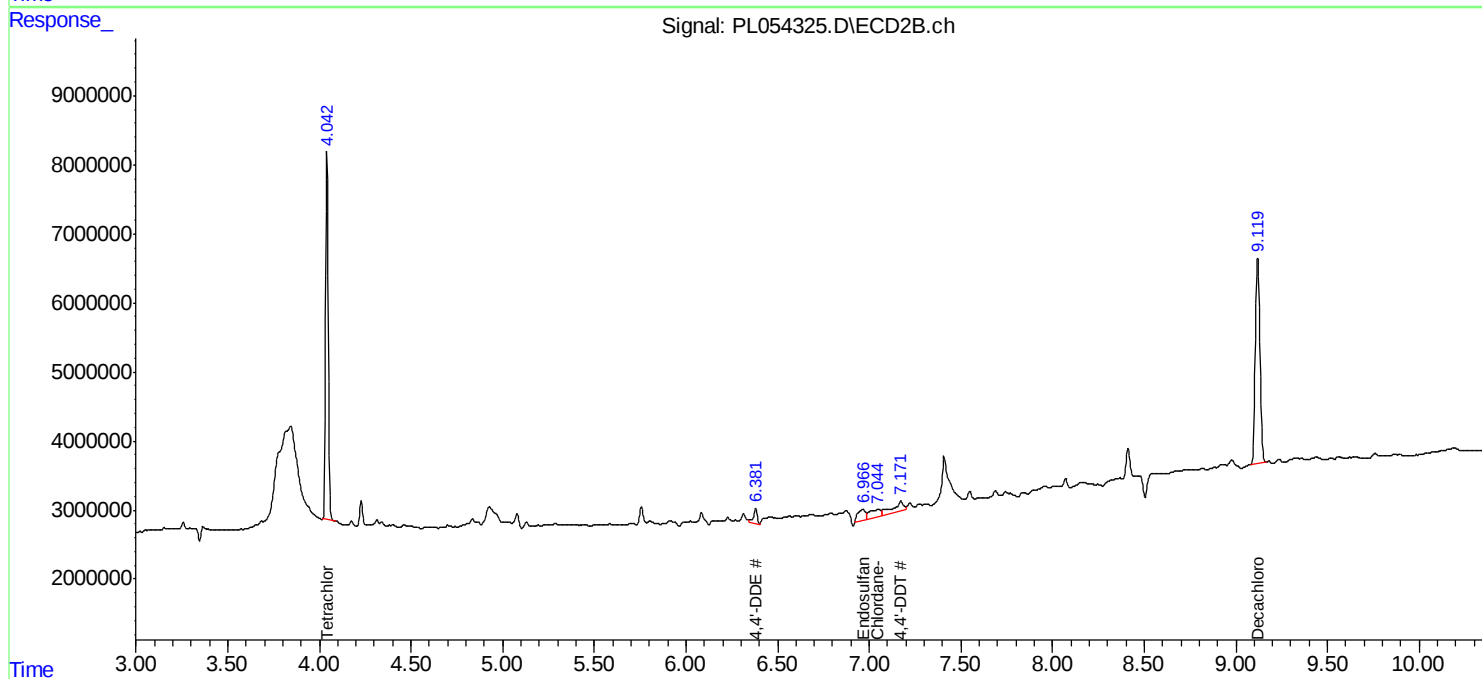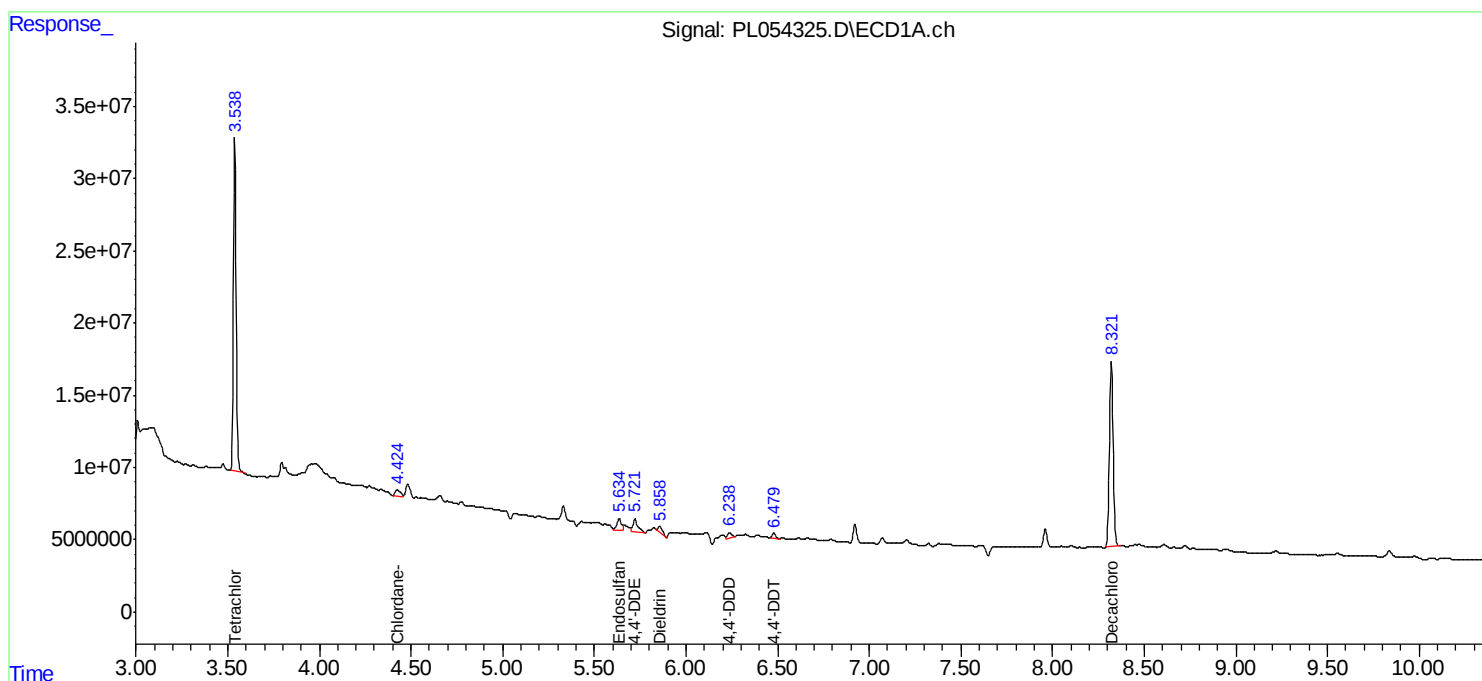


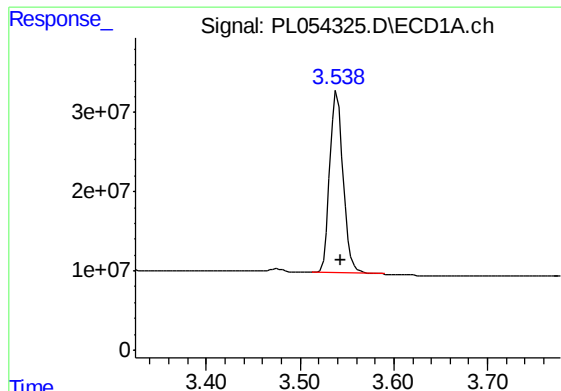

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 226799526
Conc: 20.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP

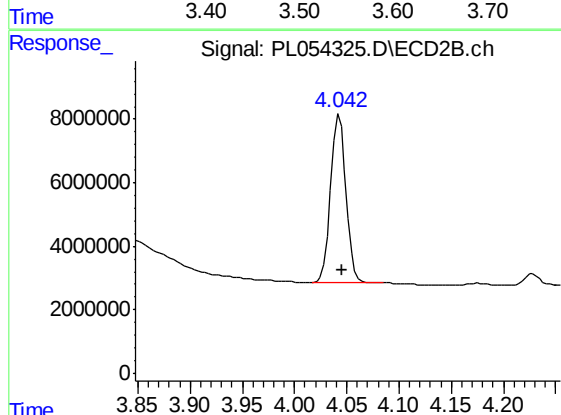


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 53818047
Conc: 21.51 ng/ml

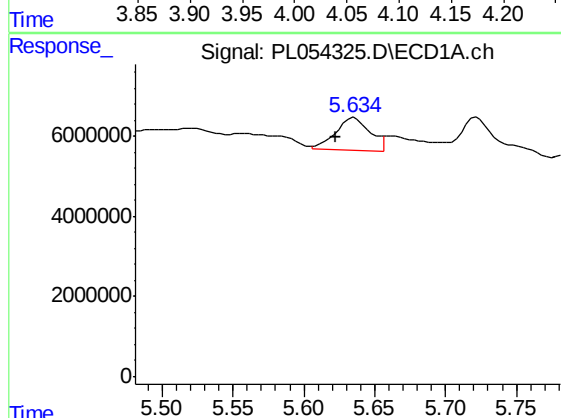


#9 Endosulfan I

R.T.: 5.636 min
Delta R.T.: 0.013 min
Response: 13660014
Conc: 1.11 ng/ml

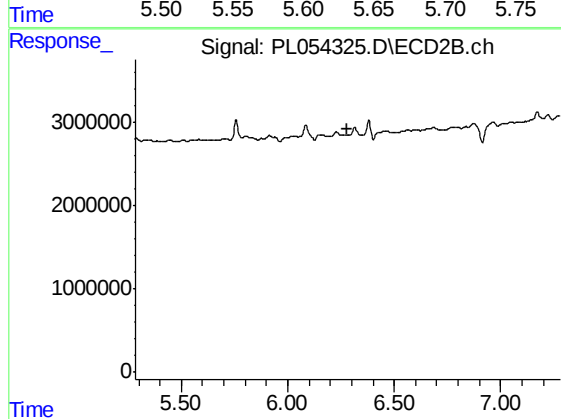

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

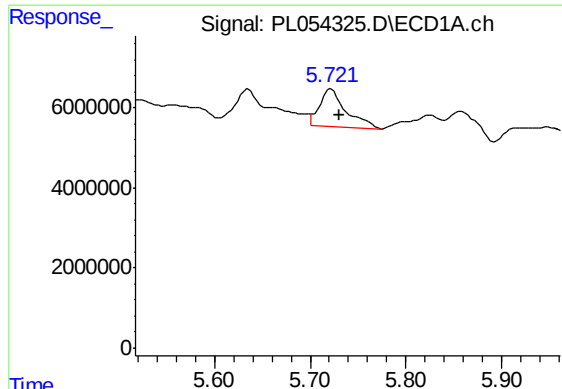

#12 4,4'-DDE


R.T.: 5.722 min
Delta R.T.: -0.009 min
Response: 17876162
Conc: 1.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP

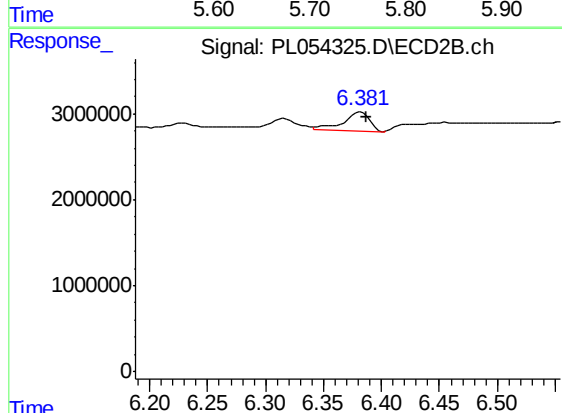


#12 4,4'-DDE

R.T.: 6.382 min
Delta R.T.: -0.005 min
Response: 3378482
Conc: 1.20 ng/ml

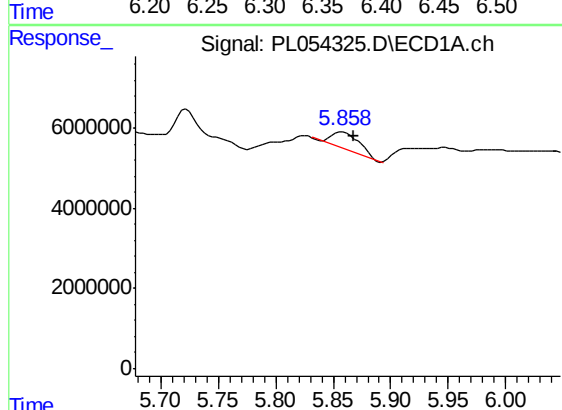


#13 Dieldrin

R.T.: 5.857 min
Delta R.T.: -0.011 min
Response: 7187503
Conc: 0.55 ng/ml

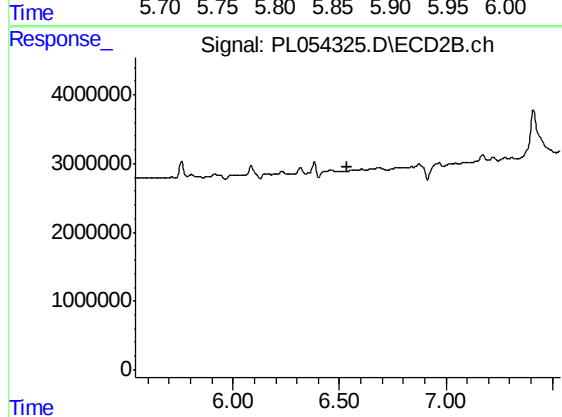

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.538 min
Response: 0
Conc: N.D.

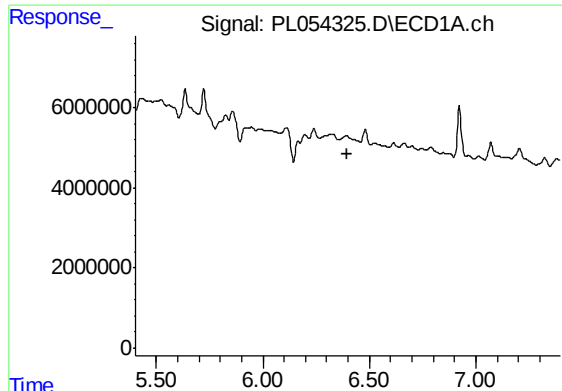

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP

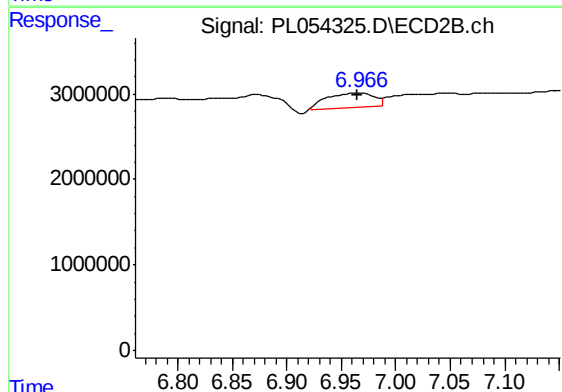


#15 Endosulfan II

R.T.: 6.968 min
Delta R.T.: 0.003 min
Response: 4912225
Conc: 1.92 ng/ml

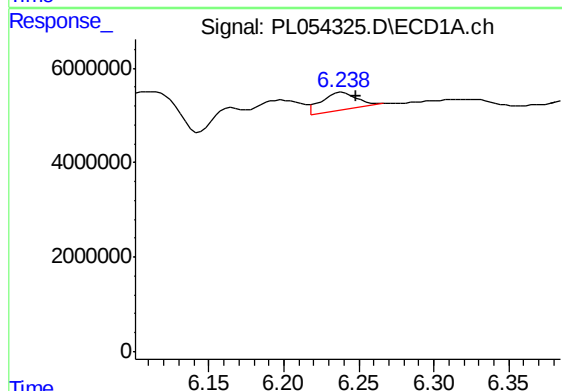


#16 4,4'-DDD

R.T.: 6.239 min
Delta R.T.: -0.009 min
Response: 6141607
Conc: 0.69 ng/ml

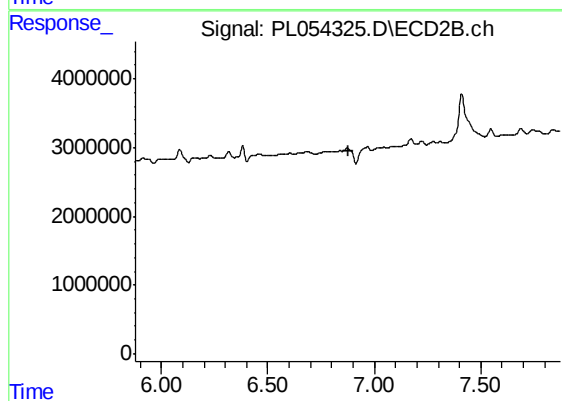

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.877 min
Response: 0
Conc: N.D.

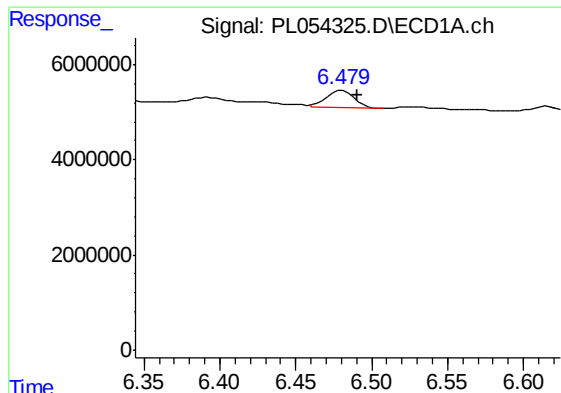

#17 4,4'-DDT


R.T.: 6.481 min
Delta R.T.: -0.010 min
Response: 4491302
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP

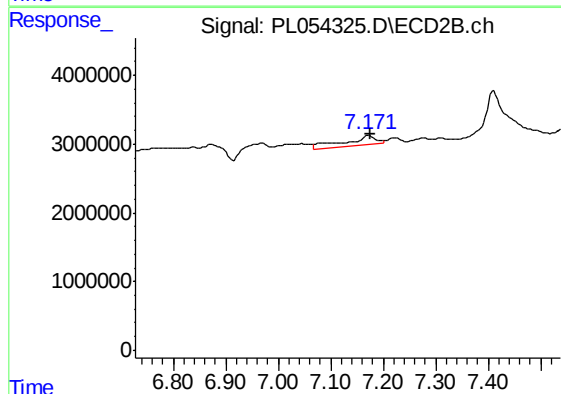


#17 4,4'-DDT

R.T.: 7.173 min
Delta R.T.: -0.003 min
Response: 6301821
Conc: 2.73 ng/ml

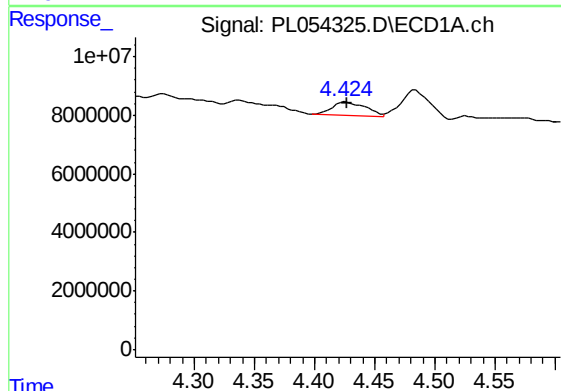


#23 Chlordane-1

R.T.: 4.426 min
Delta R.T.: -0.002 min
Response: 9213857
Conc: 25.98 ng/ml

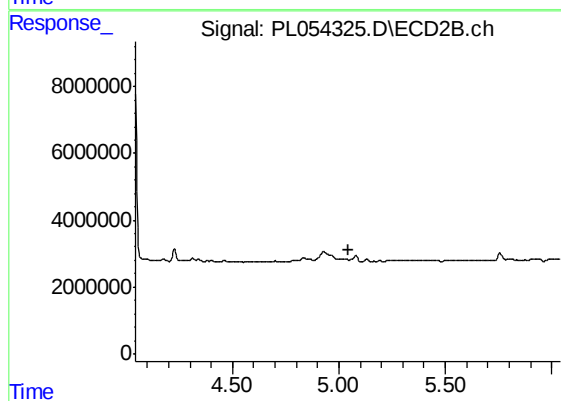

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

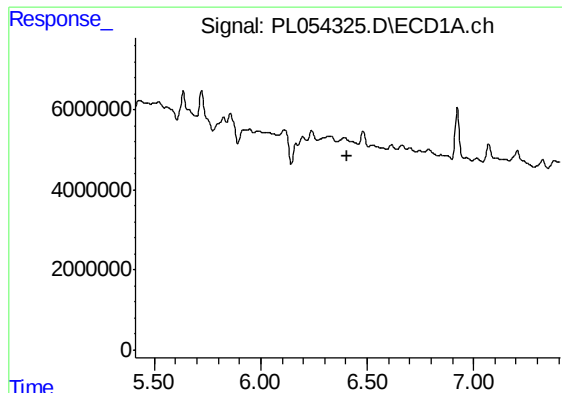

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP

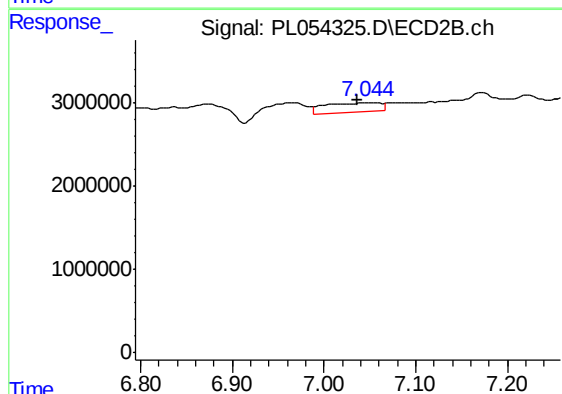


#27 Chlordane-5

R.T.: 7.046 min
Delta R.T.: 0.009 min
Response: 4692752
Conc: 61.38 ng/ml

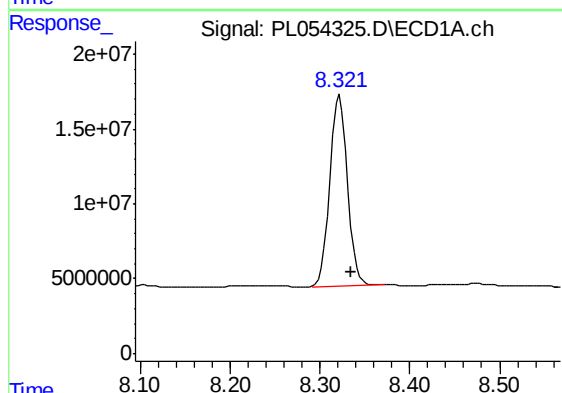

#28 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: -0.012 min
Response: 174472396
Conc: 17.78 ng/ml

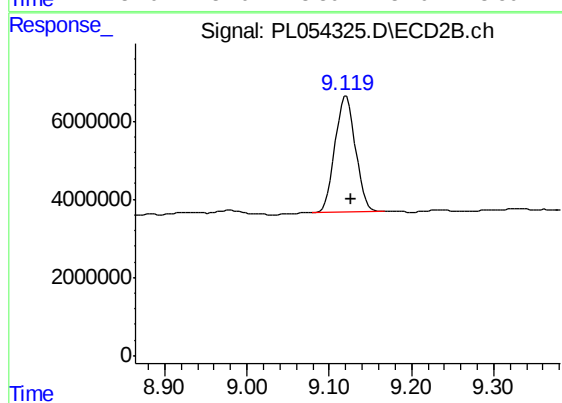

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.006 min
Response: 51458661
Conc: 18.27 ng/ml