

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
 Data File : PL054311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2019 20:39
 Operator : SG\AJ
 Sample : K5833-07
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 7-(10-12)

Manual Integrations
 APPROVED

Ankita
 11/18/2019 3:17:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 02:32:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.043	222.4E6	50796410	20.515	20.299
28)	SA Decachlor...	8.320	9.122	182.3E6	52301878	18.578m	18.573
Target Compounds							
9)	A Endosulfan I	5.636	6.275	83919660	2500328	6.827	0.922m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
Data File : PL054311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2019 20:39
Operator : SG\AJ
Sample : K5833-07
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
7-(10-12)


Manual Integrations
APPROVED

Ankita
11/18/2019 3:17:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 02:32:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

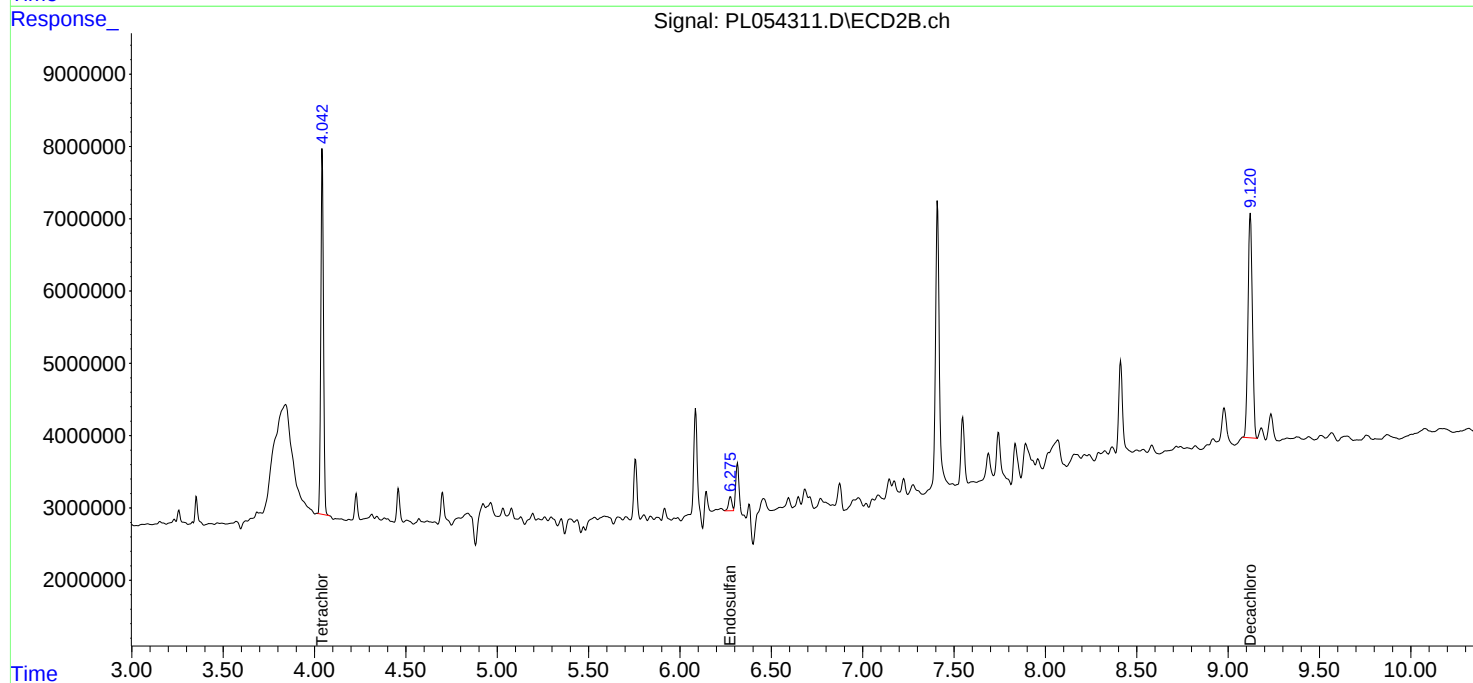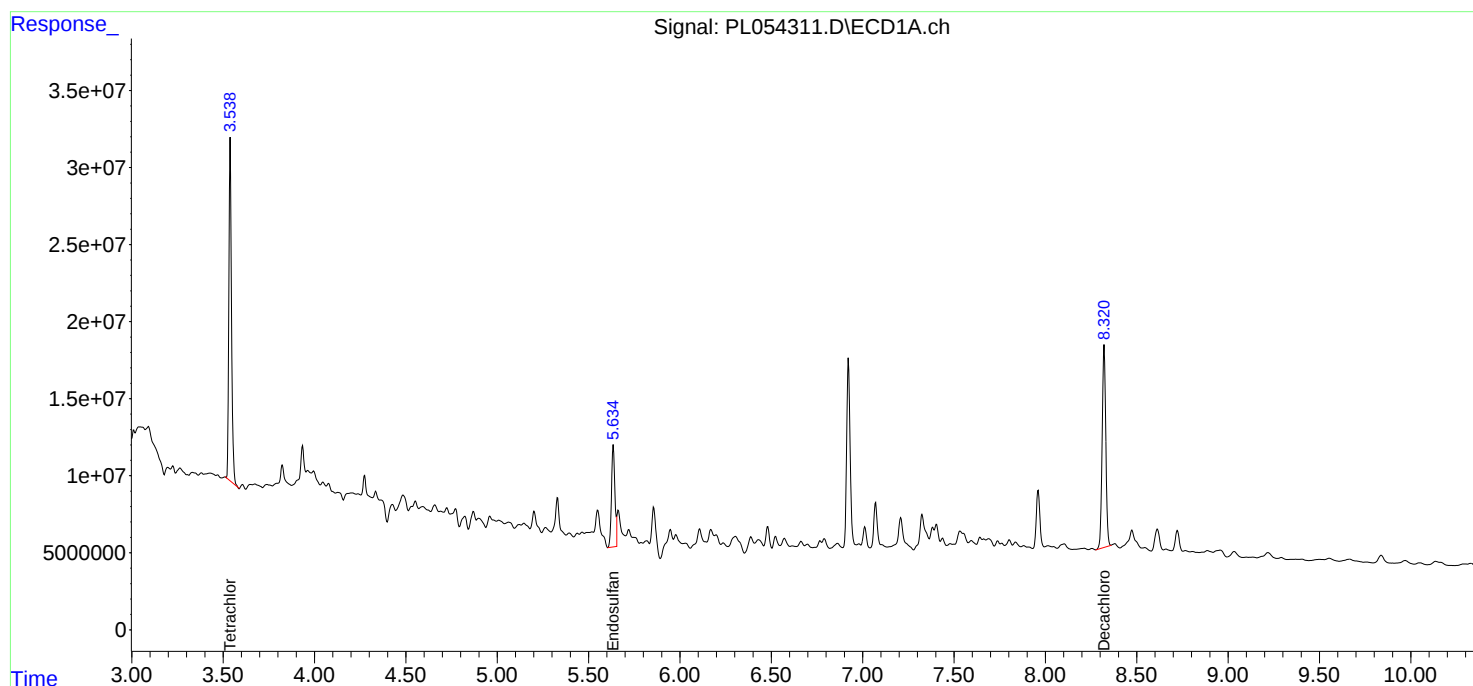

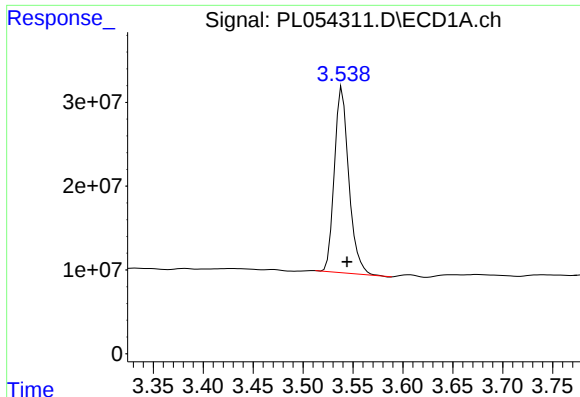


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.005 min
Response: 222369745
Conc: 20.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
7-(10-12)


Manual Integrations
APPROVED

Ankita
11/18/2019 3:17:31 PM

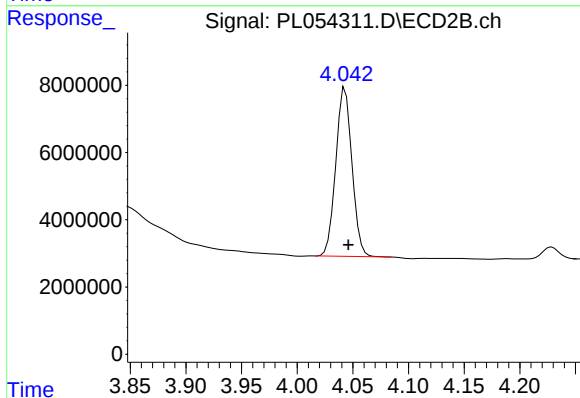


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 50796410
Conc: 20.30 ng/ml

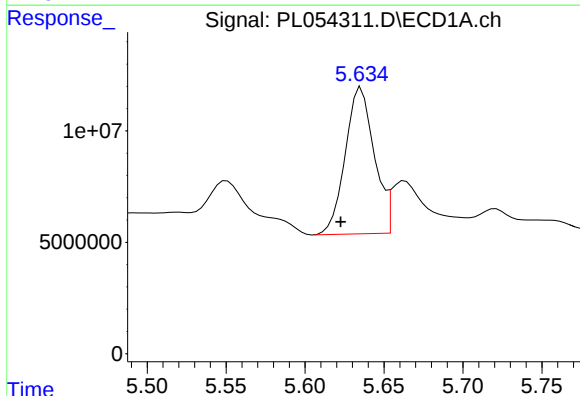


#9 Endosulfan I

R.T.: 5.636 min
Delta R.T.: 0.013 min
Response: 83919660
Conc: 6.83 ng/ml

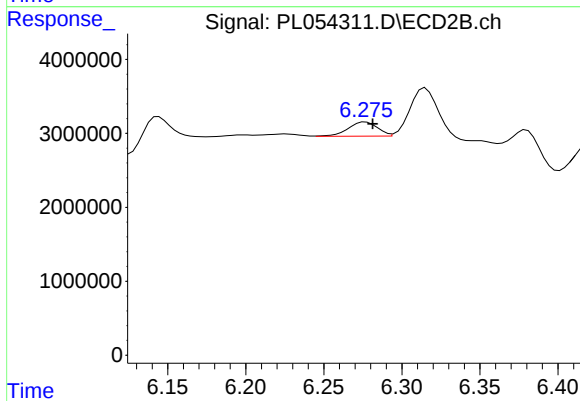

#9 Endosulfan I

R.T.: 6.275 min
Delta R.T.: -0.006 min
Response: 2500328
Conc: 0.92 ng/ml m

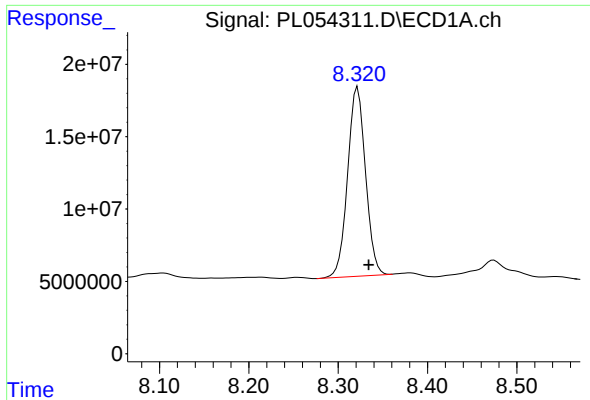


#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.014 min
Response: 182275490
Conc: 18.58 ng/ml m

Instrument :
ECD_L
ClientSampleId :
7-(10-12)

Manual Integrations
APPROVED

Ankita
11/18/2019 3:17:31 PM

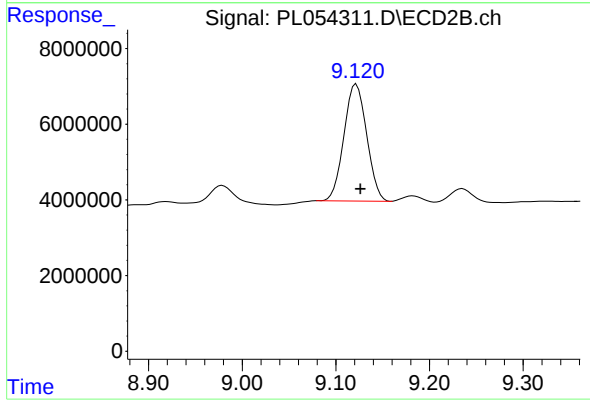

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 52301878
Conc: 18.57 ng/ml