

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
 Data File : PL054325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2019 00:09
 Operator : SG\AJ
 Sample : K5863-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-COMP

Manual Integrations
 APPROVED

Ankita
 11/18/2019 3:17:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 02:43:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.043	226.8E6	53818047	20.924	21.507
28)	SA Decachlor...	8.322	9.121	174.5E6	51458661	17.782	18.274
Target Compounds							
12)	B 4,4'-DDE	5.721	6.382	8316019	3378482	0.700m	1.200 #
17)	MA 4,4'-DDT	6.479	7.171	4675184	1711147	0.472m	0.740m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
Data File : PL054325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2019 00:09
Operator : SG\AJ
Sample : K5863-05
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-1-COMP


Manual Integrations
APPROVED

Ankita
11/18/2019 3:17:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 02:43:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

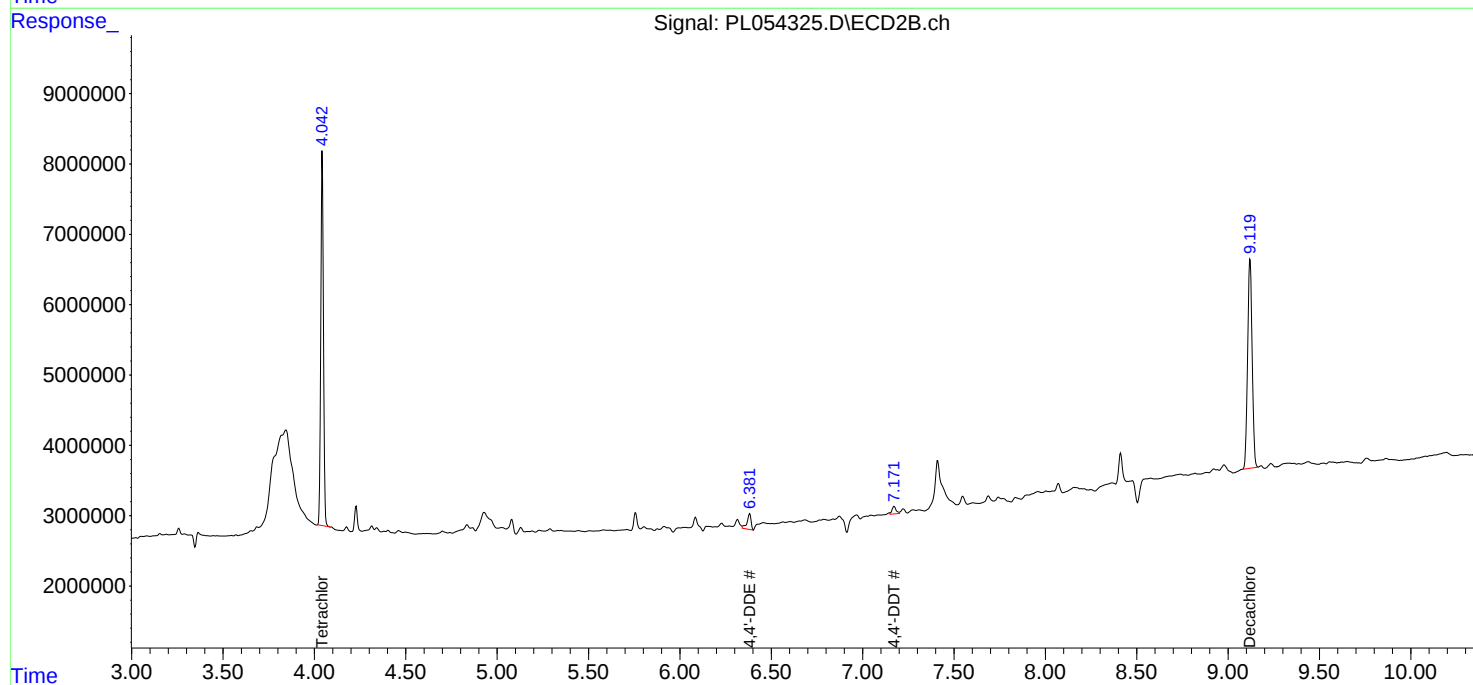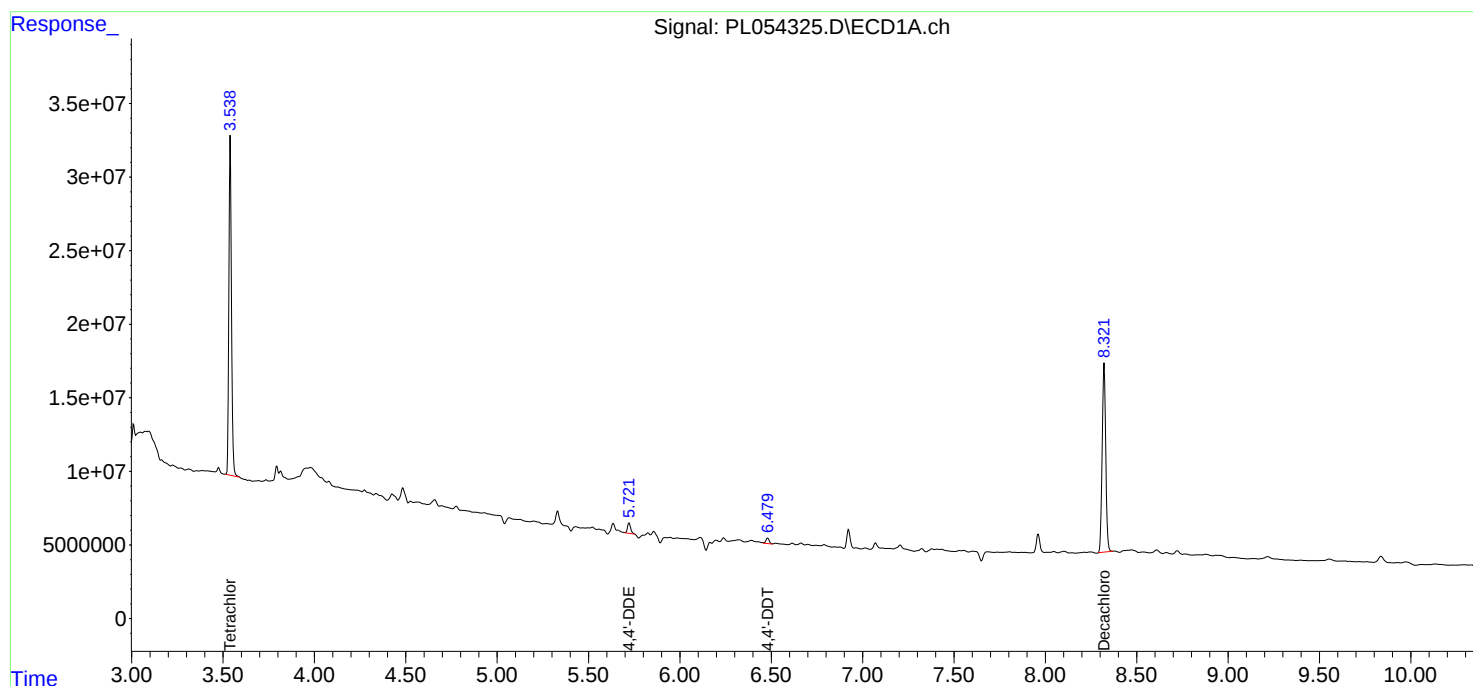

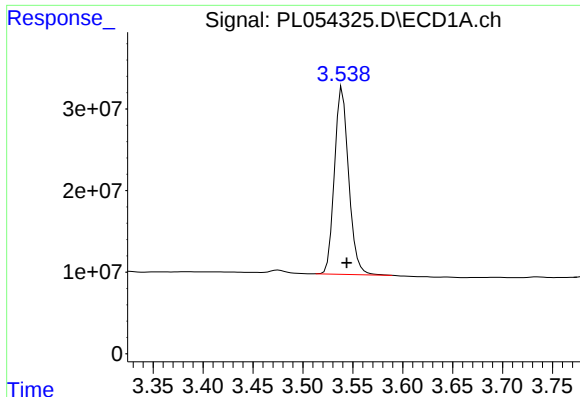


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 226799526
Conc: 20.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP


Manual Integrations
APPROVED

Ankita
11/18/2019 3:17:45 PM

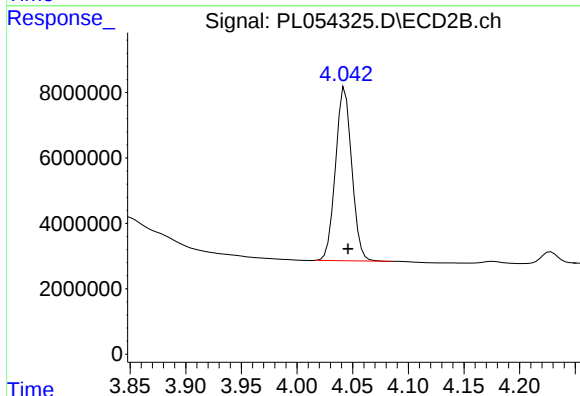


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 53818047
Conc: 21.51 ng/ml

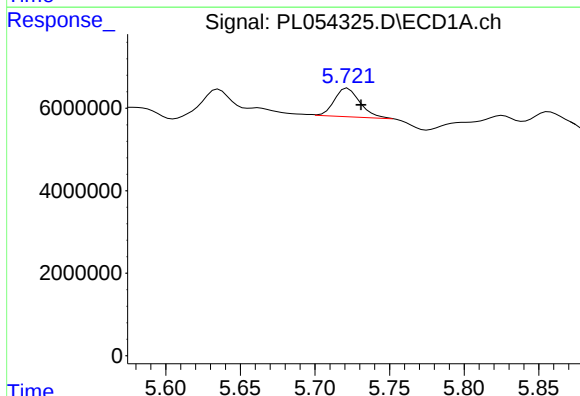


#12 4,4'-DDE

R.T.: 5.721 min
Delta R.T.: -0.010 min
Response: 8316019
Conc: 0.70 ng/ml m

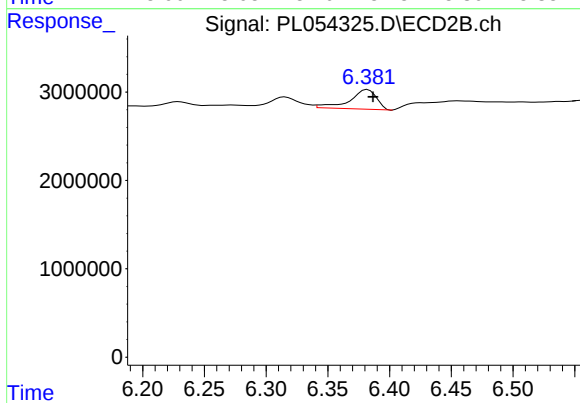

#12 4,4'-DDE

R.T.: 6.382 min
Delta R.T.: -0.005 min
Response: 3378482
Conc: 1.20 ng/ml

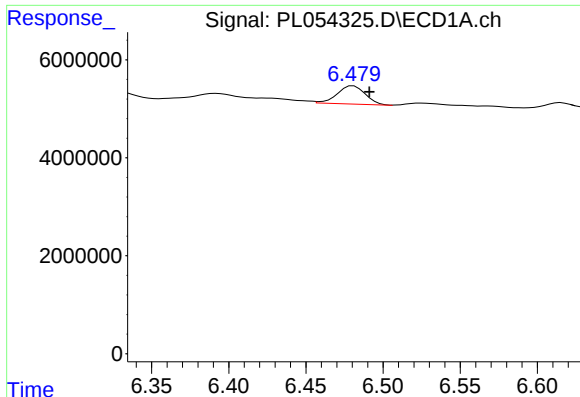


#17 4,4'-DDT

R.T.: 6.479 min
Delta R.T.: -0.012 min
Response: 4675184
Conc: 0.47 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP


Manual Integrations
APPROVED

Ankita
11/18/2019 3:17:45 PM

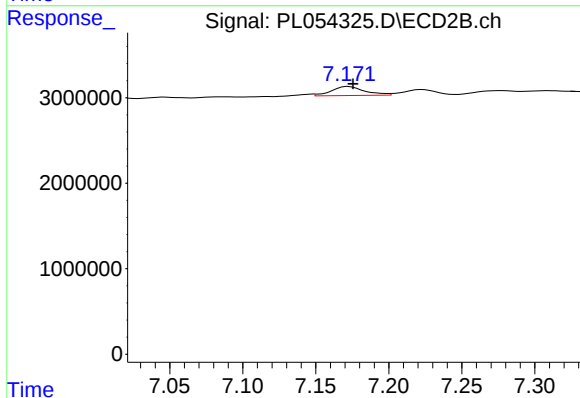


#17 4,4'-DDT

R.T.: 7.171 min
Delta R.T.: -0.005 min
Response: 1711147
Conc: 0.74 ng/ml m

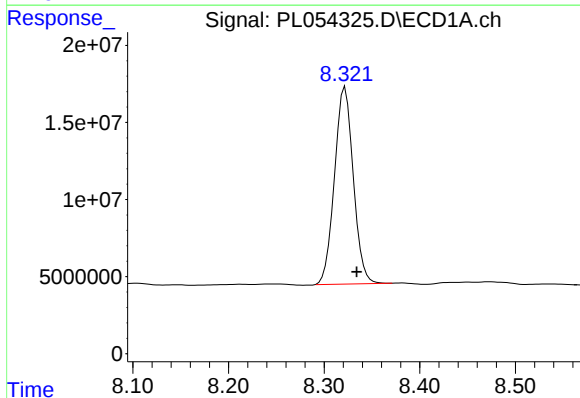

#28 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: -0.012 min
Response: 174472396
Conc: 17.78 ng/ml

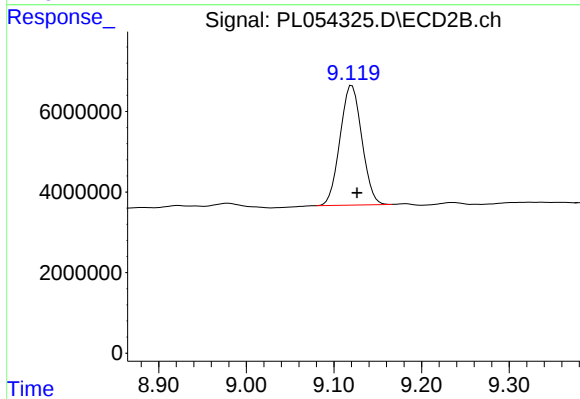

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.006 min
Response: 51458661
Conc: 18.27 ng/ml