

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
 Data File : PL054341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2019 04:09
 Operator : SG\AJ
 Sample : K5671-06
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-111419

Manual Integrations
 APPROVED

Ankita
 11/18/2019 3:17:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 05:34:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.043	159.7E6	29693985	14.736	11.866
28)	SA Decachlor...	8.322	9.123	94647038	27891289	9.646	9.904
Target Compounds							
11)	B alpha-Chl...	5.559	6.228	8006112	5637165	0.602	1.931m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111519\
Data File : PL054341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2019 04:09
Operator : SG\AJ
Sample : K5671-06
Misc :
ALS Vial : 72 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-03-111419


Manual Integrations
APPROVED

Ankita
11/18/2019 3:17:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 05:34:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

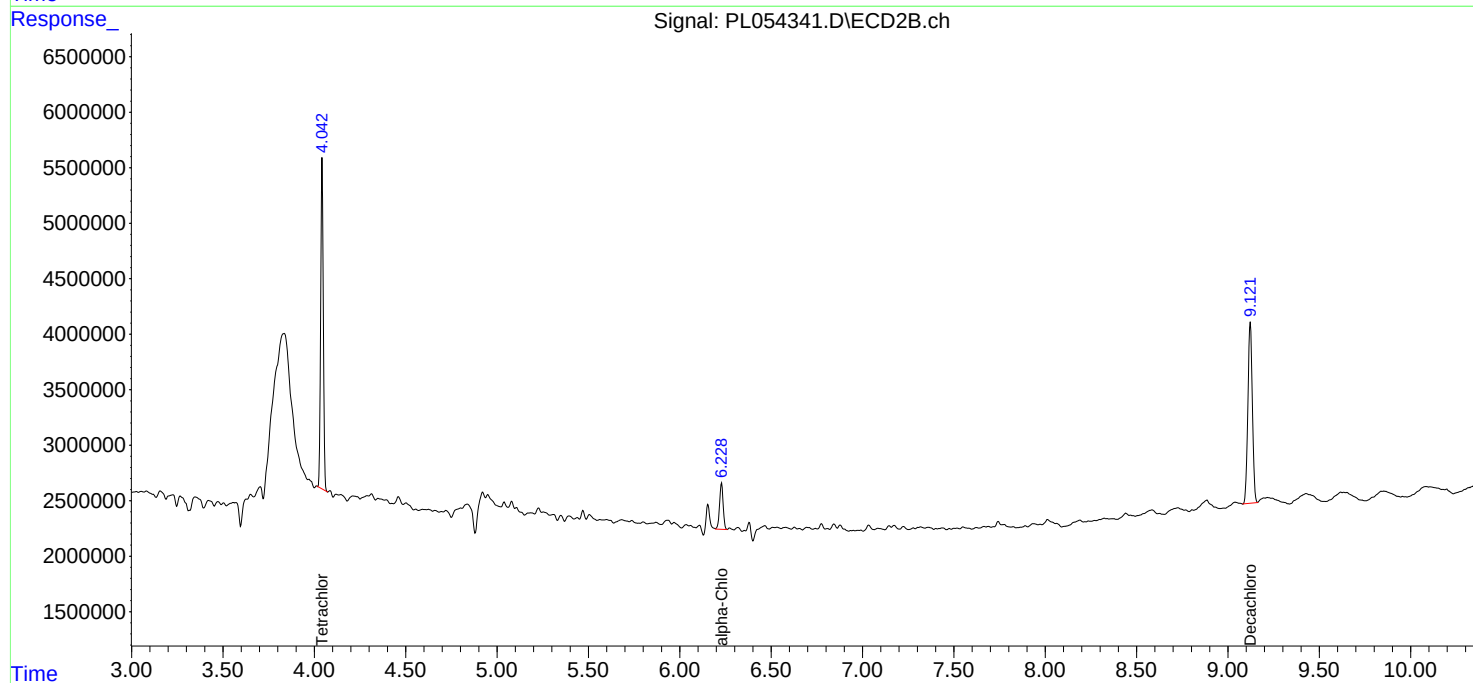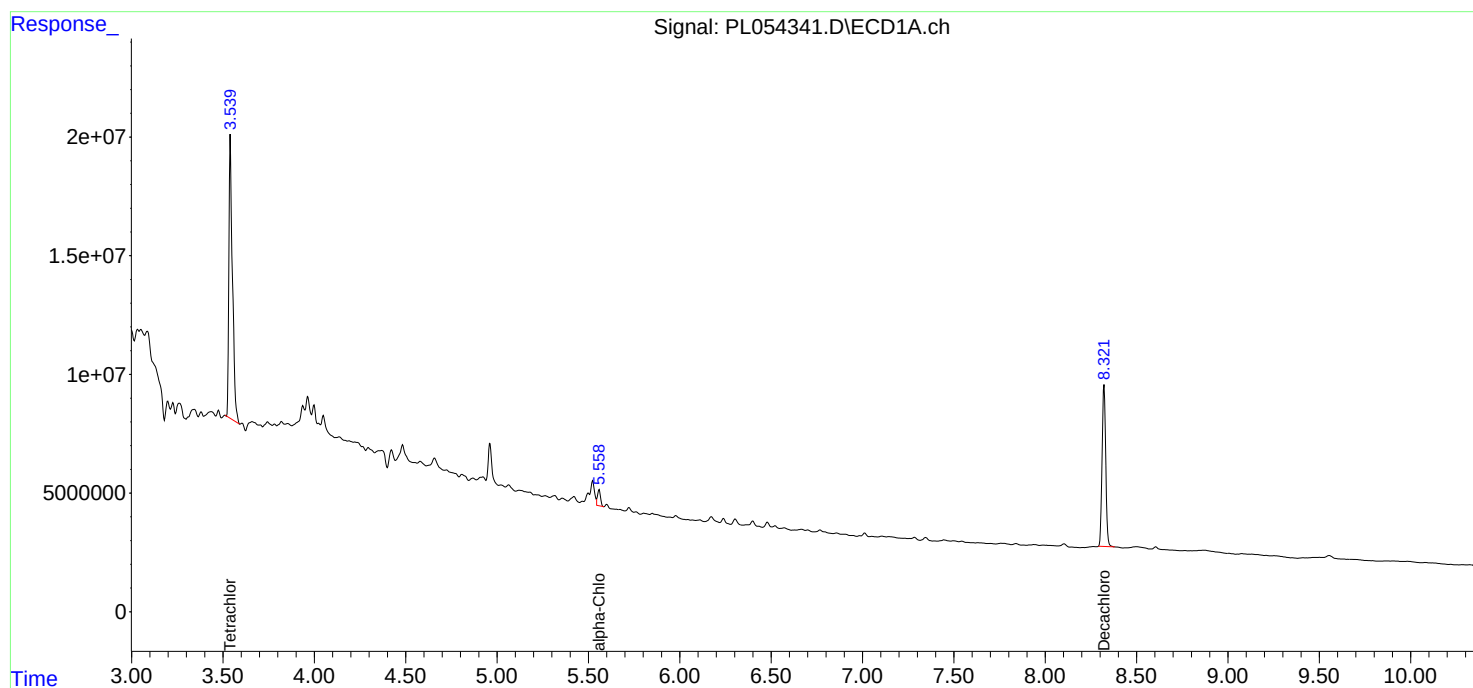

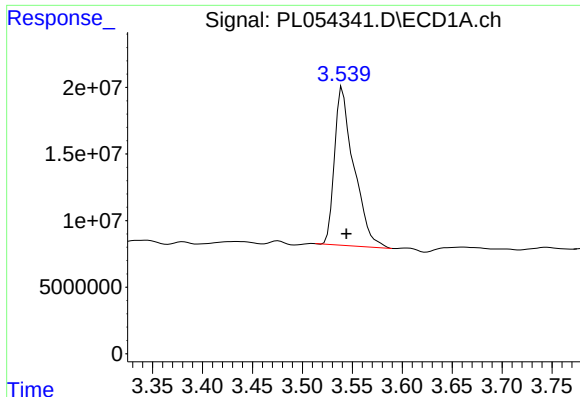


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 159731113
Conc: 14.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-111419


Manual Integrations
APPROVED

Ankita
11/18/2019 3:17:57 PM

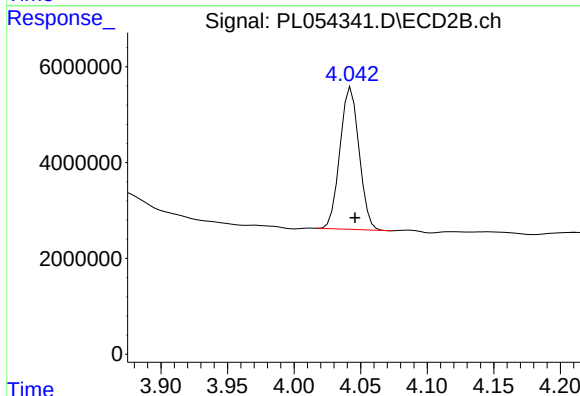


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 29693985
Conc: 11.87 ng/ml

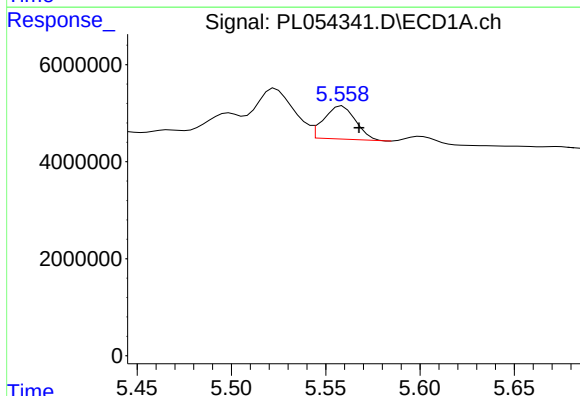


#11 alpha-Chlordane

R.T.: 5.559 min
Delta R.T.: -0.009 min
Response: 8006112
Conc: 0.60 ng/ml

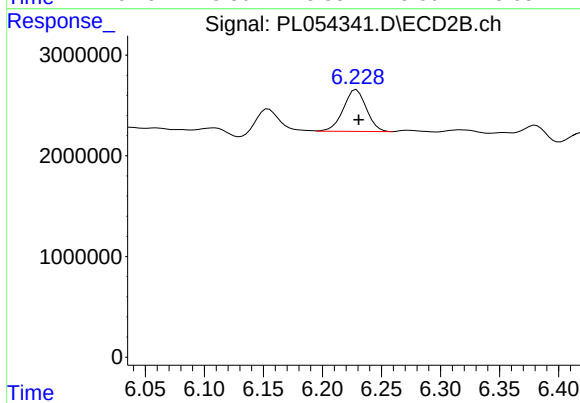

#11 alpha-Chlordane

R.T.: 6.228 min
Delta R.T.: -0.003 min
Response: 5637165
Conc: 1.93 ng/ml m

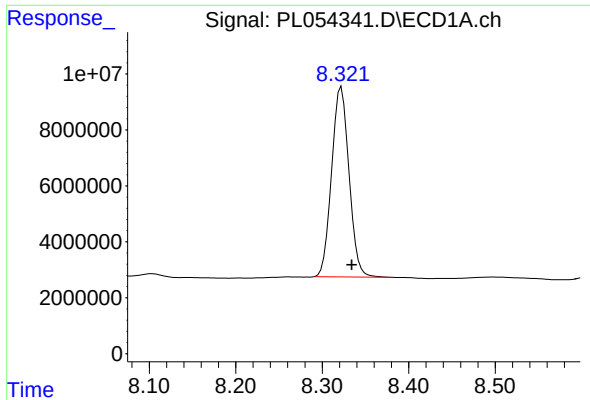


#28 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: -0.012 min
Response: 94647038
Conc: 9.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-111419

Manual Integrations
APPROVED

Ankita
11/18/2019 3:17:57 PM

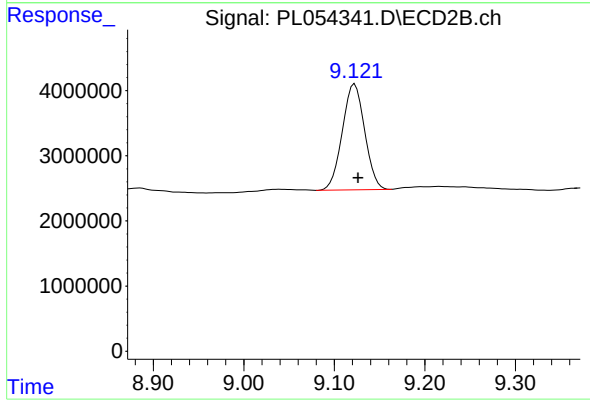

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.004 min
Response: 27891289
Conc: 9.90 ng/ml