

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111521\
 Data File : PL070983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2021 09:49
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 05:07:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.572	5.502	24975260	60485807	50.990	47.972
28)	SA Decachlor...	10.336	11.398	32059247	59307238	46.918	44.346
Target Compounds							
23)	Chlordane-1	5.898	6.885	8580013	23663112	503.225	487.300
24)	Chlordane-2	6.587	7.476	10895628	24796041	474.491	472.712m
25)	Chlordane-3	7.286	8.233	29223347	98101542	478.655m	485.343m
26)	Chlordane-4	7.355	8.316	30721831	116.0E6	467.961	478.030
27)	Chlordane-5	8.303	9.200	11211651	20964690	501.463m	506.036m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111521\
Data File : PL070983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2021 09:49
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 05:07:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

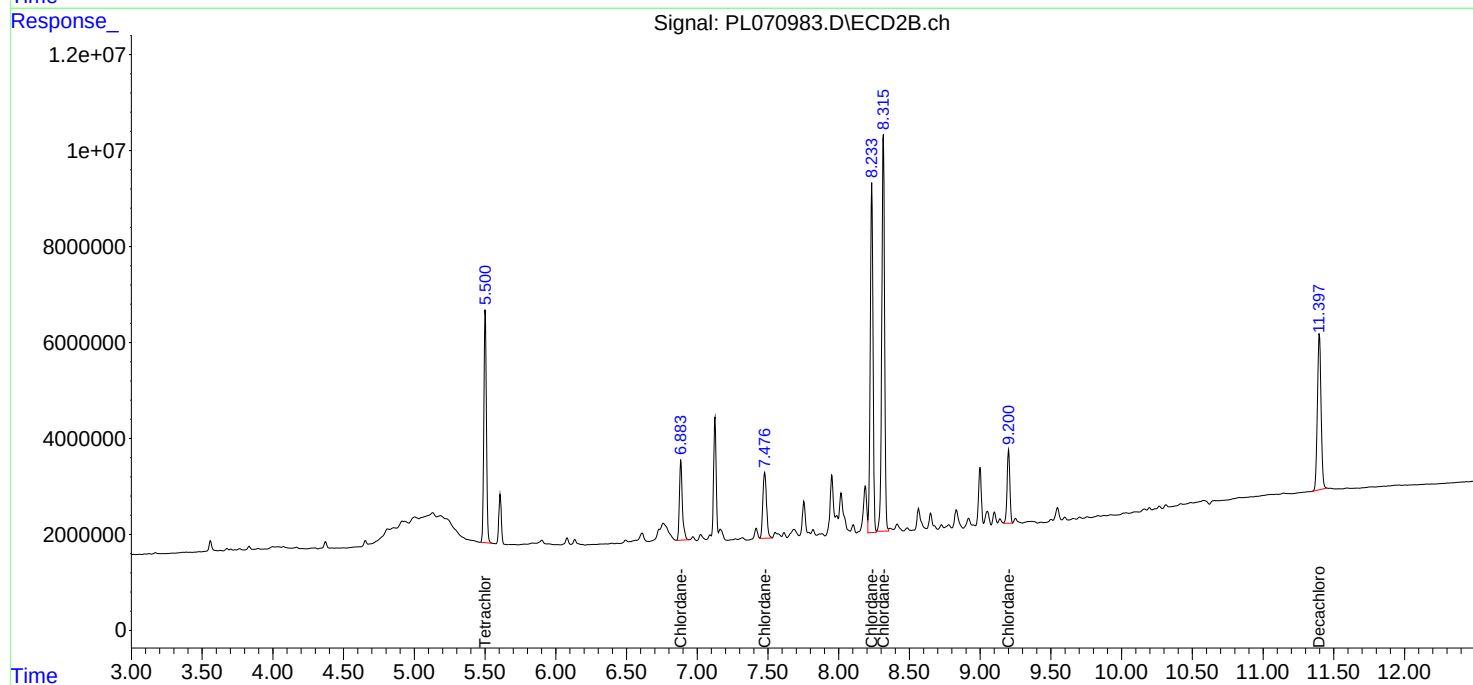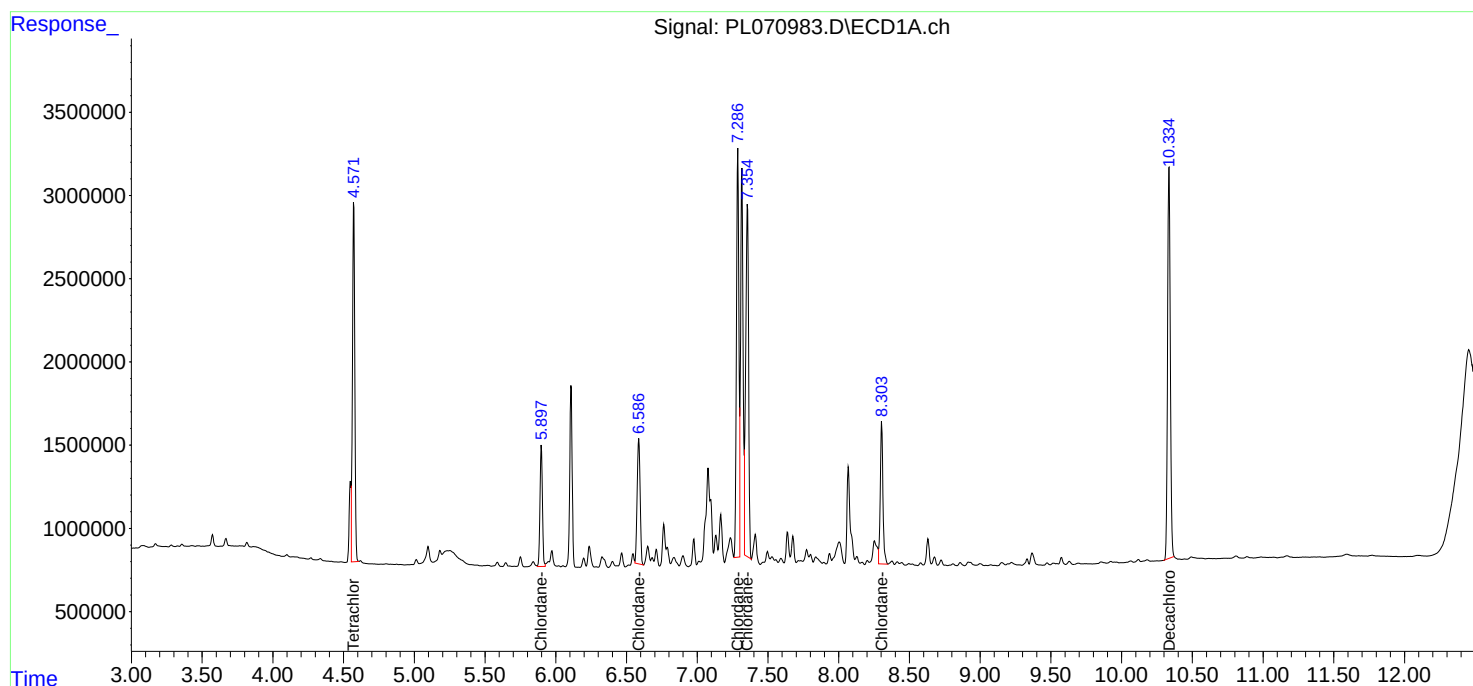


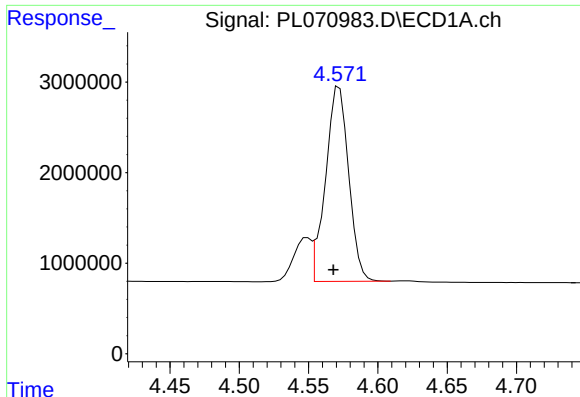

#1 Tetrachloro-m-xylene


R.T.: 4.572 min
Delta R.T.: 0.004 min
Response: 24975260
Conc: 50.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

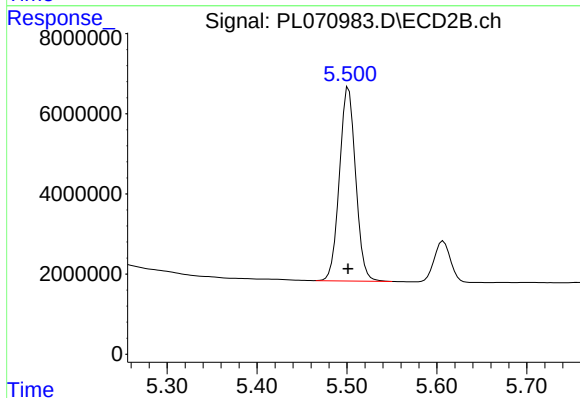


#1 Tetrachloro-m-xylene

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 60485807
Conc: 47.97 ng/ml

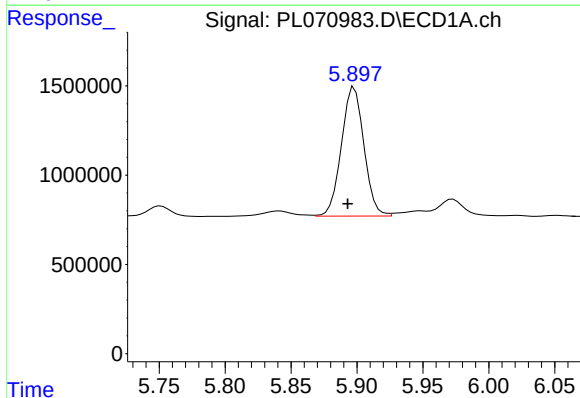


#23 Chlordane-1

R.T.: 5.898 min
Delta R.T.: 0.005 min
Response: 8580013
Conc: 503.23 ng/ml

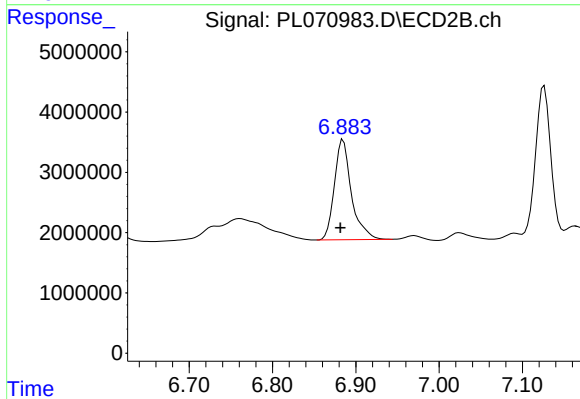

#23 Chlordane-1


R.T.: 6.885 min
Delta R.T.: 0.003 min
Response: 23663112
Conc: 487.30 ng/ml

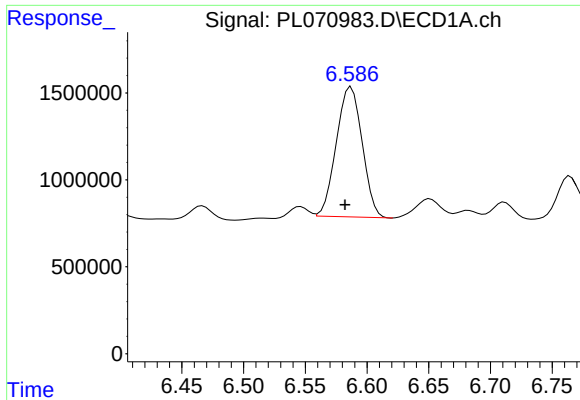

#24 Chlordane-2


R.T.: 6.587 min
Delta R.T.: 0.005 min
Response: 10895628
Conc: 474.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

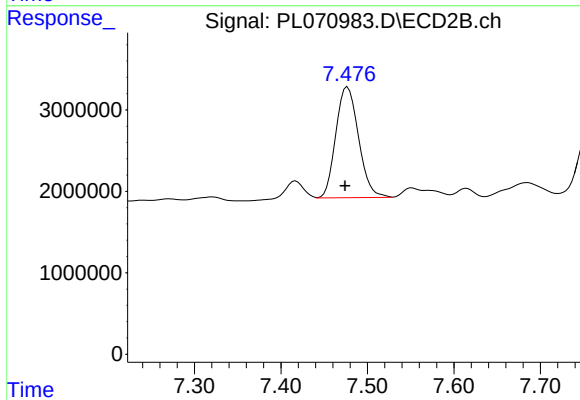


#24 Chlordane-2

R.T.: 7.476 min
Delta R.T.: 0.002 min
Response: 24796041
Conc: 472.71 ng/ml m

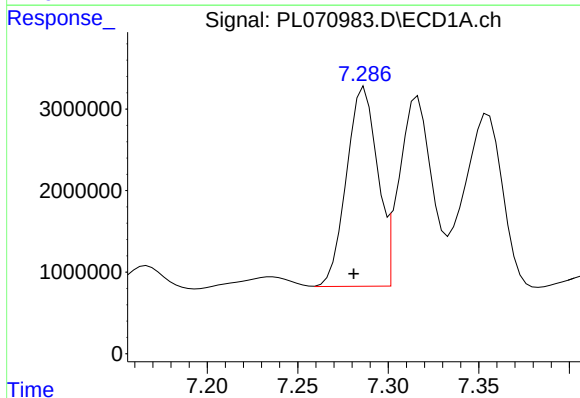


#25 Chlordane-3

R.T.: 7.286 min
Delta R.T.: 0.005 min
Response: 29223347
Conc: 478.66 ng/ml m

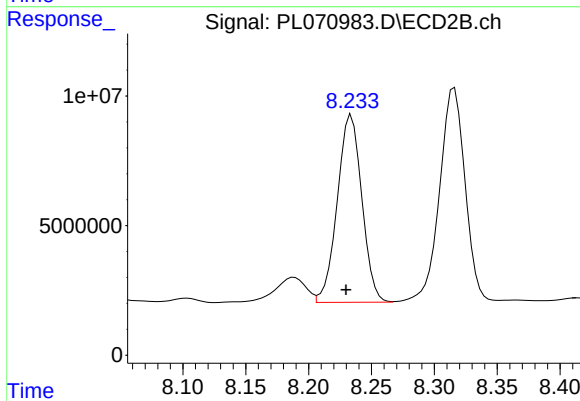

#25 Chlordane-3


R.T.: 8.233 min
Delta R.T.: 0.003 min
Response: 98101542
Conc: 485.34 ng/ml m

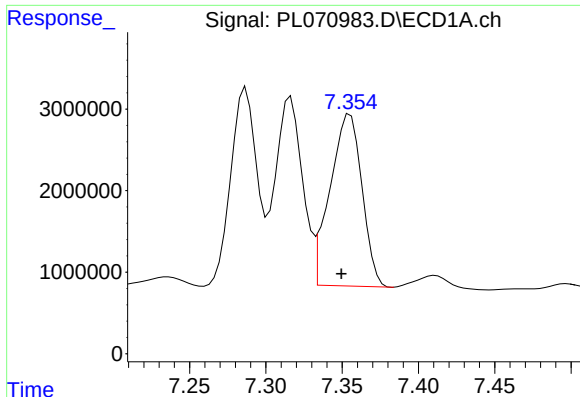

#26 Chlordane-4


R.T.: 7.355 min
Delta R.T.: 0.006 min
Response: 30721831
Conc: 467.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

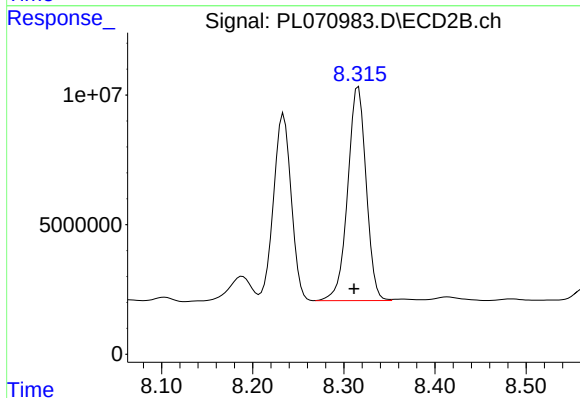


#26 Chlordane-4

R.T.: 8.316 min
Delta R.T.: 0.005 min
Response: 116003891
Conc: 478.03 ng/ml

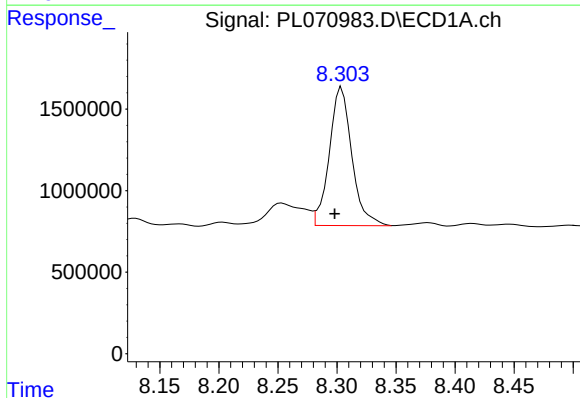


#27 Chlordane-5

R.T.: 8.303 min
Delta R.T.: 0.004 min
Response: 11211651
Conc: 501.46 ng/ml m

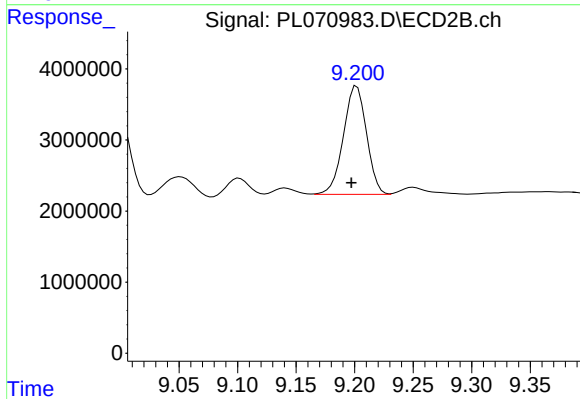

#27 Chlordane-5


R.T.: 9.200 min
Delta R.T.: 0.003 min
Response: 20964690
Conc: 506.04 ng/ml m

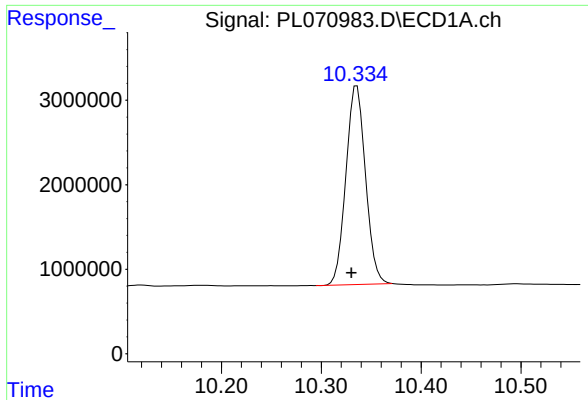

#28 Decachlorobiphenyl

R.T.: 10.336 min
Delta R.T.: 0.005 min
Response: 32059247
Conc: 46.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

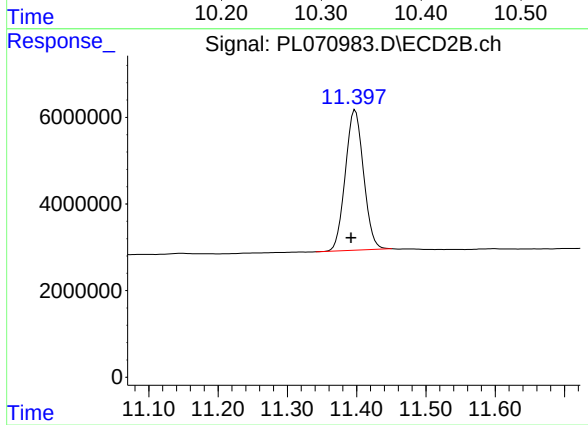

#28 Decachlorobiphenyl

R.T.: 11.398 min
Delta R.T.: 0.006 min
Response: 59307238
Conc: 44.35 ng/ml