

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111521\
 Data File : PL070994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2021 16:36
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 05:08:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.567	5.502	24962543	62157537	50.964	49.298
28)	SA Decachlor...	10.331	11.394	32005975	62488699	46.841	46.725
Target Compounds							
23)	Chlordane-1	5.893	6.883	8228843	24155704	482.629	497.444
24)	Chlordane-2	6.582	7.474	11359334	26035371	494.684	496.338m
25)	Chlordane-3	7.280	8.230	30368052	102.6E6	497.405m	507.827m
26)	Chlordane-4	7.350	8.314	30510963	121.8E6	464.749	502.008
27)	Chlordane-5	8.299	9.198	10463925	21583850	468.020	520.981m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111521\
Data File : PL070994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2021 16:36
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 05:08:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

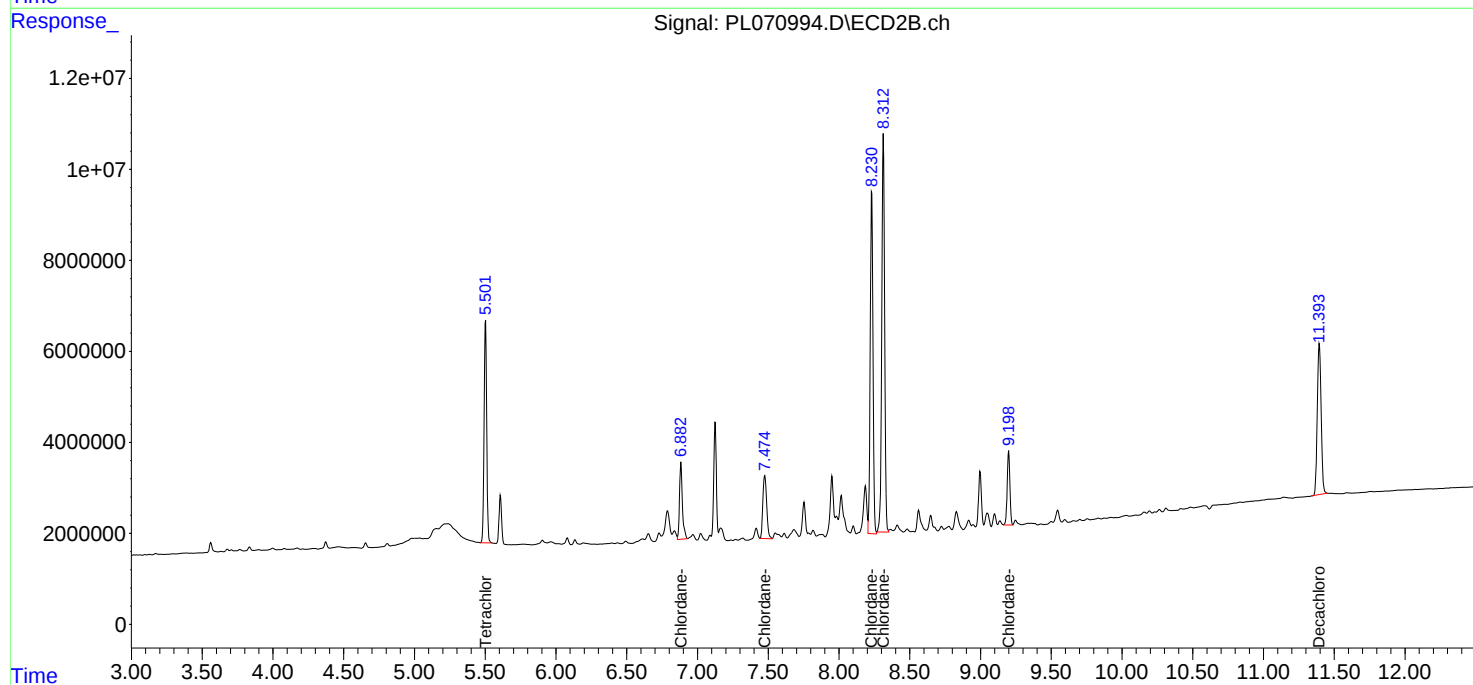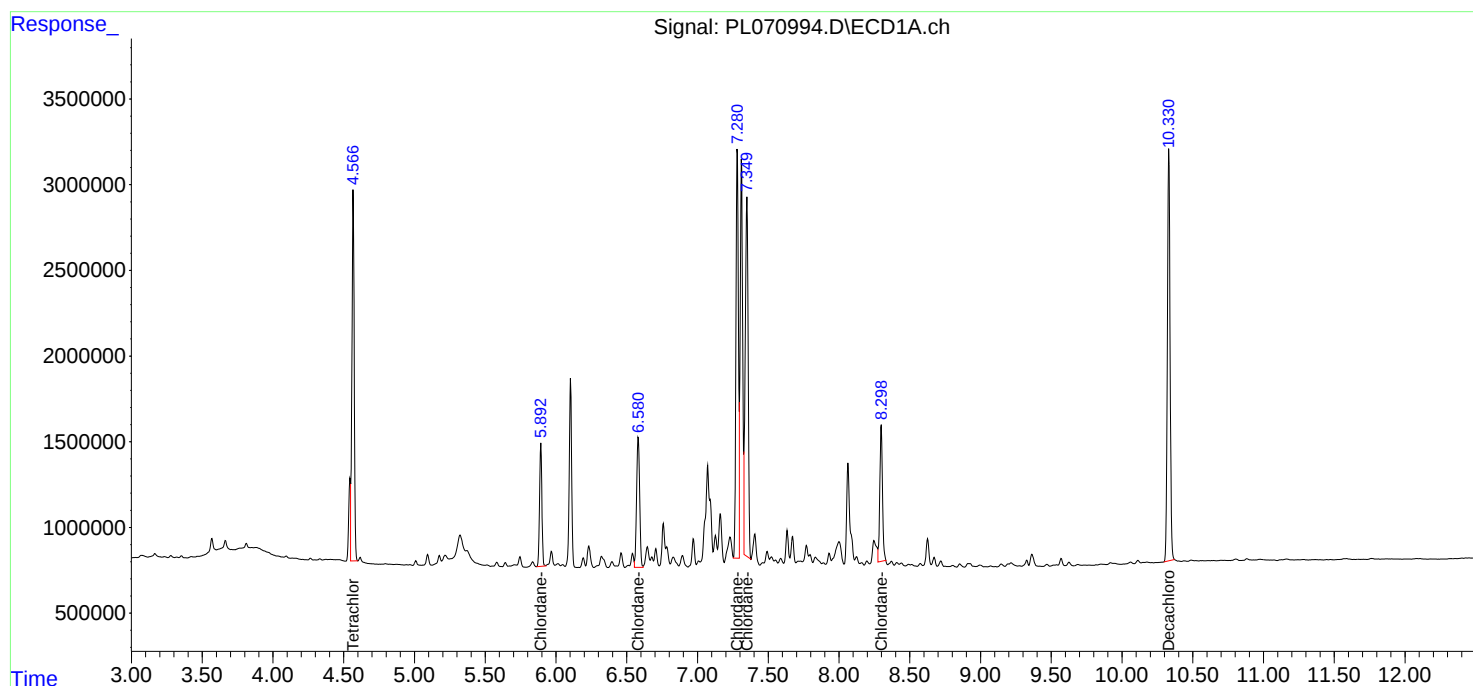


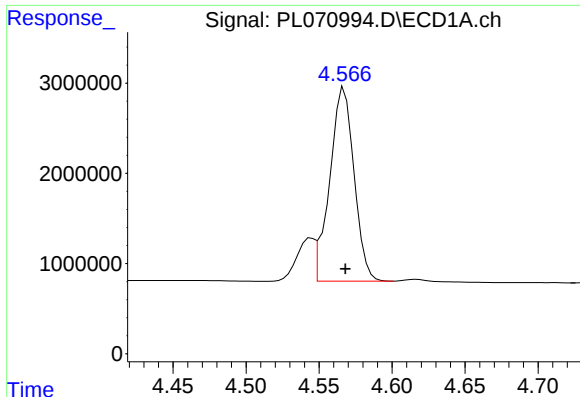

#1 Tetrachloro-m-xylene


R.T.: 4.567 min
Delta R.T.: 0.000 min
Response: 24962543
Conc: 50.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

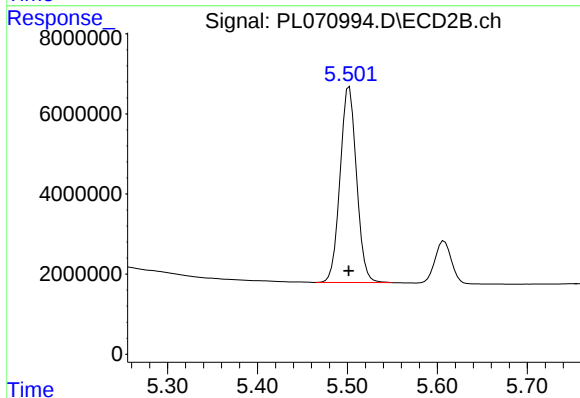


#1 Tetrachloro-m-xylene

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 62157537
Conc: 49.30 ng/ml

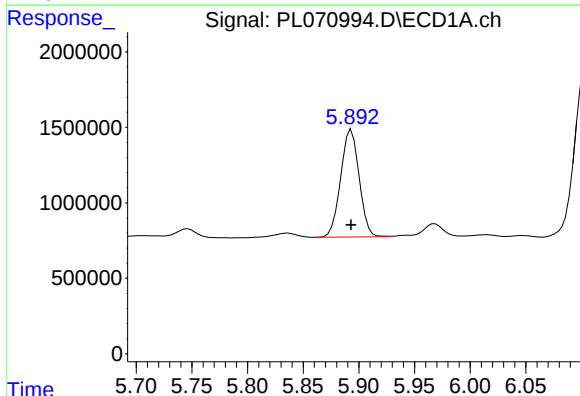


#23 Chlordane-1

R.T.: 5.893 min
Delta R.T.: 0.000 min
Response: 8228843
Conc: 482.63 ng/ml

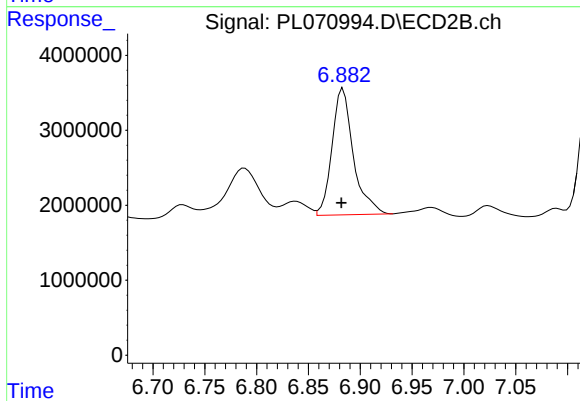

#23 Chlordane-1


R.T.: 6.883 min
Delta R.T.: 0.002 min
Response: 24155704
Conc: 497.44 ng/ml

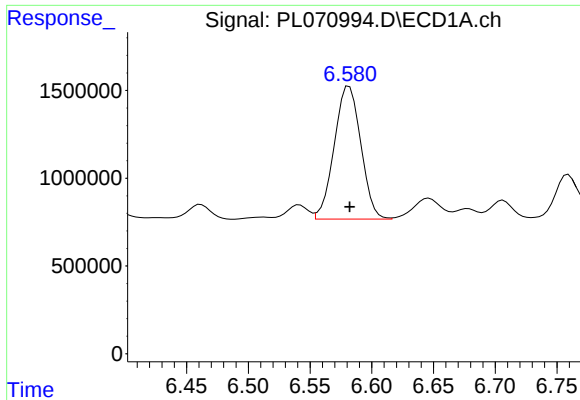

#24 Chlordane-2


R.T.: 6.582 min
Delta R.T.: 0.000 min
Response: 11359334
Conc: 494.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

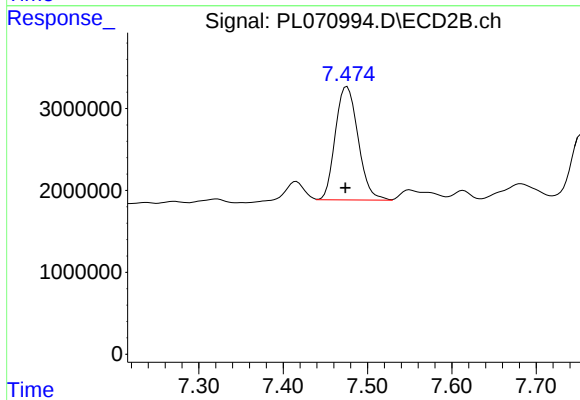


#24 Chlordane-2

R.T.: 7.474 min
Delta R.T.: 0.000 min
Response: 26035371
Conc: 496.34 ng/ml m

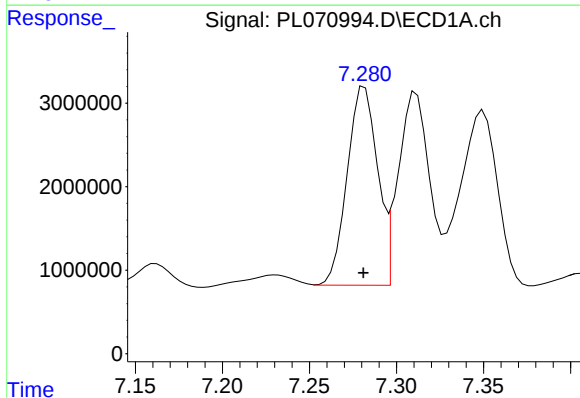


#25 Chlordane-3

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 30368052
Conc: 497.40 ng/ml m

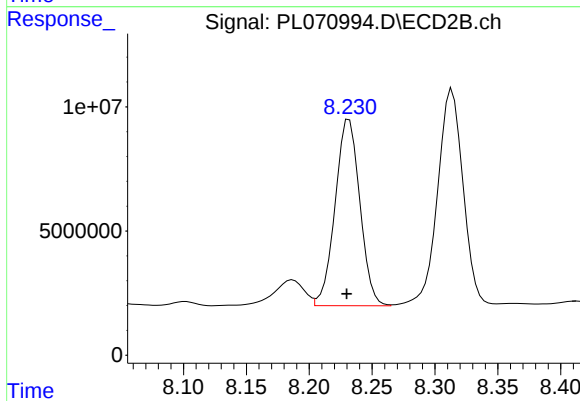

#25 Chlordane-3


R.T.: 8.230 min
Delta R.T.: 0.000 min
Response: 102646233
Conc: 507.83 ng/ml m

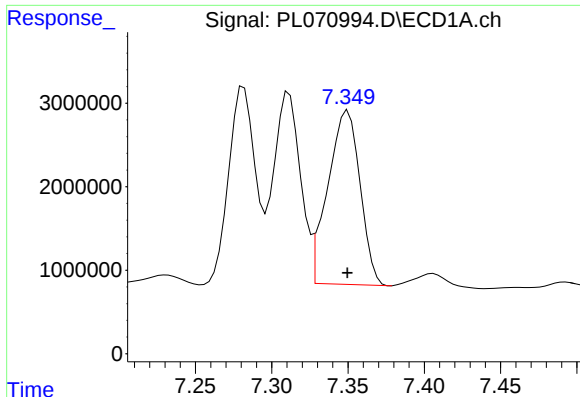

#26 Chlordane-4


R.T.: 7.350 min
Delta R.T.: 0.000 min
Response: 30510963
Conc: 464.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

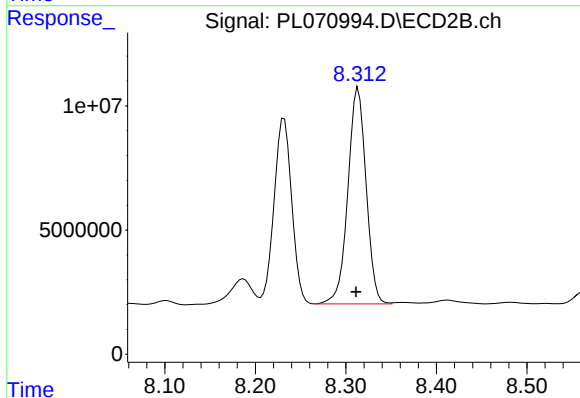


#26 Chlordane-4

R.T.: 8.314 min
Delta R.T.: 0.002 min
Response: 121822825
Conc: 502.01 ng/ml

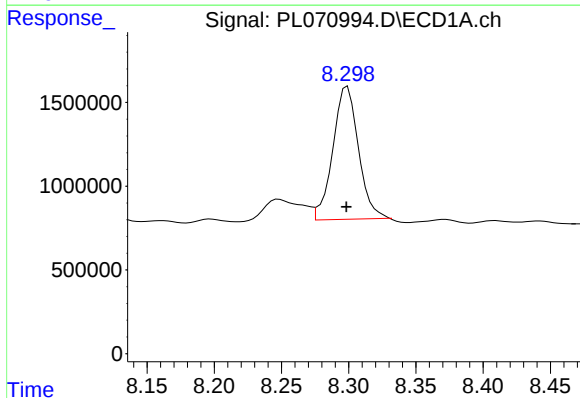


#27 Chlordane-5

R.T.: 8.299 min
Delta R.T.: 0.000 min
Response: 10463925
Conc: 468.02 ng/ml

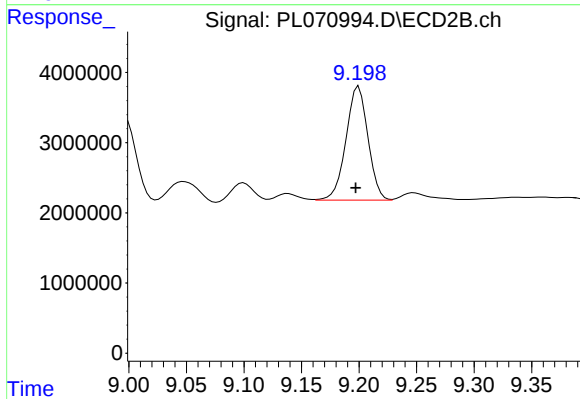

#27 Chlordane-5


R.T.: 9.198 min
Delta R.T.: 0.001 min
Response: 21583850
Conc: 520.98 ng/ml m

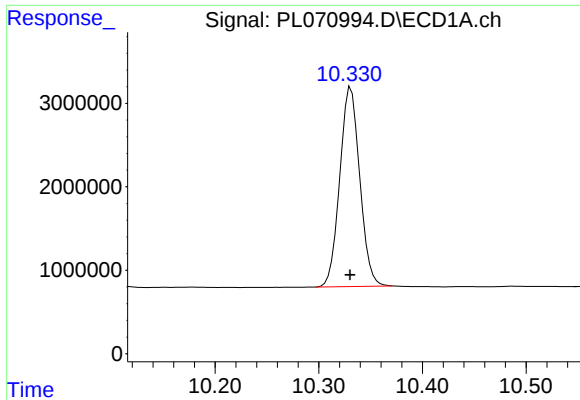

#28 Decachlorobiphenyl

R.T.: 10.331 min
Delta R.T.: 0.000 min
Response: 32005975
Conc: 46.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

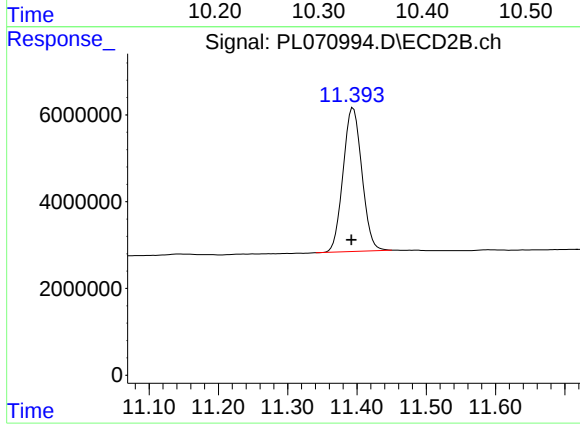

#28 Decachlorobiphenyl

R.T.: 11.394 min
Delta R.T.: 0.003 min
Response: 62488699
Conc: 46.72 ng/ml