

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111522\
 Data File : PL079106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2022 09:27
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 10:54:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) A	alpha-BHC	3.763f	0.000	39976	0	0.014	N.D. #
8) B	Heptachlo...	5.467	4.460f	7325758	4270589	3.451	1.417 #
9) A	Endosulfan I	5.838	0.000	141753	0	0.066	N.D. #
13) MA	Dieldrin	0.000	5.101	0	4586017	N.D.	1.548 #
14) MA	Endrin	0.000	5.393f	0	2389172	N.D.	0.917 #
17) MA	4,4'-DDT	6.819	0.000	748634	0	0.418	N.D. #
19) B	Endosulfa...	6.952	6.087f	70535	577477	0.038	0.243 #
20) A	Methoxychlor	7.314f	0.000	94910	0	0.103	N.D. #
24)	Chlordane-2	0.000	4.098	0	27962076	N.D.	262.736 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111522\
Data File : PL079106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2022 09:27
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 10:54:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

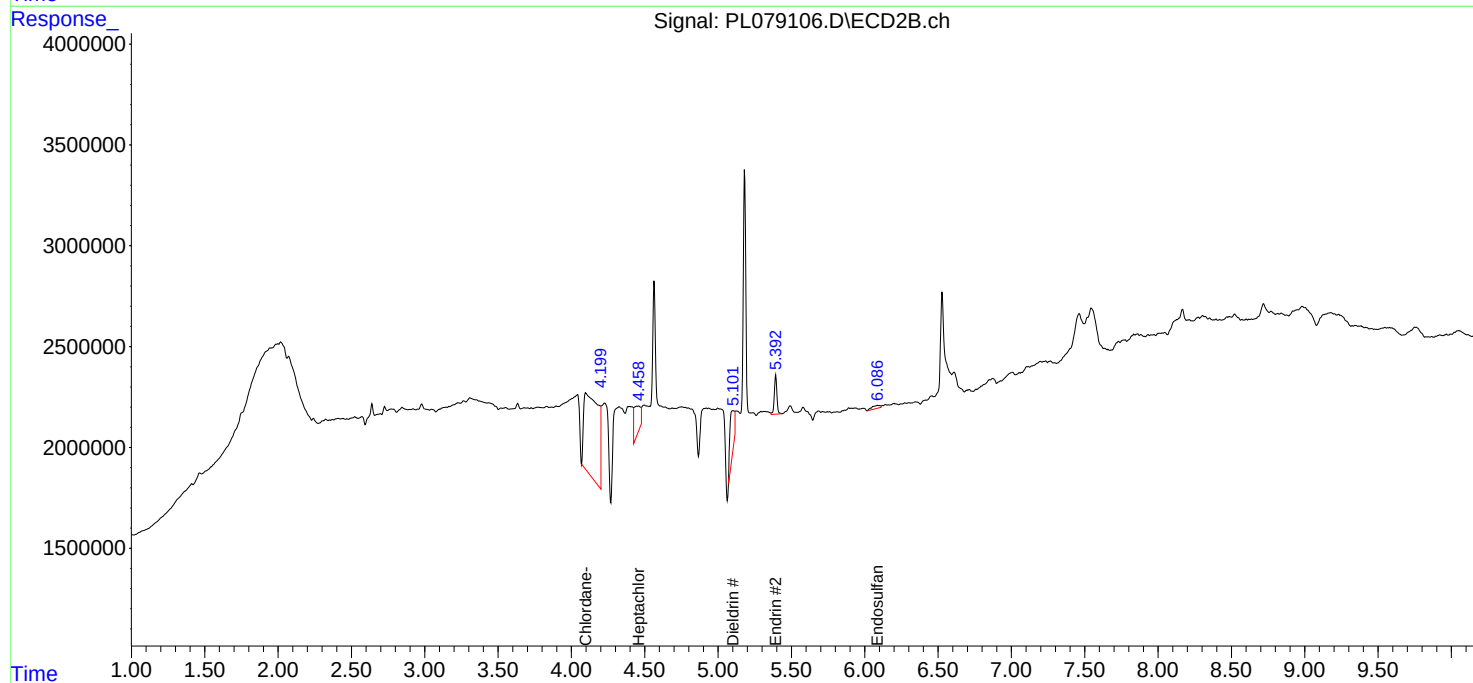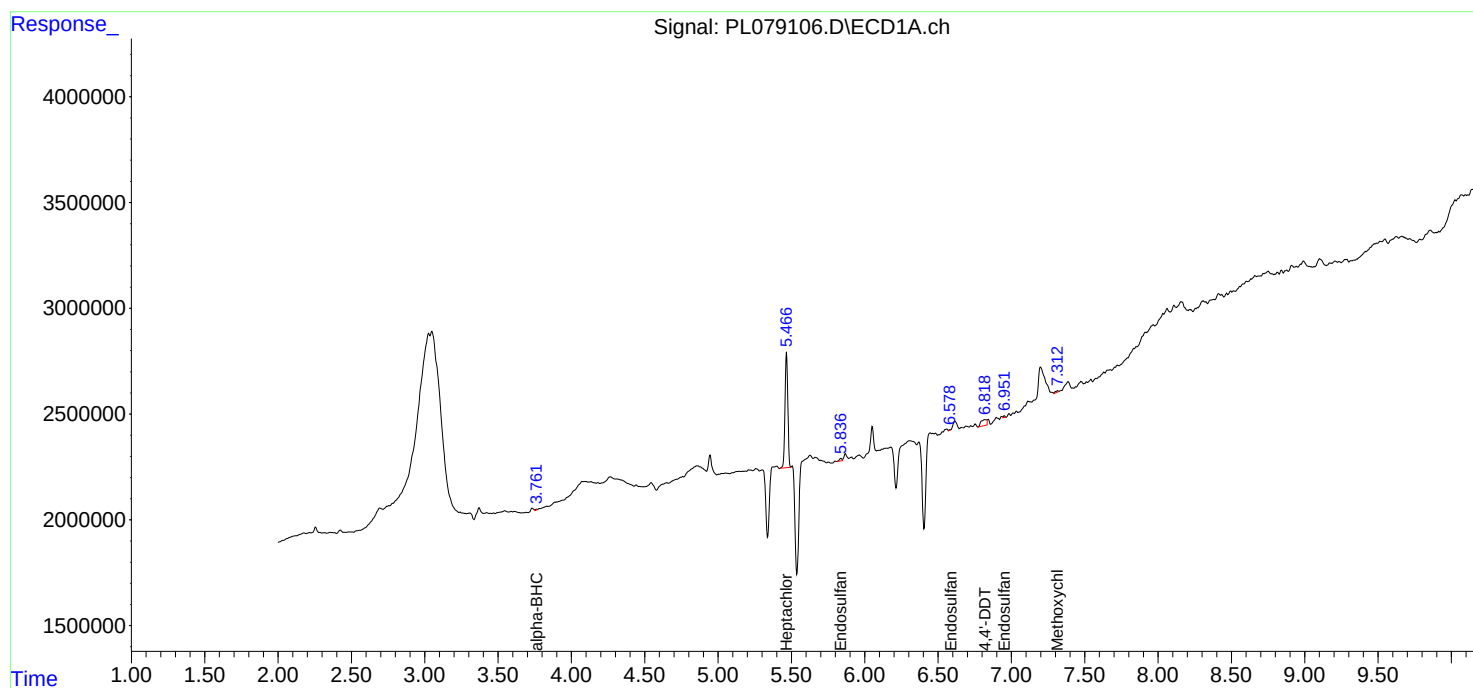


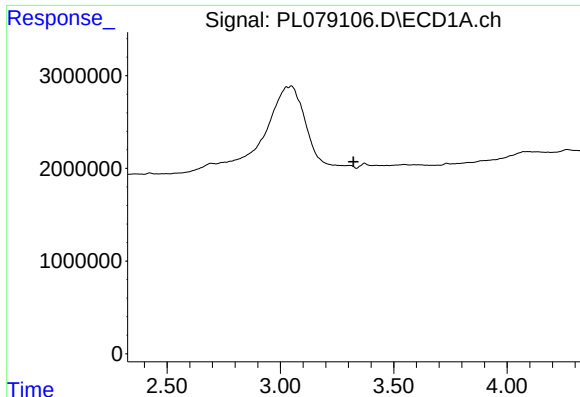

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

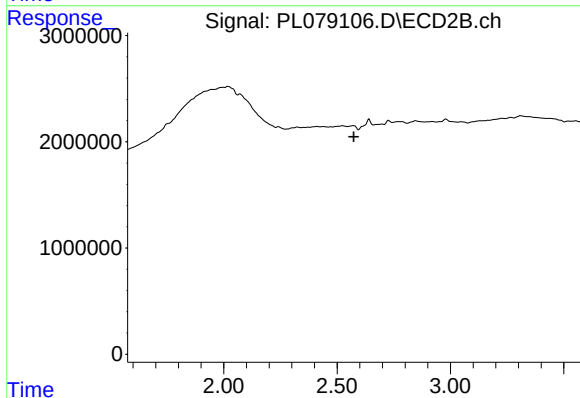


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.574 min
Response: 0
Conc: N.D.

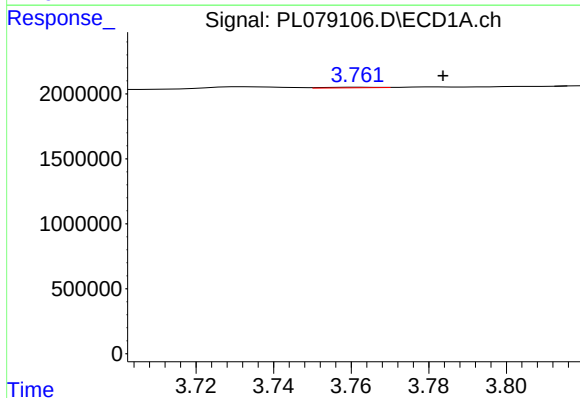


#2 alpha-BHC

R.T.: 3.763 min
Delta R.T.: -0.021 min
Response: 39976
Conc: 0.01 ng/ml

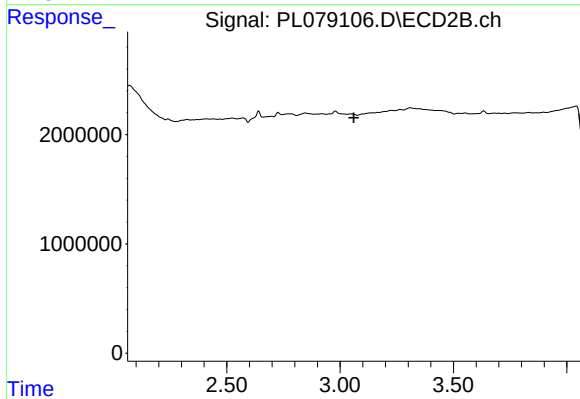

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 3.061 min
Response: 0
Conc: N.D.

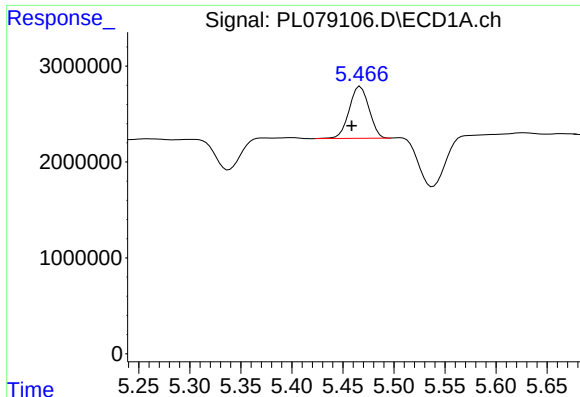

#8 Heptachlor epoxide


R.T.: 5.467 min
Delta R.T.: 0.008 min
Response: 7325758
Conc: 3.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

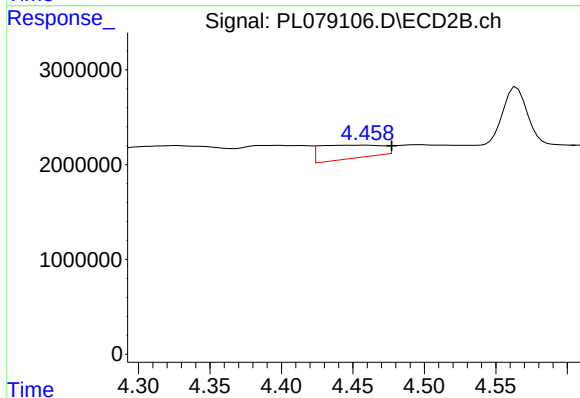


#8 Heptachlor epoxide

R.T.: 4.460 min
Delta R.T.: -0.018 min
Response: 4270589
Conc: 1.42 ng/ml

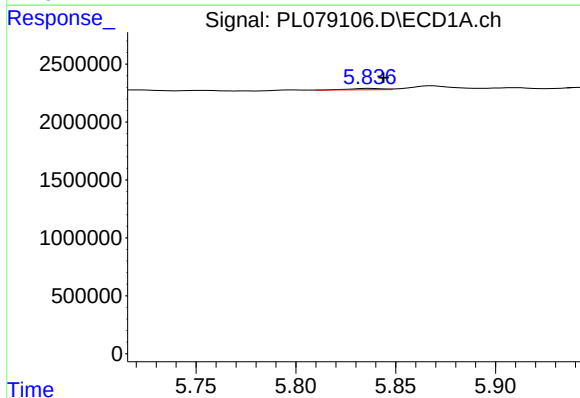


#9 Endosulfan I

R.T.: 5.838 min
Delta R.T.: -0.006 min
Response: 141753
Conc: 0.07 ng/ml

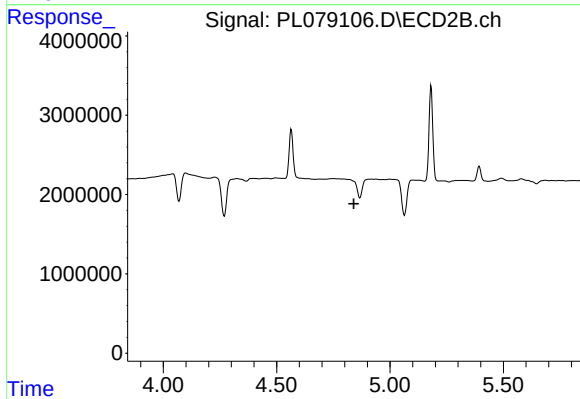

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 4.840 min
Response: 0
Conc: N.D.

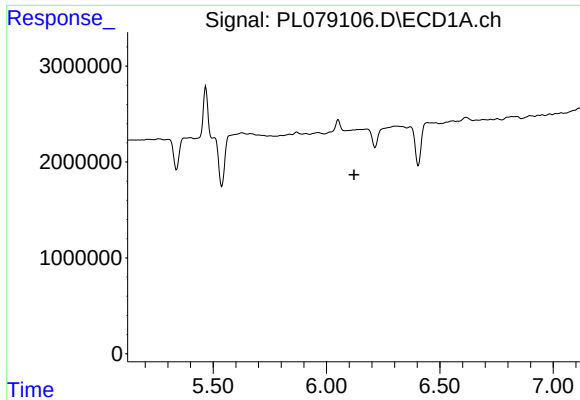

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

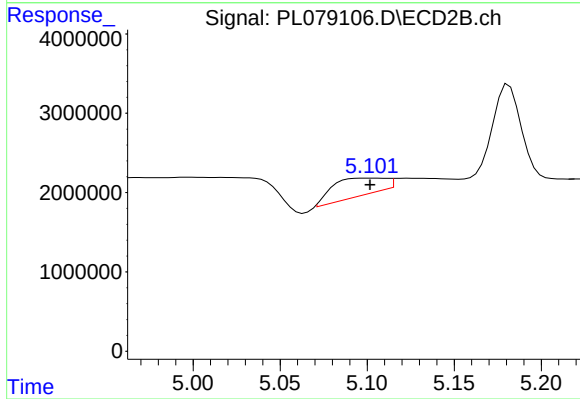


#13 Dieldrin

R.T.: 5.101 min
Delta R.T.: 0.000 min
Response: 4586017
Conc: 1.55 ng/ml

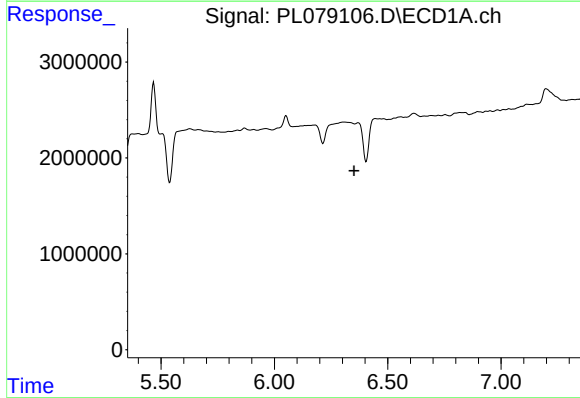


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.351 min
Response: 0
Conc: N.D.

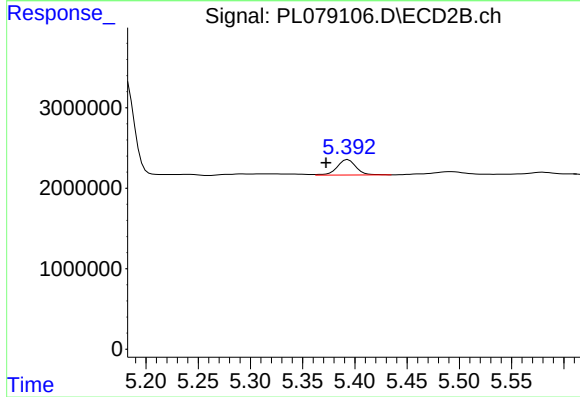

#14 Endrin


R.T.: 5.393 min
Delta R.T.: 0.021 min
Response: 2389172
Conc: 0.92 ng/ml

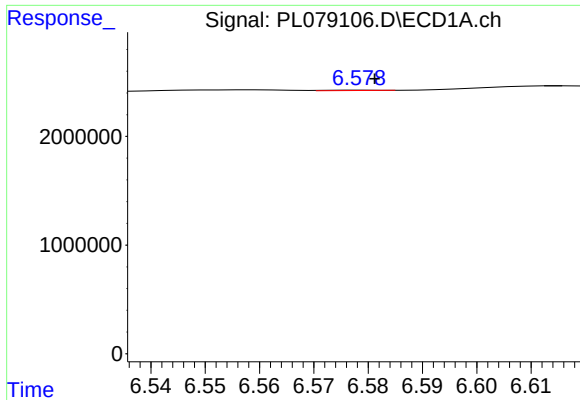

#15 Endosulfan II


R.T.: 6.579 min
Delta R.T.: -0.002 min
Response: 20604
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

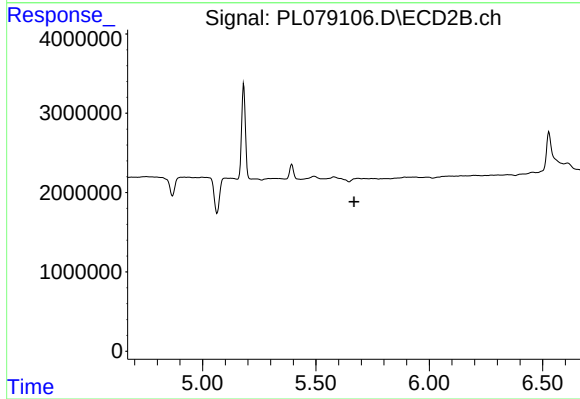


#15 Endosulfan II

R.T.: 5.685 min
Delta R.T.: 0.016 min
Response: -65331
Conc: N.D.

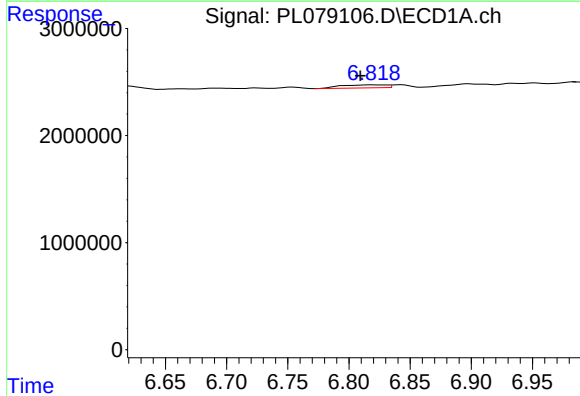


#17 4,4'-DDT

R.T.: 6.819 min
Delta R.T.: 0.010 min
Response: 748634
Conc: 0.42 ng/ml

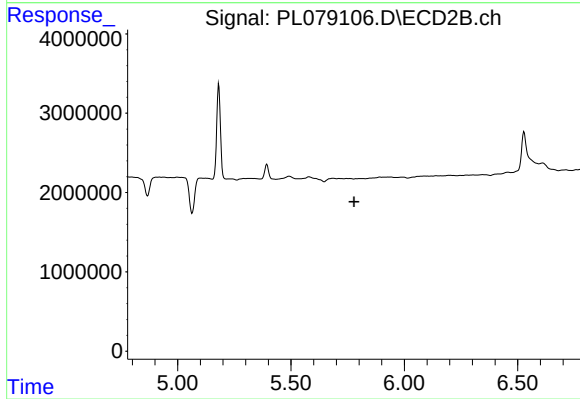

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 5.779 min
Response: 0
Conc: N.D.

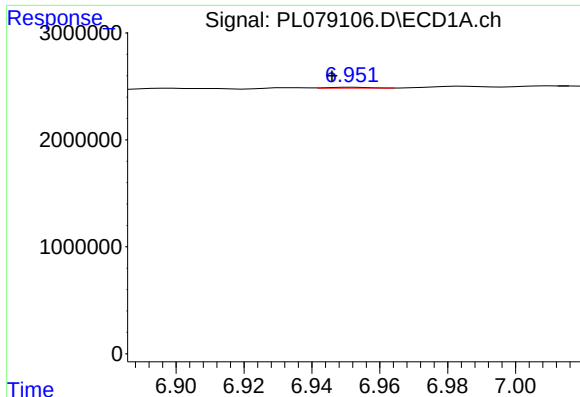

#19 Endosulfan Sulfate


R.T.: 6.952 min
Delta R.T.: 0.006 min
Response: 70535
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

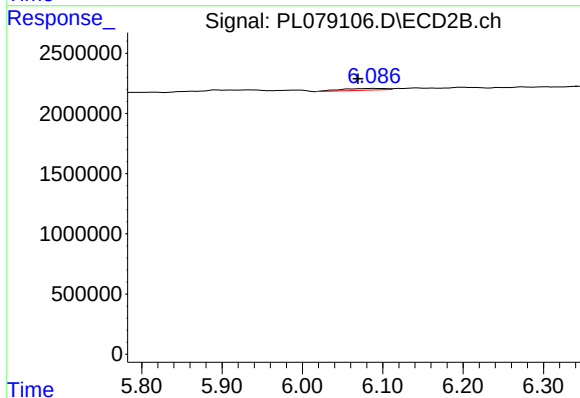


#19 Endosulfan Sulfate

R.T.: 6.087 min
Delta R.T.: 0.018 min
Response: 577477
Conc: 0.24 ng/ml

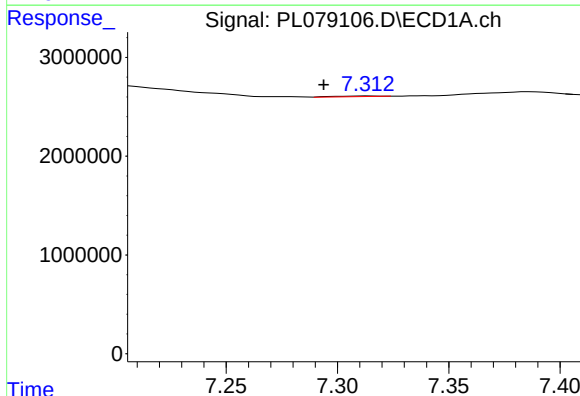


#20 Methoxychlor

R.T.: 7.314 min
Delta R.T.: 0.020 min
Response: 94910
Conc: 0.10 ng/ml

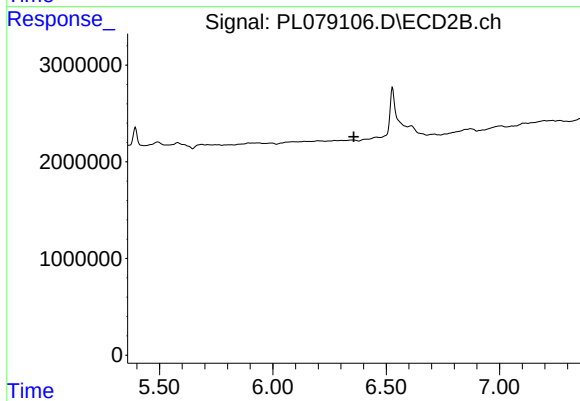

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

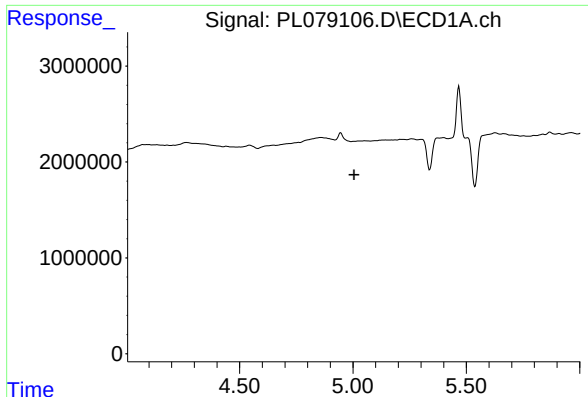

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

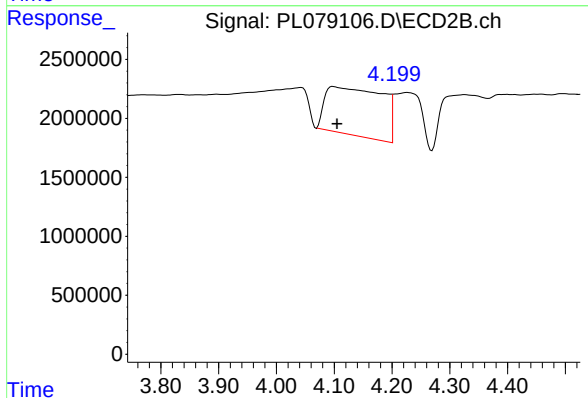


#24 Chlordane-2

R.T.: 4.098 min
Delta R.T.: -0.007 min
Response: 27962076
Conc: 262.74 ng/ml

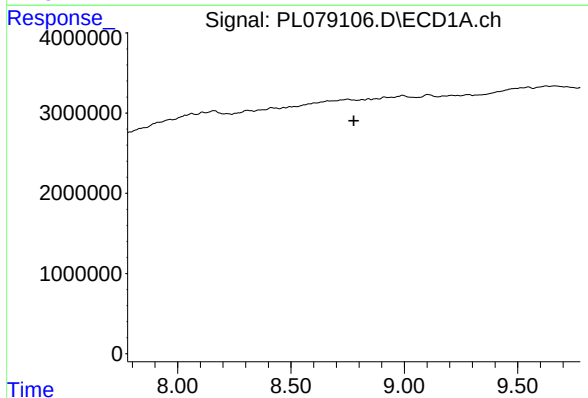

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.777 min
Response: 0
Conc: N.D.

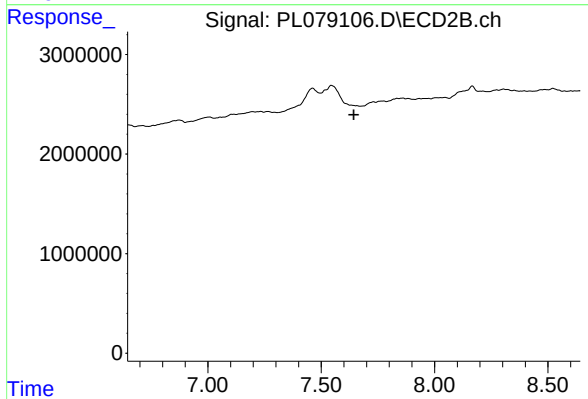

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.