

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111522\
 Data File : PL079110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2022 11:01
 Operator : AR\AJ
 Sample : N5583-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-08-111022

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/16/2022
 Supervised By : Ankita Jodhani 11/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 11:23:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.320	2.568	4309397	5082398	2.260	1.991
2) SA Decachlor...	8.768	7.632	3401196	3913599	2.261m	2.066m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111522\
Data File : PL079110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2022 11:01
Operator : AR\AJ
Sample : N5583-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-08-111022


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/16/2022
Supervised By : Ankita Jodhani 11/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 11:23:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

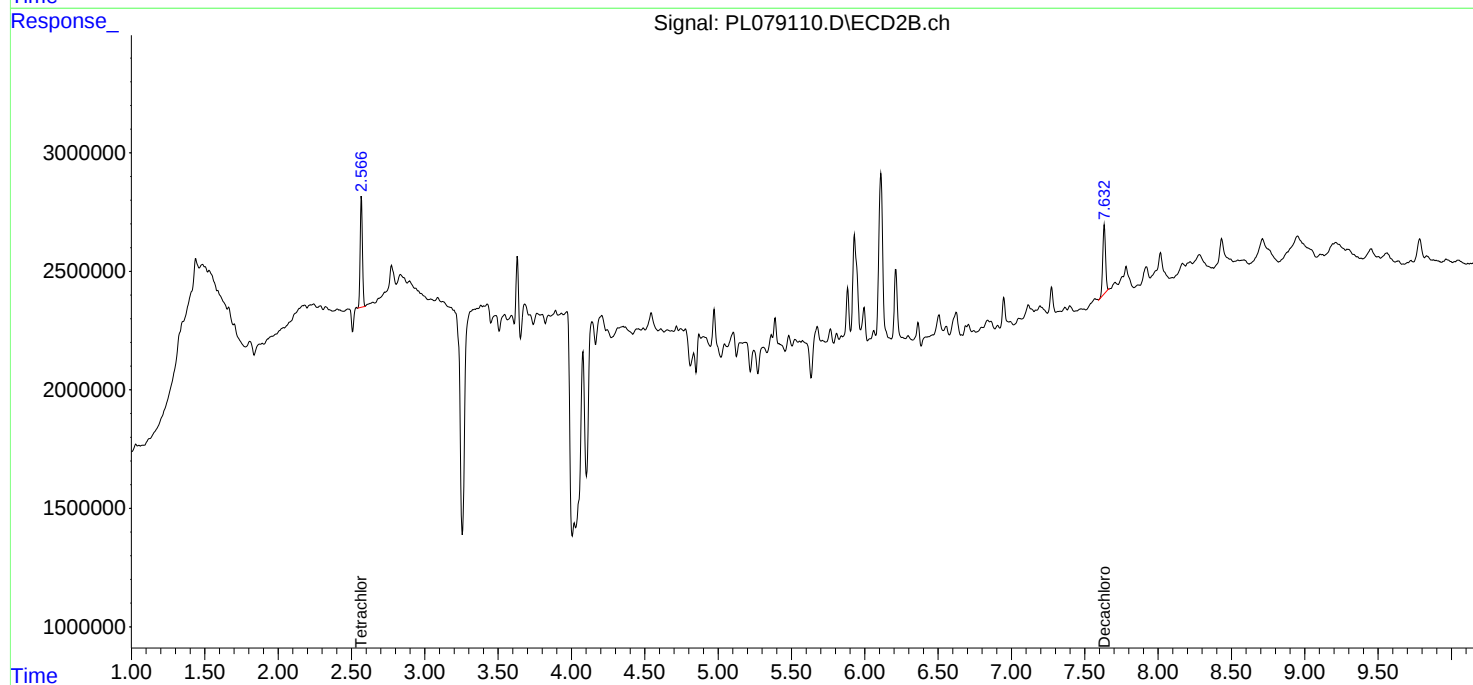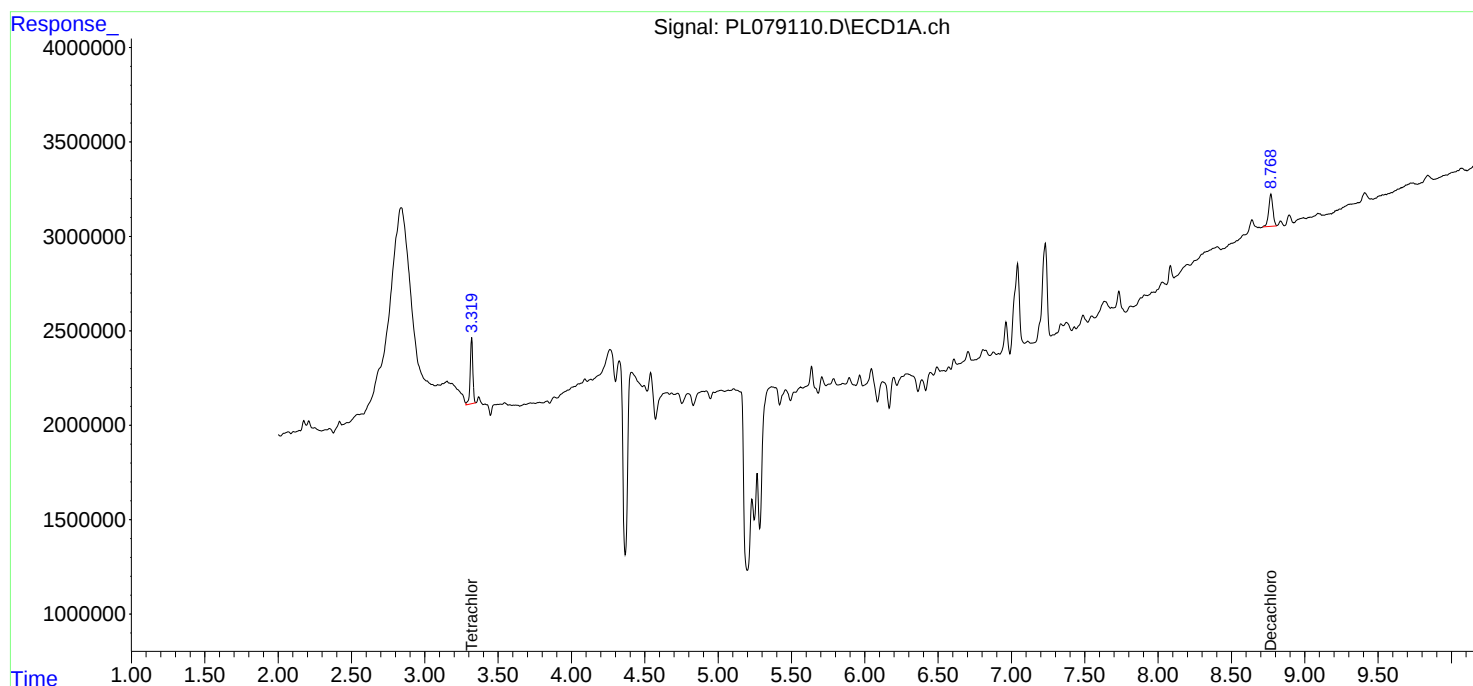

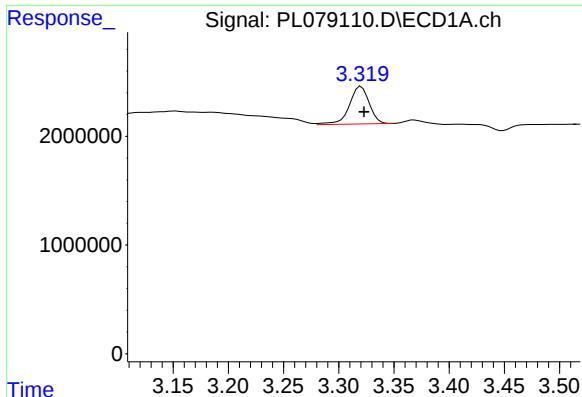


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: -0.003 min
Response: 4309397
Conc: 2.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-08-111022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/16/2022
Supervised By :Ankita Jodhani 11/16/2022

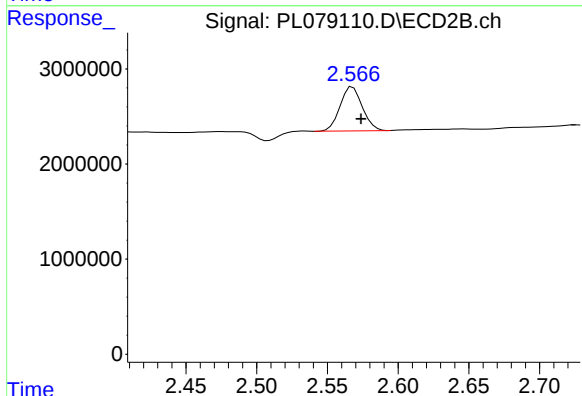


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.006 min
Response: 5082398
Conc: 1.99 ng/ml

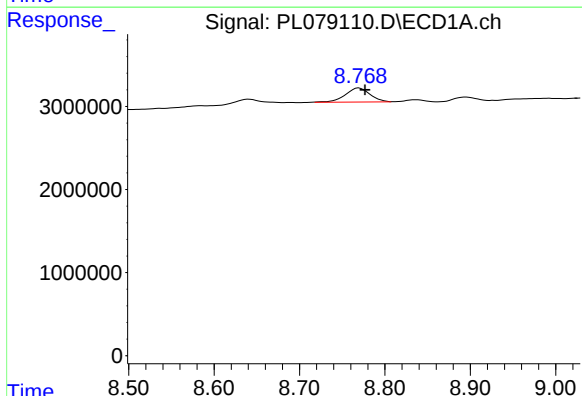

#28 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.008 min
Response: 3401196
Conc: 2.26 ng/ml m

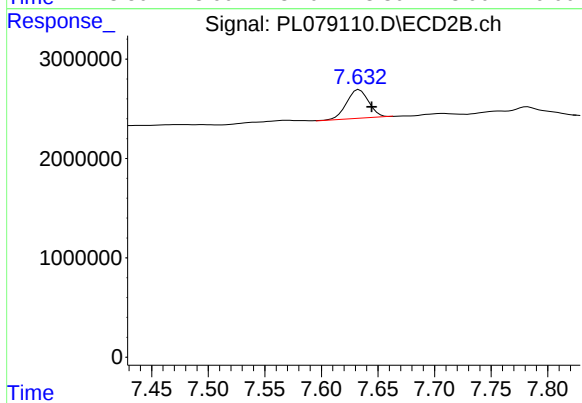

#28 Decachlorobiphenyl

R.T.: 7.632 min
Delta R.T.: -0.012 min
Response: 3913599
Conc: 2.07 ng/ml m