

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111524\
 Data File : PL093082.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2024 15:35
 Operator : AR\AJ
 Sample : P4851-01 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-11142024

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

11/18/2024

Supervised By :Ankita
 Jodhani

11/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 21:47:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.776	6981327	7111359	2.849m	2.613
28) SA Decachlor...	9.055	7.916	4456420	6901835	2.316m	2.529

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111524\
Data File : PL093082.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2024 15:35
Operator : AR\AJ
Sample : P4851-01 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-02-11142024


Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel
11/18/2024
Supervised By :Ankita
Jodhani
11/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 21:47:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

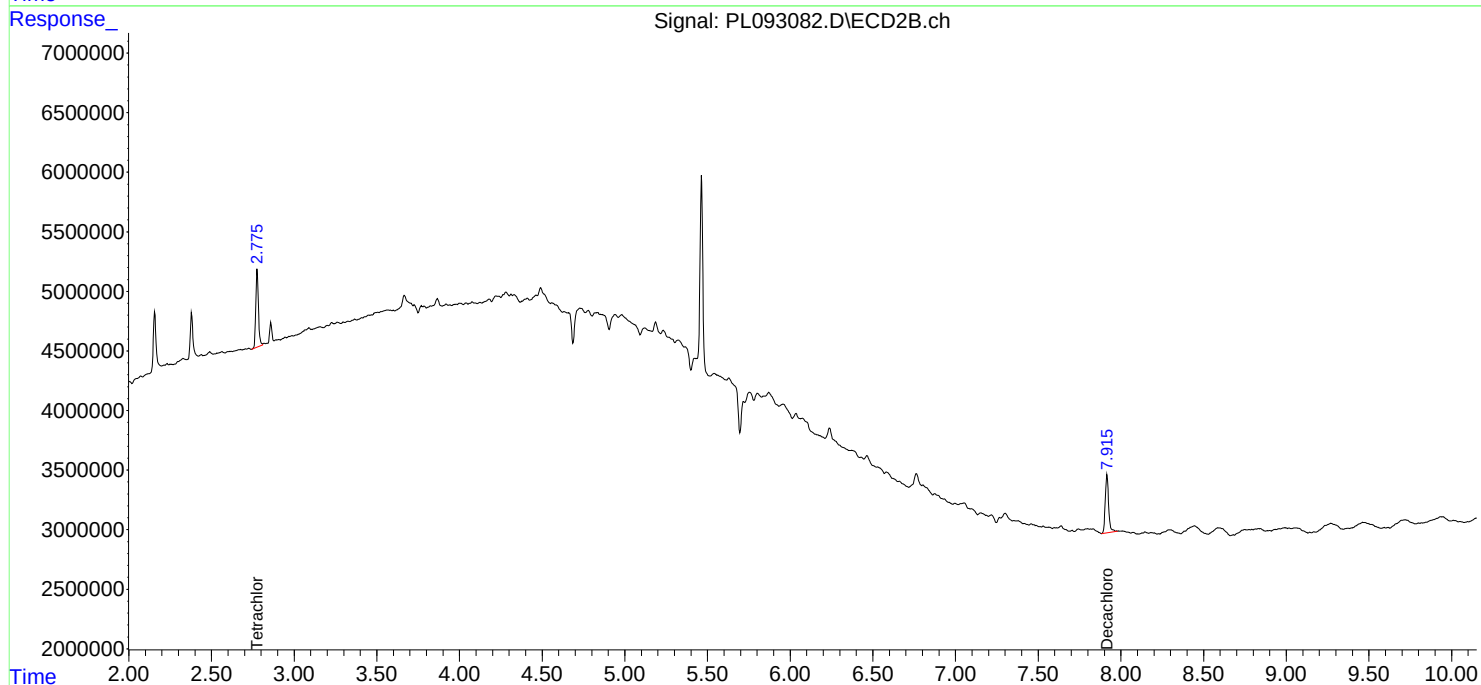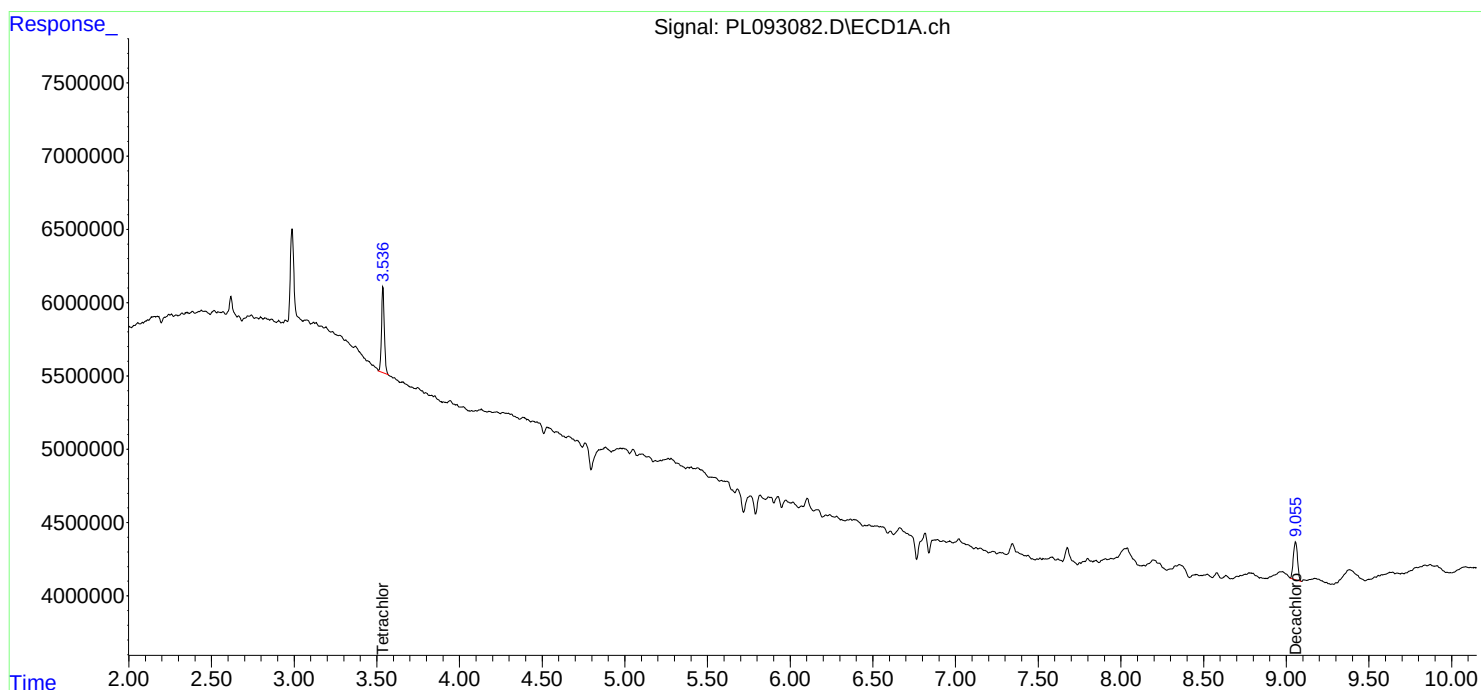

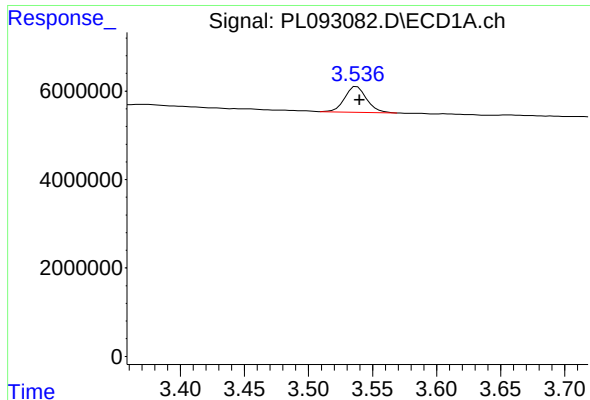

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: -0.004 min
Response: 6981327
Conc: 2.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-11142024

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
11/18/2024

Supervised By :Ankita
Jodhani
11/18/2024

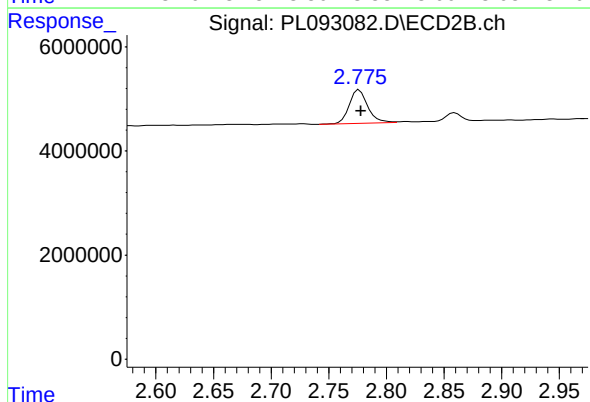


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: -0.001 min
Response: 7111359
Conc: 2.61 ng/ml

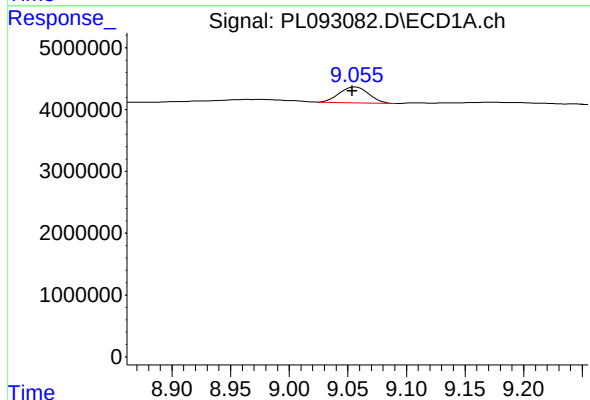

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.001 min
Response: 4456420
Conc: 2.32 ng/ml m

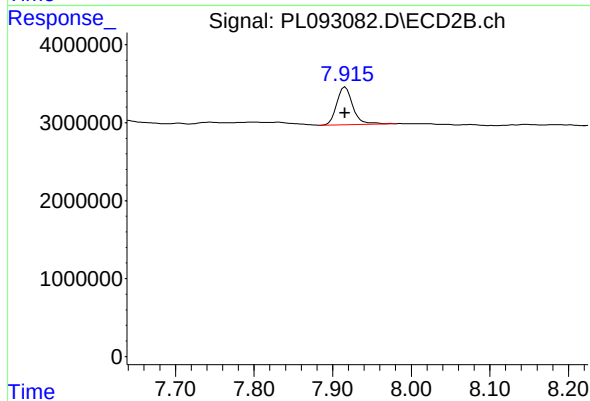

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 6901835
Conc: 2.53 ng/ml