

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111524\
 Data File : PL093088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2024 16:54
 Operator : AR\AJ
 Sample : P4857-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ETGI-328

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/18/2024
 Supervised By :Ankita Jodhani 11/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 21:53:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.805f	30490252	75382703	12.444m	27.702m#
28) SA Decachlor...	9.056	7.916	24275891	29120895	12.614m	10.670

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111524\
Data File : PL093088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2024 16:54
Operator : AR\AJ
Sample : P4857-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :Ankita Jodhani 11/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 21:53:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

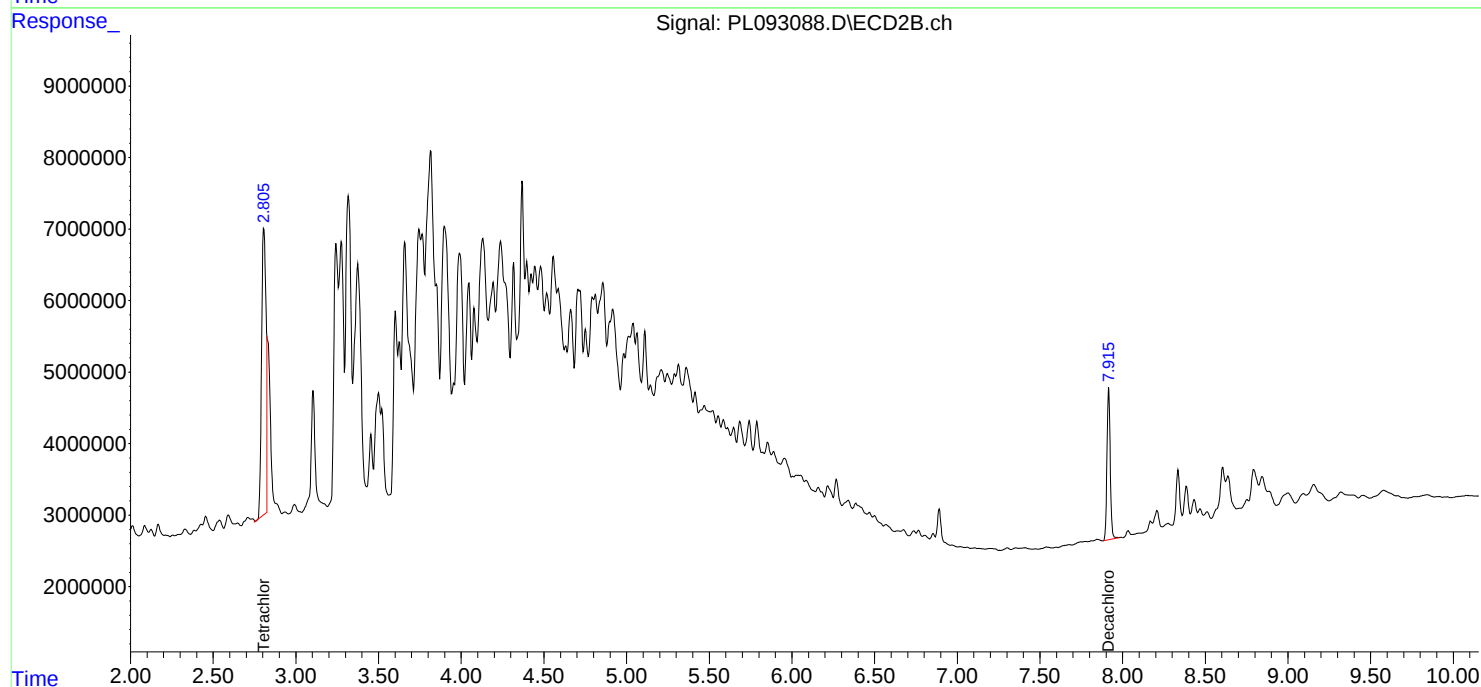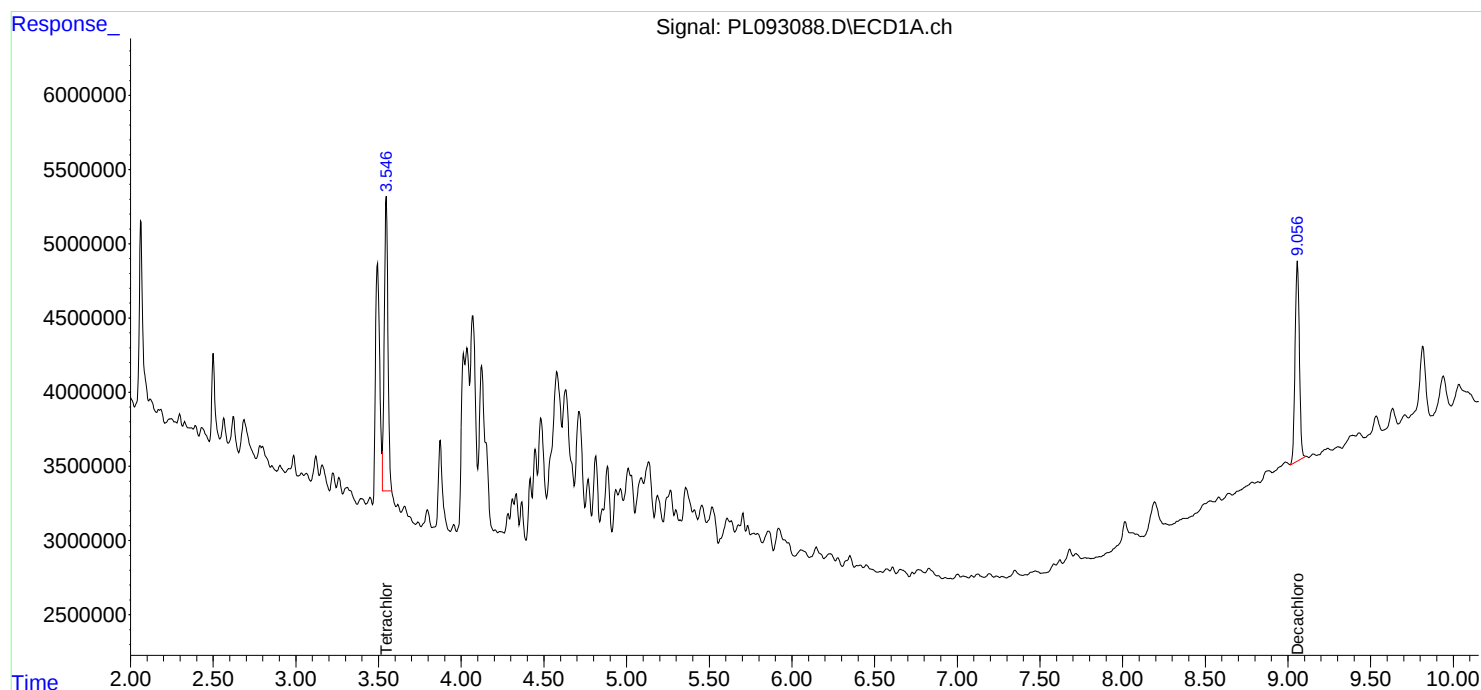

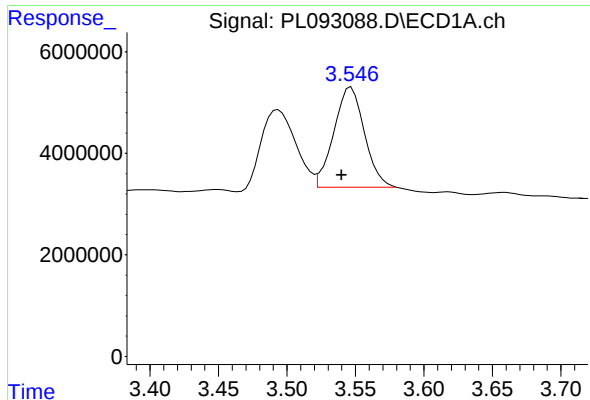


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.006 min
Response: 30490252
Conc: 12.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :Ankita Jodhani 11/18/2024

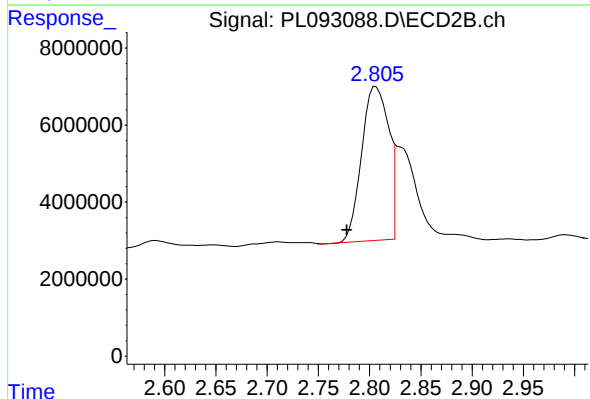


#1 Tetrachloro-m-xylene

R.T.: 2.805 min
Delta R.T.: 0.027 min
Response: 75382703
Conc: 27.70 ng/ml m

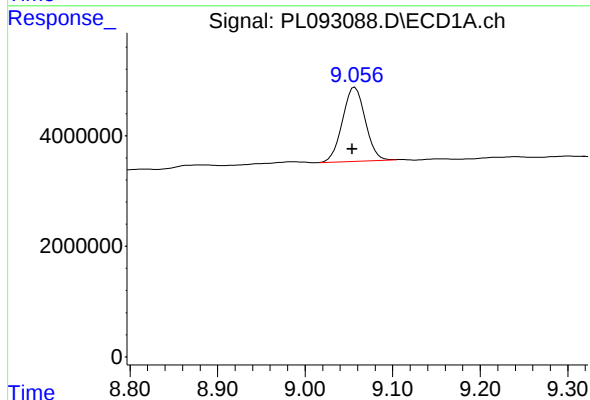

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.002 min
Response: 24275891
Conc: 12.61 ng/ml m

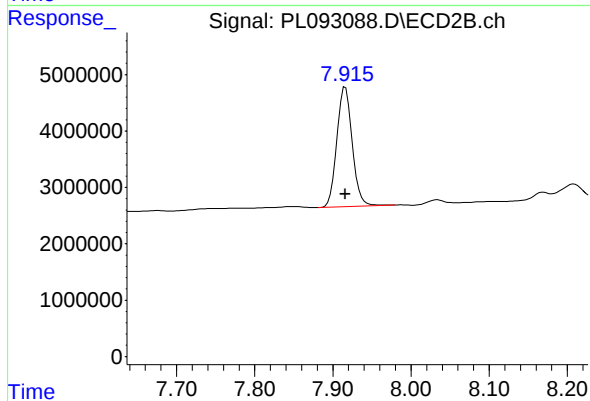

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 29120895
Conc: 10.67 ng/ml