

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL111618\  
 Data File : PL042206.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Nov 2018 20:07  
 Operator : AJ\SJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 15 05:45:32 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL110918.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Nov 09 12:38:40 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |        |       |         |         |        |          |
|------------------|--------------|--------|-------|---------|---------|--------|----------|
| 6) B             | beta-BHC     | 4.401f | 0.000 | 5147364 | 0       | 1.395  | N.D. #   |
| 7) B             | delta-BHC    | 0.000  | 5.159 | 0       | 5112346 | N.D.   | 1.293 #  |
| 8) B             | Heptachlo... | 0.000  | 5.993 | 0       | 4688881 | N.D.   | 1.305 #  |
| 15) B            | Endosulfa... | 6.230f | 0.000 | 2177189 | 0       | 0.319  | N.D. #   |
| 23)              | Chlordane-1  | 4.401  | 5.159 | 5147364 | 5112346 | 17.248 | 35.507 # |
| 27)              | Chlordane-5  | 6.230  | 0.000 | 2177189 | 0       | 8.311  | N.D. #   |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL111618\  
Data File : PL042206.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Nov 2018 20:07  
Operator : AJ\SJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 15 05:45:32 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL110918.M  
Quant Title : GC Extractables  
QLast Update : Fri Nov 09 12:38:40 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

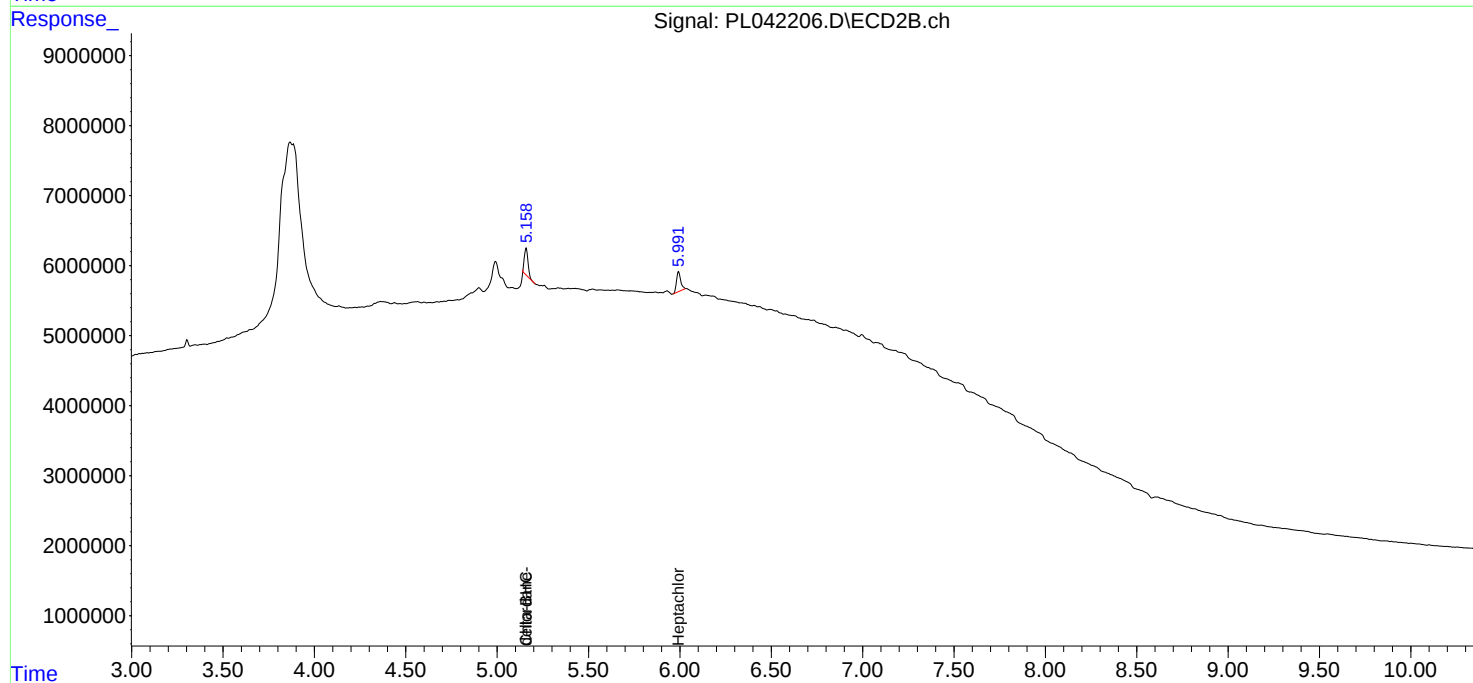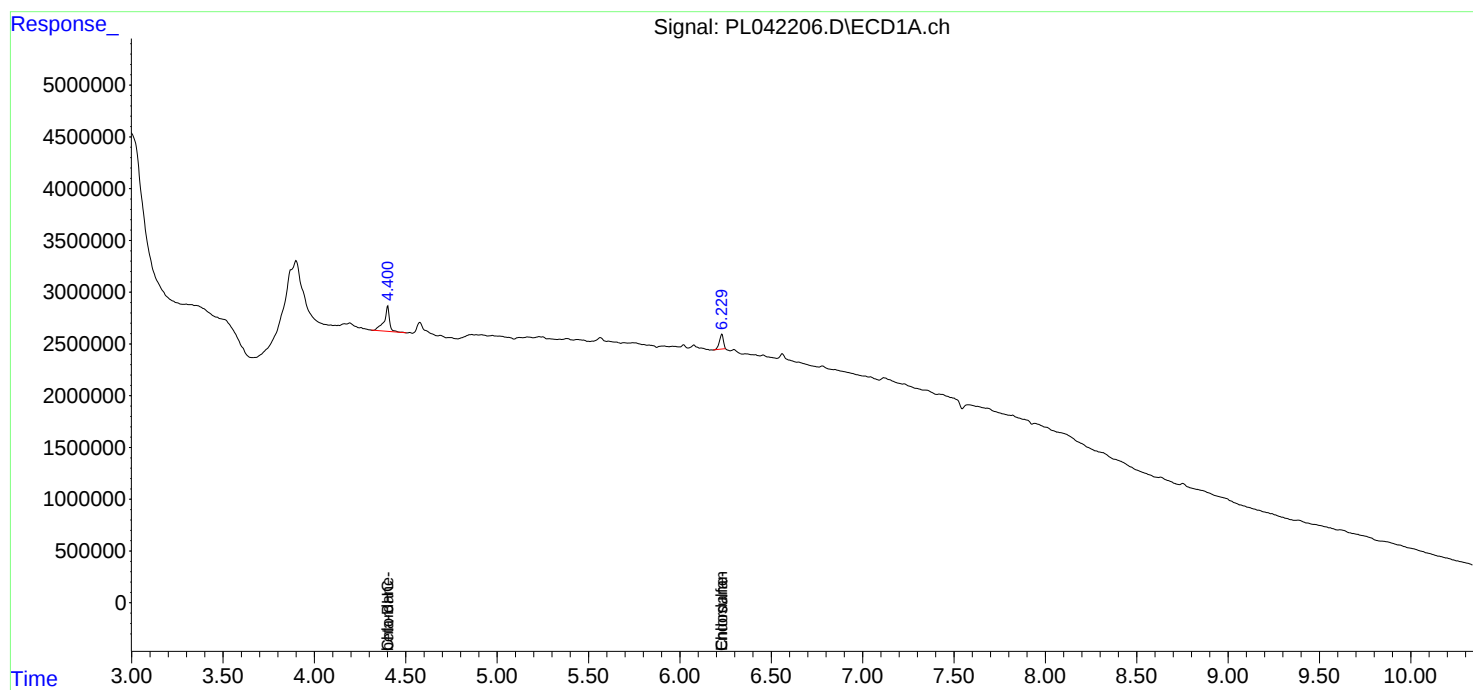


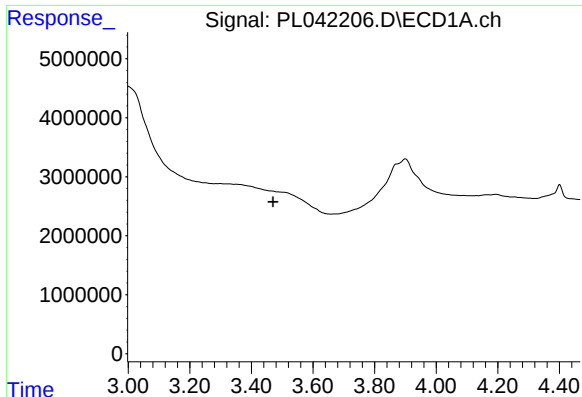

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T.: 3.470 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

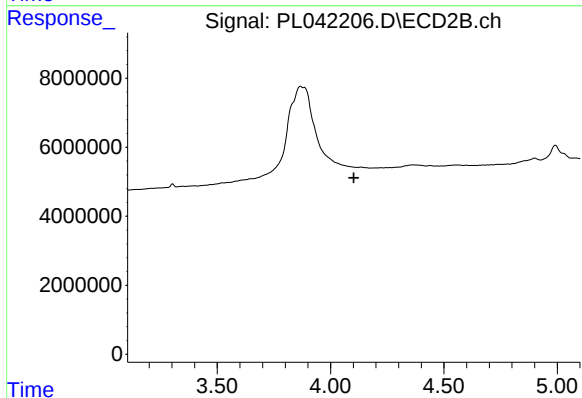


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T.: 4.102 min  
Response: 0  
Conc: N.D.

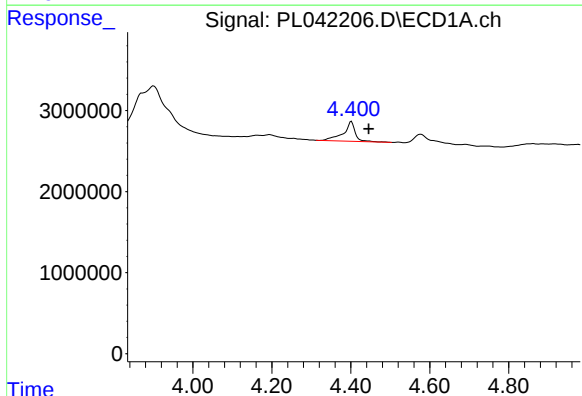


#6 beta-BHC

R.T.: 4.401 min  
Delta R.T.: -0.044 min  
Response: 5147364  
Conc: 1.39 ng/ml

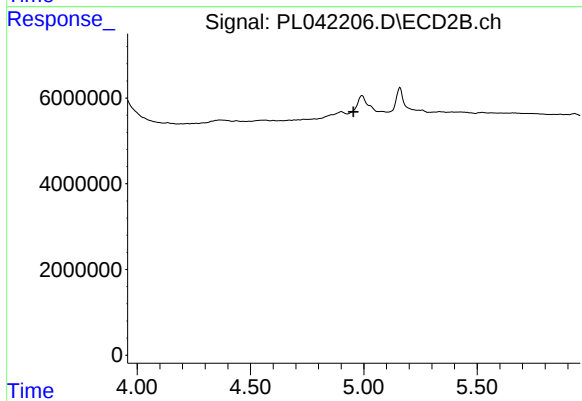

#6 beta-BHC


R.T.: 0.000 min  
Exp R.T.: 4.954 min  
Response: 0  
Conc: N.D.

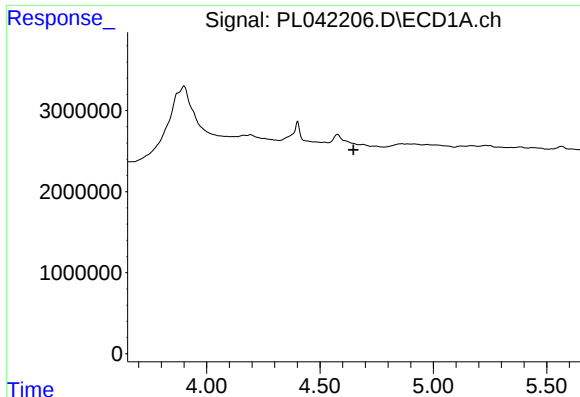

#7 delta-BHC


R.T.: 0.000 min  
Exp R.T. : 4.648 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

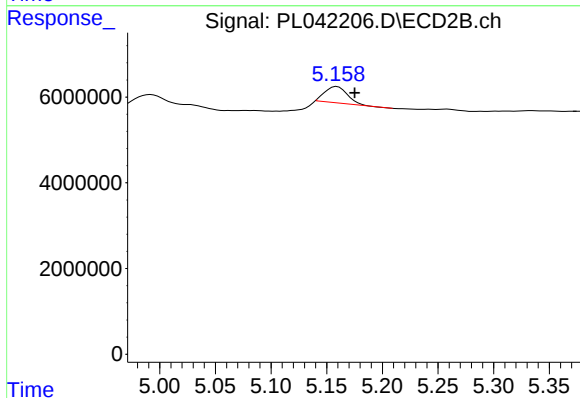


#7 delta-BHC

R.T.: 5.159 min  
Delta R.T.: -0.016 min  
Response: 5112346  
Conc: 1.29 ng/ml

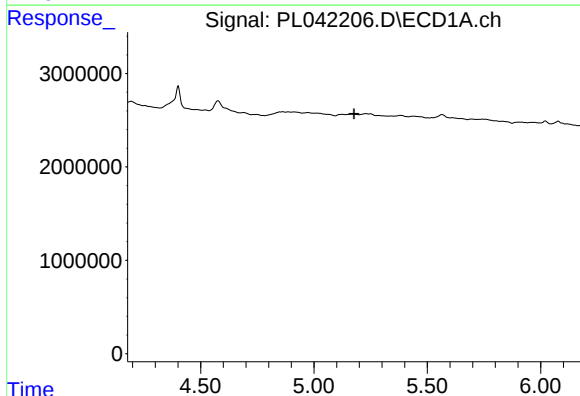


#8 Heptachlor epoxide

R.T.: 0.000 min  
Exp R.T. : 5.178 min  
Response: 0  
Conc: N.D.

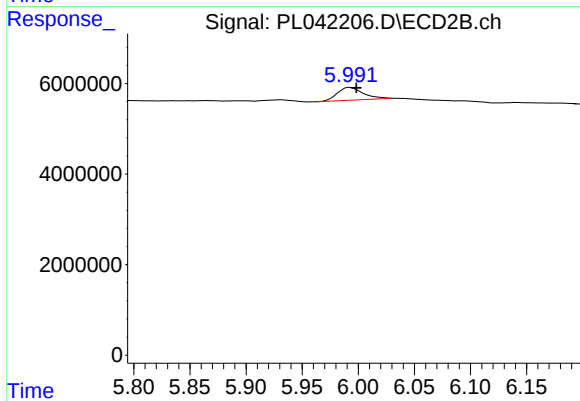

#8 Heptachlor epoxide


R.T.: 5.993 min  
Delta R.T.: -0.005 min  
Response: 4688881  
Conc: 1.31 ng/ml

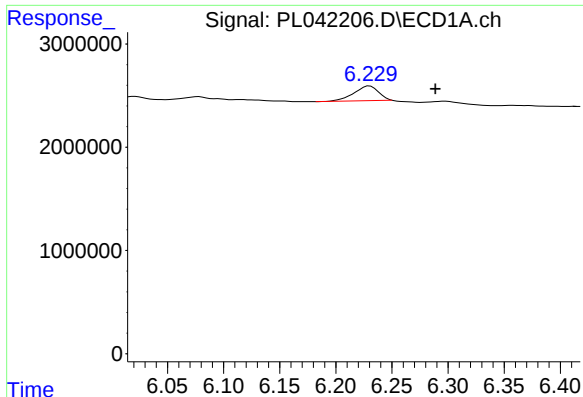

#15 Endosulfan II


R.T.: 6.230 min  
Delta R.T.: -0.058 min  
Response: 2177189  
Conc: 0.32 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

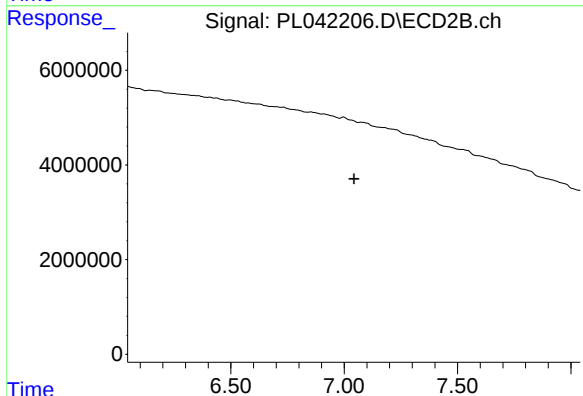


#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T. : 7.044 min  
Response: 0  
Conc: N.D.

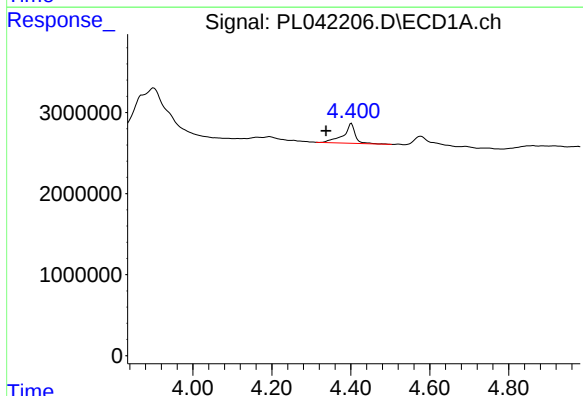


#23 Chlordane-1

R.T.: 4.401 min  
Delta R.T.: 0.064 min  
Response: 5147364  
Conc: 17.25 ng/ml

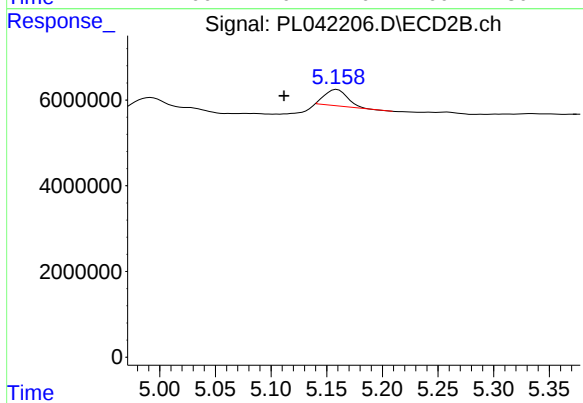

#23 Chlordane-1


R.T.: 5.159 min  
Delta R.T.: 0.048 min  
Response: 5112346  
Conc: 35.51 ng/ml

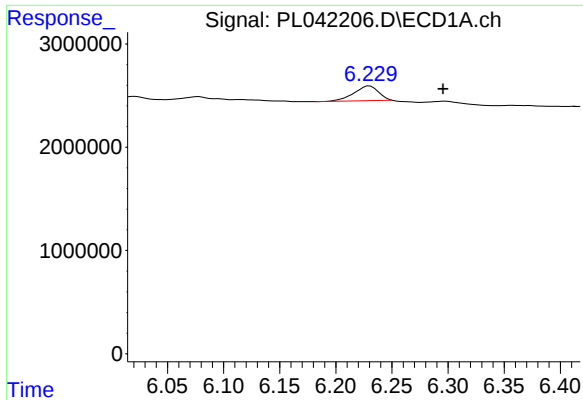

#27 Chlordane-5


R.T.: 6.230 min  
Delta R.T.: -0.065 min  
Response: 2177189  
Conc: 8.31 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

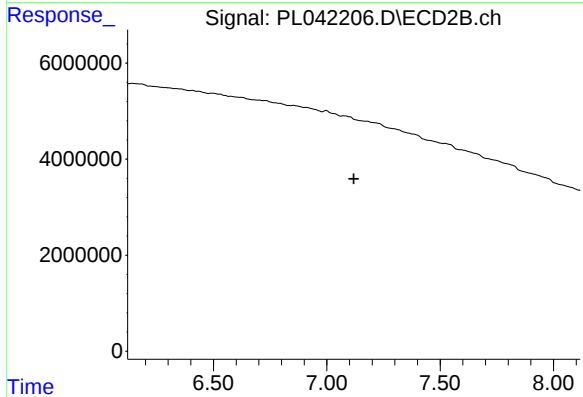


#27 Chlordane-5

R.T.: 0.000 min  
Exp R.T. : 7.119 min  
Response: 0  
Conc: N.D.

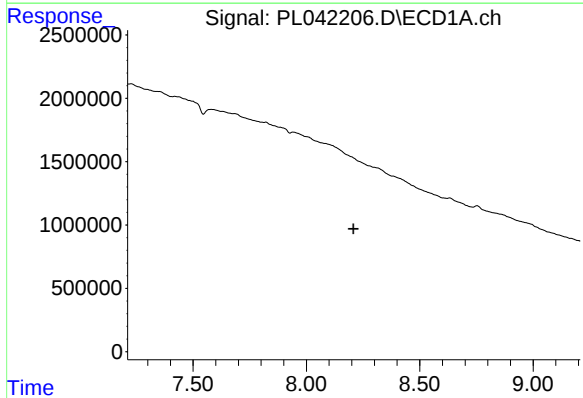

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.208 min  
Response: 0  
Conc: N.D.

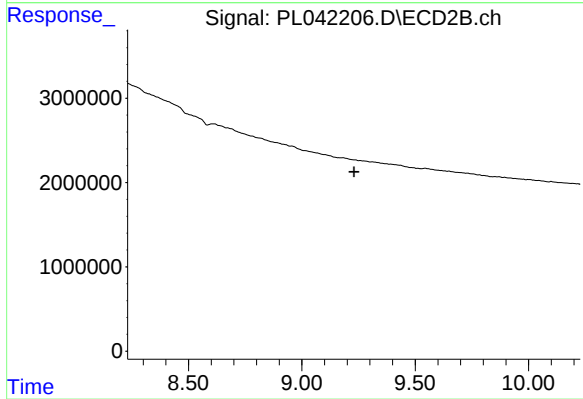

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.230 min  
Response: 0  
Conc: N.D.