

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
 Data File : PL042210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 21:03
 Operator : AJ\SJ
 Sample : PB114784BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 05:45:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	107.7E6	55651421	17.445	18.784
28)	SA Decachlor...	8.204	9.228	126.8E6	49436250	18.515	19.382
Target Compounds							
2)	A alpha-BHC	3.904	4.503	3311435	5763518	0.349	1.298 #
6)	B beta-BHC	4.407f	0.000	5798164	0	1.571	N.D. #
7)	B delta-BHC	0.000	5.150	0	2779019	N.D.	0.703 #
8)	B Heptachlo...	0.000	5.994	0	3201964	N.D.	0.891 #
15)	B Endosulfa...	6.230f	0.000	1598258	0	0.234	N.D. #
19)	B Endosulfa...	6.653	7.383	8106603	10544943	1.271	3.877 #
20)	A Methoxychlor	0.000	7.645f	0	13085143	N.D.	9.523 #
21)	B Endrin ke...	7.197f	0.000	4080964	0	0.566	N.D. #
23)	Chlordane-1	4.365	5.150	1700565	2779019	5.698	19.301 #
27)	Chlordane-5	6.230	0.000	1598258	0	6.101	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
Data File : PL042210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 21:03
Operator : AJ\SJ
Sample : PB114784BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 05:45:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

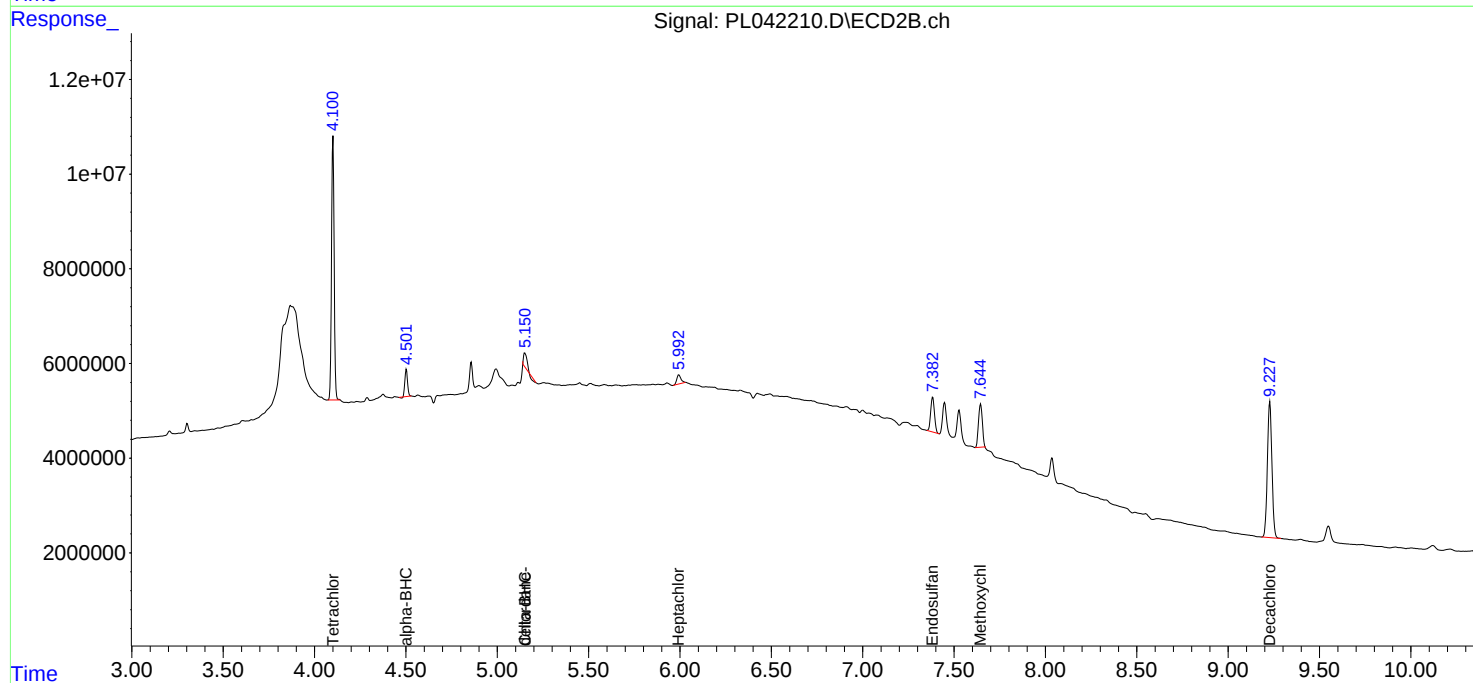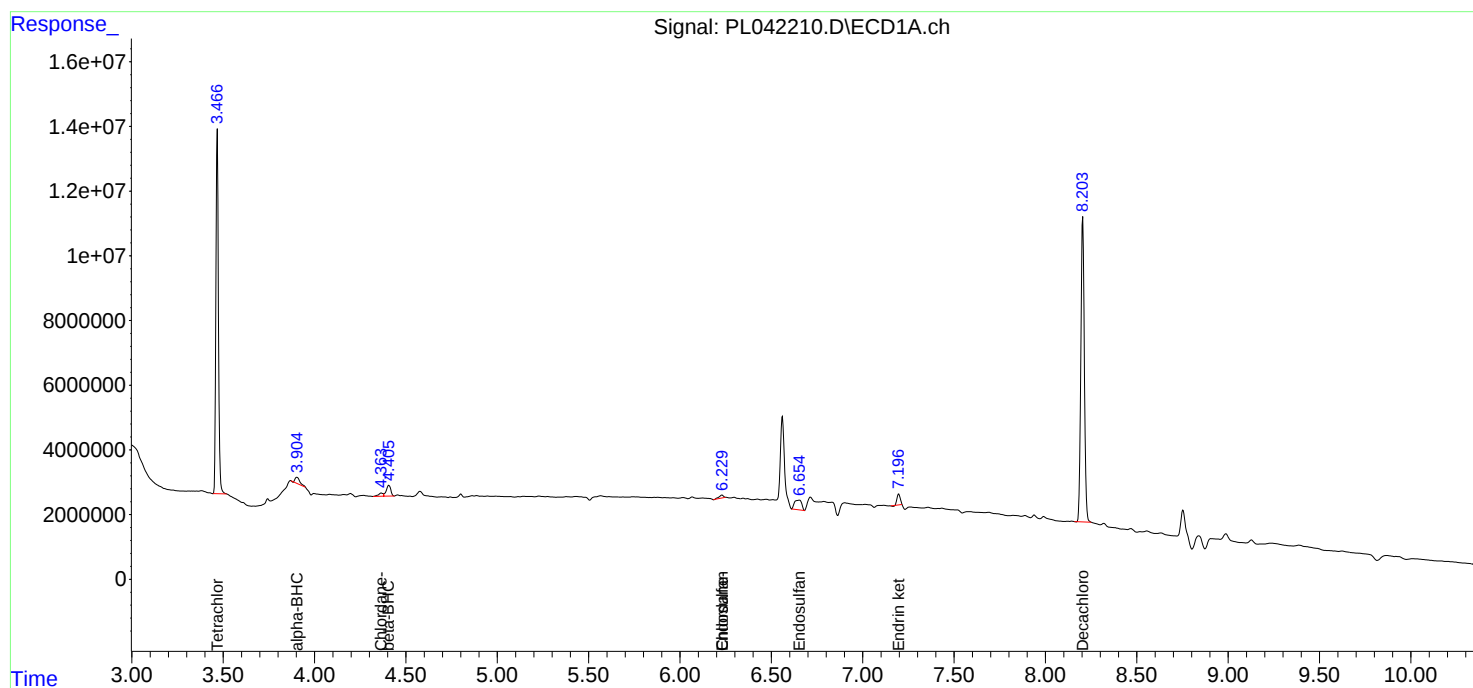


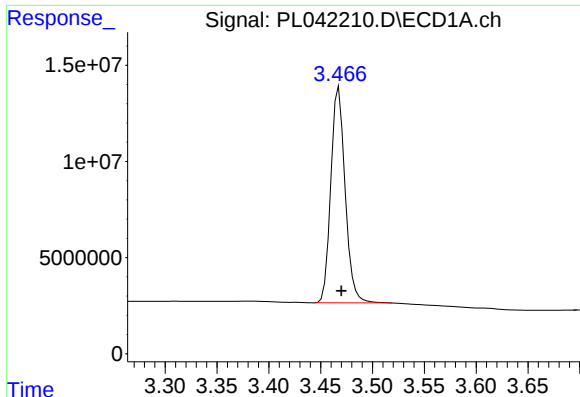

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: -0.002 min
Response: 107722321
Conc: 17.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

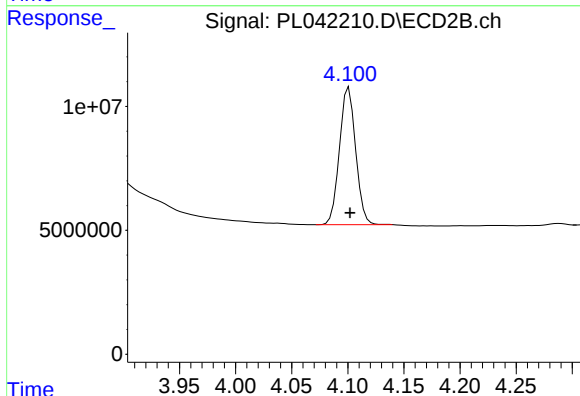


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.001 min
Response: 55651421
Conc: 18.78 ng/ml

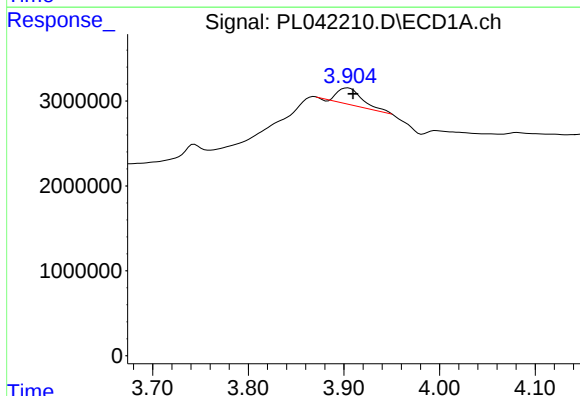


#2 alpha-BHC

R.T.: 3.904 min
Delta R.T.: -0.005 min
Response: 3311435
Conc: 0.35 ng/ml

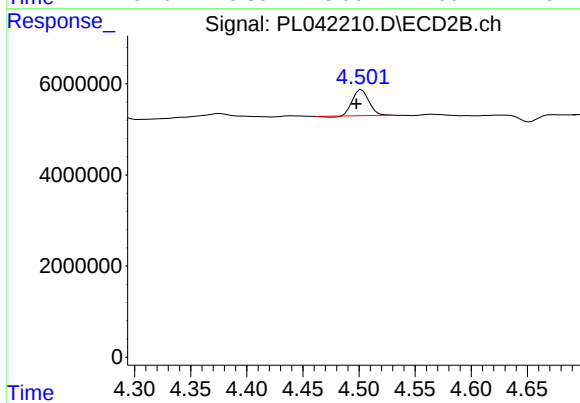

#2 alpha-BHC


R.T.: 4.503 min
Delta R.T.: 0.005 min
Response: 5763518
Conc: 1.30 ng/ml

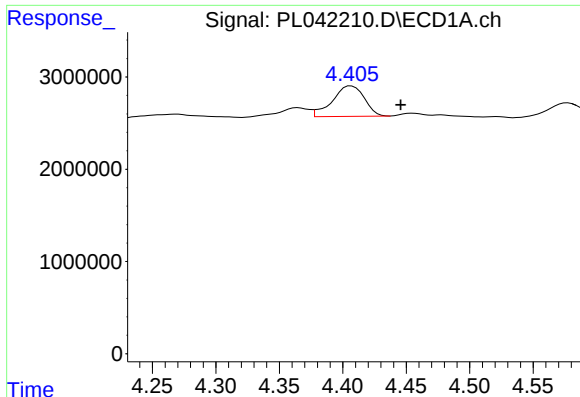

#6 beta-BHC


R.T.: 4.407 min
Delta R.T.: -0.039 min
Response: 5798164
Conc: 1.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

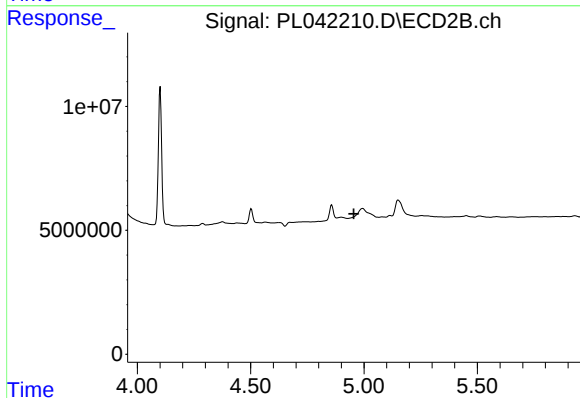


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

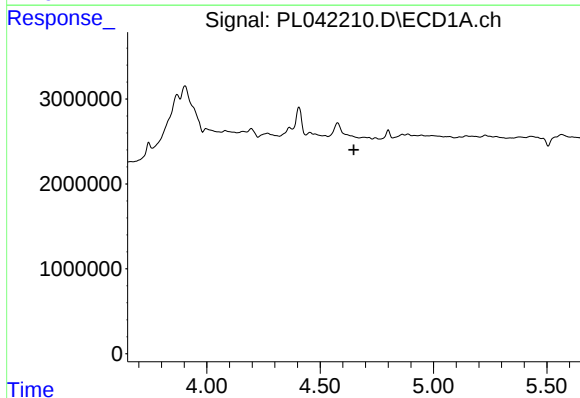


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

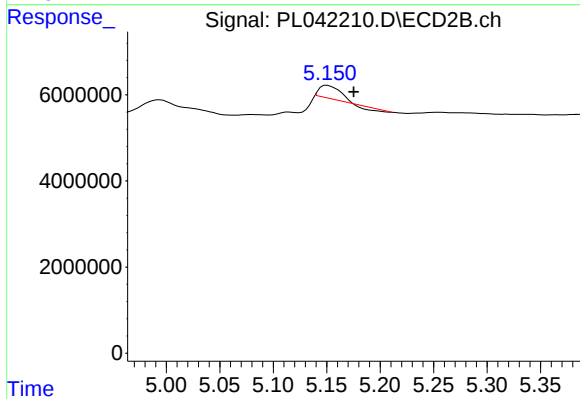

#7 delta-BHC


R.T.: 5.150 min
Delta R.T.: -0.025 min
Response: 2779019
Conc: 0.70 ng/ml

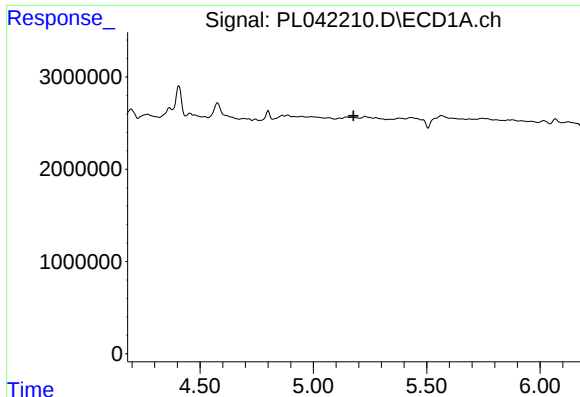

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

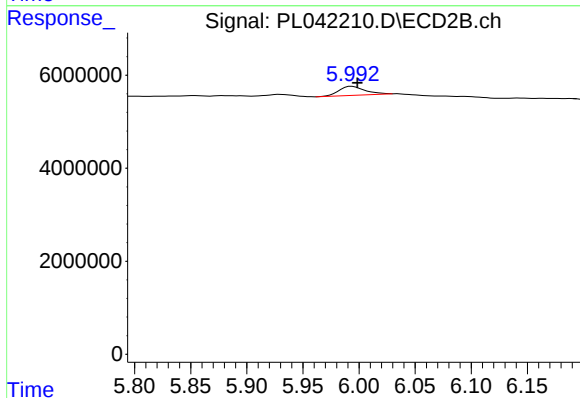


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.005 min
Response: 3201964
Conc: 0.89 ng/ml

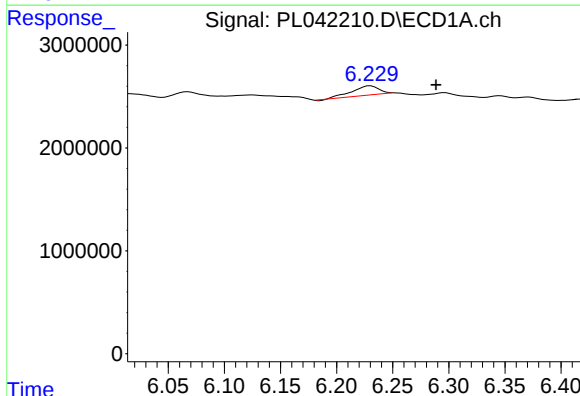


#15 Endosulfan II

R.T.: 6.230 min
Delta R.T.: -0.059 min
Response: 1598258
Conc: 0.23 ng/ml

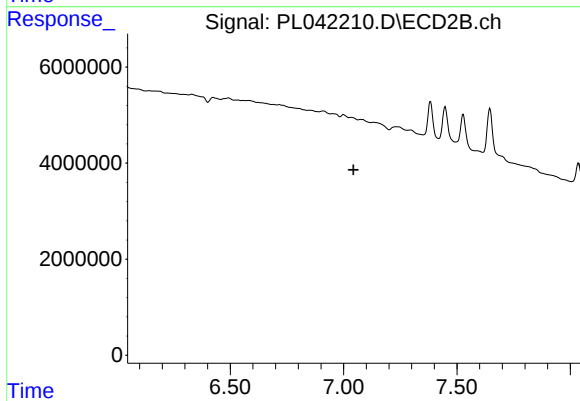

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.044 min
Response: 0
Conc: N.D.

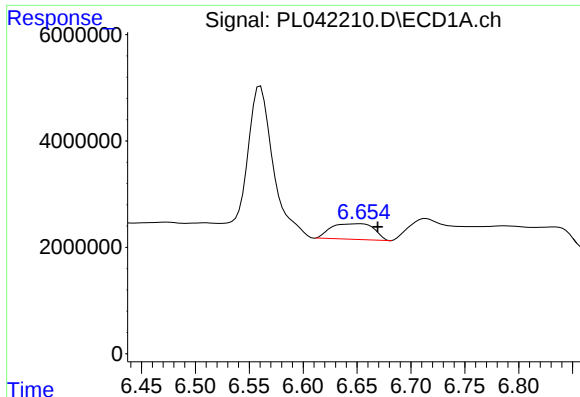

#19 Endosulfan Sulfate


R.T.: 6.653 min
Delta R.T.: -0.016 min
Response: 8106603
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

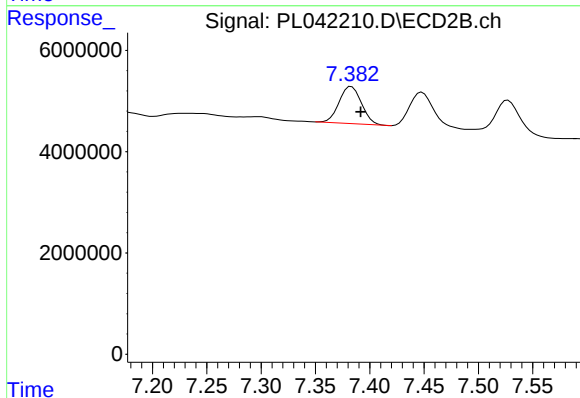


#19 Endosulfan Sulfate

R.T.: 7.383 min
Delta R.T.: -0.009 min
Response: 10544943
Conc: 3.88 ng/ml

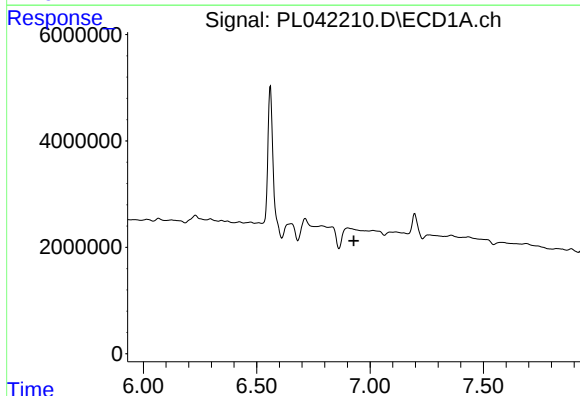


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

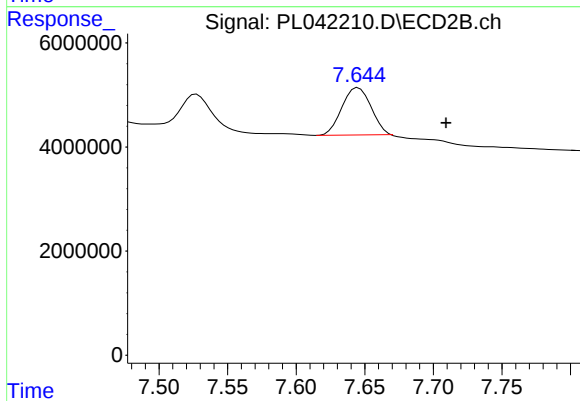

#20 Methoxychlor


R.T.: 7.645 min
Delta R.T.: -0.064 min
Response: 13085143
Conc: 9.52 ng/ml

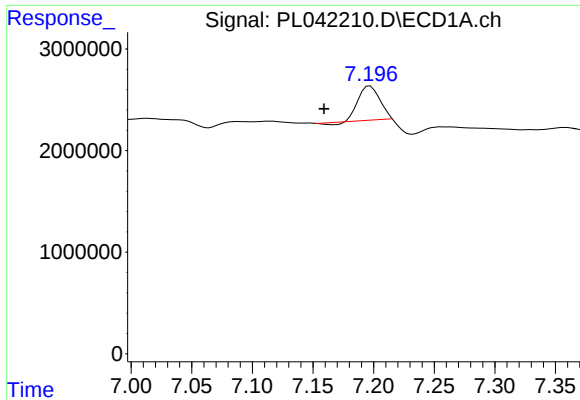

#21 Endrin ketone


R.T.: 7.197 min
Delta R.T.: 0.038 min
Response: 4080964
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

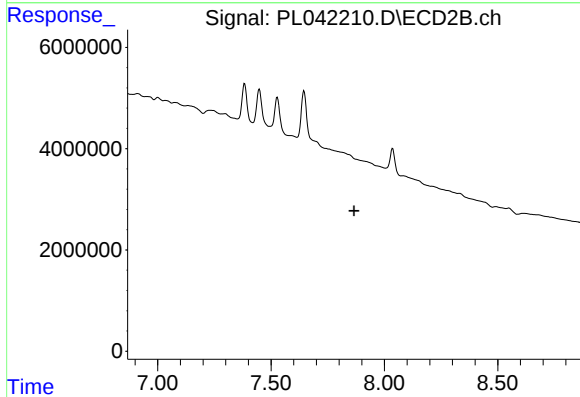


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.867 min
Response: 0
Conc: N.D.

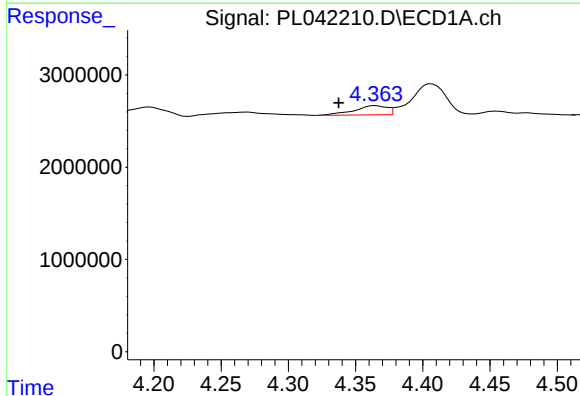


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.027 min
Response: 1700565
Conc: 5.70 ng/ml

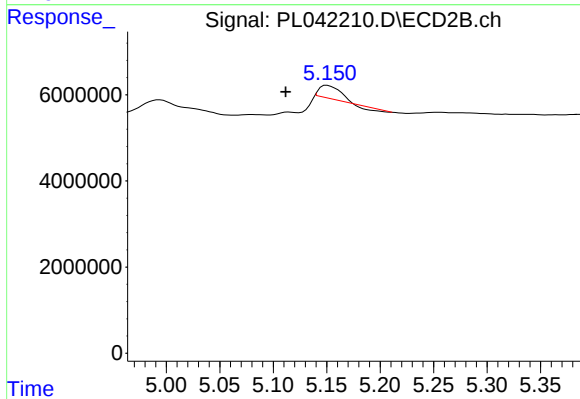

#23 Chlordane-1


R.T.: 5.150 min
Delta R.T.: 0.039 min
Response: 2779019
Conc: 19.30 ng/ml

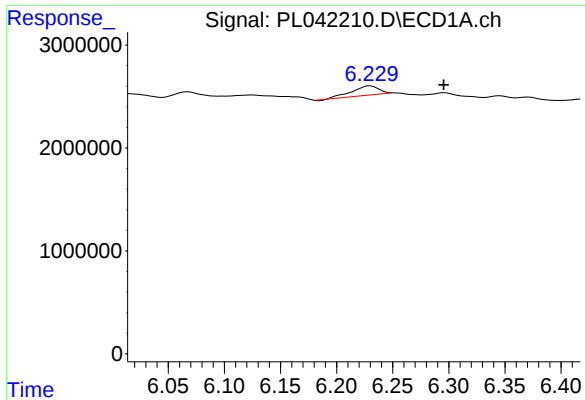

#27 Chlordane-5


R.T.: 6.230 min
Delta R.T.: -0.065 min
Response: 1598258
Conc: 6.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

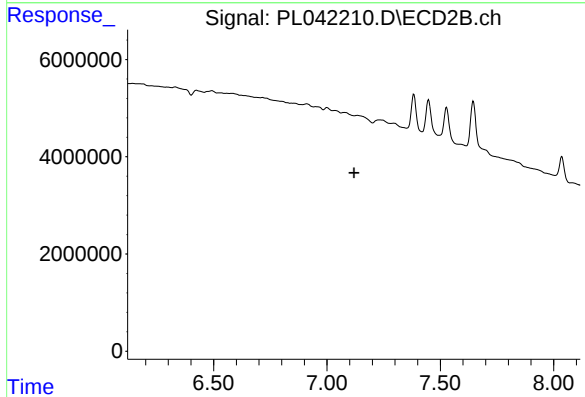


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.119 min
Response: 0
Conc: N.D.

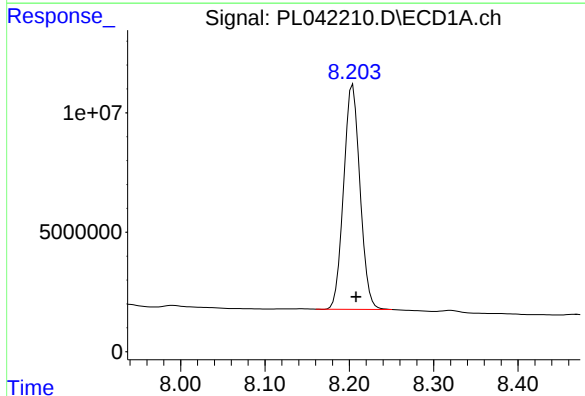

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.004 min
Response: 126835152
Conc: 18.52 ng/ml

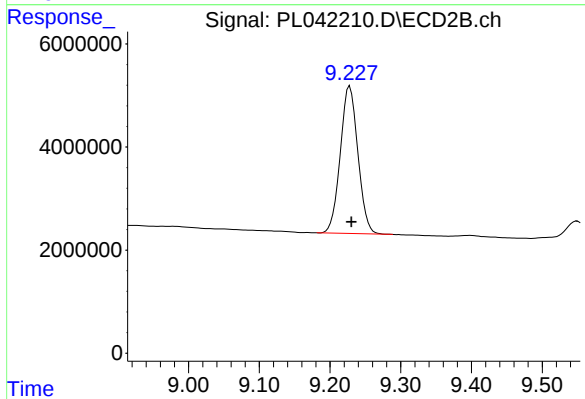

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: -0.002 min
Response: 49436250
Conc: 19.38 ng/ml