

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
 Data File : PL042212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 21:31
 Operator : AJ\SJ
 Sample : PB114784TB
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 05:46:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	104.7E6	55049501	16.960	18.581
28)	SA Decachlor...	8.204	9.228	125.1E6	47924467	18.258	18.790
Target Compounds							
2)	A alpha-BHC	3.901	4.502	3493462	3321452	0.368	0.748 #
6)	B beta-BHC	4.404f	0.000	4725678	0	1.280	N.D. #
7)	B delta-BHC	0.000	5.152	0	1747805	N.D.	0.442 #
8)	B Heptachlo...	0.000	5.993	0	2124636	N.D.	0.591 #
15)	B Endosulfa...	6.229f	0.000	1842561	0	0.270	N.D. #
19)	B Endosulfa...	6.655	7.383	6006645	6447441	0.942	2.370 #
20)	A Methoxychlor	0.000	7.646f	0	8075373	N.D.	5.877 #
21)	B Endrin ke...	7.197f	0.000	2267084	0	0.315	N.D. #
23)	Chlordane-1	4.365	5.152	1741635	1747805	5.836	12.139 #
27)	Chlordane-5	6.229	0.000	1842561	0	7.034	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
Data File : PL042212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 21:31
Operator : AJ\SJ
Sample : PB114784TB
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 05:46:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

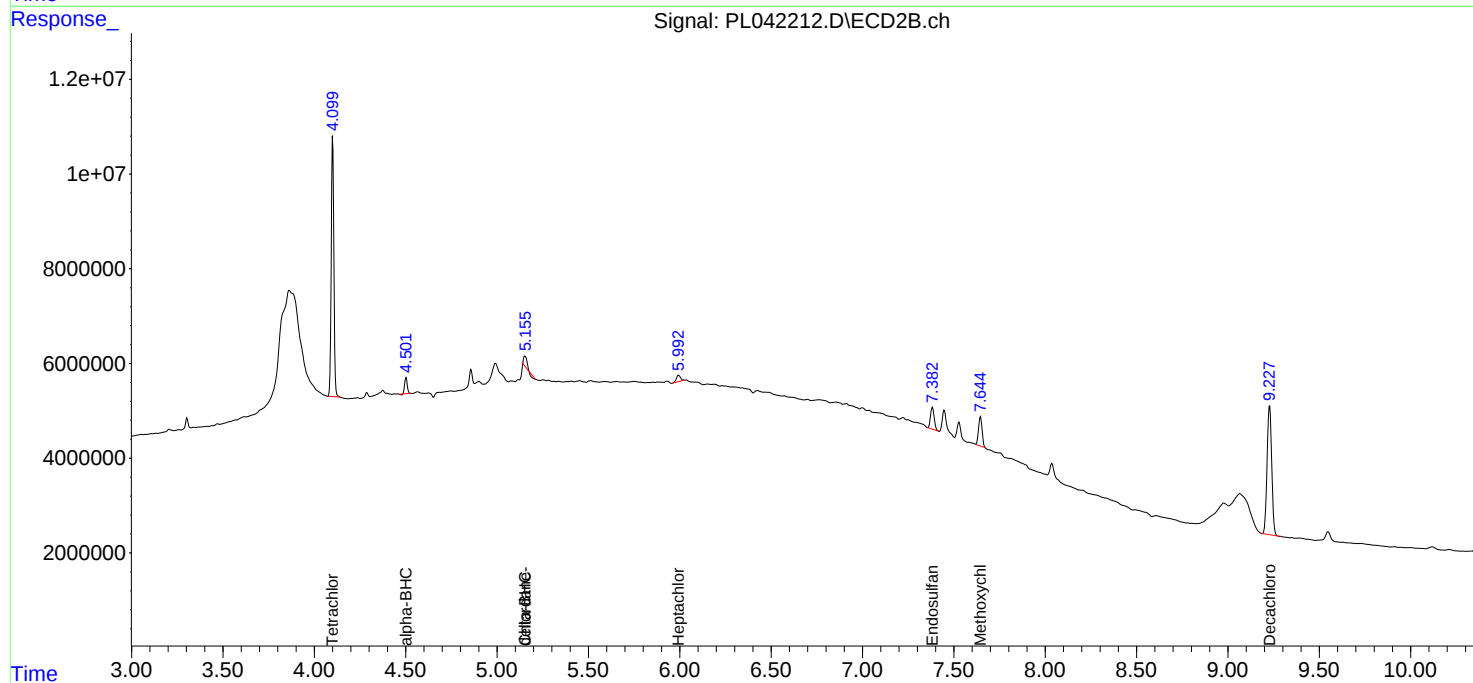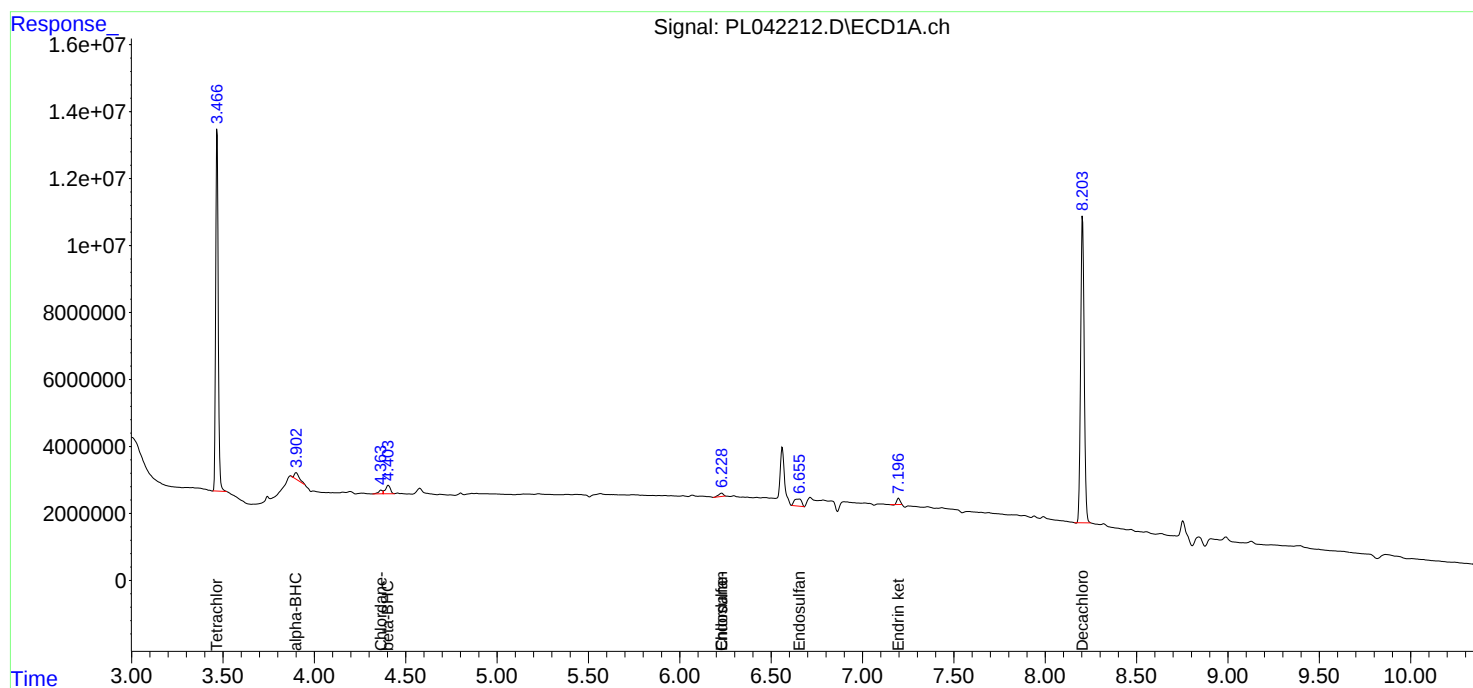


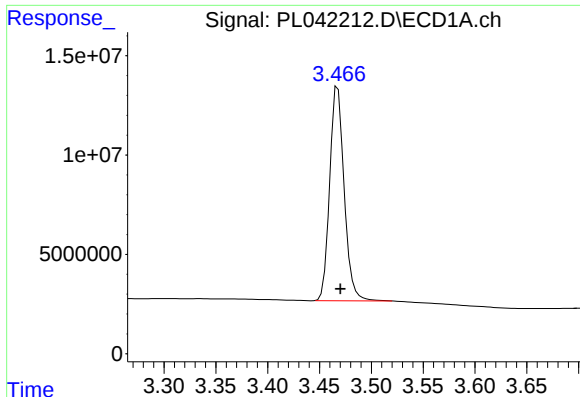

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: -0.002 min
Response: 104727651
Conc: 16.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

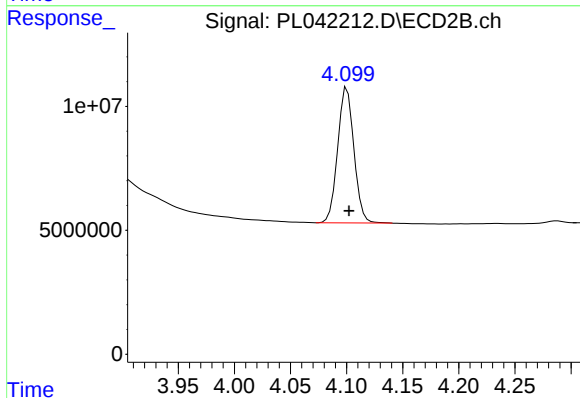


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.002 min
Response: 55049501
Conc: 18.58 ng/ml

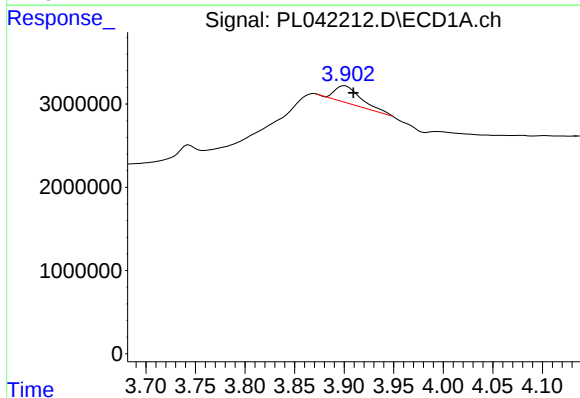


#2 alpha-BHC

R.T.: 3.901 min
Delta R.T.: -0.009 min
Response: 3493462
Conc: 0.37 ng/ml

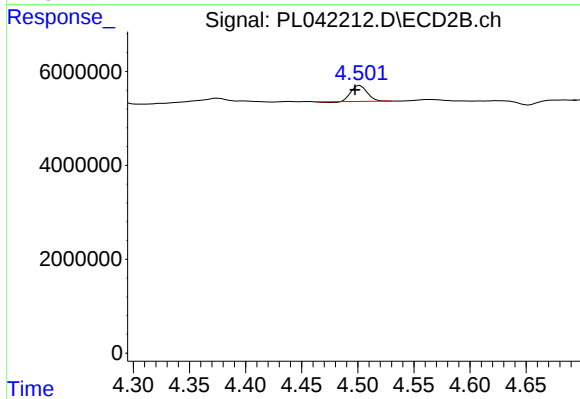

#2 alpha-BHC


R.T.: 4.502 min
Delta R.T.: 0.005 min
Response: 3321452
Conc: 0.75 ng/ml

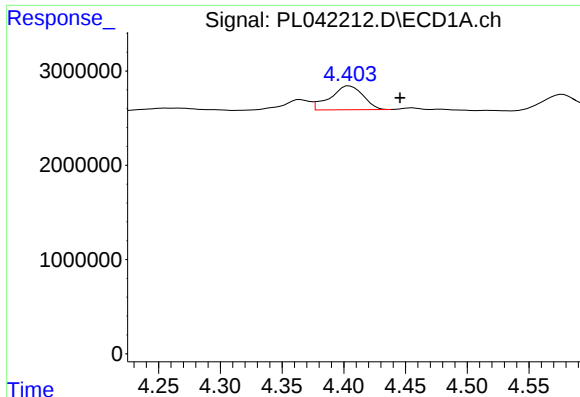

#6 beta-BHC


R.T.: 4.404 min
Delta R.T.: -0.041 min
Response: 4725678
Conc: 1.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

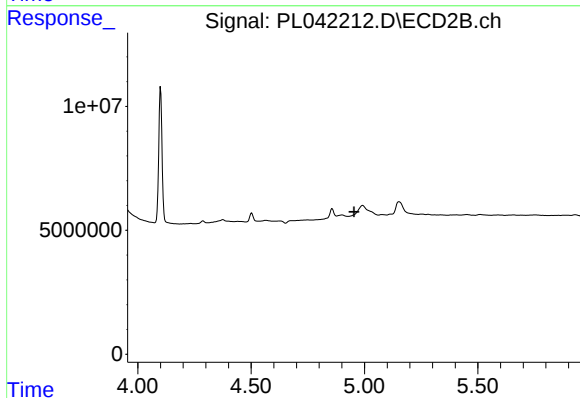


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

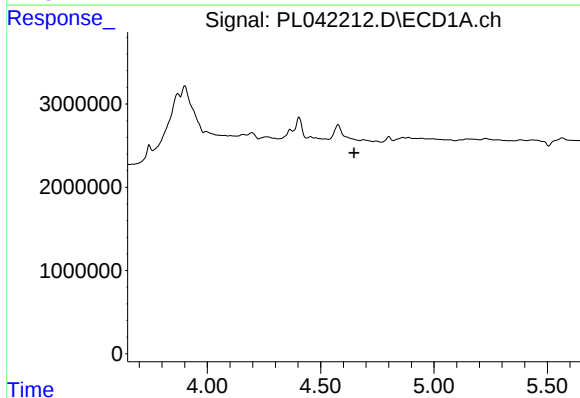


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

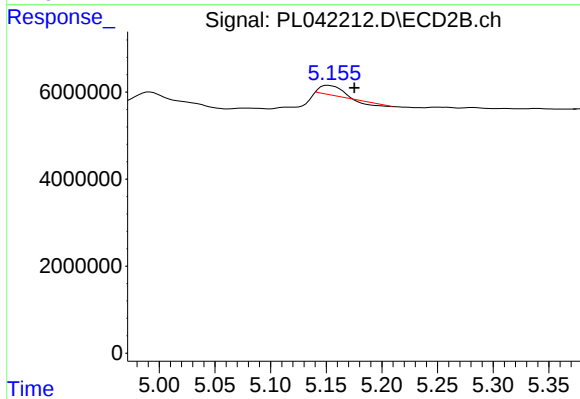

#7 delta-BHC


R.T.: 5.152 min
Delta R.T.: -0.023 min
Response: 1747805
Conc: 0.44 ng/ml

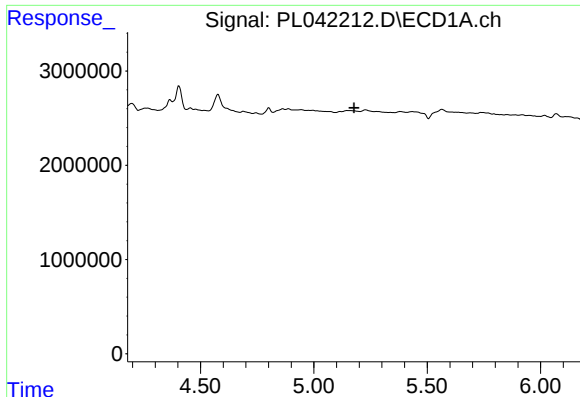

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

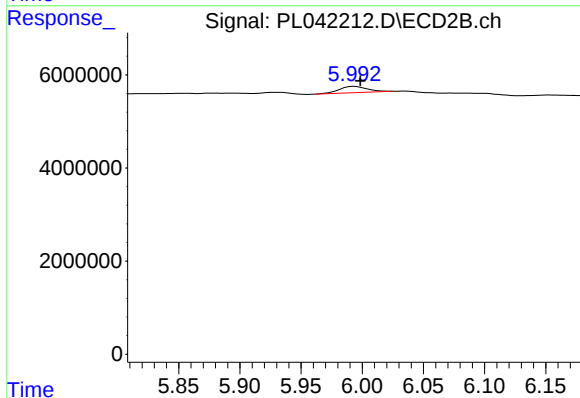


#8 Heptachlor epoxide

R.T.: 5.993 min
Delta R.T.: -0.005 min
Response: 2124636
Conc: 0.59 ng/ml

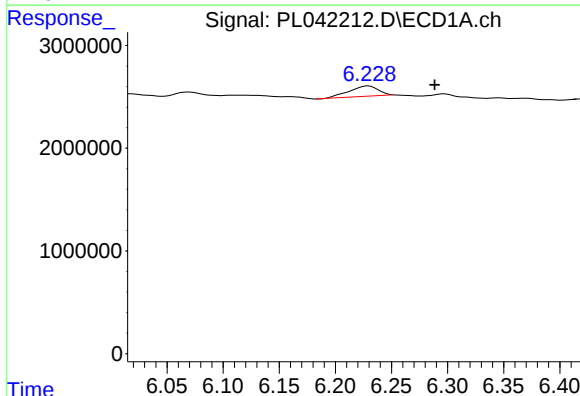


#15 Endosulfan II

R.T.: 6.229 min
Delta R.T.: -0.059 min
Response: 1842561
Conc: 0.27 ng/ml

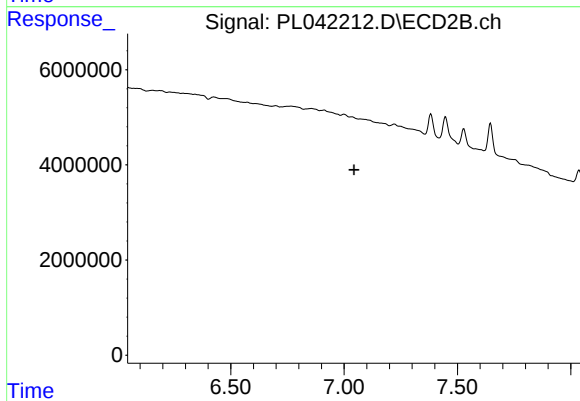

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.044 min
Response: 0
Conc: N.D.

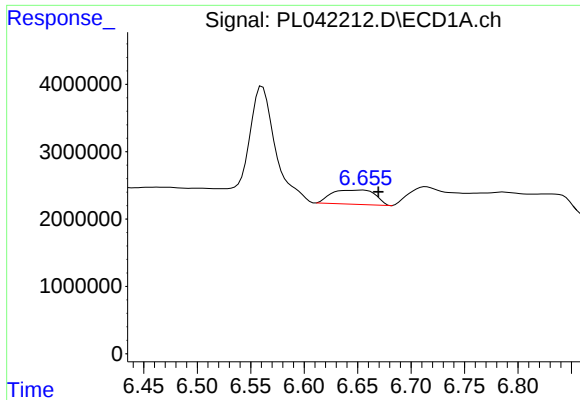

#19 Endosulfan Sulfate


R.T.: 6.655 min
Delta R.T.: -0.014 min
Response: 6006645
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

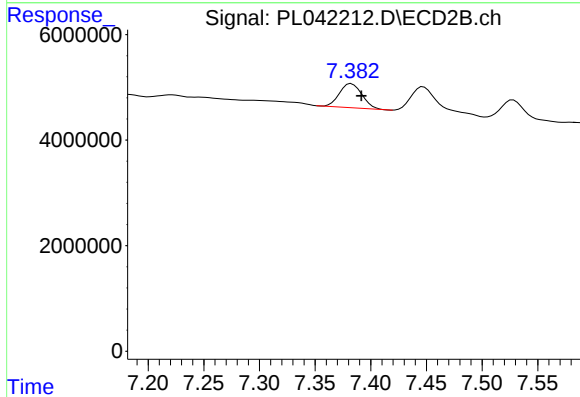


#19 Endosulfan Sulfate

R.T.: 7.383 min
Delta R.T.: -0.009 min
Response: 6447441
Conc: 2.37 ng/ml

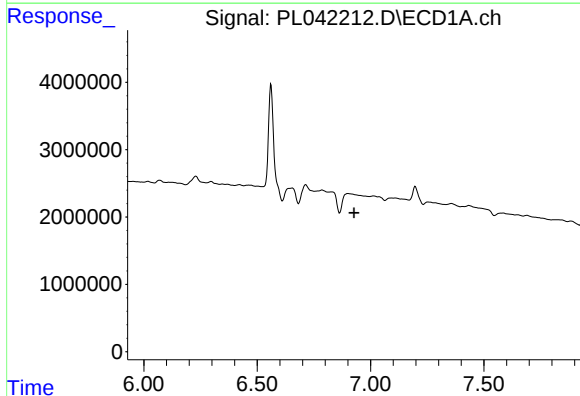


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

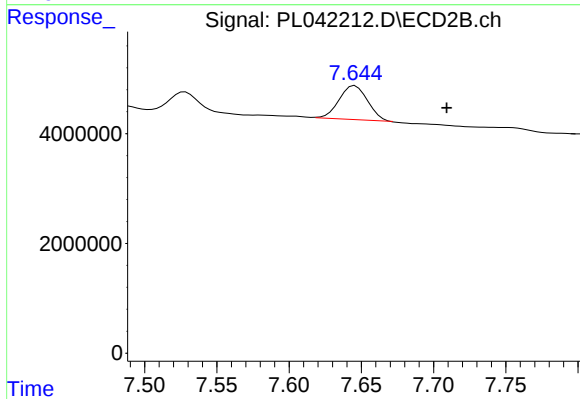

#20 Methoxychlor


R.T.: 7.646 min
Delta R.T.: -0.064 min
Response: 8075373
Conc: 5.88 ng/ml

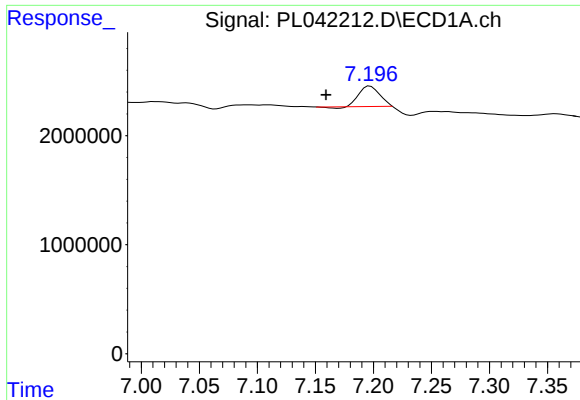

#21 Endrin ketone


R.T.: 7.197 min
Delta R.T.: 0.038 min
Response: 2267084
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

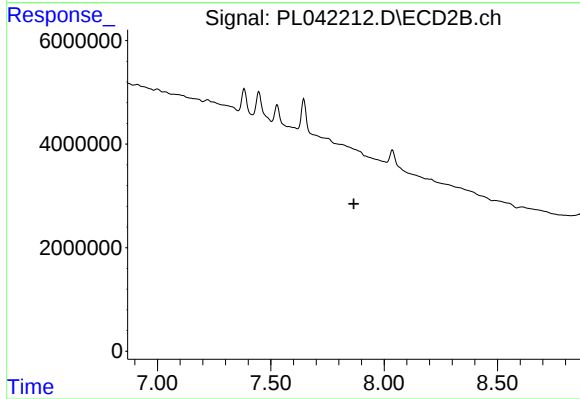


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.867 min
Response: 0
Conc: N.D.

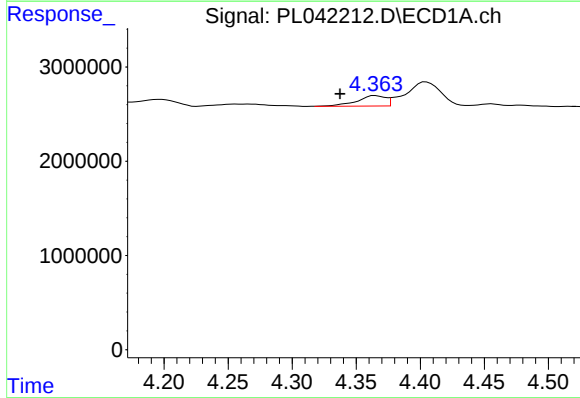


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.028 min
Response: 1741635
Conc: 5.84 ng/ml

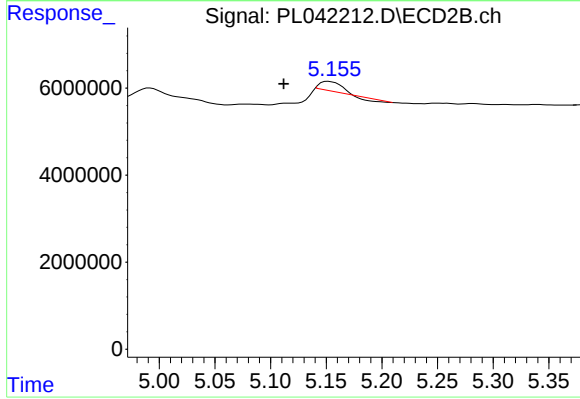

#23 Chlordane-1


R.T.: 5.152 min
Delta R.T.: 0.041 min
Response: 1747805
Conc: 12.14 ng/ml

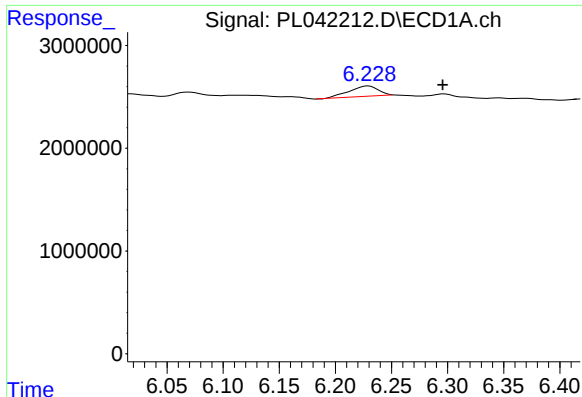

#27 Chlordane-5


R.T.: 6.229 min
Delta R.T.: -0.066 min
Response: 1842561
Conc: 7.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

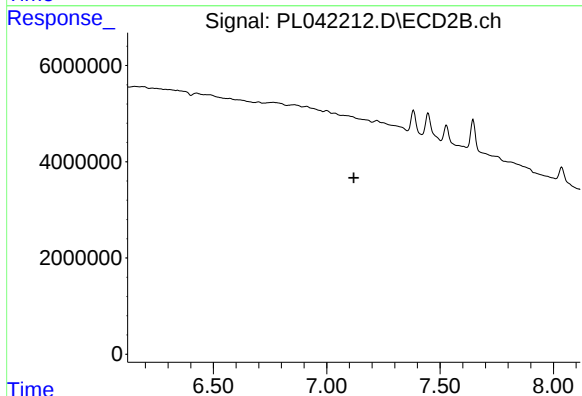


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.119 min
Response: 0
Conc: N.D.

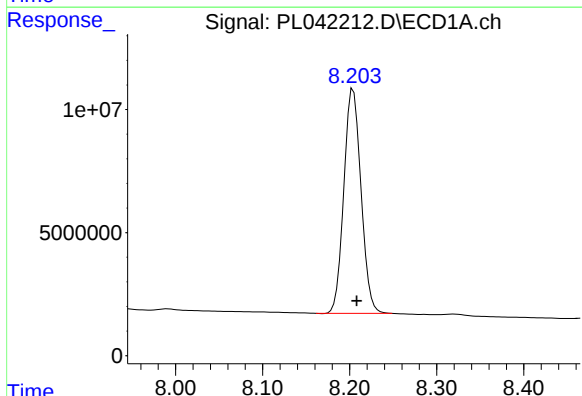

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.004 min
Response: 125072070
Conc: 18.26 ng/ml

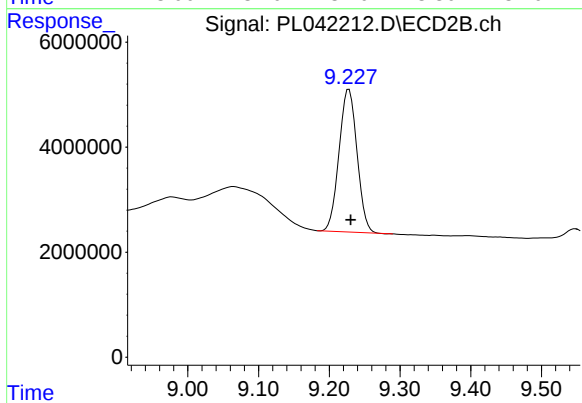

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: -0.002 min
Response: 47924467
Conc: 18.79 ng/ml