

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
 Data File : PL042216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 22:28
 Operator : AJ\SJ
 Sample : J5925-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 05:46:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	96397065	51350305	15.611	17.332
28)	SA Decachlor...	8.203	9.228	118.3E6	47295563	17.275	18.543
Target Compounds							
6)	B beta-BHC	4.403f	0.000	7541724	0	2.044	N.D. #
7)	B delta-BHC	0.000	5.149f	0	669757	N.D.	0.169 #
8)	B Heptachlo...	0.000	5.993	0	3131973	N.D.	0.872 #
15)	B Endosulfa...	6.228f	0.000	934231	0	0.137	N.D. #
19)	B Endosulfa...	6.657	0.000	3247577	0	0.509	N.D. #
20)	A Methoxychlor	0.000	7.645f	0	1571197	N.D.	1.143 #
23)	Chlordane-1	4.378	5.149	1858315	669757	6.227	4.652 #
27)	Chlordane-5	6.228	0.000	934231	0	3.566	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
Data File : PL042216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 22:28
Operator : AJ\SJ
Sample : J5925-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 05:46:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

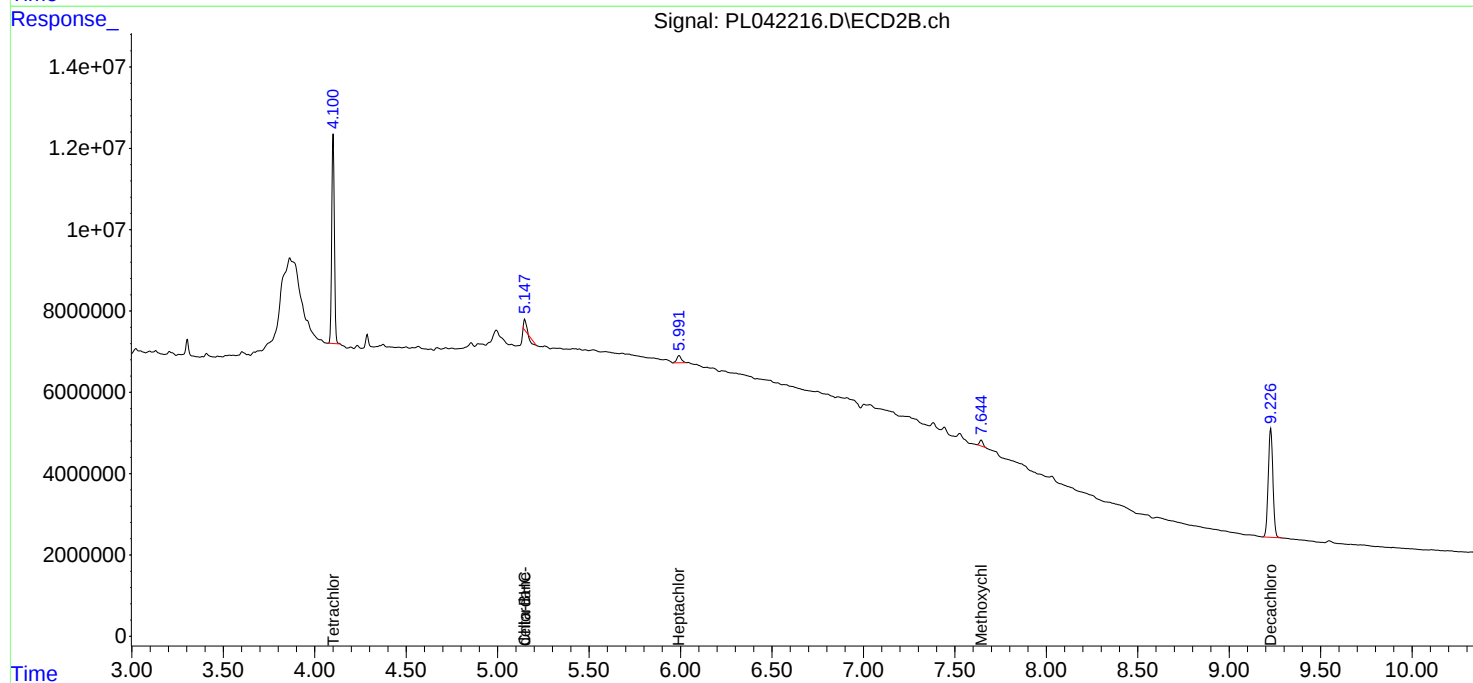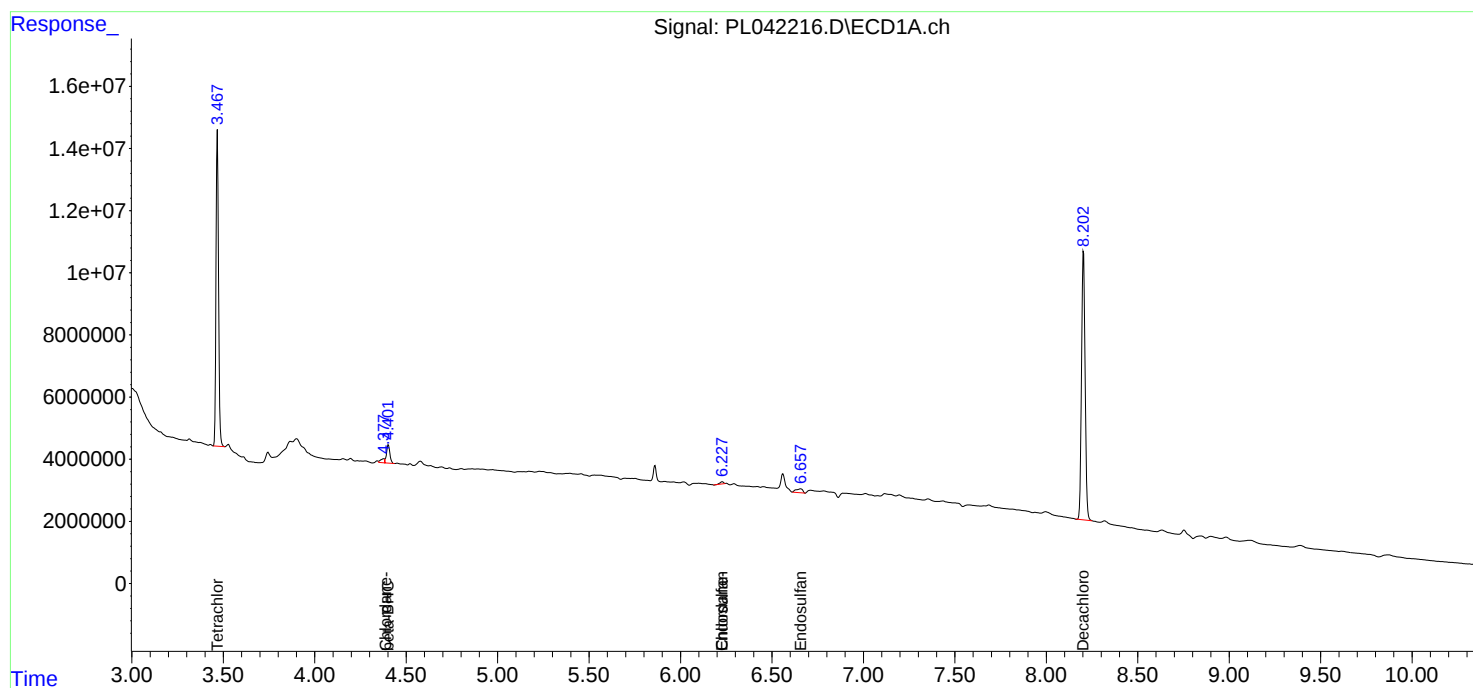


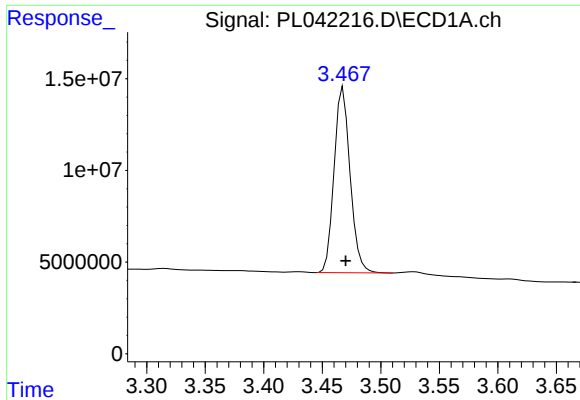

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: -0.002 min
Response: 96397065
Conc: 15.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

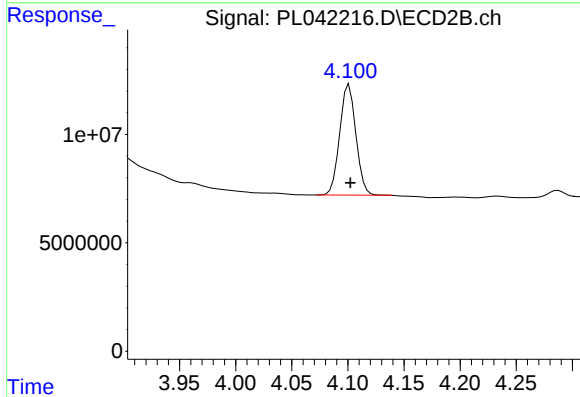


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 51350305
Conc: 17.33 ng/ml

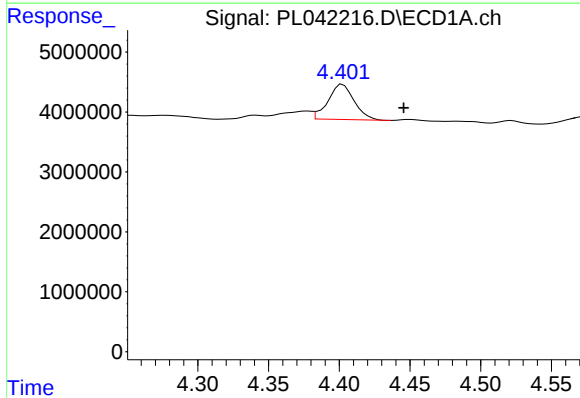


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: -0.043 min
Response: 7541724
Conc: 2.04 ng/ml

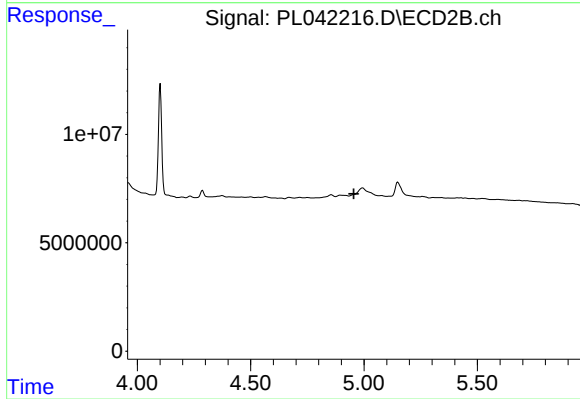

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

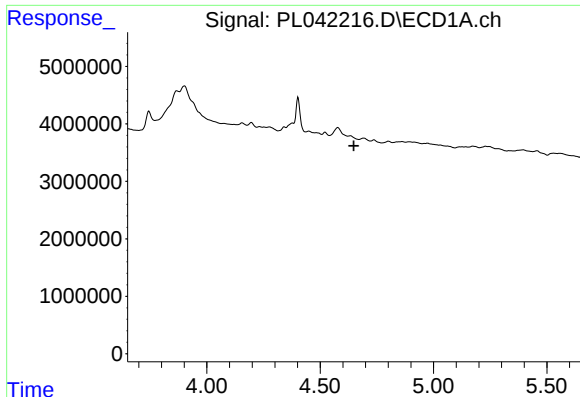

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

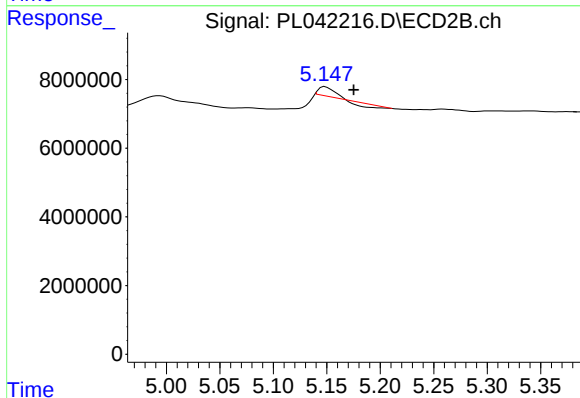


#7 delta-BHC

R.T.: 5.149 min
Delta R.T.: -0.027 min
Response: 669757
Conc: 0.17 ng/ml

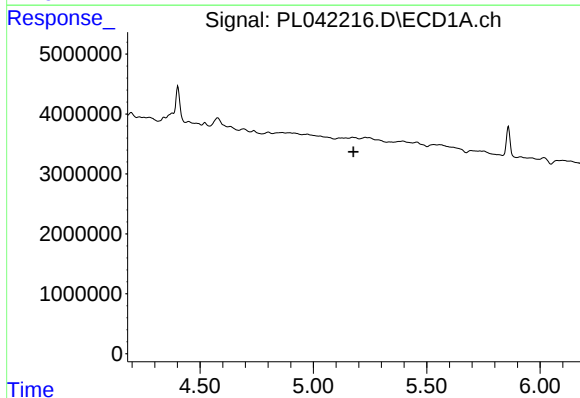


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.178 min
Response: 0
Conc: N.D.

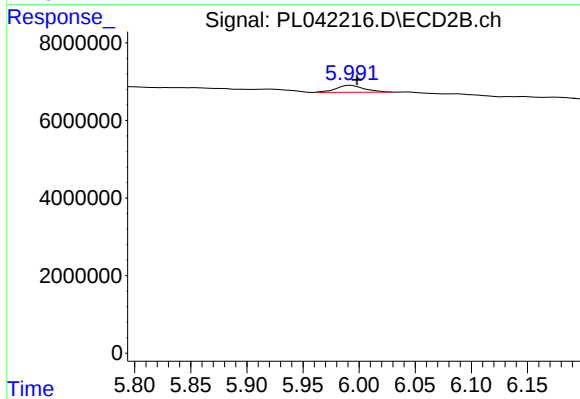

#8 Heptachlor epoxide


R.T.: 5.993 min
Delta R.T.: -0.006 min
Response: 3131973
Conc: 0.87 ng/ml

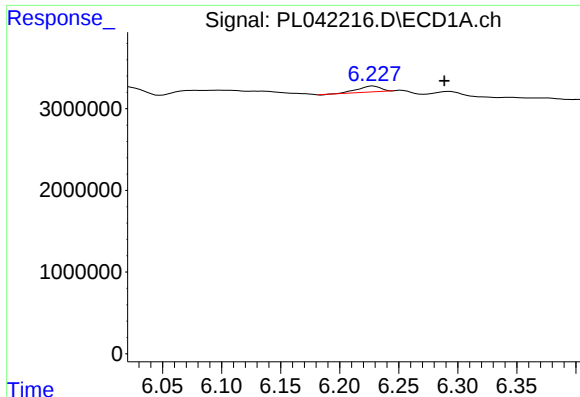

#15 Endosulfan II


R.T.: 6.228 min
Delta R.T.: -0.060 min
Response: 934231
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

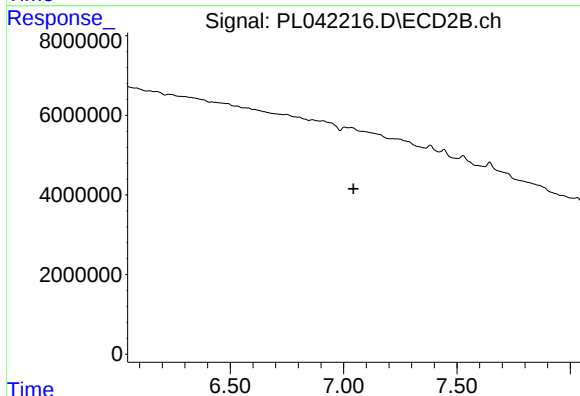


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

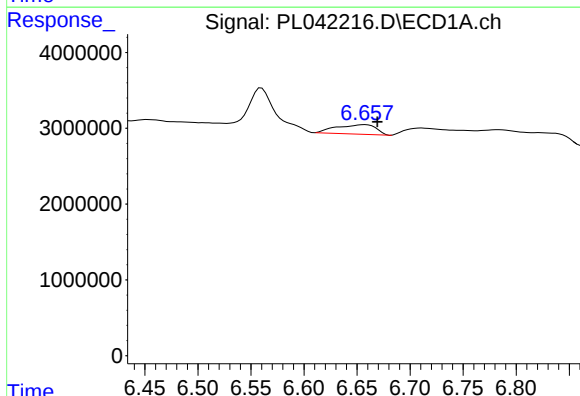


#19 Endosulfan Sulfate

R.T.: 6.657 min
Delta R.T.: -0.012 min
Response: 3247577
Conc: 0.51 ng/ml

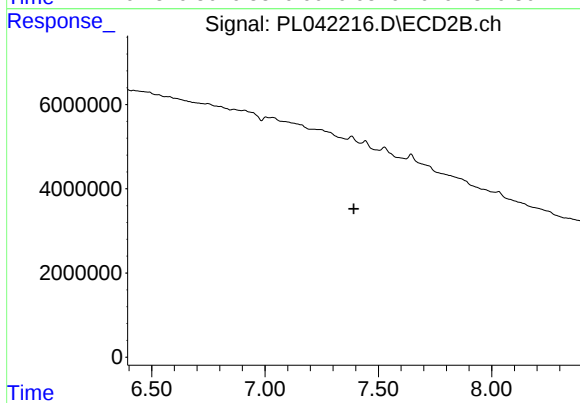

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

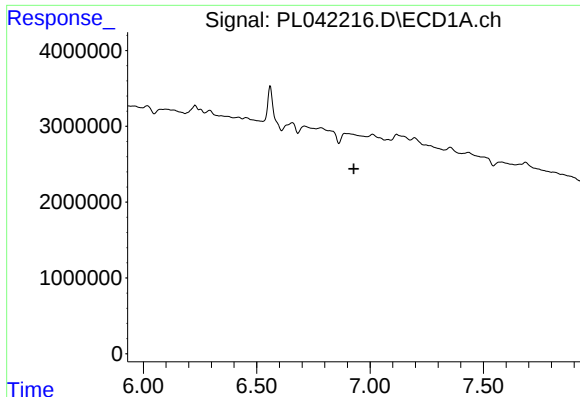

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.928 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

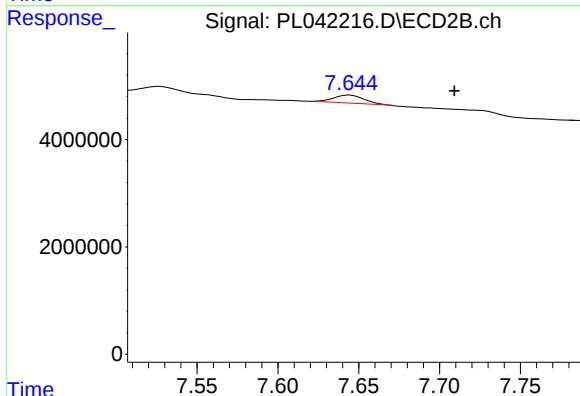


#20 Methoxychlor

R.T.: 7.645 min
Delta R.T.: -0.065 min
Response: 1571197
Conc: 1.14 ng/ml

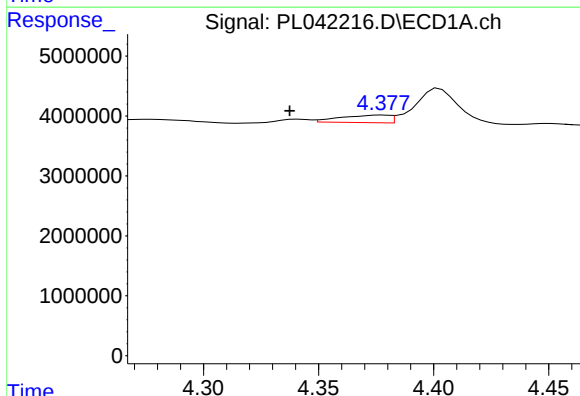


#23 Chlordane-1

R.T.: 4.378 min
Delta R.T.: 0.040 min
Response: 1858315
Conc: 6.23 ng/ml

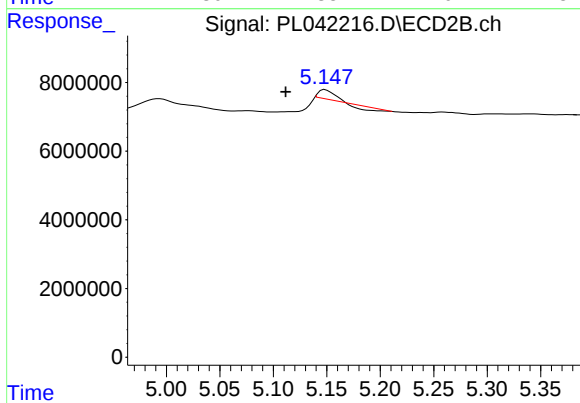

#23 Chlordane-1


R.T.: 5.149 min
Delta R.T.: 0.037 min
Response: 669757
Conc: 4.65 ng/ml

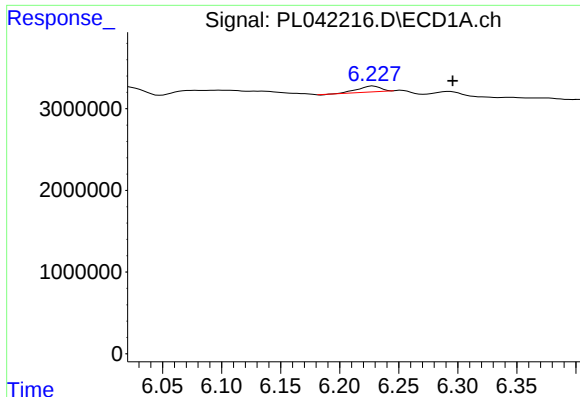

#27 Chlordane-5


R.T.: 6.228 min
Delta R.T.: -0.067 min
Response: 934231
Conc: 3.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

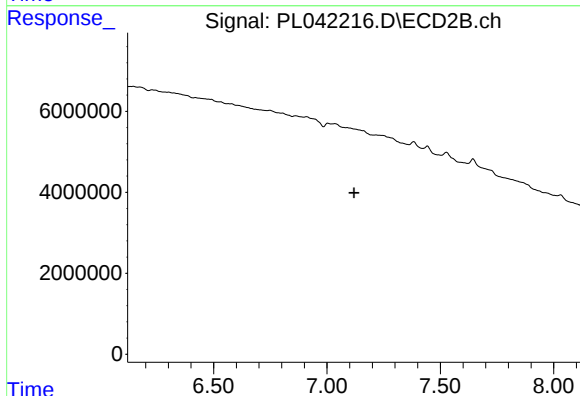


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.119 min
Response: 0
Conc: N.D.

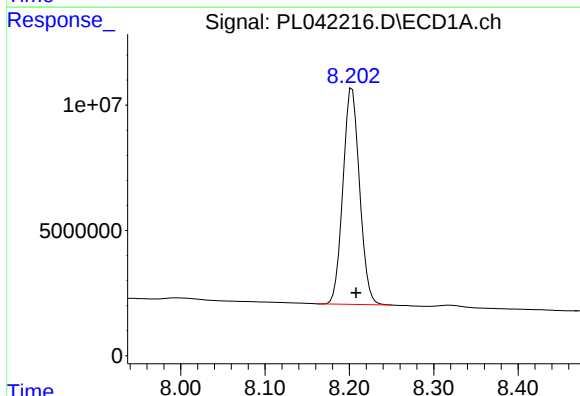

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.005 min
Response: 118337743
Conc: 17.27 ng/ml

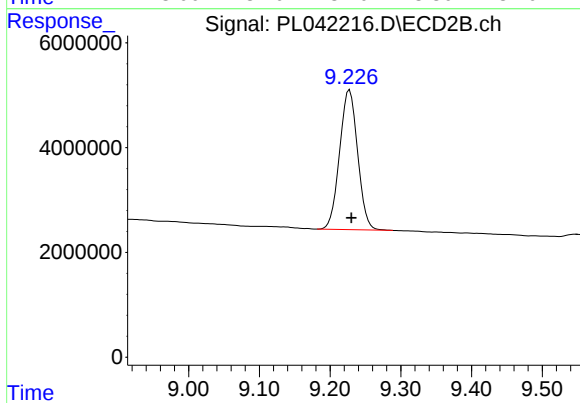

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: -0.003 min
Response: 47295563
Conc: 18.54 ng/ml